

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
 Data File : BN015315.D
 Acq On : 03 Jul 2021 02:33
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Jul 03 03:03:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 09:06:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.734	152	23039	0.40	ng	# 0.00
7) Naphthalene-d8	10.495	136	102210	0.40	ng	0.00
13) Acenaphthene-d10	14.345	164	54365	0.40	ng	0.00
19) Phenanthrene-d10	17.090	188	103564	0.40	ng	# 0.00
29) Chrysene-d12	21.280	240	80355	0.40	ng	#-0.02
35) Perylene-d12	23.529	264	66117	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.355	112	27404	0.47	ng	0.00
5) Phenol-d6	6.905	99	33285	0.45	ng	0.00
8) Nitrobenzene-d5	8.860	82	27824	0.49	ng	0.00
11) 2-Methylnaphthalene-d10	12.083	152	65990	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.842	330	7359	0.53	ng	0.00
15) 2-Fluorobiphenyl	12.962	172	84064	0.38	ng	0.00
27) Fluoranthene-d10	19.127	212	117227	0.38	ng	0.00
31) Terphenyl-d14	19.728	244	82390	0.44	ng	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.355	88	4356	0.40	ng	# 59
3) n-Nitrosodimethylamine	3.696	42	7960	0.39	ng	# 78
6) bis(2-Chloroethyl)ether	7.163	93	29544	0.41	ng	# 85
9) Naphthalene	10.546	128	115722	0.39	ng	97
10) Hexachlorobutadiene	10.837	225	21517	0.39	ng	# 98
12) 2-Methylnaphthalene	12.154	142	75603	0.40	ng	# 90
16) Acenaphthylene	14.053	152	96404	0.40	ng	98
17) Acenaphthene	14.408	154	65661	0.39	ng	98
18) Fluorene	15.398	166	79853	0.39	ng	99
20) 4,6-Dinitro-2-methylph...	15.474	198	253	0.33	ng	90
21) 4-Bromophenyl-phenylether	16.287	248	24849	0.38	ng	94
22) Hexachlorobenzene	16.397	284	27859	0.37	ng	# 92
23) Atrazine	16.555	200	17387	0.48	ng	94
24) Pentachlorophenol	16.750	266	4735	0.61	ng	100
25) Phenanthrene	17.127	178	127870	0.38	ng	99
26) Anthracene	17.224	178	109875	0.38	ng	99
28) Fluoranthene	19.157	202	141875	0.40	ng	# 97
30) Pyrene	19.519	202	140388	0.46	ng	99
32) Benzo(a)anthracene	21.270	228	109559	0.40	ng	97
33) Chrysene	21.323	228	118776	0.40	ng	98
34) Bis(2-ethylhexyl)phtha...	21.206	149	64497	0.77	ng	# 87
36) Indeno(1,2,3-cd)pyrene	25.788	276	73029	0.31	ng	# 88
37) Benzo(b)fluoranthene	22.858	252	106100	0.41	ng	# 93
38) Benzo(k)fluoranthene	22.902	252	106316	0.38	ng	# 94
39) Benzo(a)pyrene	23.429	252	89749	0.38	ng	# 84
40) Dibenzo(a,h)anthracene	25.802	278	54984	0.30	ng	# 90
41) Benzo(g,h,i)perylene	26.472	276	66411	0.32	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015315.D
Acq On : 03 Jul 2021 02:33
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Jul 03 03:03:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 01 09:06:31 2021
Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.734 min Scan# 505
 Delta R.T. 0.002 min
 Lab File: BN015315.D
 Acq: 03 Jul 2021 02:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:152 Resp: 23039
 Ion Ratio Lower Upper
 152 100
 150 153.5 119.0 178.6
 115 58.5 62.2 93.4#



#2
 1,4-Dioxane
 Concen: 0.40 ng
 RT: 3.355 min Scan# 30
 Delta R.T. 0.003 min
 Lab File: BN015315.D
 Acq: 03 Jul 2021 02:33

Tgt Ion: 88 Resp: 4356
 Ion Ratio Lower Upper
 88 100
 43 27.2 12.9 19.3#
 58 78.4 38.1 57.1#









#3
n-Nitrosodimethylamine
Concen: 0.39 ng
RT: 3.696 min Scan# 67
Delta R.T. 0.003 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 42 Resp: 7960
Ion Ratio Lower Upper
42 100
74 153.8 149.5 224.3
44 7.8 4.2 6.2#

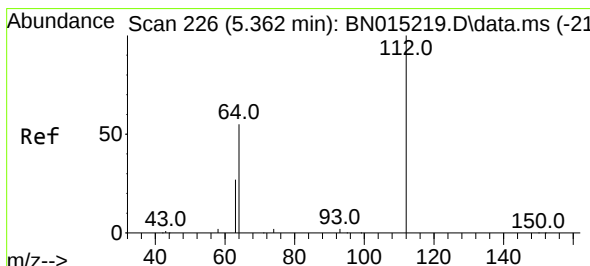

#4
2-Fluorophenol
Concen: 0.47 ng
RT: 5.355 min Scan# 247
Delta R.T. -0.007 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion: 112 Resp: 27404
Ion Ratio Lower Upper
112 100
64 55.9 39.0 58.6
63 27.9 20.6 30.8









#5
Phenol-d6
Concen: 0.45 ng
RT: 6.905 min Scan# 415
Delta R.T. 0.003 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 99 Resp: 33285
Ion Ratio Lower Upper
99 100
42 16.7 8.9 13.3#
71 30.1 35.6 53.4#



#6
bis(2-Chloroethyl)ether
Concen: 0.41 ng
RT: 7.163 min Scan# 443
Delta R.T. -0.007 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion: 93 Resp: 29544
Ion Ratio Lower Upper
93 100
63 74.4 46.6 70.0#
95 32.9 28.6 42.8









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.495 min Scan# 740
Delta R.T. 0.003 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:136	Resp:	102210
Ion Ratio	Lower	Upper
136	100	
137	11.0	9.8 14.8
54	5.8	5.4 8.2
68	5.0	4.9 7.3



#8
Nitrobenzene-d5
Concen: 0.49 ng
RT: 8.860 min Scan# 611
Delta R.T. -0.010 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion: 82	Resp:	27824
Ion Ratio	Lower	Upper
82	100	
128	34.5	31.6 47.4
54	54.0	29.0 43.4#









#9
Naphthalene
Concen: 0.39 ng
RT: 10.546 min Scan# 744
Delta R.T. 0.003 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:128 Resp: 115722
Ion Ratio Lower Upper
128 100
129 11.0 9.1 13.7
127 12.7 11.8 17.6



#10
Hexachlorobutadiene
Concen: 0.39 ng
RT: 10.837 min Scan# 767
Delta R.T. 0.003 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:225 Resp: 21517
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.3 50.2 75.2









#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 12.083 min Scan# 949
Delta R.T. -0.006 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 65990
Ion Ratio Lower Upper
152 100
151 20.3 16.7 25.1

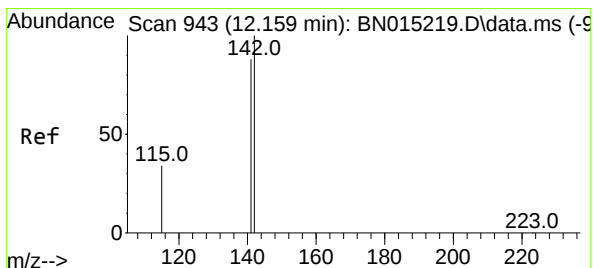

#12
2-Methylnaphthalene
Concen: 0.40 ng
RT: 12.154 min Scan# 965
Delta R.T. -0.006 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:142 Resp: 75603
Ion Ratio Lower Upper
142 100
141 89.2 72.3 108.5
115 33.7 40.7 61.1#









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.345 min Scan# 1189
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:164 Resp: 54365
Ion Ratio Lower Upper
164 100
162 99.0 83.8 125.6
160 43.8 37.4 56.0



#14
2,4,6-Tribromophenol
Concen: 0.53 ng
RT: 15.842 min Scan# 1307
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:330 Resp: 7359
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.7 22.4 33.6#









#15
2-Fluorobiphenyl
Concen: 0.38 ng
RT: 12.962 min Scan# 1080
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:172 Resp: 84064
Ion Ratio Lower Upper
172 100
171 34.4 30.6 45.8
170 22.8 20.2 30.4



#16
Acenaphthylene
Concen: 0.40 ng
RT: 14.053 min Scan# 1166
Delta R.T. -0.014 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:152 Resp: 96404
Ion Ratio Lower Upper
152 100
151 19.5 16.7 25.1
153 13.1 10.5 15.7









#17
Acenaphthene
Concen: 0.39 ng
RT: 14.408 min Scan# 1194
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 65661
Ion Ratio Lower Upper
154 100
153 112.9 90.9 136.3
152 54.5 45.8 68.8



#18
Fluorene
Concen: 0.39 ng
RT: 15.398 min Scan# 1272
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:166 Resp: 79853
Ion Ratio Lower Upper
166 100
165 97.4 79.2 118.8
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.090 min Scan# 1409
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:188 Resp: 103564
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.2 9.0 13.4#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.33 ng
RT: 15.474 min Scan# 1278
Delta R.T. -0.014 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:198 Resp: 253
Ion Ratio Lower Upper
198 100
182 36.7 34.5 51.7
77 0.0 0.0 0.0







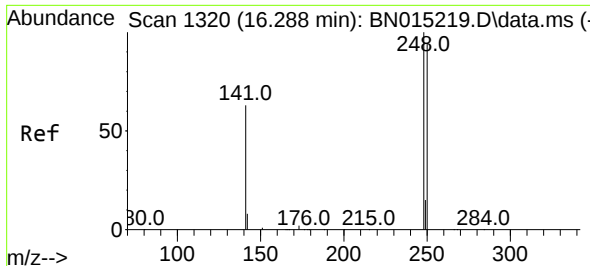

#21
4-Bromophenyl-phenylether
Concen: 0.38 ng
RT: 16.287 min Scan# 1343
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 24849
Ion Ratio Lower Upper
248 100
250 99.4 86.2 129.4
141 46.4 36.2 54.2



#22
Hexachlorobenzene
Concen: 0.37 ng
RT: 16.397 min Scan# 1352
Delta R.T. -0.013 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:284 Resp: 27859
Ion Ratio Lower Upper
284 100
142 34.6 22.2 33.2#
249 30.7 26.6 39.8









#23
Atrazine
Concen: 0.48 ng
RT: 16.555 min Scan# 1365
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:200 Resp: 17387
Ion Ratio Lower Upper
200 100
173 24.6 21.7 32.5
215 48.8 43.1 64.7



#24
Pentachlorophenol
Concen: 0.61 ng
RT: 16.750 min Scan# 1381
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:266 Resp: 4735
Ion Ratio Lower Upper
266 100
264 63.6 51.0 76.4
268 63.5 50.6 76.0









#25
Phenanthrene
Concen: 0.38 ng
RT: 17.127 min Scan# 1412
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178 Resp: 127870
Ion Ratio Lower Upper
178 100
176 18.9 15.6 23.4
179 15.3 12.1 18.1



#26
Anthracene
Concen: 0.38 ng
RT: 17.224 min Scan# 1420
Delta R.T. -0.001 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:178 Resp: 109875
Ion Ratio Lower Upper
178 100
176 18.1 15.1 22.7
179 15.4 12.2 18.2









#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 19.127 min Scan# 1709
Delta R.T. -0.006 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 117227
Ion Ratio Lower Upper
212 100
106 14.4 7.0 10.6#
104 7.8 4.1 6.1#



#28
Fluoranthene
Concen: 0.40 ng
RT: 19.157 min Scan# 1715
Delta R.T. -0.006 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:202 Resp: 141875
Ion Ratio Lower Upper
202 100
101 11.9 6.6 10.0#
203 17.3 13.9 20.9









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.280 min Scan# 2006
Delta R.T. -0.023 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 80355
Ion Ratio Lower Upper
240 100
120 16.0 4.2 6.4#
236 27.1 21.4 32.2



#30
Pyrene
Concen: 0.46 ng
RT: 19.519 min Scan# 1788
Delta R.T. -0.011 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:202 Resp: 140388
Ion Ratio Lower Upper
202 100
200 20.6 16.9 25.3
203 17.4 13.9 20.9









#31
 Terphenyl-d14
 Concen: 0.44 ng
 RT: 19.728 min Scan# 1830
 Delta R.T. -0.011 min
 Lab File: BN015315.D
 Acq: 03 Jul 2021 02:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:244 Resp: 82390
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.3 9.5
 122 14.3 6.2 9.2#



#32
 Benzo(a)anthracene
 Concen: 0.40 ng
 RT: 21.270 min Scan# 2005
 Delta R.T. -0.011 min
 Lab File: BN015315.D
 Acq: 03 Jul 2021 02:33

Tgt Ion:228 Resp: 109559
 Ion Ratio Lower Upper
 228 100
 226 26.4 23.0 34.6
 229 19.6 15.7 23.5









#33
Chrysene
Concen: 0.40 ng
RT: 21.323 min Scan# 2010
Delta R.T. -0.012 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	228	Resp:	118776
Ion Ratio	Lower	Upper	
228	100		
226	29.5	25.0	37.6
229	19.6	15.9	23.9

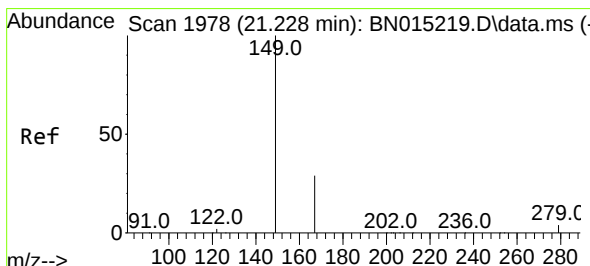

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.77 ng
RT: 21.206 min Scan# 1999
Delta R.T. -0.022 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33


Tgt Ion:	149	Resp:	64497
Ion Ratio	Lower	Upper	
149	100		
167	28.0	28.9	43.3#
279	3.6	4.9	7.3#








#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.529 min Scan# 2440
 Delta R.T. -0.021 min
 Lab File: BN015315.D
 Acq: 03 Jul 2021 02:33


Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC





Tgt Ion:264 Resp: 66117
 Ion Ratio Lower Upper
 264 100
 260 25.0 20.6 31.0
 265 22.9 21.4 32.2



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.31 ng
 RT: 25.788 min Scan# 3100
 Delta R.T. -0.025 min
 Lab File: BN015315.D
 Acq: 03 Jul 2021 02:33




Tgt Ion:276 Resp: 73029
 Ion Ratio Lower Upper
 276 100
 138 25.6 10.0 15.0#
 277 25.0 20.4 30.6








#37
Benzo(b)fluoranthene
Concen: 0.41 ng
RT: 22.858 min Scan# 2244
Delta R.T. -0.018 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC






Tgt Ion:252 Resp: 106100
Ion Ratio Lower Upper
252 100
253 23.1 18.5 27.7
125 18.0 5.8 8.6#



#38
Benzo(k)fluoranthene
Concen: 0.38 ng
RT: 22.902 min Scan# 2257
Delta R.T. -0.018 min
Lab File: BN015315.D
Acq: 03 Jul 2021 02:33

Tgt Ion:252 Resp: 106316
Ion Ratio Lower Upper
252 100
253 22.0 19.1 28.7
125 11.0 5.4 8.0#





#39

Benzo(a)pyrene

Concen: 0.38 ng

RT: 23.429 min Scan# 2411

Delta R.T. -0.025 min

Lab File: BN015315.D

Acq: 03 Jul 2021 02:33





Tgt Ion:252	Resp:	89749
Ion Ratio	Lower	Upper
252	100	
253	24.5	19.4 29.2
125	30.4	7.4 11.2#

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC



#40

Dibenzo(a,h)anthracene

Concen: 0.30 ng




RT: 25.802 min Scan# 3104


Delta R.T. -0.025 min

Lab File: BN015315.D

Acq: 03 Jul 2021 02:33

Tgt Ion:278	Resp:	54984
Ion Ratio	Lower	Upper
278	100	
139	19.2	9.0 13.4#
279	23.6	21.0 31.4



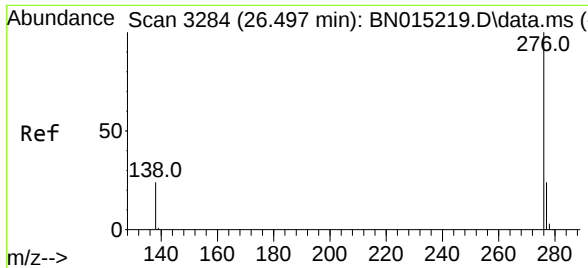

#41
 Benzo(g,h,i)perylene
 Concen: 0.32 ng
 RT: 26.472 min Scan# 3300
 Delta R.T. -0.025 min
 Lab File: BN015315.D
 Acq: 03 Jul 2021 02:33

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:	276	Resp:	66411
Ion	Ratio	Lower	Upper
276	100		
277	23.8	19.7	29.5
138	23.9	9.8	14.6#

