
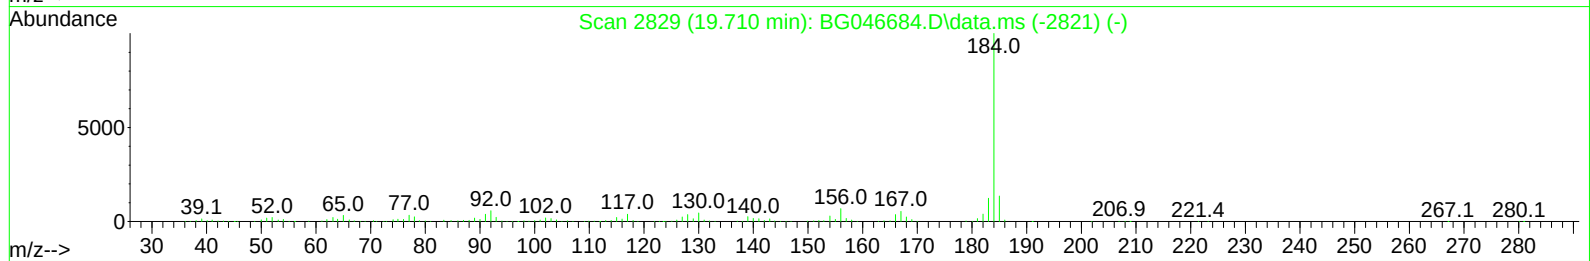
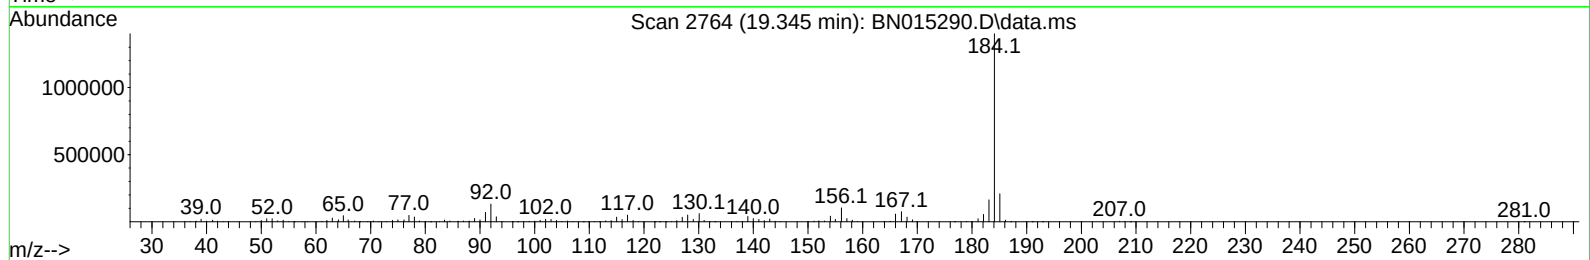


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015290.D
Acq On : 02 Jul 2021 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 12:03:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

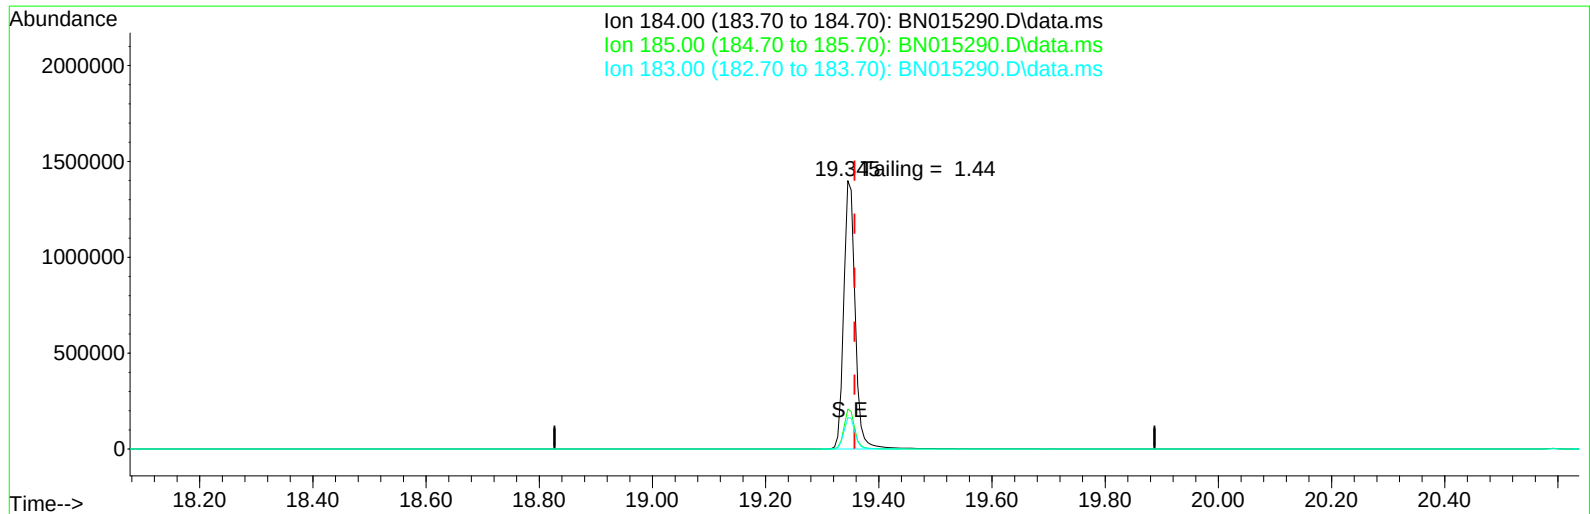

TIC: BN015290.D\data.ms

(77) Benzidine




19.345min (-0.012) 0.00 ng

response 1962176

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.88
183.00	13.20	11.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
 Data File : BN015290.D
 Acq On : 02 Jul 2021 10:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 12:03:53 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 10:10:58 2021
 Response via : Initial Calibration

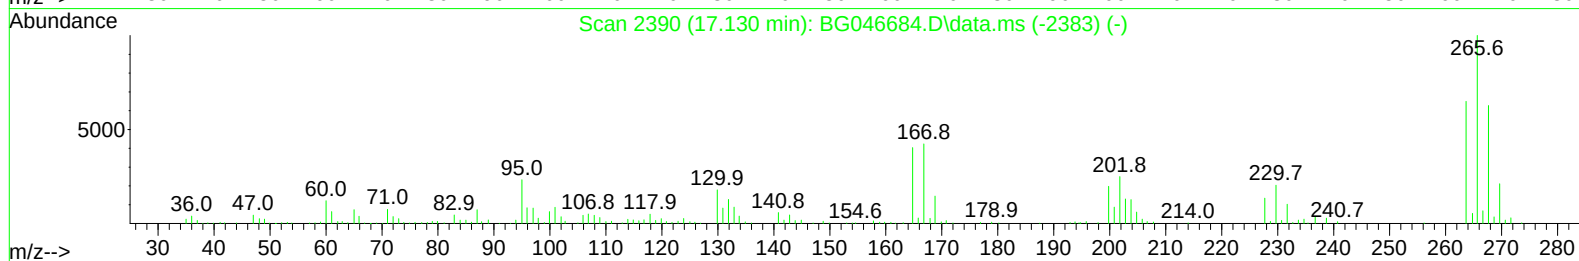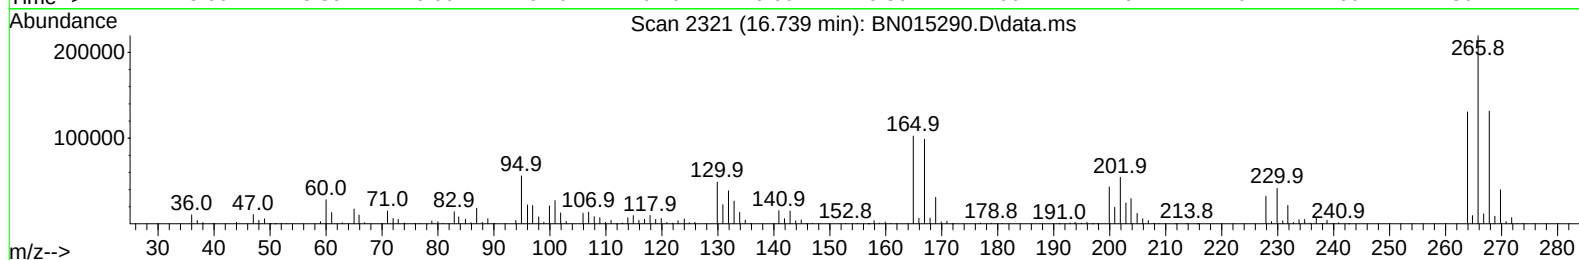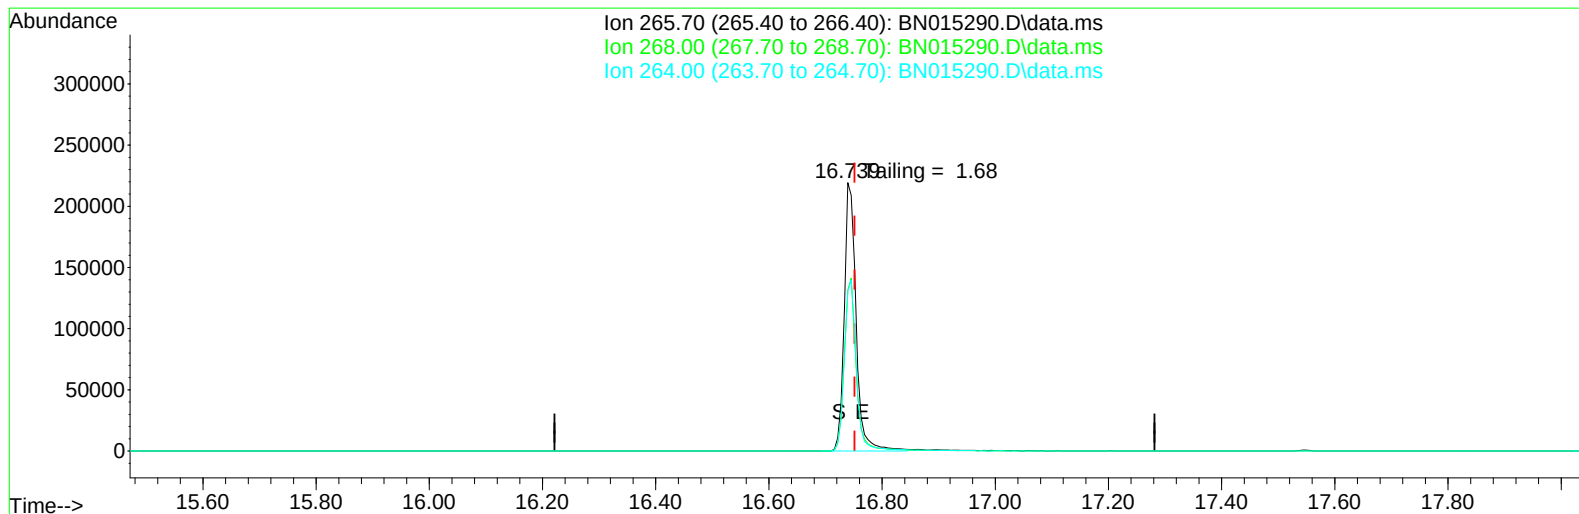

TIC: BN015290.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 23483.69 ng

response 320856

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.99
264.00	61.60	59.55
0.00	0.00	0.00