
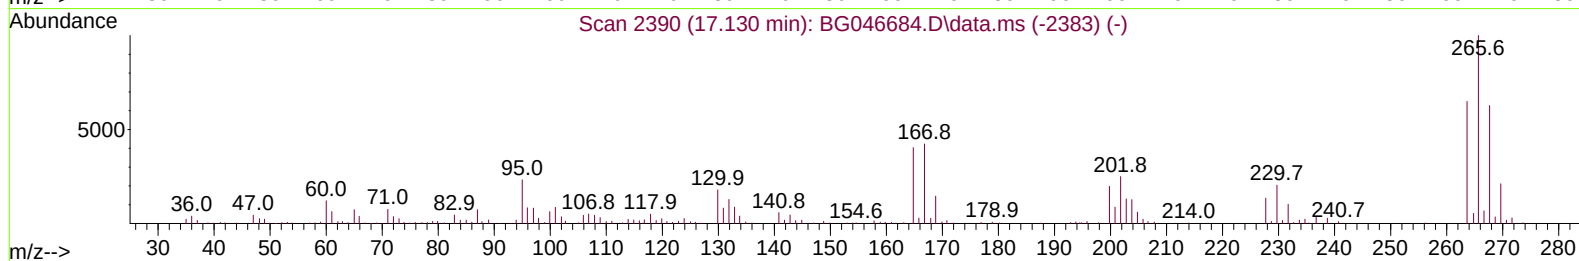
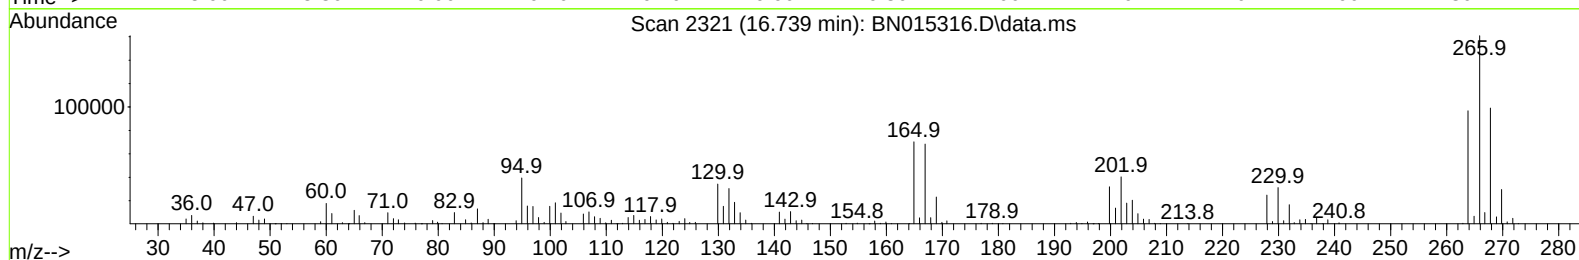


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\  
Data File : BN015316.D  
Acq On    : 03 Jul 2021  04:20  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 03 05:02:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

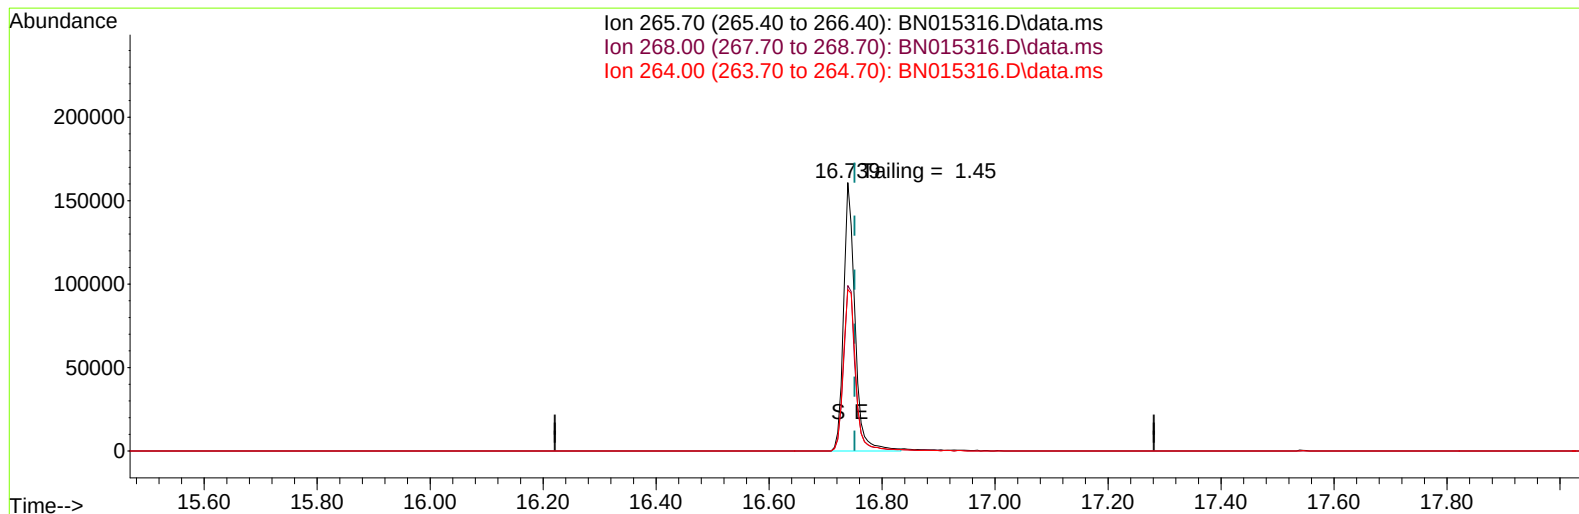

TIC: BN015316.D\data.ms

(70) Pentachlorophenol (C)




16.739min (-0.012) 22931.18 ng

response **227647**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.63
264.00	61.60	60.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015316.D
Acq On : 03 Jul 2021 04:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 05:02:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

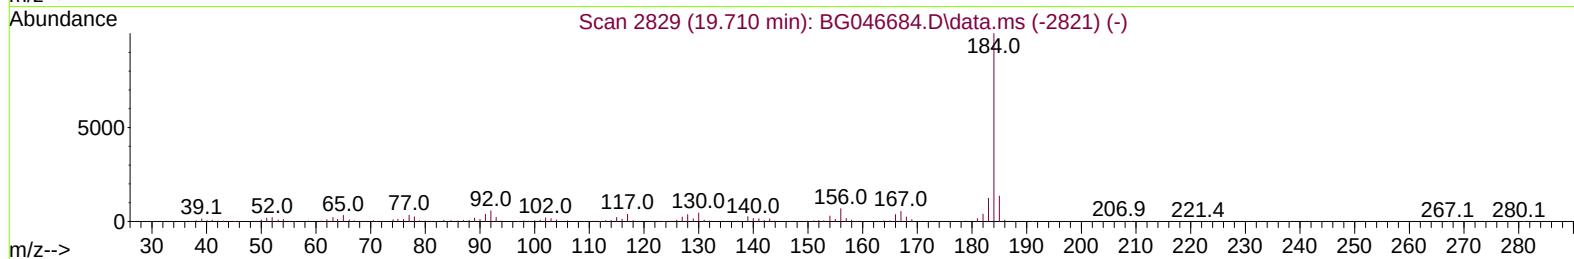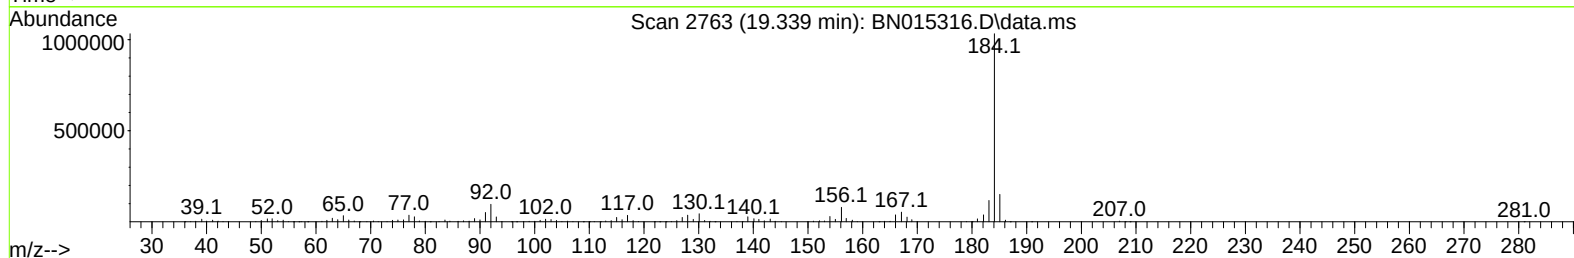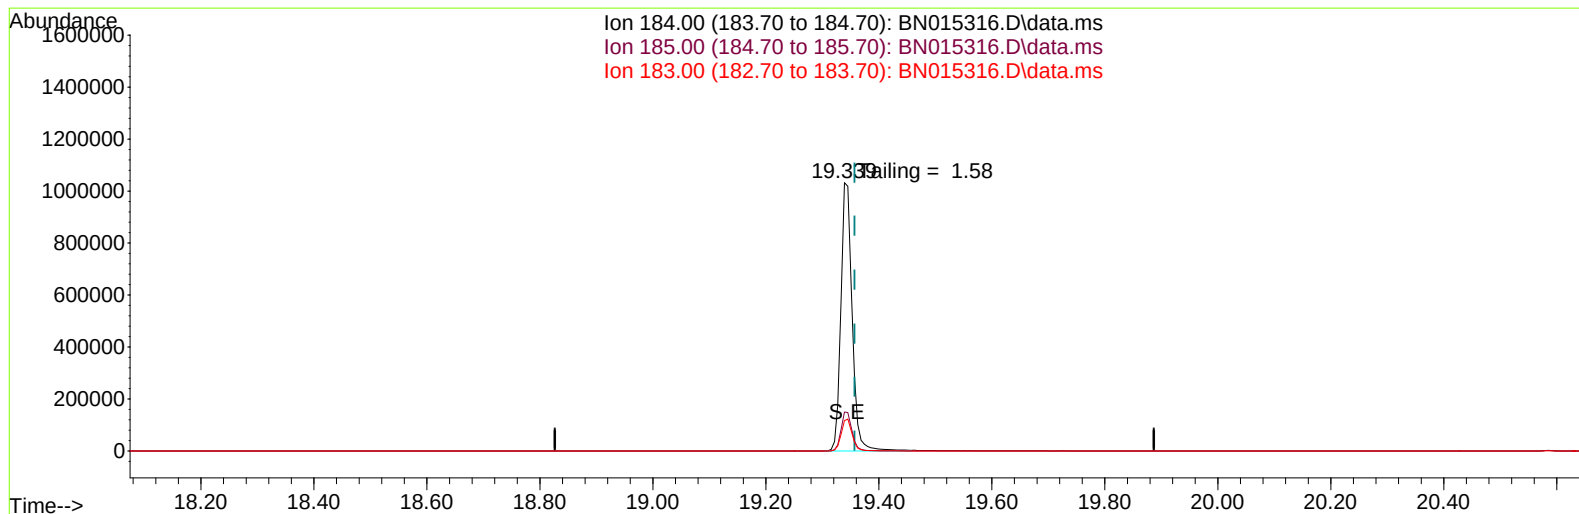

TIC: BN015316.D\data.ms

(77) Benzidine

19.339min (-0.018) 0.00 ng

response 1429184

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.57
183.00	13.20	11.37
0.00	0.00	0.00