

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
 Data File : BN015298.D
 Acq On : 02 Jul 2021 16:18
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Manual Integrations
 APPROVED

mohammad
 7/6/2021 10:02:58 AM

Quant Time: Jul 02 17:07:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 09:06:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.735	152	19519	0.40	ng	# 0.00
7) Naphthalene-d8	10.495	136	85409	0.40	ng	0.00
13) Acenaphthene-d10	14.345	164	43906	0.40	ng	0.00
19) Phenanthrene-d10	17.090	188	82073	0.40	ng	0.00
29) Chrysene-d12	21.291	240	59462	0.40	ng	#-0.01
35) Perylene-d12	23.543	264	42994	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.356	112	21515	0.43	ng	0.00
5) Phenol-d6	6.905	99	25920	0.41	ng	0.00
8) Nitrobenzene-d5	8.860	82	21062	0.44	ng	0.00
11) 2-Methylnaphthalene-d10	12.083	152	54365	0.38	ng	0.00
14) 2,4,6-Tribromophenol	15.842	330	4647	0.47	ng	0.00
15) 2-Fluorobiphenyl	12.962	172	70251	0.39	ng	0.00
27) Fluoranthene-d10	19.127	212	89198	0.37	ng	0.00
31) Terphenyl-d14	19.733	244	63273	0.45	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.345	88	3312m	0.36	ng	
3) n-Nitrosodimethylamine	3.696	42	6296	0.37	ng	# 76
6) bis(2-Chloroethyl)ether	7.163	93	24912	0.40	ng	# 85
9) Naphthalene	10.546	128	96705	0.39	ng	97
10) Hexachlorobutadiene	10.837	225	18201	0.39	ng	# 99
12) 2-Methylnaphthalene	12.158	142	62639	0.40	ng	# 88
16) Acenaphthylene	14.066	152	73626	0.38	ng	98
17) Acenaphthene	14.408	154	52918	0.39	ng	99
18) Fluorene	15.398	166	64059	0.39	ng	99
20) 4,6-Dinitro-2-methylph...	15.474	198	286	0.38	ng	92
21) 4-Bromophenyl-phenylether	16.287	248	19844	0.38	ng	89
22) Hexachlorobenzene	16.397	284	23073	0.39	ng	# 91
23) Atrazine	16.555	200	11754	0.43	ng	93
24) Pentachlorophenol	16.750	266	2940	0.53	ng	99
25) Phenanthrene	17.127	178	103931	0.39	ng	99
26) Anthracene	17.224	178	83757	0.37	ng	99
28) Fluoranthene	19.157	202	110151	0.39	ng	# 97
30) Pyrene	19.525	202	106788	0.47	ng	99
32) Benzo(a)anthracene	21.280	228	73480	0.36	ng	96
33) Chrysene	21.323	228	87422	0.39	ng	99
34) Bis(2-ethylhexyl)phtha...	21.217	149	28144	0.53	ng	# 87
36) Indeno(1,2,3-cd)pyrene	25.805	276	43066	0.28	ng	# 88
37) Benzo(b)fluoranthene	22.865	252	69538	0.41	ng	# 95
38) Benzo(k)fluoranthene	22.909	252	70907	0.39	ng	# 95
39) Benzo(a)pyrene	23.443	252	55987	0.36	ng	# 93
40) Dibenzo(a,h)anthracene	25.822	278	31178	0.26	ng	# 91
41) Benzo(g,h,i)perylene	26.486	276	41553	0.31	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015298.D
Acq On : 02 Jul 2021 16:18
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM


Quant Time: Jul 02 17:07:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 01 09:06:31 2021
Response via : Initial Calibration





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.735 min Scan# 505
 Delta R.T. 0.003 min
 Lab File: BN015298.D
 Acq: 02 Jul 2021 16:18




Instrument :
 BNA_N
 ClientSampled :
 SSTDCCC0.4




Tgt Ion:152 Resp: 19519
 Ion Ratio Lower Upper
 152 100
 150 155.6 119.0 178.6
 115 60.0 62.2 93.4#

Manual Integrations
 APPROVED



mohammad
 7/6/2021 10:02:58 AM



#2
 1,4-Dioxane
 Concen: 0.36 ng m
 RT: 3.345 min Scan# 29
 Delta R.T. -0.006 min
 Lab File: BN015298.D
 Acq: 02 Jul 2021 16:18



Tgt Ion: 88 Resp: 3312
 Ion Ratio Lower Upper
 88 100
 43 27.2 12.9 19.3#
 58 75.9 38.1 57.1#









#3
n-Nitrosodimethylamine
Concen: 0.37 ng
RT: 3.696 min Scan# 67
Delta R.T. 0.003 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion: 42 Resp: 6296
Ion Ratio Lower Upper
42 100
74 151.8 149.5 224.3
44 7.4 4.2 6.2#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
7/6/2021 10:02:58 AM



#4
2-Fluorophenol
Concen: 0.43 ng
RT: 5.356 min Scan# 247
Delta R.T. -0.006 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion: 112 Resp: 21515
Ion Ratio Lower Upper
112 100
64 55.9 39.0 58.6
63 27.9 20.6 30.8



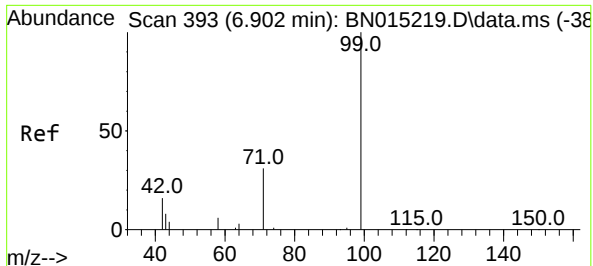





#5
Phenol-d6
Concen: 0.41 ng
RT: 6.905 min Scan# 415
Delta R.T. 0.003 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion: 99 Resp: 25920
Ion Ratio Lower Upper
99 100
42 16.7 8.9 13.3#
71 30.2 35.6 53.4#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM



#6
bis(2-Chloroethyl)ether
Concen: 0.40 ng
RT: 7.163 min Scan# 443
Delta R.T. -0.006 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18


Tgt Ion: 93 Resp: 24912
Ion Ratio Lower Upper
93 100
63 74.2 46.6 70.0#
95 32.8 28.6 42.8





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.495 min Scan# 740
Delta R.T. 0.003 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



Tgt Ion:	136	Resp:	85409
Ion Ratio	Lower	Upper	
136	100		
137	11.0	9.8	14.8
54	6.2	5.4	8.2
68	5.4	4.9	7.3




Manual Integrations
APPROVED


mohammad
7/6/2021 10:02:58 AM



#8
Nitrobenzene-d5
Concen: 0.44 ng
RT: 8.860 min Scan# 611
Delta R.T. -0.010 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:	82	Resp:	21062
Ion Ratio	Lower	Upper	
82	100		
128	33.2	31.6	47.4
54	54.6	29.0	43.4



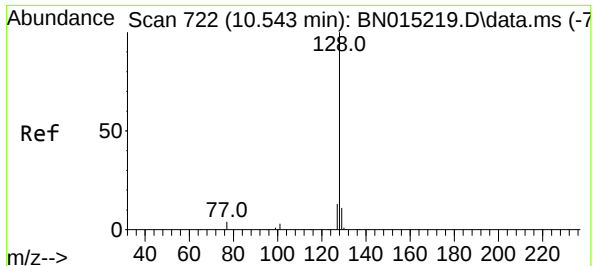





#9
Naphthalene
Concen: 0.39 ng
RT: 10.546 min Scan# 744
Delta R.T. 0.003 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:	128	Resp:	96705
Ion Ratio	Lower	Upper	
128	100		
129	10.9	9.1	13.7
127	12.7	11.8	17.6

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM



#10
Hexachlorobutadiene
Concen: 0.39 ng
RT: 10.837 min Scan# 767
Delta R.T. 0.003 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:	225	Resp:	18201
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.5	50.2	75.2









#11
2-Methylnaphthalene-d10
Concen: 0.38 ng
RT: 12.083 min Scan# 949
Delta R.T. -0.005 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:152 Resp: 54365
Ion Ratio Lower Upper
152 100
151 20.4 16.7 25.1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
7/6/2021 10:02:58 AM



#12
2-Methylnaphthalene
Concen: 0.40 ng
RT: 12.158 min Scan# 966
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18


Tgt Ion:142 Resp: 62639
Ion Ratio Lower Upper
142 100
141 87.1 72.3 108.5
115 32.5 40.7 61.1#





#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.345 min Scan# 1189
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



Tgt Ion:164 Resp: 43906
Ion Ratio Lower Upper
164 100
162 100.9 83.8 125.6
160 45.4 37.4 56.0




Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM




#14
2,4,6-Tribromophenol
Concen: 0.47 ng
RT: 15.842 min Scan# 1307
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:330 Resp: 4647
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 37.3 22.4 33.6#









#15
2-Fluorobiphenyl
Concen: 0.39 ng
RT: 12.962 min Scan# 1080
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18





Tgt Ion:172 Resp: 70251
Ion Ratio Lower Upper
172 100
171 34.9 30.6 45.8
170 23.5 20.2 30.4



#16
Acenaphthylene
Concen: 0.38 ng
RT: 14.066 min Scan# 1167
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18



Tgt Ion:152 Resp: 73626
Ion Ratio Lower Upper
152 100
151 19.5 16.7 25.1
153 13.0 10.5 15.7




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED




mohammad
7/6/2021 10:02:58 AM




#17
Acenaphthene
Concen: 0.39 ng
RT: 14.408 min Scan# 1194
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18





Tgt Ion:154 Resp: 52918
Ion Ratio Lower Upper
154 100
153 113.1 90.9 136.3
152 55.5 45.8 68.8



#18
Fluorene
Concen: 0.39 ng
RT: 15.398 min Scan# 1272
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18




Tgt Ion:166 Resp: 64059
Ion Ratio Lower Upper
166 100
165 97.6 79.2 118.8
167 13.5 10.7 16.1



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM







#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.090 min Scan# 1409
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:188 Resp: 82073
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.6 9.0 13.4

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
7/6/2021 10:02:58 AM




#20
4,6-Dinitro-2-methylphenol
Concen: 0.38 ng
RT: 15.474 min Scan# 1278
Delta R.T. -0.014 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:198 Resp: 286
Ion Ratio Lower Upper
198 100
182 37.9 34.5 51.7
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.38 ng
RT: 16.287 min Scan# 1343
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18





Tgt Ion:248 Resp: 19844
Ion Ratio Lower Upper
248 100
250 97.8 86.2 129.4
141 53.6 36.2 54.2



#22
Hexachlorobenzene
Concen: 0.39 ng
RT: 16.397 min Scan# 1352
Delta R.T. -0.013 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18




Tgt Ion:284 Resp: 23073
Ion Ratio Lower Upper
284 100
142 34.9 22.2 33.2#
249 30.7 26.6 39.8



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM



#23

Atrazine

Concen: 0.43 ng

RT: 16.555 min Scan# 1365

Delta R.T. -0.001 min

Lab File: BN015298.D

Acq: 02 Jul 2021 16:18

Tgt Ion:	200	Resp:	11754
Ion Ratio	Lower	Upper	
200	100		
173	25.8	21.7	32.5
215	47.6	43.1	64.7

Instrument :





BNA_N

ClientSampleId :

SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM



#24

Pentachlorophenol

Concen: 0.53 ng




RT: 16.750 min Scan# 1381

Delta R.T. -0.001 min

Lab File: BN015298.D

Acq: 02 Jul 2021 16:18


Tgt Ion:	266	Resp:	2940
Ion Ratio	Lower	Upper	
266	100		
264	62.8	51.0	76.4
268	64.7	50.6	76.0





#25
Phenanthrene
Concen: 0.39 ng
RT: 17.127 min Scan# 1412
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



Tgt Ion:178 Resp: 103931
Ion Ratio Lower Upper
178 100
176 18.8 15.6 23.4
179 15.3 12.1 18.1




Manual Integrations
APPROVED


mohammad
7/6/2021 10:02:58 AM




#26
Anthracene
Concen: 0.37 ng
RT: 17.224 min Scan# 1420
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:178 Resp: 83757
Ion Ratio Lower Upper
178 100
176 18.2 15.1 22.7
179 15.3 12.2 18.2






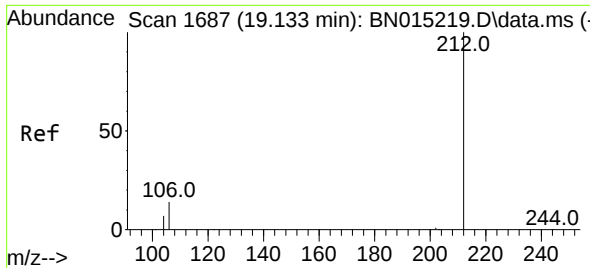


#27
Fluoranthene-d10
Concen: 0.37 ng
RT: 19.127 min Scan# 1709
Delta R.T. -0.006 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18





Tgt Ion:212 Resp: 89198
Ion Ratio Lower Upper
212 100
106 14.3 7.0 10.6#
104 7.8 4.1 6.1#



#28
Fluoranthene
Concen: 0.39 ng
RT: 19.157 min Scan# 1715
Delta R.T. -0.006 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18




Tgt Ion:202 Resp: 110151
Ion Ratio Lower Upper
202 100
101 11.9 6.6 10.0#
203 17.4 13.9 20.9




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED




mohammad
7/6/2021 10:02:58 AM




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.291 min Scan# 2007
Delta R.T. -0.012 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18





Tgt Ion:240 Resp: 59462
Ion Ratio Lower Upper
240 100
120 9.9 4.2 6.4#
236 26.2 21.4 32.2



#30
Pyrene
Concen: 0.47 ng
RT: 19.525 min Scan# 1789
Delta R.T. -0.005 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18




Tgt Ion:202 Resp: 106788
Ion Ratio Lower Upper
202 100
200 20.6 16.9 25.3
203 17.4 13.9 20.9



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM



#31
Terphenyl-d14
Concen: 0.45 ng
RT: 19.733 min Scan# 1831
Delta R.T. -0.006 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Tgt Ion:244 Resp: 63273
Ion Ratio Lower Upper
244 100
212 7.7 6.3 9.5
122 13.0 6.2 9.2#

Manual Integrations
APPROVED



mohammad
7/6/2021 10:02:58 AM



#32
Benzo(a)anthracene
Concen: 0.36 ng
RT: 21.280 min Scan# 2006
Delta R.T. -0.001 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18



Tgt Ion:228 Resp: 73480
Ion Ratio Lower Upper
228 100
226 25.6 23.0 34.6
229 20.1 15.7 23.5









#33
Chrysene
Concen: 0.39 ng
RT: 21.323 min Scan# 2010
Delta R.T. -0.012 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:228 Resp: 87422
Ion Ratio Lower Upper
228 100
226 30.7 25.0 37.6
229 19.2 15.9 23.9

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED


mohammad
7/6/2021 10:02:58 AM



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.53 ng
RT: 21.217 min Scan# 2000
Delta R.T. -0.011 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:149 Resp: 28144
Ion Ratio Lower Upper
149 100
167 27.8 28.9 43.3#
279 3.4 4.9 7.3#





#35

Perylene-d12

Concen: 0.40 ng

RT: 23.543 min Scan# 2444

Delta R.T. -0.007 min

Lab File: BN015298.D

Acq: 02 Jul 2021 16:18

Tgt Ion:	264	Resp:	42994
Ion Ratio	Lower	Upper	
264	100		
260	25.1	20.6	31.0
265	23.7	21.4	32.2

Instrument :





BNA_N

ClientSampleId :

SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.28 ng




RT: 25.805 min Scan# 3105

Delta R.T. -0.008 min

Lab File: BN015298.D

Acq: 02 Jul 2021 16:18

Tgt Ion:	276	Resp:	43066
Ion Ratio	Lower	Upper	
276	100		
138	25.5	10.0	15.0#
277	25.0	20.4	30.6









#37
Benzo(b)fluoranthene
Concen: 0.41 ng
RT: 22.865 min Scan# 2246
Delta R.T. -0.011 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:252 Resp: 69538
Ion Ratio Lower Upper
252 100
253 22.1 18.5 27.7
125 11.8 5.8 8.6#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM



#38
Benzo(k)fluoranthene
Concen: 0.39 ng
RT: 22.909 min Scan# 2259
Delta R.T. -0.011 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18

Tgt Ion:252 Resp: 70907
Ion Ratio Lower Upper
252 100
253 22.3 19.1 28.7
125 10.8 5.4 8.0#





#39

Benzo(a)pyrene

Concen: 0.36 ng

RT: 23.443 min Scan# 2415

Delta R.T. -0.011 min

Lab File: BN015298.D

Acq: 02 Jul 2021 16:18

Tgt Ion:	252	Resp:	55987
Ion Ratio	Lower	Upper	
252	100		
253	23.0	19.4	29.2
125	15.5	7.4	11.2#

Instrument :





BNA_N

ClientSampleId :

SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM



#40

Dibenzo(a,h)anthracene

Concen: 0.26 ng




RT: 25.822 min Scan# 3110


Delta R.T. -0.004 min

Lab File: BN015298.D


Acq: 02 Jul 2021 16:18

Tgt Ion:	278	Resp:	31178
Ion Ratio	Lower	Upper	
278	100		
139	18.6	9.0	13.4#
279	23.9	21.0	31.4







#41
Benzo(g,h,i)perylene
Concen: 0.31 ng
RT: 26.486 min Scan# 3304
Delta R.T. -0.011 min
Lab File: BN015298.D
Acq: 02 Jul 2021 16:18



Tgt Ion: 276 Resp: 41553
Ion Ratio Lower Upper
276 100
277 24.0 19.7 29.5
138 24.0 9.8 14.6#



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
7/6/2021 10:02:58 AM