

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
 Data File : BN015334.D
 Acq On : 03 Jul 2021 15:00
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Manual Integrations
 APPROVED

mohammad
 7/6/2021 10:04:18 AM

Quant Time: Jul 05 05:50:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 09:06:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.726	152	23456	0.40	ng	# 0.00
7) Naphthalene-d8	10.496	136	103435	0.40	ng	# 0.00
13) Acenaphthene-d10	14.345	164	55106	0.40	ng	0.00
19) Phenanthrene-d10	17.091	188	102517	0.40	ng	# 0.00
29) Chrysene-d12	21.291	240	78310	0.40	ng	-0.01
35) Perylene-d12	23.533	264	61938	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.356	112	27532	0.46	ng	0.00
5) Phenol-d6	6.896	99	33468	0.44	ng	0.00
8) Nitrobenzene-d5	8.861	82	28464	0.49	ng	0.00
11) 2-Methylnaphthalene-d10	12.079	152	67060	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.829	330	7215	0.52	ng	-0.01
15) 2-Fluorobiphenyl	12.962	172	86015	0.38	ng	0.00
27) Fluoranthene-d10	19.128	212	116427	0.38	ng	0.00
31) Terphenyl-d14	19.728	244	82153	0.45	ng	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.346	88	3933m	0.36	ng	
3) n-Nitrosodimethylamine	3.687	42	7954	0.39	ng	# 77
6) bis(2-Chloroethyl)ether	7.163	93	30230	0.41	ng	# 85
9) Naphthalene	10.546	128	116977	0.39	ng	97
10) Hexachlorobutadiene	10.838	225	22064	0.39	ng	# 99
12) 2-Methylnaphthalene	12.154	142	76938	0.40	ng	# 90
16) Acenaphthylene	14.053	152	97755	0.40	ng	98
17) Acenaphthene	14.408	154	66434	0.39	ng	99
18) Fluorene	15.385	166	80674	0.39	ng	99
20) 4,6-Dinitro-2-methylph...	15.474	198	347	0.37	ng	# 81
21) 4-Bromophenyl-phenylether	16.288	248	25253	0.39	ng	94
22) Hexachlorobenzene	16.397	284	28492	0.39	ng	# 92
23) Atrazine	16.555	200	17251	0.48	ng	93
24) Pentachlorophenol	16.750	266	4504	0.60	ng	99
25) Phenanthrene	17.127	178	128942	0.39	ng	99
26) Anthracene	17.225	178	109137	0.39	ng	99
28) Fluoranthene	19.157	202	141276	0.40	ng	# 97
30) Pyrene	19.520	202	139648	0.47	ng	99
32) Benzo(a)anthracene	21.270	228	108176	0.40	ng	98
33) Chrysene	21.323	228	113186	0.39	ng	98
34) Bis(2-ethylhexyl)phtha...	21.206	149	56298	0.71	ng	# 87
36) Indeno(1,2,3-cd)pyrene	25.788	276	65556	0.30	ng	# 88
37) Benzo(b)fluoranthene	22.858	252	102472	0.42	ng	# 93
38) Benzo(k)fluoranthene	22.903	252	98034	0.38	ng	# 94
39) Benzo(a)pyrene	23.433	252	82106	0.37	ng	# 86
40) Dibenzo(a,h)anthracene	25.805	278	48823	0.28	ng	# 91
41) Benzo(g,h,i)perylene	26.473	276	59840	0.31	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015334.D
Acq On : 03 Jul 2021 15:00
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED


mohammad
7/6/2021 10:04:18 AM

Quant Time: Jul 05 05:50:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 01 09:06:31 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.726 min Scan# 504
 Delta R.T. -0.006 min
 Lab File: BN015334.D
 Acq: 03 Jul 2021 15:00





Tgt Ion: 152 Resp: 23456
 Ion Ratio Lower Upper
 152 100
 150 157.7 119.0 178.6
 115 61.6 62.2 93.4#



#2
 1,4-Dioxane
 Concen: 0.36 ng m
 RT: 3.346 min Scan# 29
 Delta R.T. -0.006 min
 Lab File: BN015334.D
 Acq: 03 Jul 2021 15:00



Tgt Ion: 88 Resp: 3933
 Ion Ratio Lower Upper
 88 100
 43 27.7 12.9 19.3#
 58 76.7 38.1 57.1#



Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Manual Integrations
 APPROVED

mohammad
 7/6/2021 10:04:18 AM







#3
n-Nitrosodimethylamine
Concen: 0.39 ng
RT: 3.687 min Scan# 66
Delta R.T. -0.006 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion: 42 Resp: 7954
Ion Ratio Lower Upper
42 100
74 152.6 149.5 224.3
44 6.9 4.2 6.2#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED

mohammad
7/6/2021 10:04:18 AM




#4
2-Fluorophenol
Concen: 0.46 ng
RT: 5.356 min Scan# 247
Delta R.T. -0.006 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion: 112 Resp: 27532
Ion Ratio Lower Upper
112 100
64 56.1 39.0 58.6
63 28.0 20.6 30.8









#5
Phenol-d6
Concen: 0.44 ng
RT: 6.896 min Scan# 414
Delta R.T. -0.006 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00





Tgt Ion: 99 Resp: 33468
Ion Ratio Lower Upper
99 100
42 16.9 8.9 13.3#
71 30.0 35.6 53.4#



#6
bis(2-Chloroethyl)ether
Concen: 0.41 ng
RT: 7.163 min Scan# 443
Delta R.T. -0.006 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00



Tgt Ion: 93 Resp: 30230
Ion Ratio Lower Upper
93 100
63 74.1 46.6 70.0#
95 32.8 28.6 42.8



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Manual Integrations
APPROVED

mohammad
7/6/2021 10:04:18 AM



#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.496 min Scan# 740
Delta R.T. 0.003 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:136 Resp: 103435
Ion Ratio Lower Upper
136 100
137 11.0 9.8 14.8
54 5.3 5.4 8.2#
68 4.6 4.9 7.3#

Manual Integrations
APPROVED



mohammad
7/6/2021 10:04:18 AM



#8
Nitrobenzene-d5
Concen: 0.49 ng
RT: 8.861 min Scan# 611
Delta R.T. -0.009 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00



Tgt Ion: 82 Resp: 28464
Ion Ratio Lower Upper
82 100
128 36.3 31.6 47.4
54 51.7 29.0 43.4#









#9
Naphthalene
Concen: 0.39 ng
RT: 10.546 min Scan# 744
Delta R.T. 0.003 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:	128	Resp:	116977
Ion Ratio	Lower	Upper	
128	100		
129	11.0	9.1	13.7
127	12.6	11.8	17.6

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED

mohammad
7/6/2021 10:04:18 AM



#10
Hexachlorobutadiene
Concen: 0.39 ng
RT: 10.838 min Scan# 767
Delta R.T. 0.003 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:	225	Resp:	22064
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.8	50.2	75.2









#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 12.079 min Scan# 948
Delta R.T. -0.010 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:152 Resp: 67060
Ion Ratio Lower Upper
152 100
151 20.4 16.7 25.1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
7/6/2021 10:04:18 AM



#12
2-Methylnaphthalene
Concen: 0.40 ng
RT: 12.154 min Scan# 965
Delta R.T. -0.005 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00


Tgt Ion:142 Resp: 76938
Ion Ratio Lower Upper
142 100
141 88.5 72.3 108.5
115 33.6 40.7 61.1#





#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.345 min Scan# 1189
Delta R.T. -0.001 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion:164 Resp: 55106
Ion Ratio Lower Upper
164 100
162 98.3 83.8 125.6
160 43.0 37.4 56.0




Manual Integrations
APPROVED

mohammad
7/6/2021 10:04:18 AM



#14
2,4,6-Tribromophenol
Concen: 0.52 ng
RT: 15.829 min Scan# 1306
Delta R.T. -0.014 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00


Tgt Ion:330 Resp: 7215
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 36.3 22.4 33.6#





#15
2-Fluorobiphenyl
Concen: 0.38 ng
RT: 12.962 min Scan# 1080
Delta R.T. -0.001 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:172 Resp: 86015
Ion Ratio Lower Upper
172 100
171 34.3 30.6 45.8
170 22.5 20.2 30.4

Manual Integrations
APPROVED



mohammad
7/6/2021 10:04:18 AM



#16
Acenaphthylene
Concen: 0.40 ng
RT: 14.053 min Scan# 1166
Delta R.T. -0.014 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00



Tgt Ion:152 Resp: 97755
Ion Ratio Lower Upper
152 100
151 19.3 16.7 25.1
153 13.0 10.5 15.7









#17
Acenaphthene
Concen: 0.39 ng
RT: 14.408 min Scan# 1194
Delta R.T. -0.001 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:154 Resp: 66434
Ion Ratio Lower Upper
154 100
153 113.1 90.9 136.3
152 54.8 45.8 68.8

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
7/6/2021 10:04:18 AM



#18
Fluorene
Concen: 0.39 ng
RT: 15.385 min Scan# 1271
Delta R.T. -0.014 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:166 Resp: 80674
Ion Ratio Lower Upper
166 100
165 97.6 79.2 118.8
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.091 min Scan# 1409
Delta R.T. -0.000 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:188 Resp: 102517
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.7 9.0 13.4#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
7/6/2021 10:04:18 AM




#20
4,6-Dinitro-2-methylphenol
Concen: 0.37 ng
RT: 15.474 min Scan# 1278
Delta R.T. -0.014 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:198 Resp: 347
Ion Ratio Lower Upper
198 100
182 31.1 34.5 51.7#
77 0.0 0.0 0.0






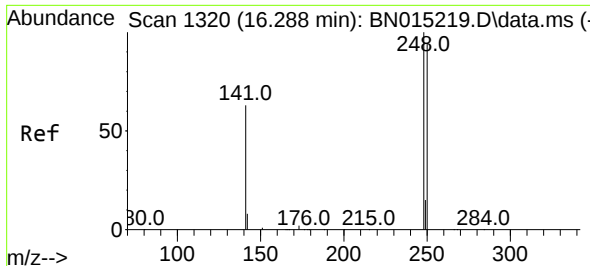


#21
4-Bromophenyl-phenylether
Concen: 0.39 ng
RT: 16.288 min Scan# 1343
Delta R.T. -0.000 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00





Tgt Ion:248 Resp: 25253
Ion Ratio Lower Upper
248 100
250 101.6 86.2 129.4
141 41.3 36.2 54.2



#22
Hexachlorobenzene
Concen: 0.39 ng
RT: 16.397 min Scan# 1352
Delta R.T. -0.013 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00




Tgt Ion:284 Resp: 28492
Ion Ratio Lower Upper
284 100
142 34.6 22.2 33.2#
249 30.8 26.6 39.8




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED




mohammad
7/6/2021 10:04:18 AM

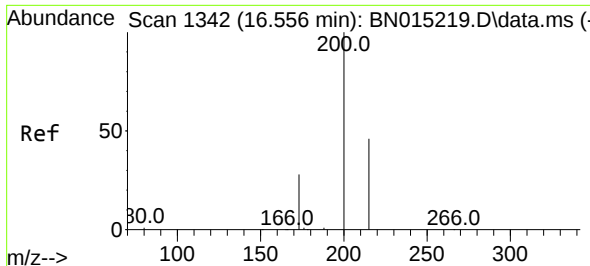


#23
Atrazine
Concen: 0.48 ng
RT: 16.555 min Scan# 1365
Delta R.T. -0.001 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00





Tgt Ion:200 Resp: 17251
Ion Ratio Lower Upper
200 100
173 23.8 21.7 32.5
215 48.1 43.1 64.7



#24
Pentachlorophenol
Concen: 0.60 ng
RT: 16.750 min Scan# 1381
Delta R.T. -0.001 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00



Tgt Ion:266 Resp: 4504
Ion Ratio Lower Upper
266 100
264 63.0 51.0 76.4
268 64.2 50.6 76.0




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED




mohammad
7/6/2021 10:04:18 AM




#25
Phenanthrene
Concen: 0.39 ng
RT: 17.127 min Scan# 1412
Delta R.T. -0.001 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00





Tgt Ion:178 Resp: 128942
Ion Ratio Lower Upper
178 100
176 18.8 15.6 23.4
179 15.4 12.1 18.1



#26
Anthracene
Concen: 0.39 ng
RT: 17.225 min Scan# 1420
Delta R.T. -0.000 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00




Tgt Ion:178 Resp: 109137
Ion Ratio Lower Upper
178 100
176 18.1 15.1 22.7
179 15.3 12.2 18.2




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED




mohammad
7/6/2021 10:04:18 AM

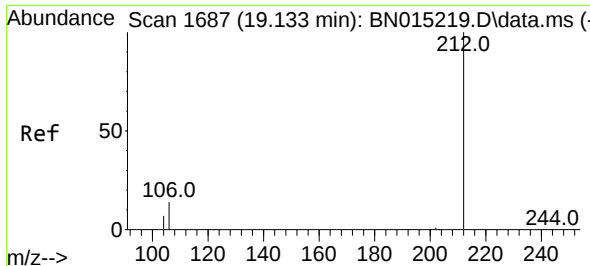


#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 19.128 min Scan# 1709
Delta R.T. -0.005 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00





Tgt Ion:212 Resp: 116427
Ion Ratio Lower Upper
212 100
106 14.4 7.0 10.6#
104 7.9 4.1 6.1#



#28
Fluoranthene
Concen: 0.40 ng
RT: 19.157 min Scan# 1715
Delta R.T. -0.006 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00




Tgt Ion:202 Resp: 141276
Ion Ratio Lower Upper
202 100
101 11.9 6.6 10.0#
203 17.4 13.9 20.9



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
7/6/2021 10:04:18 AM







#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.291 min Scan# 2007
Delta R.T. -0.012 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:240 Resp: 78310
Ion Ratio Lower Upper
240 100
120 6.2 4.2 6.4
236 25.6 21.4 32.2

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
7/6/2021 10:04:18 AM




#30
Pyrene
Concen: 0.47 ng
RT: 19.520 min Scan# 1788
Delta R.T. -0.010 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:202 Resp: 139648
Ion Ratio Lower Upper
202 100
200 20.5 16.9 25.3
203 17.4 13.9 20.9









#31
Terphenyl-d14
Concen: 0.45 ng
RT: 19.728 min Scan# 1830
Delta R.T. -0.011 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00





Tgt Ion:244 Resp: 82153
Ion Ratio Lower Upper
244 100
212 7.7 6.3 9.5
122 13.4 6.2 9.2#



#32
Benzo(a)anthracene
Concen: 0.40 ng
RT: 21.270 min Scan# 2005
Delta R.T. -0.011 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00



Tgt Ion:228 Resp: 108176
Ion Ratio Lower Upper
228 100
226 26.9 23.0 34.6
229 19.2 15.7 23.5



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
7/6/2021 10:04:18 AM







#33
Chrysene
Concen: 0.39 ng
RT: 21.323 min Scan# 2010
Delta R.T. -0.012 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:228 Resp: 113186
Ion Ratio Lower Upper
228 100
226 29.3 25.0 37.6
229 19.6 15.9 23.9

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED

mohammad
7/6/2021 10:04:18 AM



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.71 ng
RT: 21.206 min Scan# 1999
Delta R.T. -0.022 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00


Tgt Ion:149 Resp: 56298
Ion Ratio Lower Upper
149 100
167 28.0 28.9 43.3#
279 3.6 4.9 7.3#





#35
Perylene-d12
Concen: 0.40 ng
RT: 23.533 min Scan# 2441
Delta R.T. -0.017 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:264 Resp: 61938
Ion Ratio Lower Upper
264 100
260 25.0 20.6 31.0
265 23.1 21.4 32.2

Manual Integrations
APPROVED



mohammad
7/6/2021 10:04:18 AM



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.30 ng
RT: 25.788 min Scan# 3100
Delta R.T. -0.025 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00



Tgt Ion:276 Resp: 65556
Ion Ratio Lower Upper
276 100
138 25.4 10.0 15.0#
277 24.9 20.4 30.6









#37
Benzo(b)fluoranthene
Concen: 0.42 ng
RT: 22.858 min Scan# 2244
Delta R.T. -0.018 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:252 Resp: 102472
Ion Ratio Lower Upper
252 100
253 22.7 18.5 27.7
125 16.2 5.8 8.6#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
7/6/2021 10:04:18 AM




#38
Benzo(k)fluoranthene
Concen: 0.38 ng
RT: 22.903 min Scan# 2257
Delta R.T. -0.018 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00

Tgt Ion:252 Resp: 98034
Ion Ratio Lower Upper
252 100
253 21.8 19.1 28.7
125 10.9 5.4 8.0#









#39
Benzo(a)pyrene
Concen: 0.37 ng
RT: 23.433 min Scan# 2412
Delta R.T. -0.021 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00





Tgt Ion:252 Resp: 82106
Ion Ratio Lower Upper
252 100
253 24.2 19.4 29.2
125 28.1 7.4 11.2#



#40
Dibenzo(a,h)anthracene
Concen: 0.28 ng
RT: 25.805 min Scan# 3105
Delta R.T. -0.021 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00




Tgt Ion:278 Resp: 48823
Ion Ratio Lower Upper
278 100
139 18.7 9.0 13.4#
279 24.1 21.0 31.4




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED



mohammad
7/6/2021 10:04:18 AM



#41
Benzo(g,h,i)perylene
Concen: 0.31 ng
RT: 26.473 min Scan# 3300
Delta R.T. -0.025 min
Lab File: BN015334.D
Acq: 03 Jul 2021 15:00



Tgt Ion: 276 Resp: 59840
Ion Ratio Lower Upper
276 100
277 23.8 19.7 29.5
138 23.8 9.8 14.6#



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
7/6/2021 10:04:18 AM