
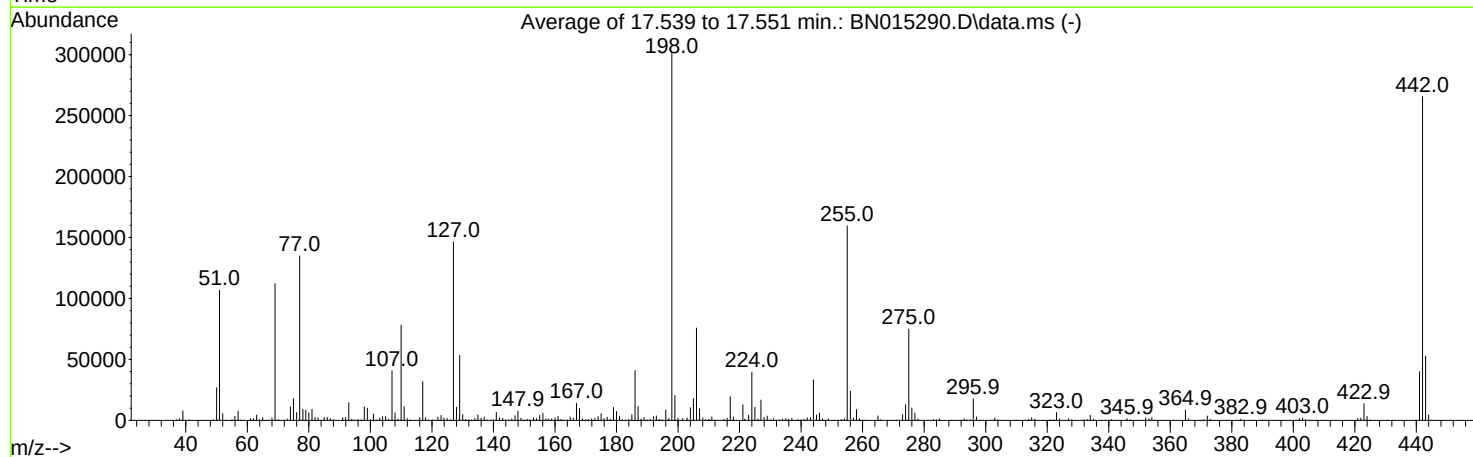


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
 Data File : BN015290.D
 Acq On : 02 Jul 2021 10:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 01 09:06:31 2021

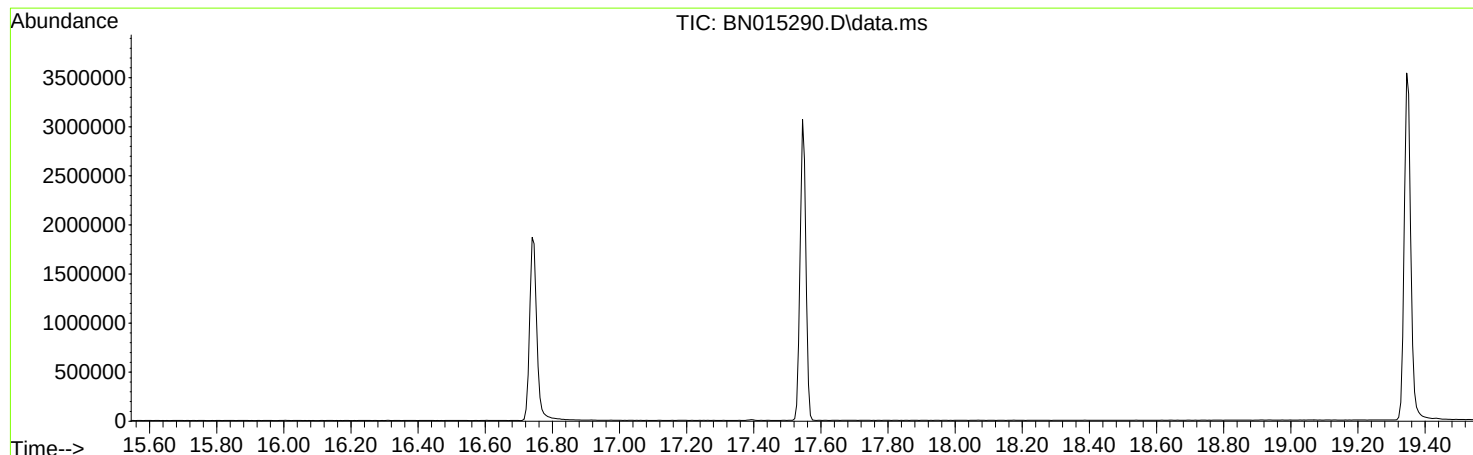

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	106755	PASS
68	69	0.00	2	1.7	1869	PASS
69	198	0.00	100	37.2	112291	PASS
70	69	0.00	2	0.5	602	PASS
127	198	10	80	48.6	146552	PASS
197	198	0.00	2	0.5	1451	PASS
198	198	100	100	100.0	301781	PASS
199	198	5	9	6.8	20501	PASS
275	198	10	60	24.8	74824	PASS
365	198	1	100	2.8	8425	PASS
441	198	0.01	100	13.2	39864	PASS
442	442	50	100	100.0	265728	PASS
443	442	15	24	19.8	52741	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/2/2021	BNA_N	<u>BN015290.D</u>
Compound Name	Response	Retention Time
DDT	839815	20.59
DDD	36029	20.14
DDE	2640	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38669	878484	4.40

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015290.D
Acq On : 02 Jul 2021 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 02 12:03:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

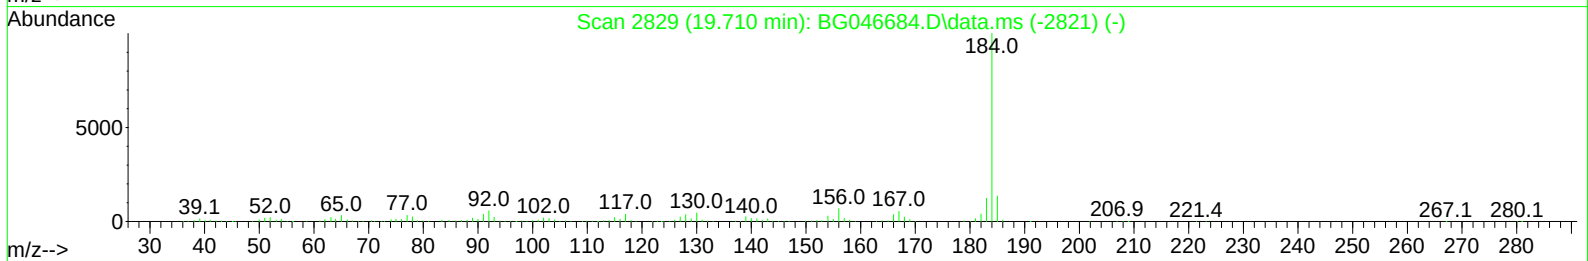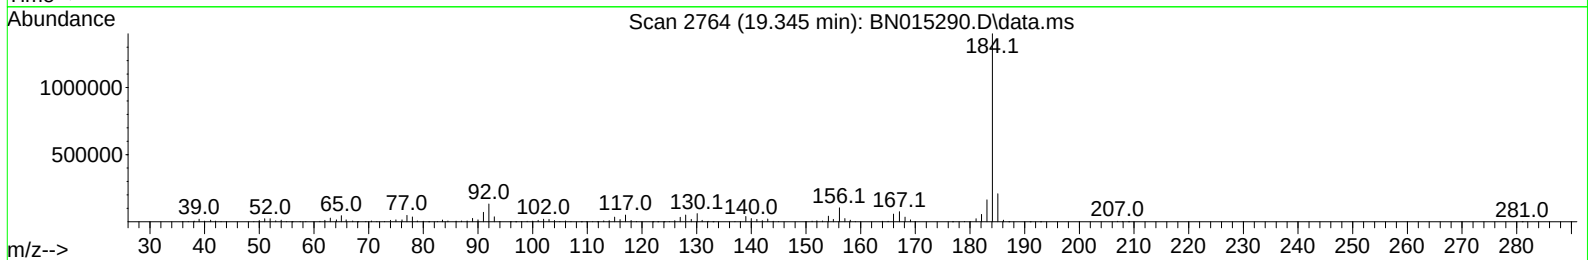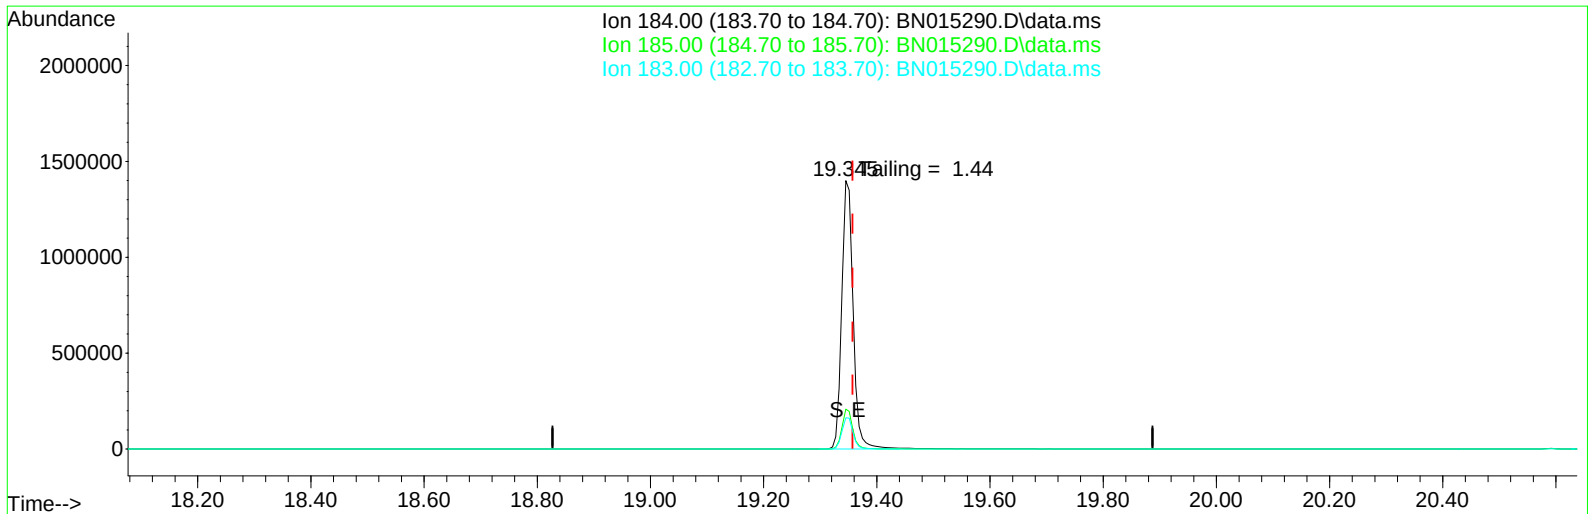

TIC: BN015290.D\data.ms

(77) Benzidine

19.345min (-0.012) 0.00 ng




response 1962176

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.88
183.00	13.20	11.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015290.D
Acq On : 02 Jul 2021 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 02 12:03:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

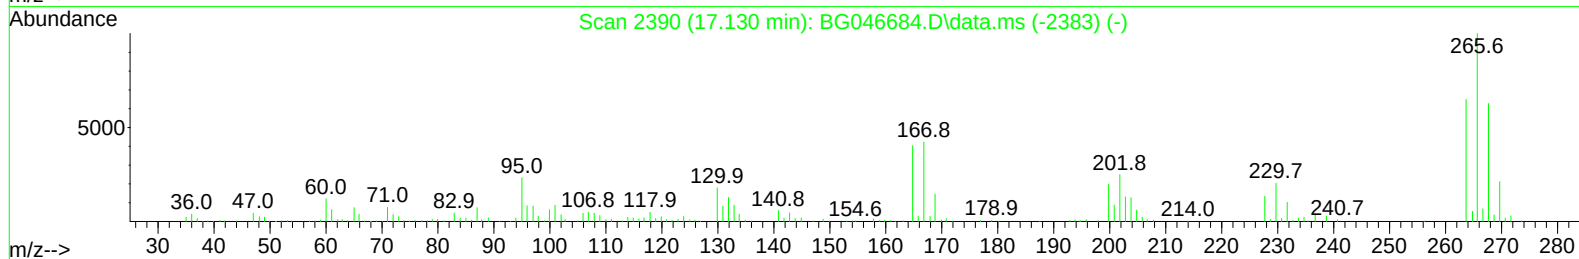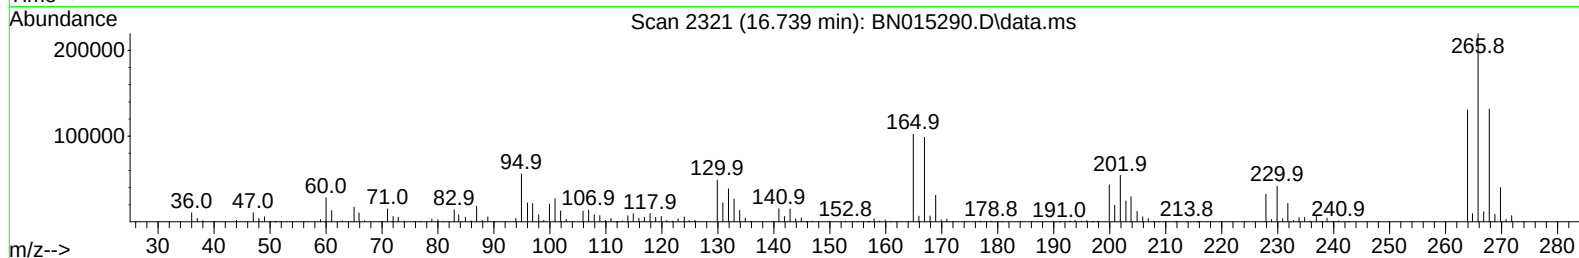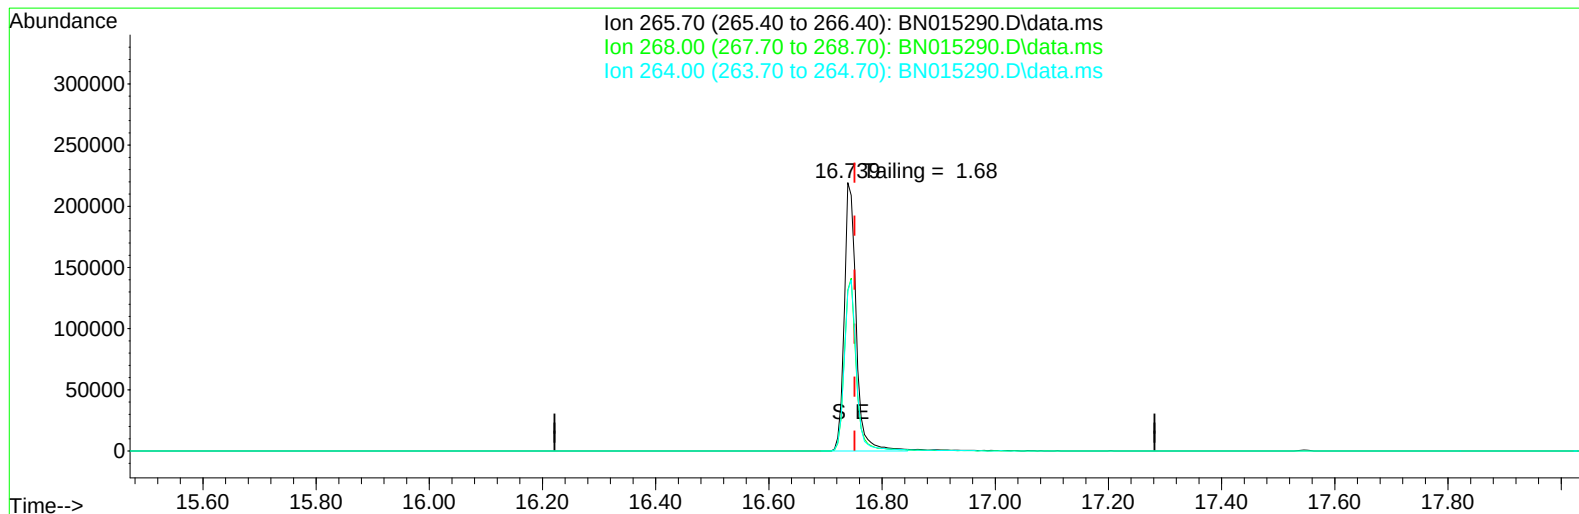

TIC: BN015290.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 23483.69 ng

response 320856

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.99
264.00	61.60	59.55
0.00	0.00	0.00