


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
 Data File : BN015297.D
 Acq On : 02 Jul 2021 15:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 01 09:06:31 2021

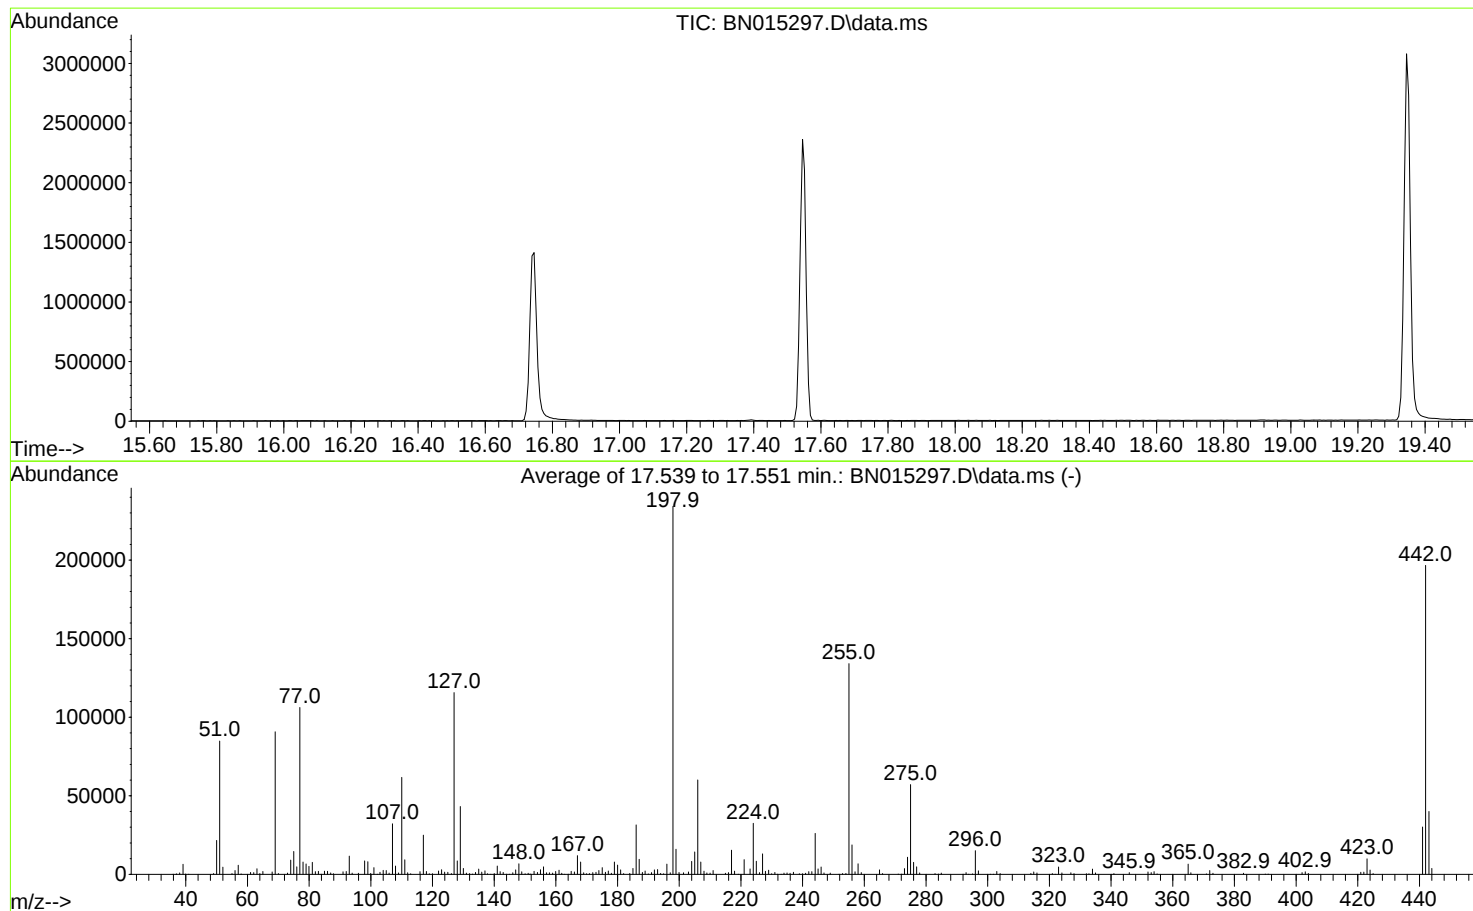

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	84811	PASS
68	69	0.00	2	1.7	1506	PASS
69	198	0.00	100	38.8	90781	PASS
70	69	0.00	2	0.6	518	PASS
127	198	10	80	49.4	115709	PASS
197	198	0.00	2	0.5	1061	PASS
198	198	100	100	100.0	234112	PASS
199	198	5	9	6.8	15988	PASS
275	198	10	60	24.4	57149	PASS
365	198	1	100	2.8	6526	PASS
441	198	0.01	100	12.9	30181	PASS
442	442	50	100	100.0	196595	PASS
443	442	15	24	20.4	40077	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/2/2021	BNA_N	<u>BN015297.D</u>
Compound Name	Response	Retention Time
DDT	687303	20.59
DDD	23801	20.14
DDE	1846	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25647	712950	3.60

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015297.D
Acq On : 02 Jul 2021 15:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 02 16:34:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

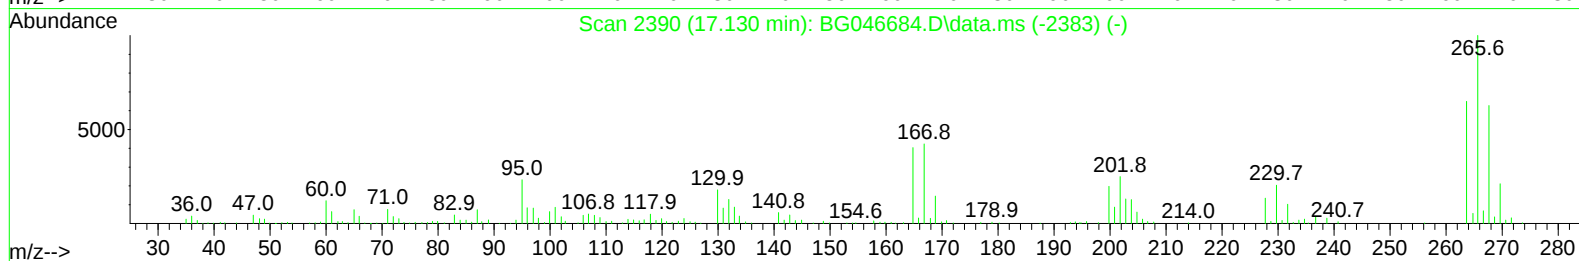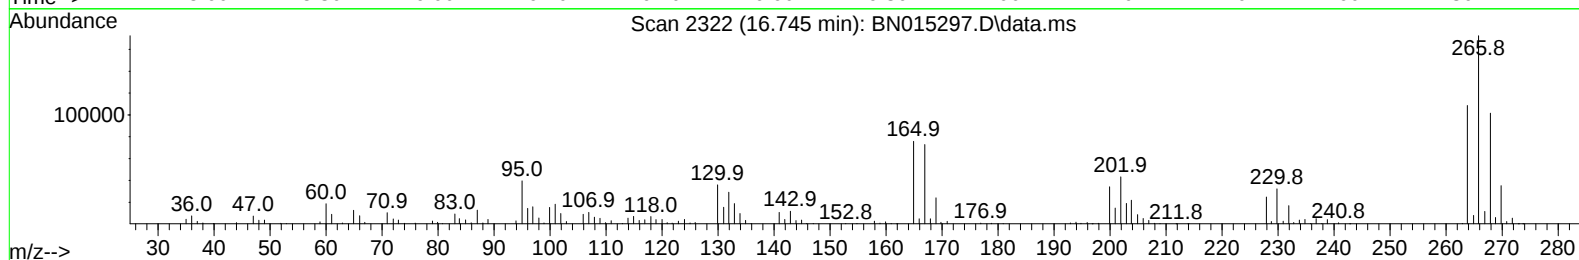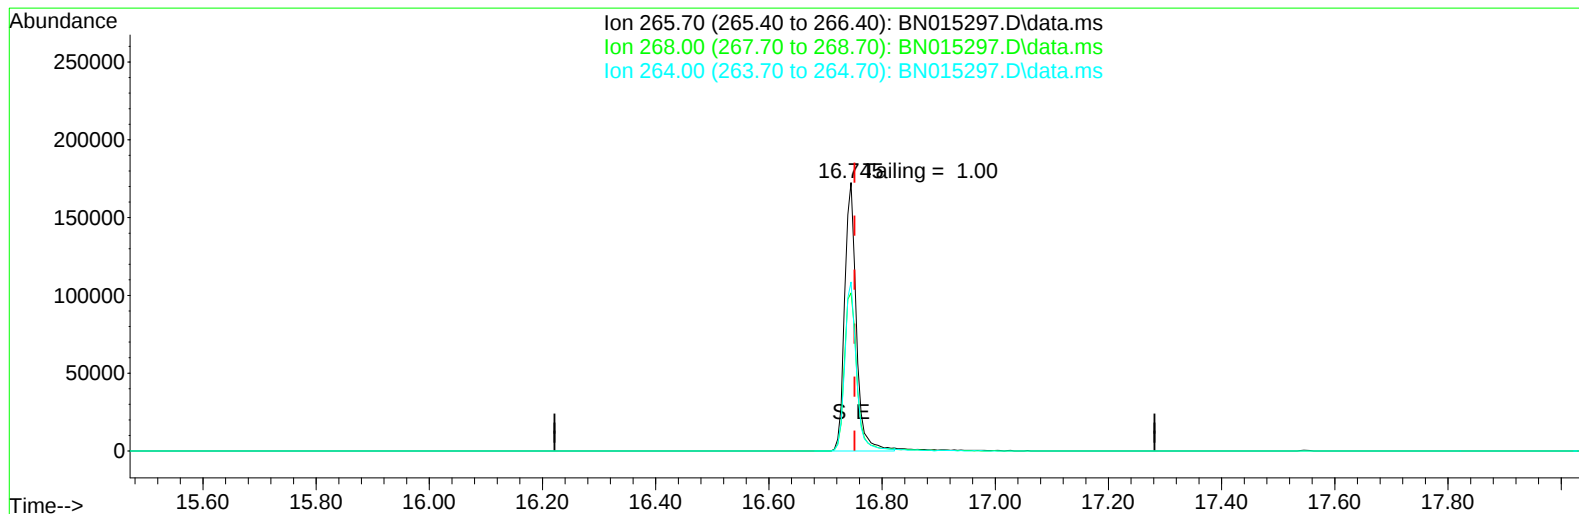

TIC: BN015297.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 19390.32 ng




response 252755

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.92
264.00	61.60	62.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015297.D
Acq On : 02 Jul 2021 15:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 02 16:34:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

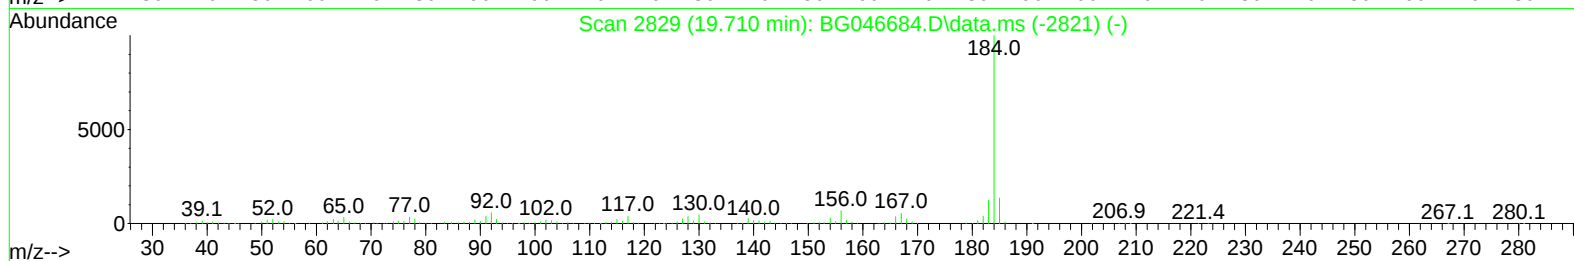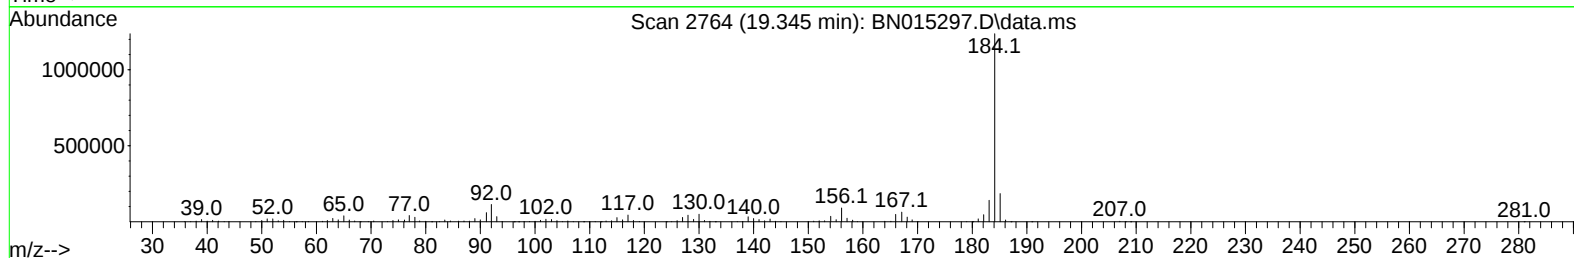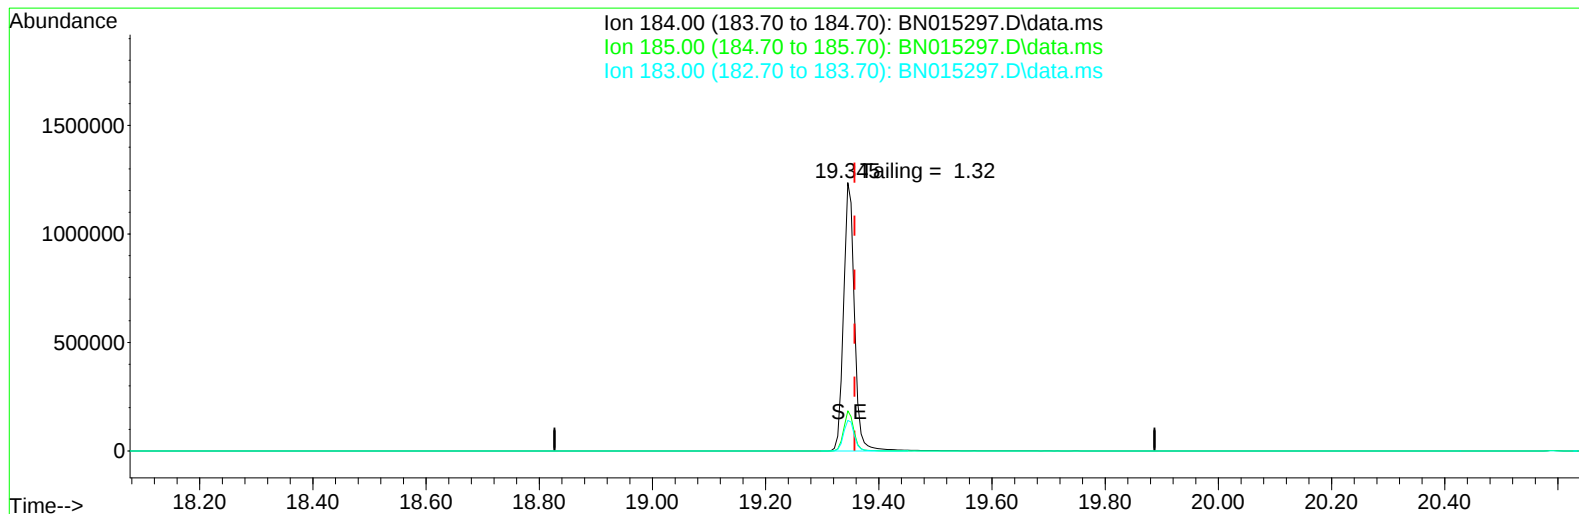

TIC: BN015297.D\data.ms

(77) Benzidine

19.345min (-0.012) 0.00 ng

response 1666266

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.96
183.00	13.20	11.40
0.00	0.00	0.00