


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
 Data File : BN015316.D
 Acq On : 03 Jul 2021 04:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 01 09:06:31 2021

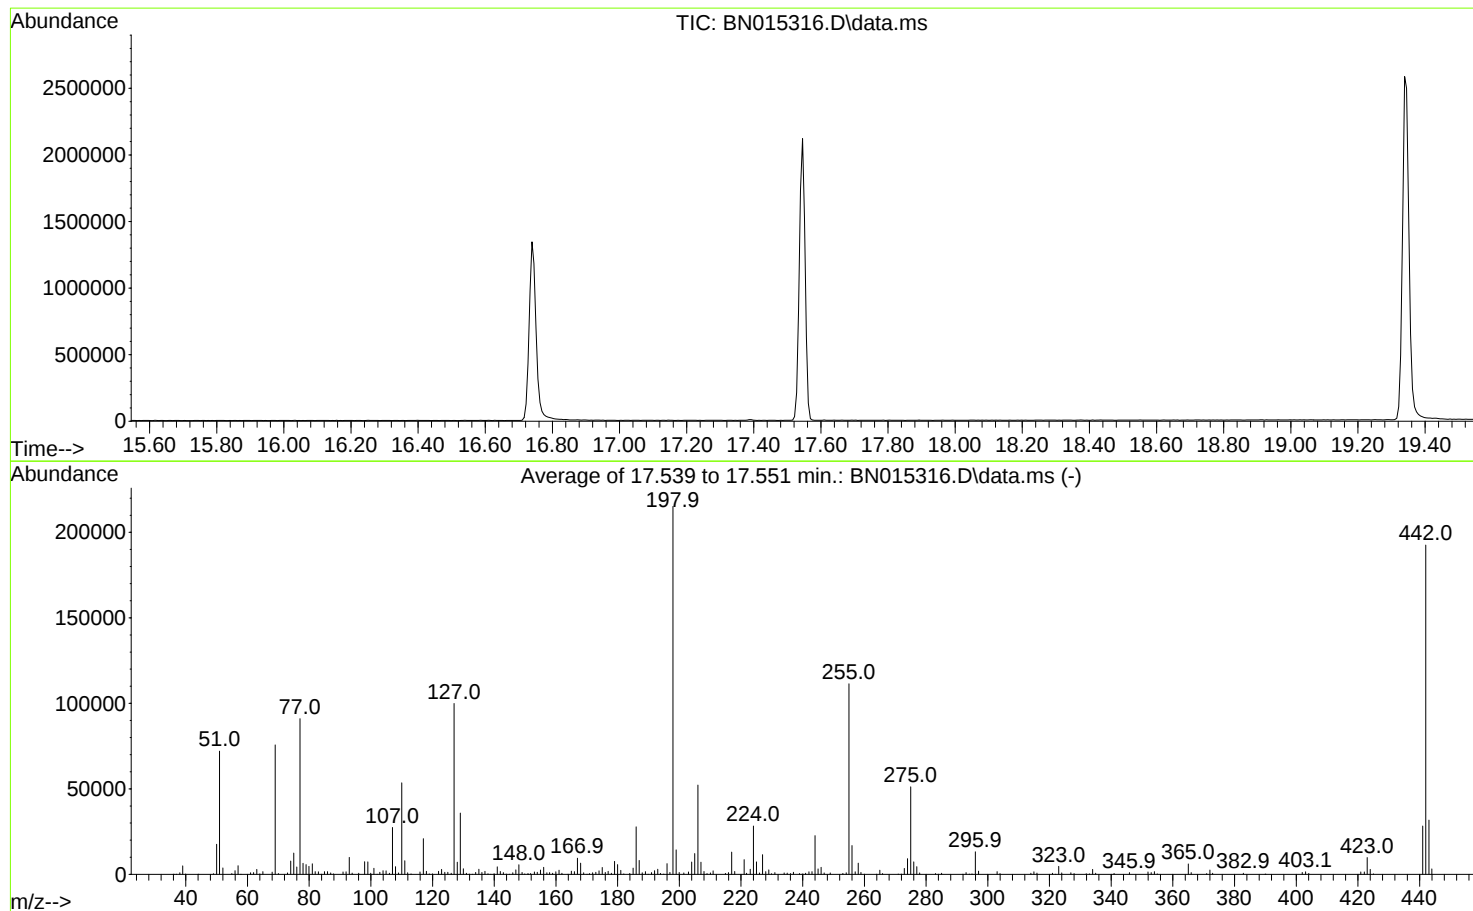

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	72080	PASS
68	69	0.00	2	1.8	1336	PASS
69	198	0.00	100	35.2	75728	PASS
70	69	0.00	2	0.6	436	PASS
127	198	10	80	46.5	99939	PASS
197	198	0.00	2	0.5	1099	PASS
198	198	100	100	100.0	215104	PASS
199	198	5	9	6.6	14304	PASS
275	198	10	60	23.8	51189	PASS
365	198	1	100	2.8	6067	PASS
441	198	0.01	100	13.1	28253	PASS
442	442	50	100	100.0	192512	PASS
443	442	15	24	16.5	31685	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/2/2021	BNA_N	<u>BN015316.D</u>
Compound Name	Response	Retention Time
DDT	622553	20.586
DDD	26098	20.145
DDE	1581	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27679	650232	4.26

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015316.D
Acq On : 03 Jul 2021 04:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 03 05:02:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

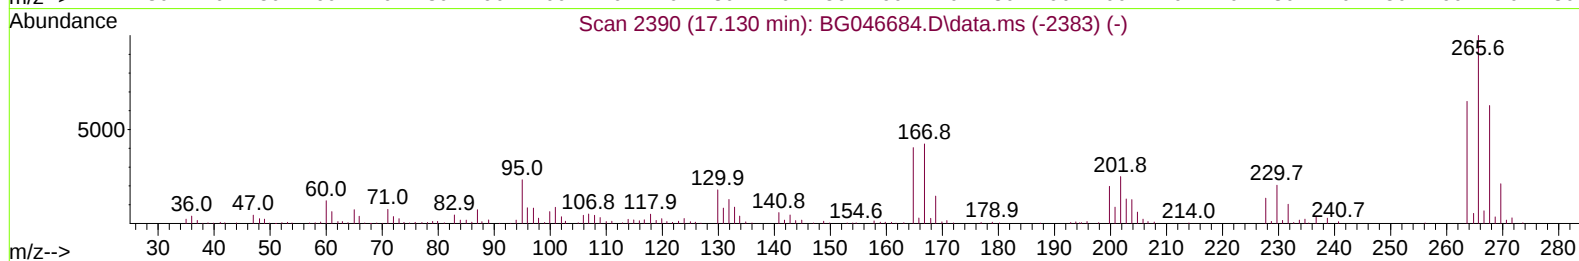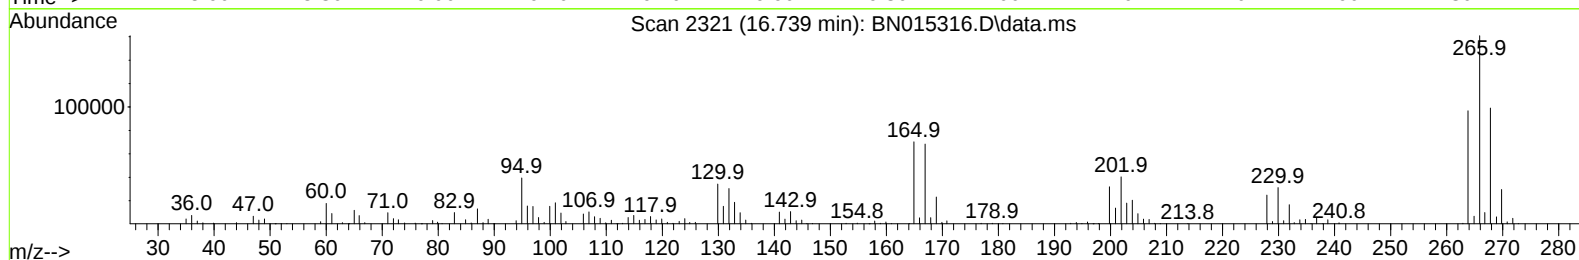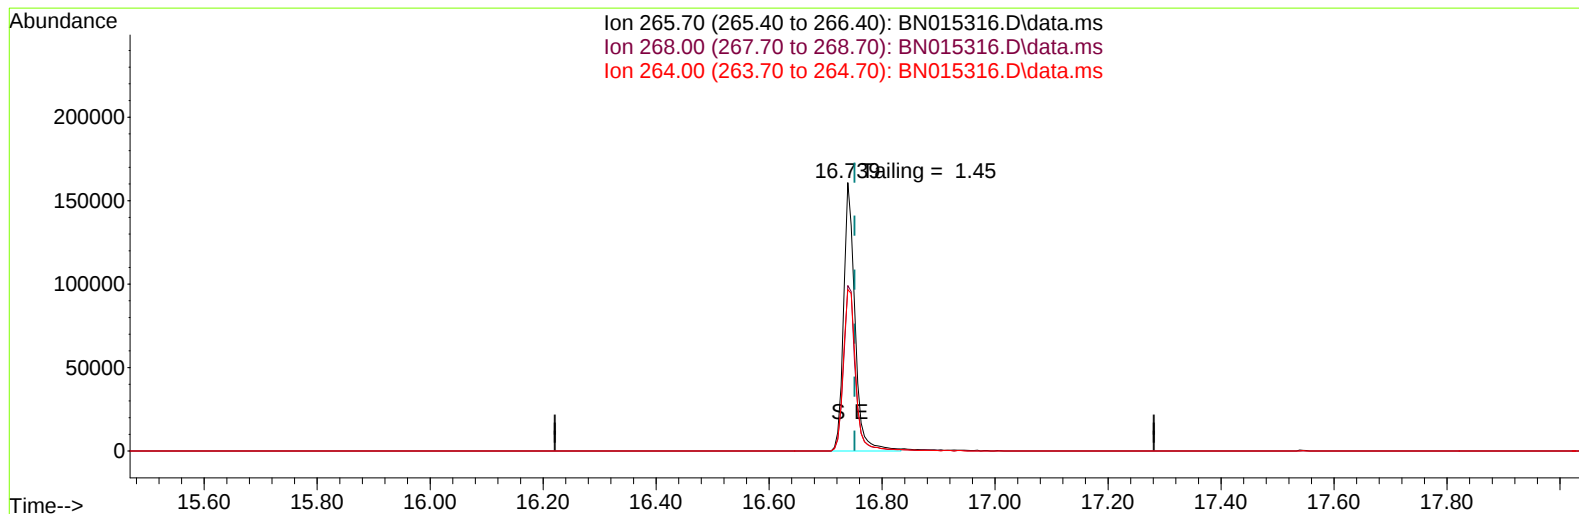

TIC: BN015316.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 22931.18 ng




response 227647

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.63
264.00	61.60	60.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070221\
Data File : BN015316.D
Acq On : 03 Jul 2021 04:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 03 05:02:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

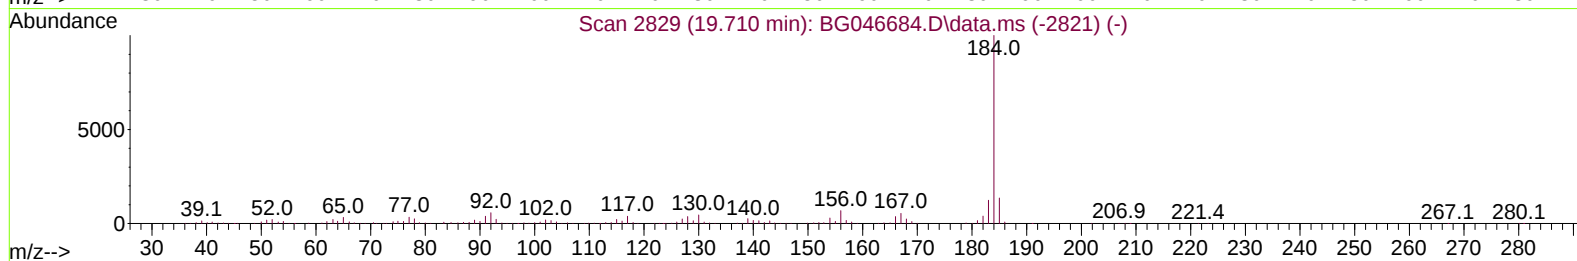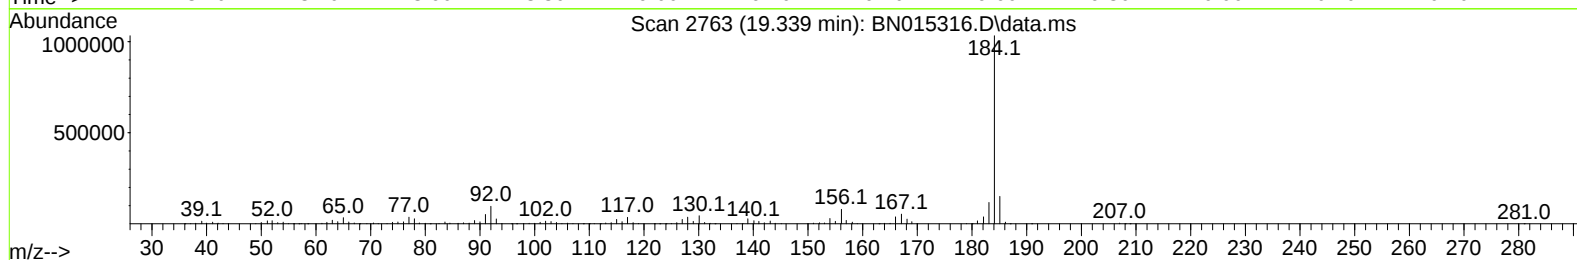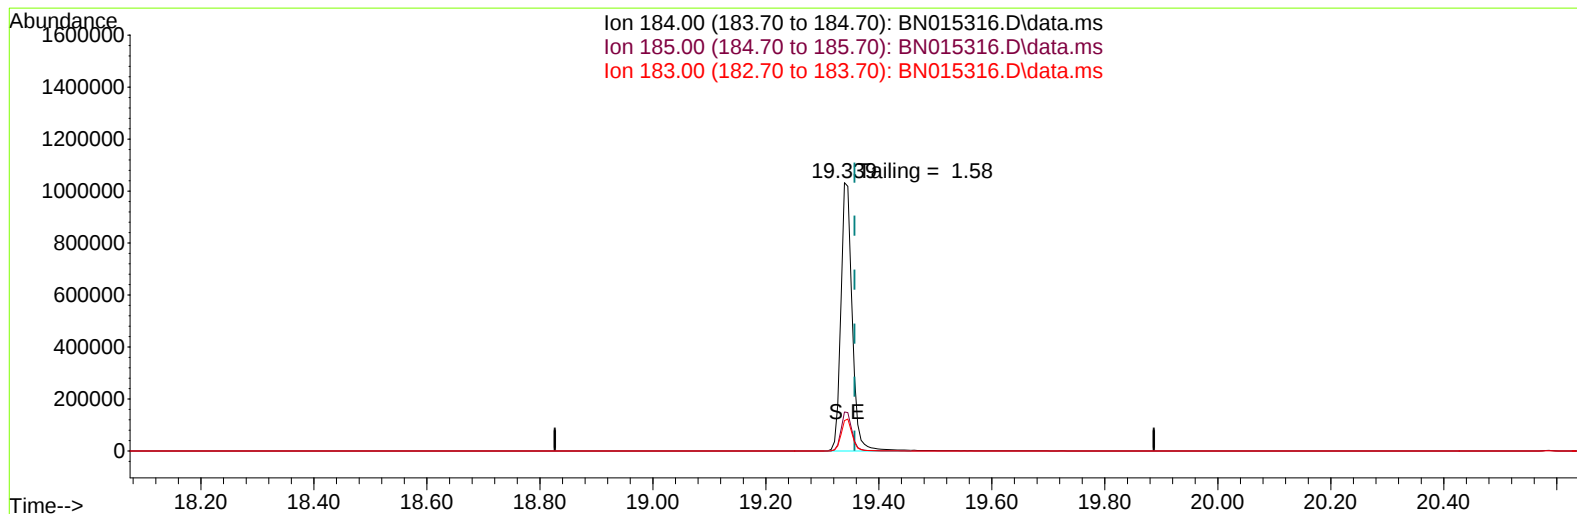

TIC: BN015316.D\data.ms

(77) Benzidine

19.339min (-0.018) 0.00 ng

response 1429184

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.57
183.00	13.20	11.37
0.00	0.00	0.00