
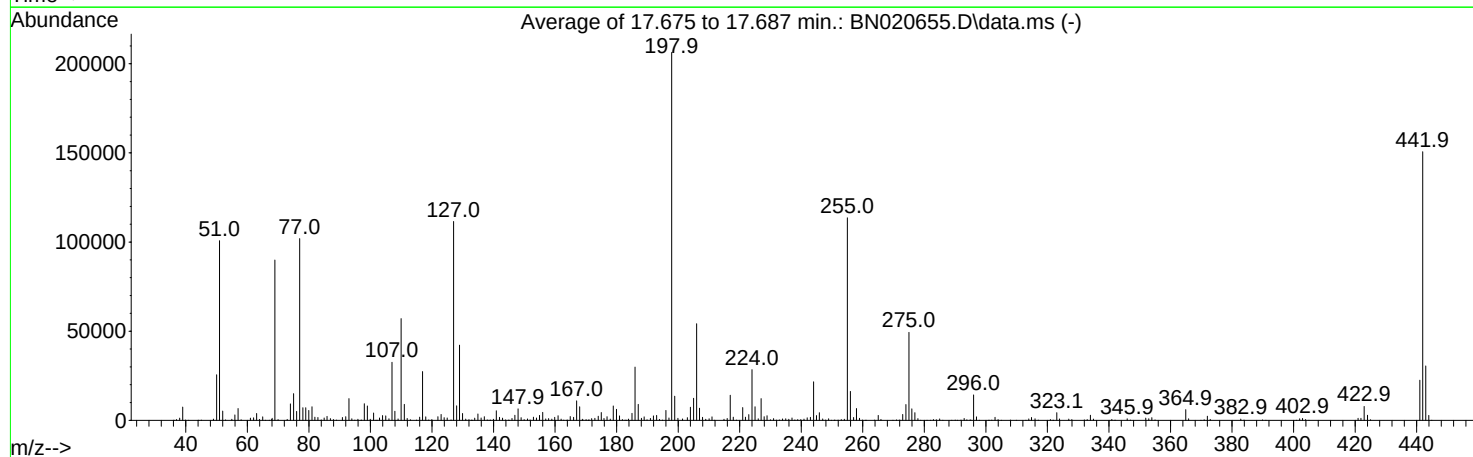


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070522\
 Data File : BN020655.D
 Acq On : 05 Jul 2022 10:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 02 03:10:12 2022

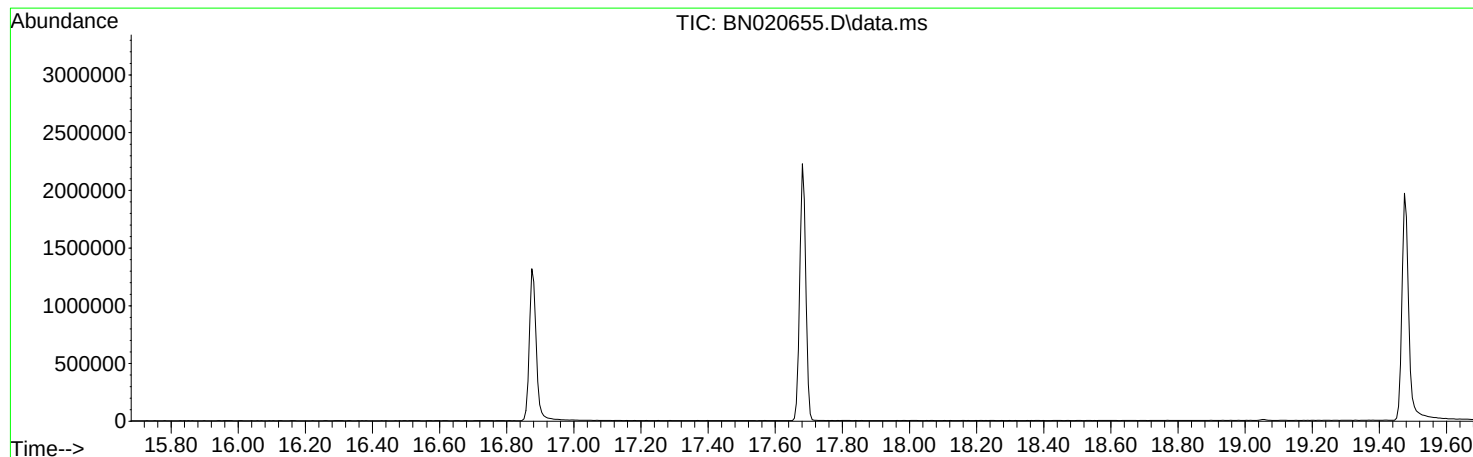




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	100815	PASS
68	69	0.00	2	1.3	1130	PASS
69	198	0.00	100	43.6	89907	PASS
70	69	0.00	2	0.5	439	PASS
127	198	10	80	54.1	111555	PASS
197	198	0.00	2	0.6	1305	PASS
198	198	100	100	100.0	206293	PASS
199	198	5	9	6.6	13527	PASS
275	198	10	60	23.9	49397	PASS
365	198	1	100	2.9	6009	PASS
441	198	0.01	100	10.9	22538	PASS
442	442	50	100	100.0	150688	PASS
443	442	15	24	20.2	30509	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070522\
Data File : BN020655.D
Acq On : 05 Jul 2022 10:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 06 03:10:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 06 03:10:51 2022
Response via : Initial Calibration

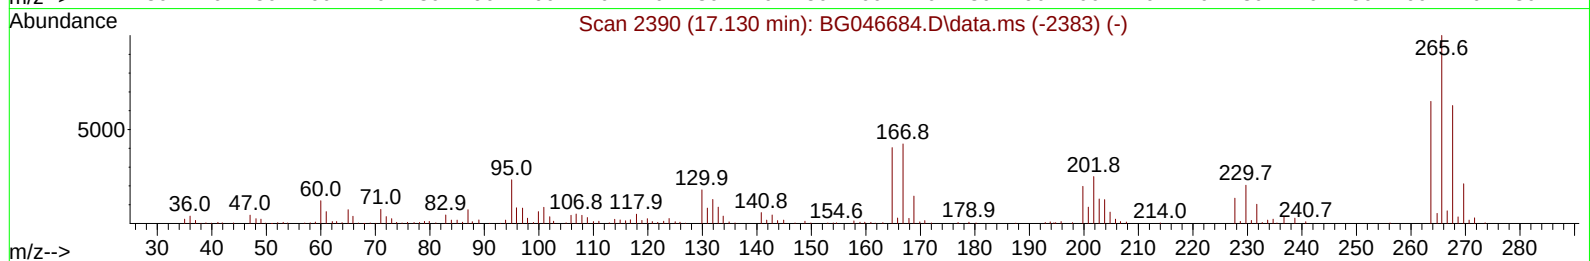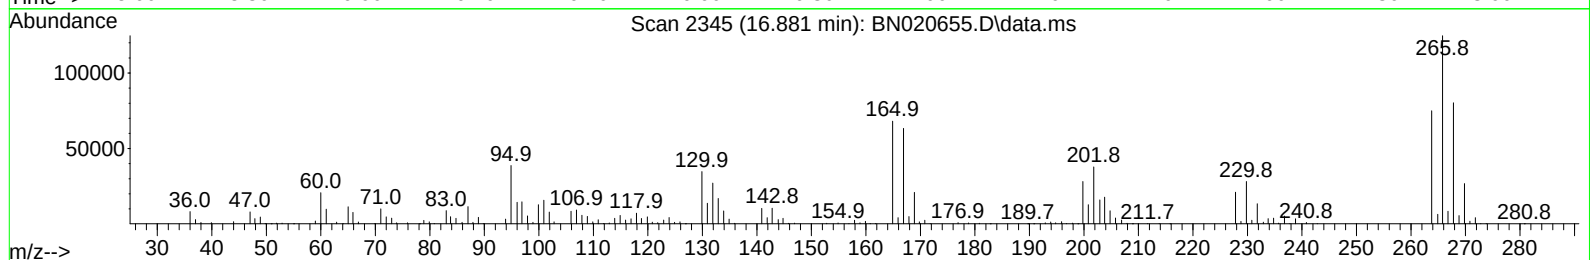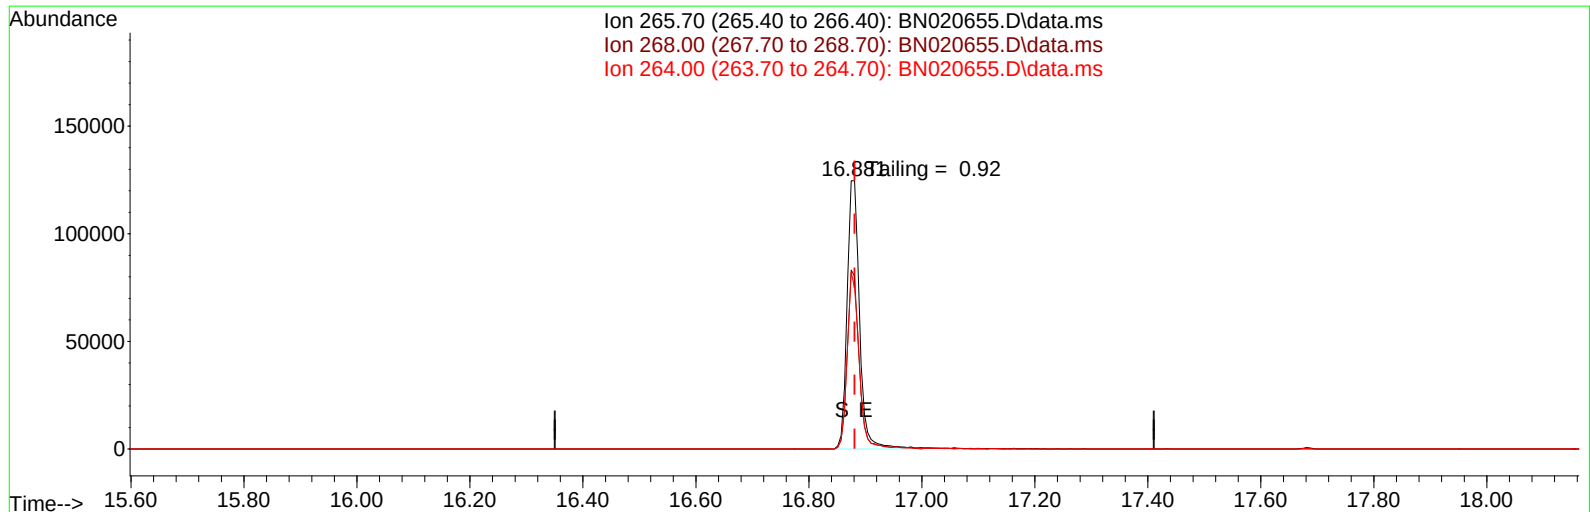

TIC: BN020655.D\data.ms

(70) Pentachlorophenol (C)

16.881min (0.000) 14825.93 ng




response 191396

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.38
264.00	61.60	60.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070522\
 Data File : BN020655.D
 Acq On : 05 Jul 2022 10:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 06 03:10:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 06 03:10:51 2022
 Response via : Initial Calibration

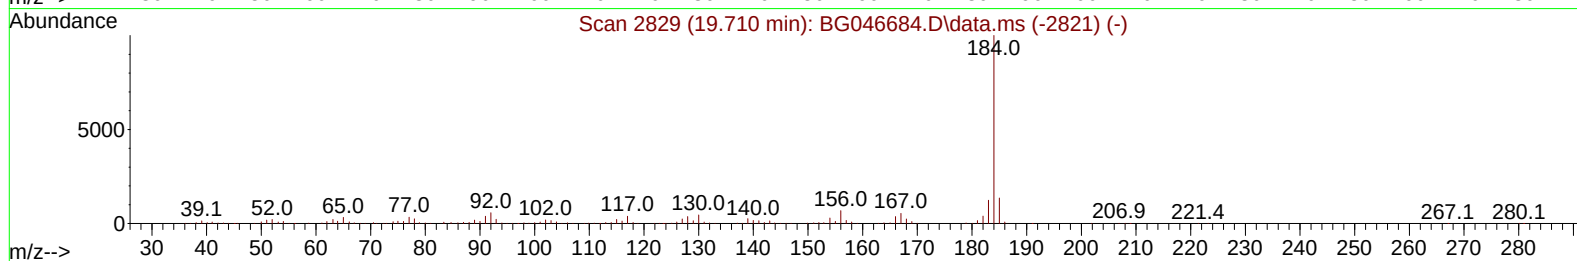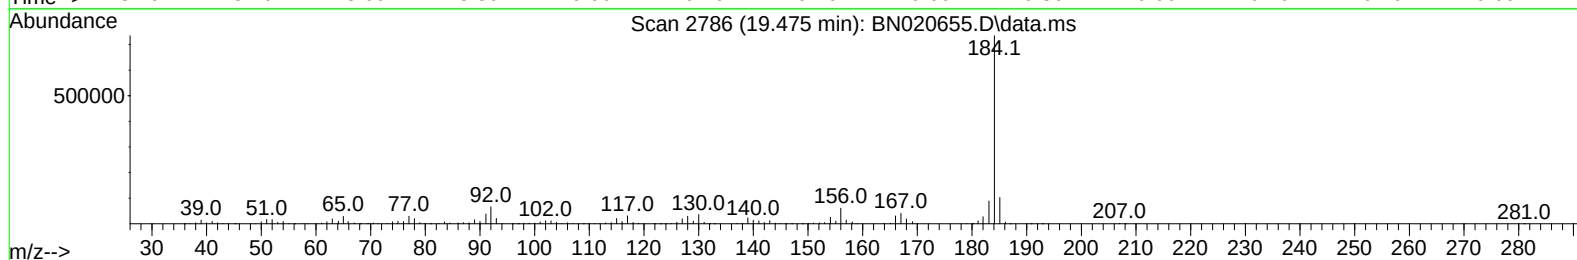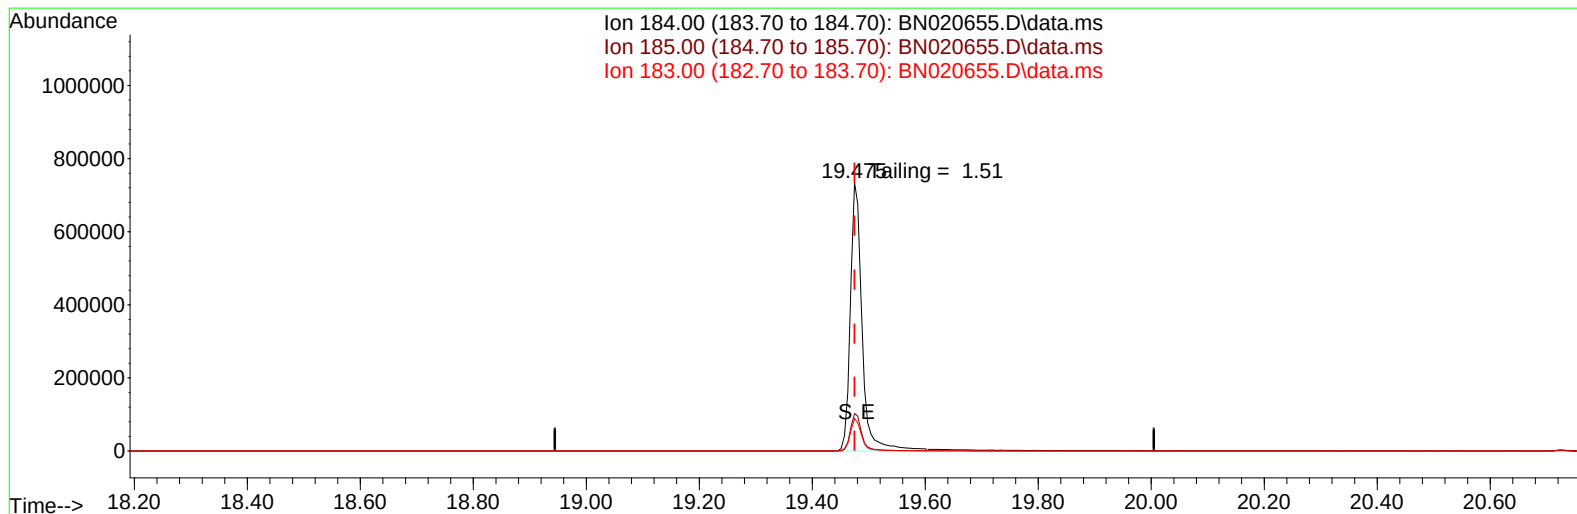

TIC: BN020655.D\data.ms

(77) Benzidine

19.475min (0.000) 0.00 ng

response 1086043

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/5/2022	BNA_N	<u>BN020655.D</u>
Compound Name	Response	Retention Time
DDT	713125	20.728
DDD	16123	20.286
DDE	2154	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18277	731402	2.50

Instrument :
BNA_N
ClientSampleId :
DFTPP