

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
 Data File : BN032514.D
 Acq On : 05 Jul 2024 18:53
 Operator : MA/JU
 Sample : PB161679BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK679

Quant Time: Jul 05 23:28:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.595	152	6214	0.400	ng/ul	0.00
4) Naphthalene-d8	10.365	136	17852	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.239	164	9303	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.096	188	1017614	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.21
23) Perylene-d12	23.424	264	21692	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	38184	5.528	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.977	152	6603	0.247	ng/ul	0.00
18) Fluoranthene-d10	19.036	212	11847	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
24) Benzo(b)fluoranthene	22.757	252	2397	0.025	ng/ul#	1
26) Benzo(a)pyrene	23.278	252	4518	0.069	ng/ul#	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
Data File : BN032514.D
Acq On : 05 Jul 2024 18:53
Operator : MA/JU
Sample : PB161679BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK679

Quant Time: Jul 05 23:28:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

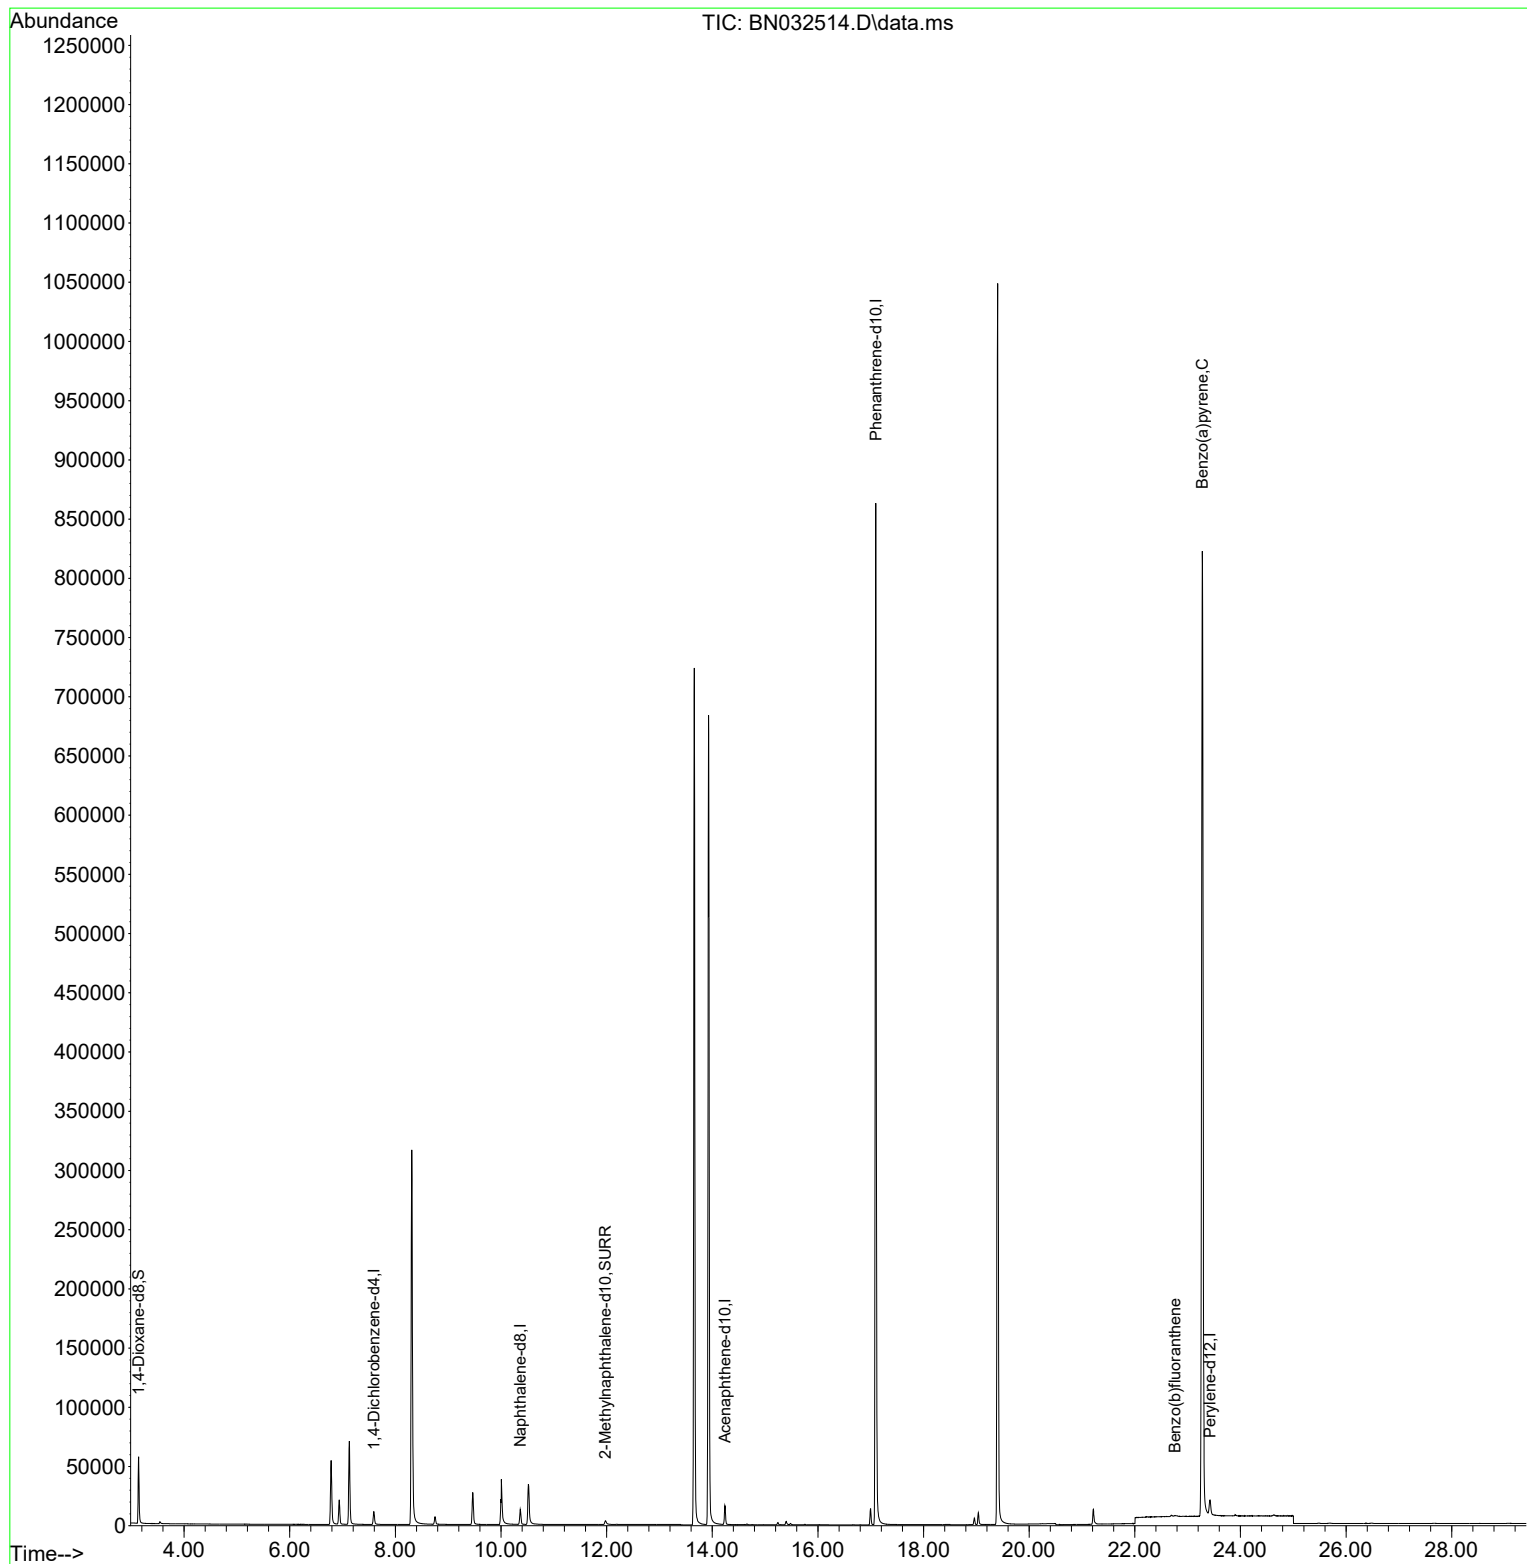

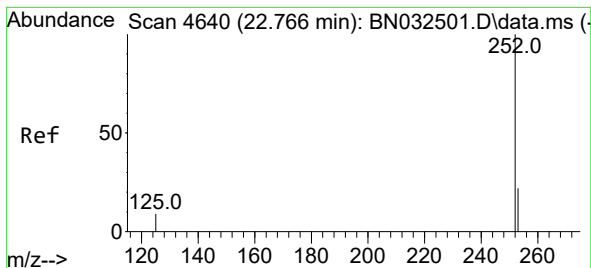

#24

Benzo(b)fluoranthene

Concen: 0.025 ng/ul

RT: 22.757 min Scan# 4637

Delta R.T. -0.000 min

Lab File: BN032514.D

Acq: 05 Jul 2024 18:53

Instrument :

BNA_N

ClientSampleId :

SBLK679





Tgt Ion:252 Resp: 2397

Ion Ratio Lower Upper

252 100

253 87.0 0.0 50.2#

125 98.2 0.0 32.0#

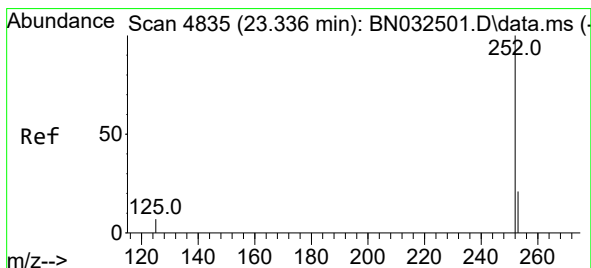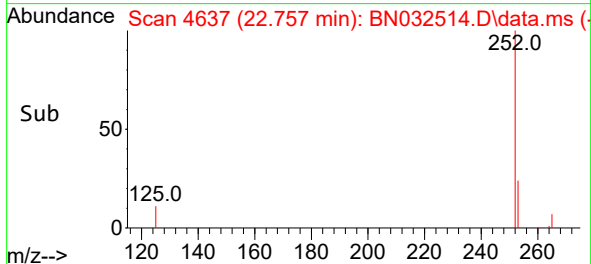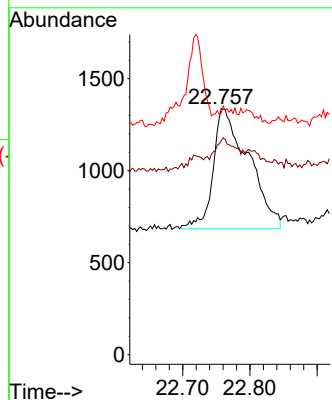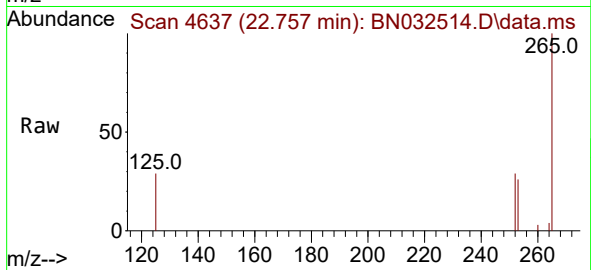

#26

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.278 min Scan# 4815

Delta R.T. -0.050 min

Lab File: BN032514.D

Acq: 05 Jul 2024 18:53

Tgt Ion:252 Resp: 4518

Ion Ratio Lower Upper

252 100

253 60.7 22.2 33.2#

125 77.8 16.4 24.6#

