




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
Data File : BN032514.D
Acq On : 05 Jul 2024 18:53
Operator : MA/JU
Sample : PB161679BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK679

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

Quant Time: Jul 05 23:28:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

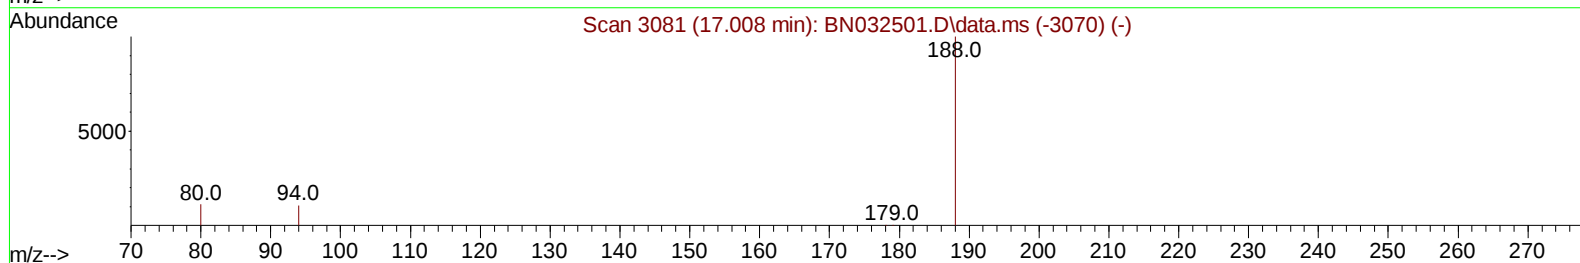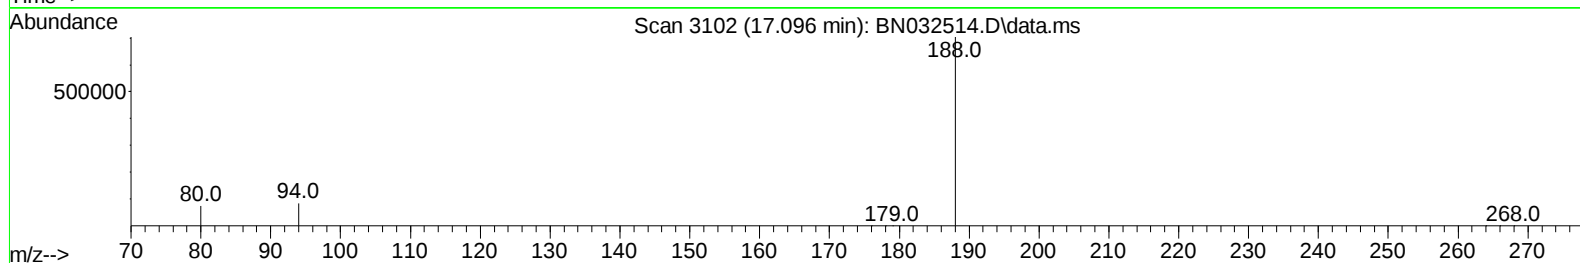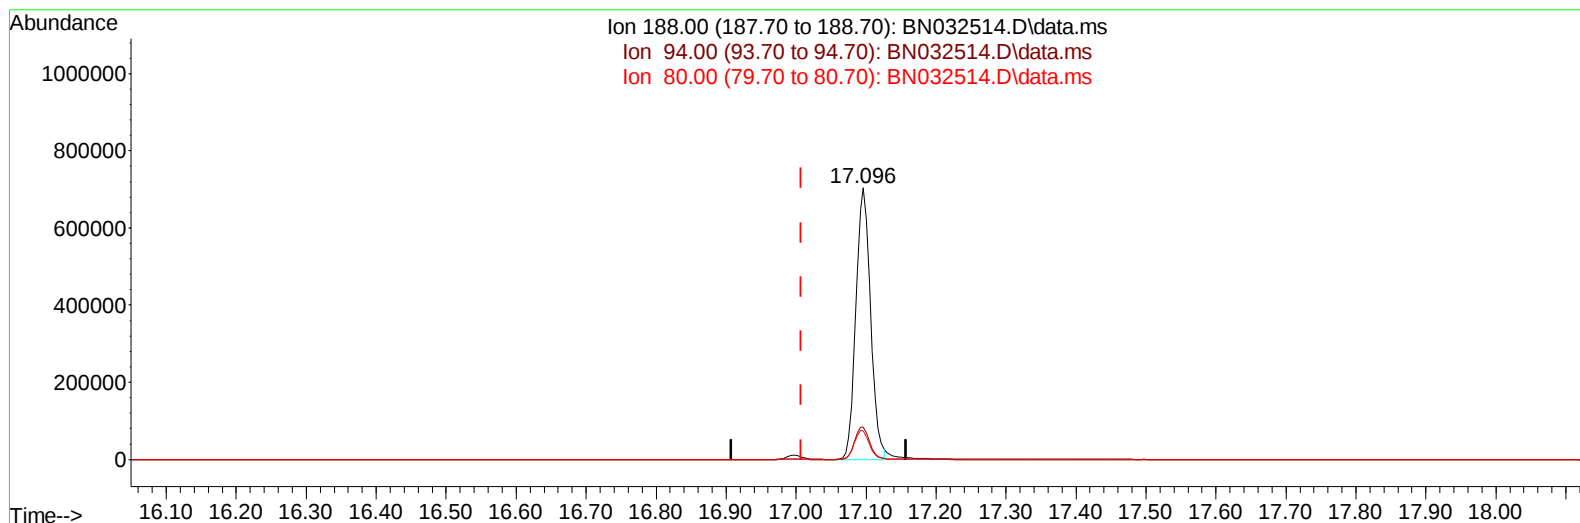

TIC: BN032514.D\data.ms

(13) Phenanthrene-d10 (I)

17.096min (+ 0.089) 0.40 ng/u1

response 1017614

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	11.88
80.00	10.50	10.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
Data File : BN032514.D
Acq On : 05 Jul 2024 18:53
Operator : MA/JU
Sample : PB161679BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK679

Manual IntegrationsAPPROVED

Quant Time: Jul 05 23:28:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

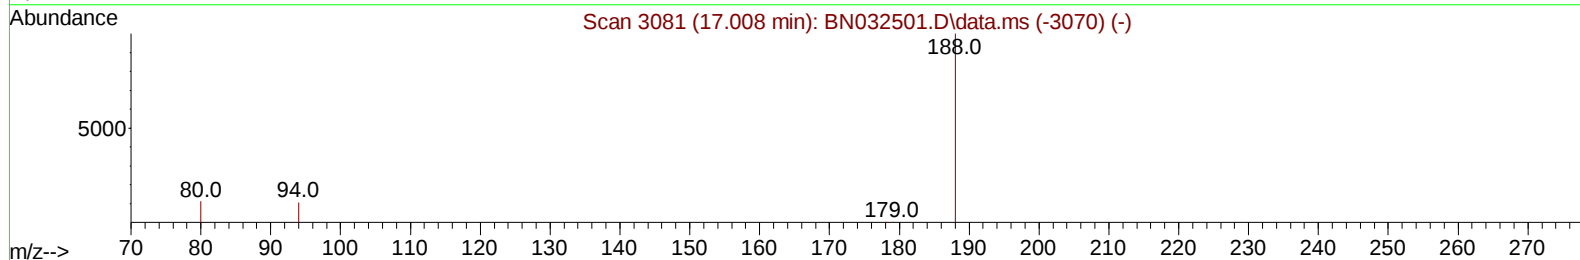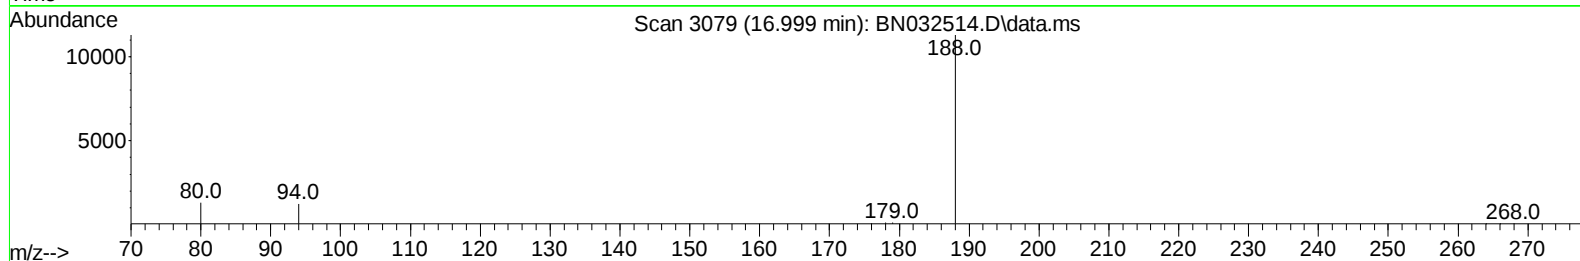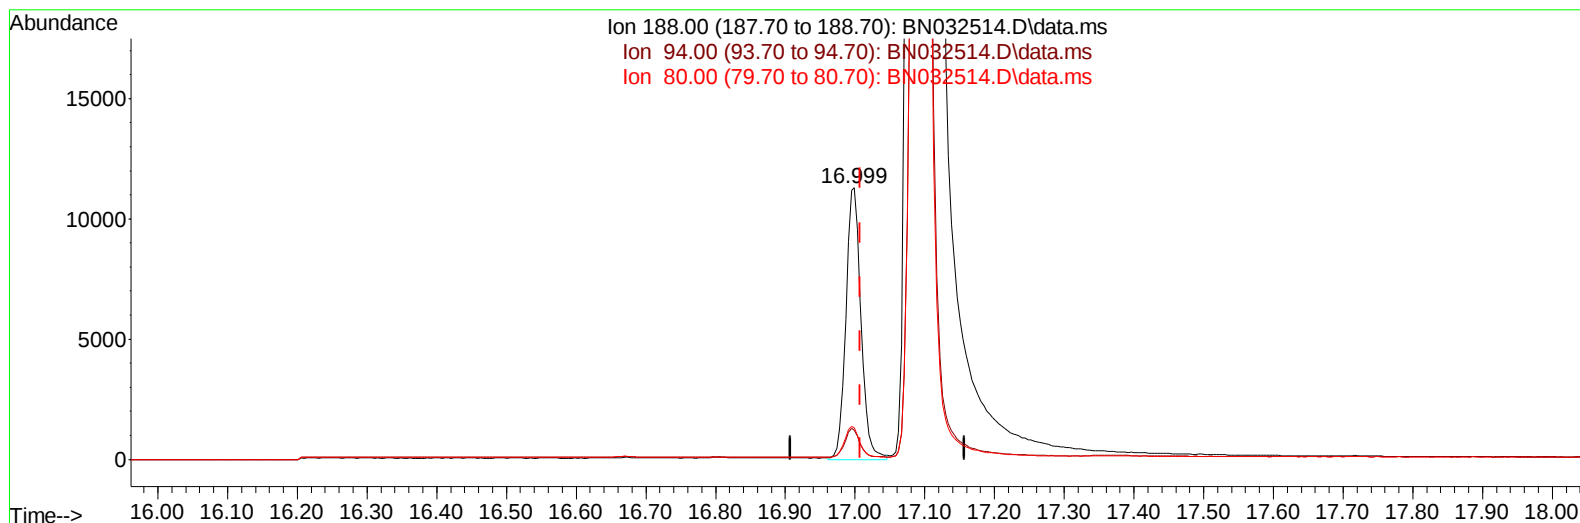

TIC: BN032514.D\data.ms

(13) Phenanthrene-d10 (I)

16.999min (-0.009) 0.40 ng/u1 m

response 17072

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	10.83
80.00	10.50	11.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
Data File : BN032514.D
Acq On : 05 Jul 2024 18:53
Operator : MA/JU
Sample : PB161679BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK679

Manual IntegrationsAPPROVED

Quant Time: Jul 05 23:28:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

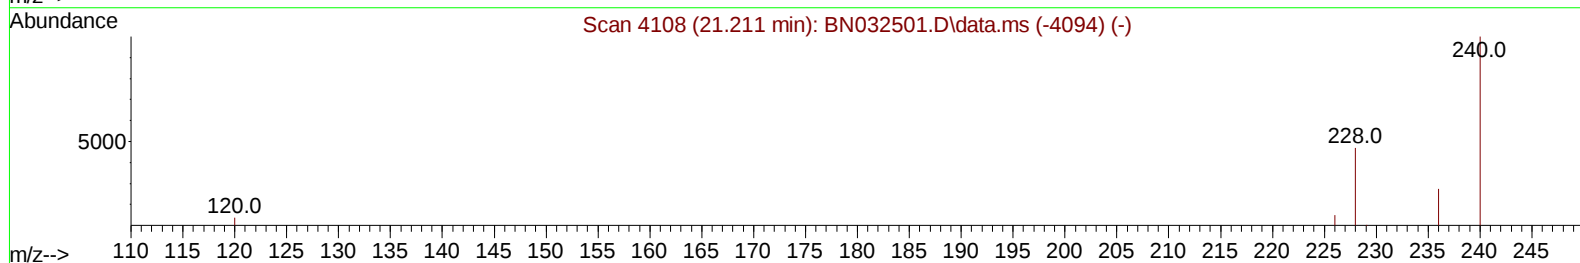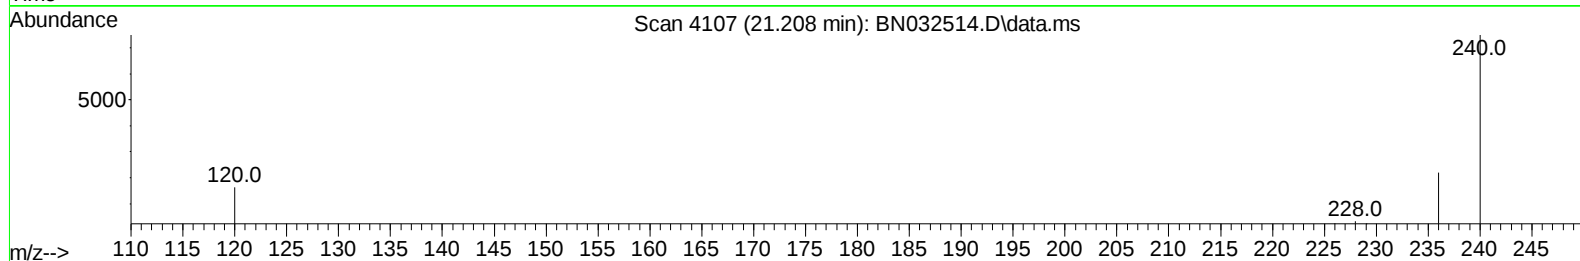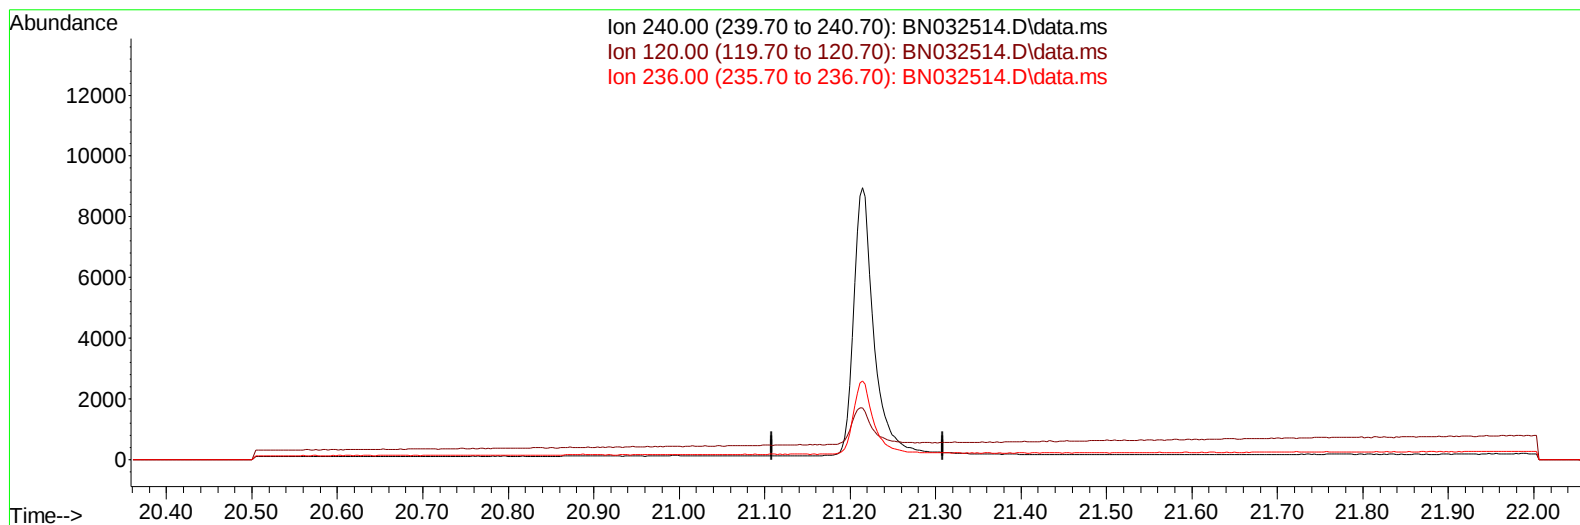

TIC: BN032514.D\data.ms

(17) Chrysene-d12

21.209min (-21.209) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.80	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
Data File : BN032514.D
Acq On : 05 Jul 2024 18:53
Operator : MA/JU
Sample : PB161679BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK679

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

Quant Time: Jul 05 23:28:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

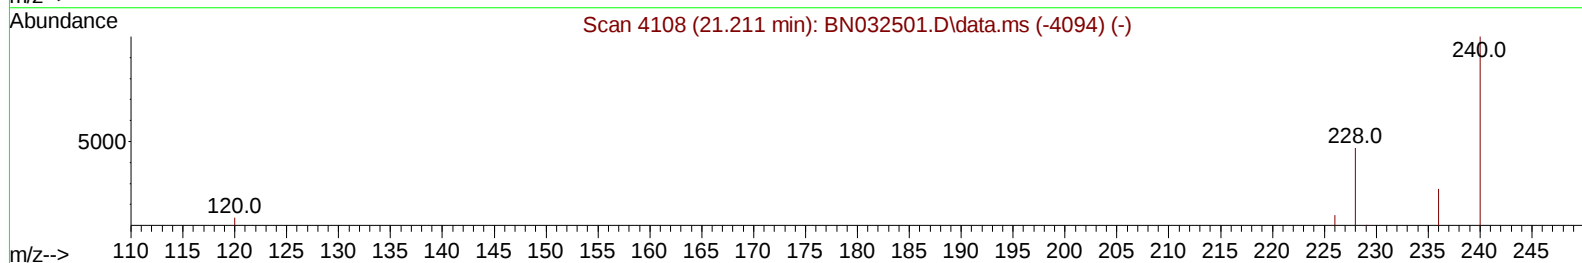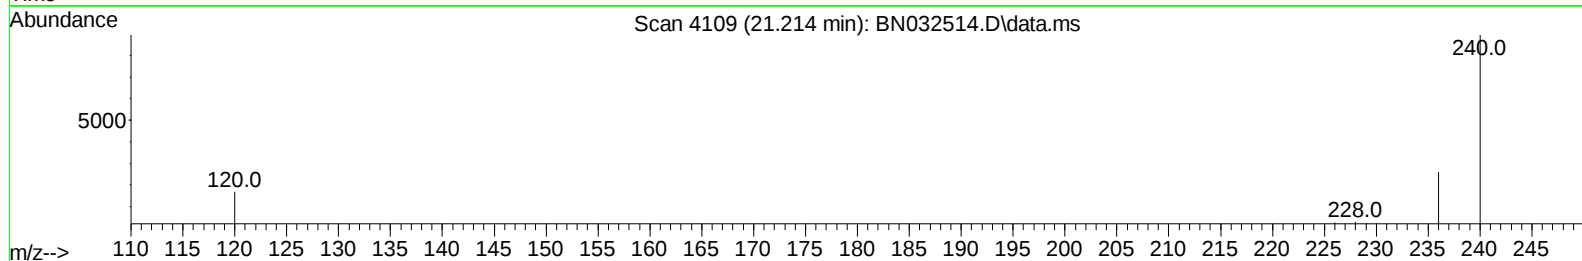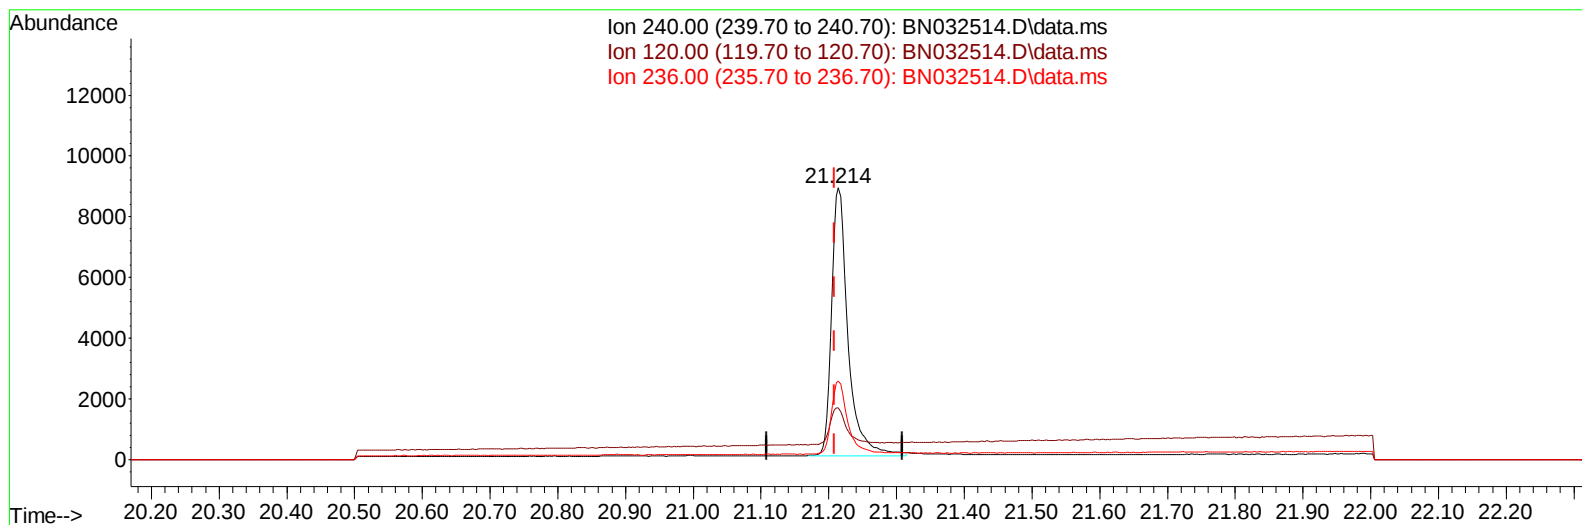

TIC: BN032514.D\data.ms

(17) Chrysene-d12

21.214min (+ 0.006) 0.40 ng/ul m

response 14850

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	18.97
236.00	28.40	28.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
Data File : BN032514.D
Acq On : 05 Jul 2024 18:53
Operator : MA/JU
Sample : PB161679BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK679

Manual IntegrationsAPPROVED

Quant Time: Jul 05 23:28:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

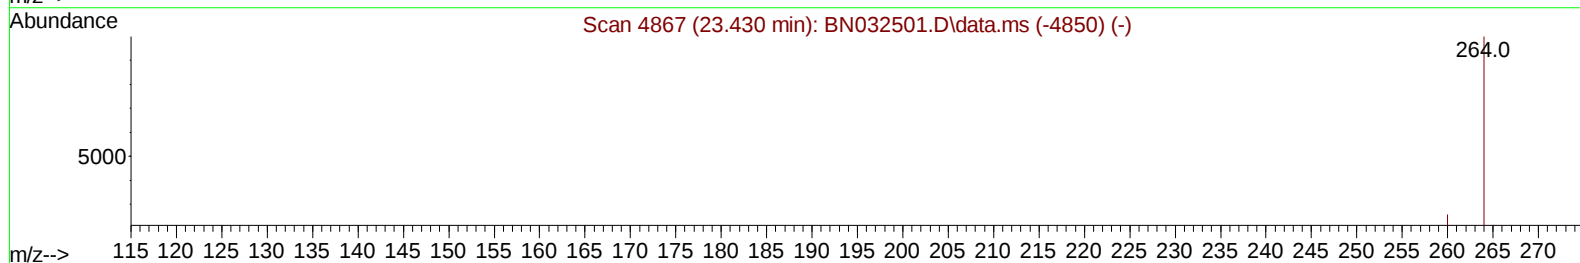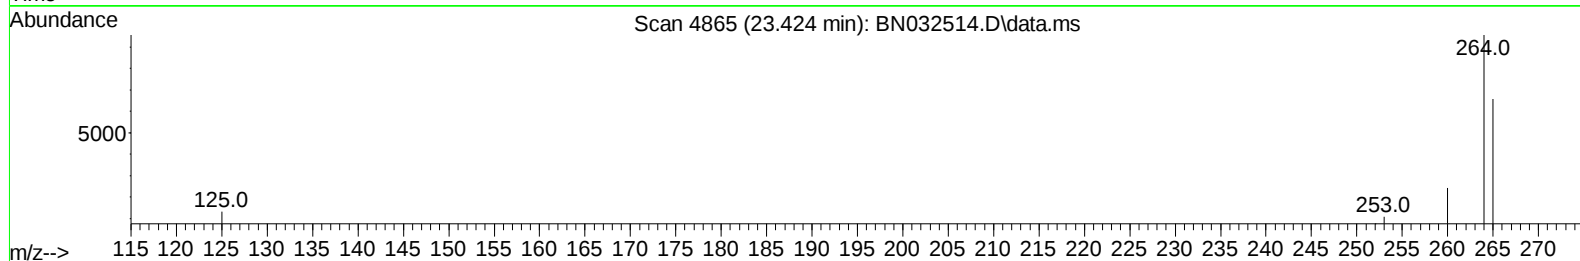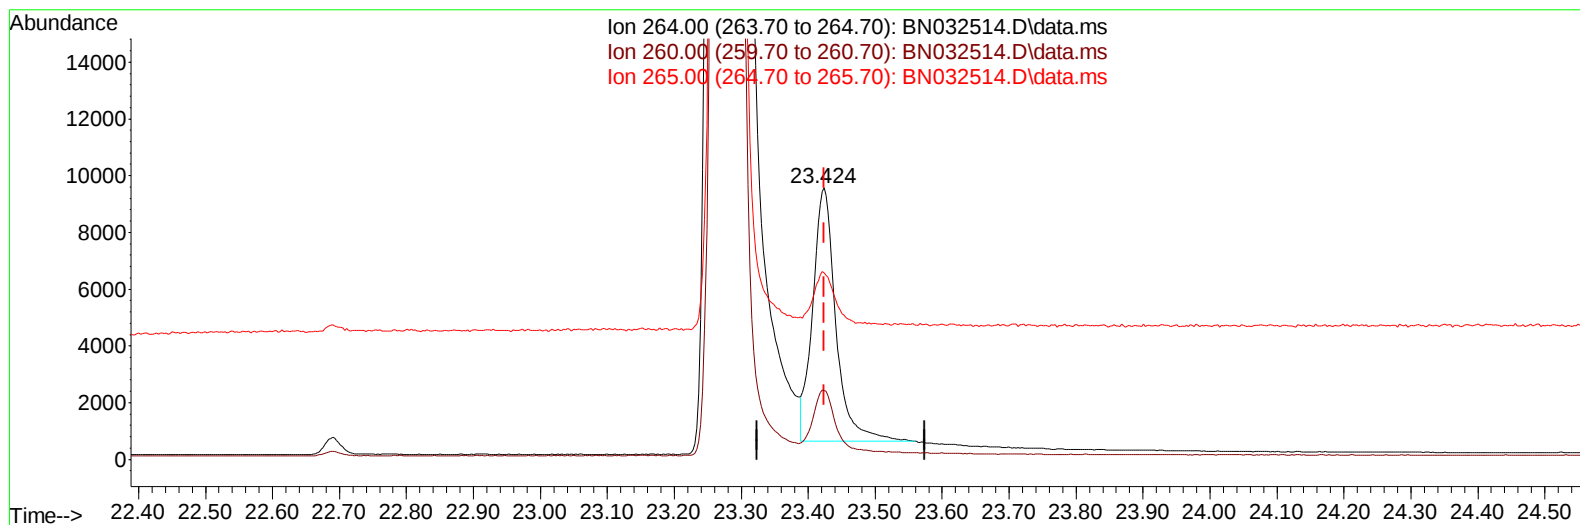

TIC: BN032514.D\data.ms

(23) Perylene-d12 (I)

23.424min (-0.000) 0.40 ng/u1

response 21692

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.36
265.00	67.20	68.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
Data File : BN032514.D
Acq On : 05 Jul 2024 18:53
Operator : MA/JU
Sample : PB161679BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK679

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

Quant Time: Jul 05 23:28:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

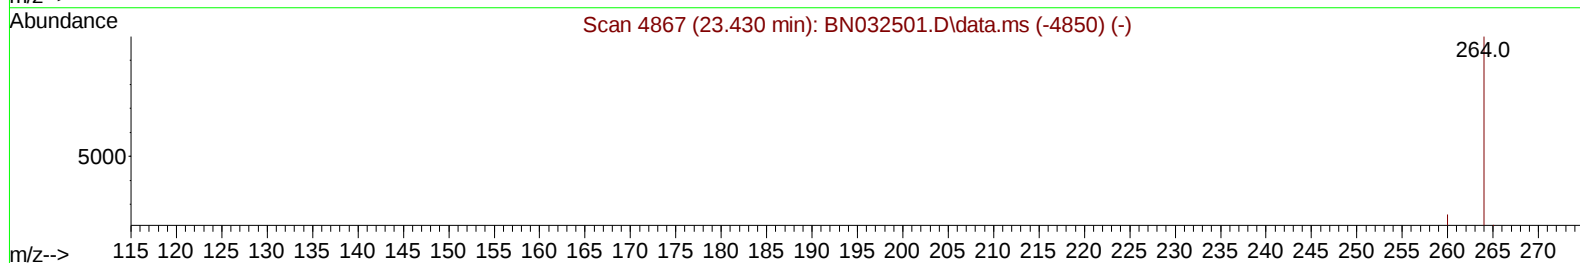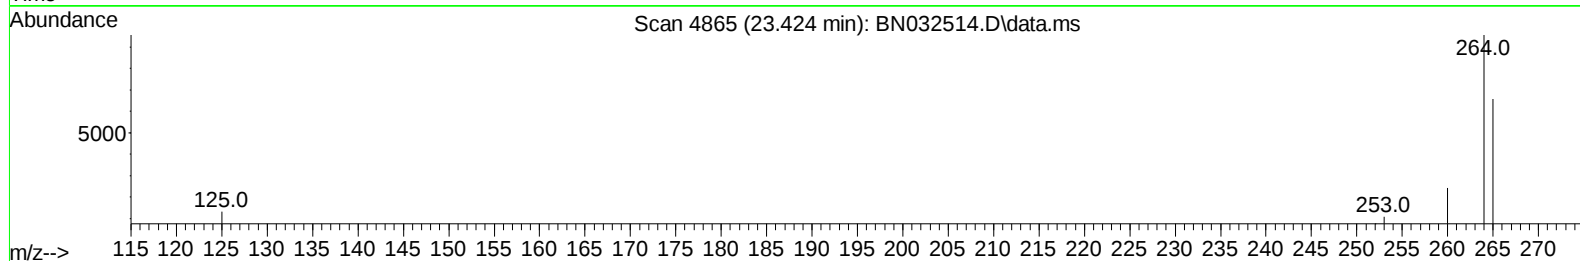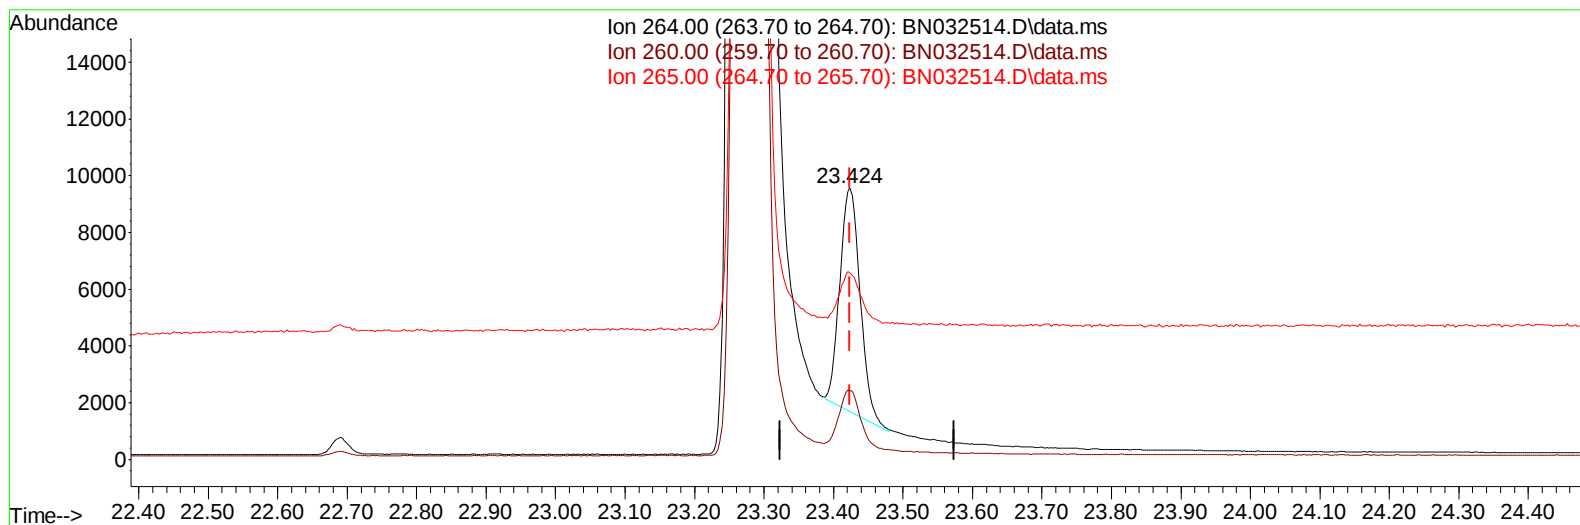

TIC: BN032514.D\data.ms

(23) Perylene-d12 (I)

23.424min (-0.000) 0.40 ng/ul m

response 15900

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.36
265.00	67.20	68.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
 Data File : BN032514.D
 Acq On : 05 Jul 2024 18:53
 Operator : MA/JU
 Sample : PB161679BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK679

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/08/2024
 Supervised By :mohammad ahmed 07/08/2024

Quant Time: Jul 05 23:28:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.595	152	6214	0.400	ng/ul	0.00
4) Naphthalene-d8	10.365	136	17852	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.239	164	9303	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.999	188	17072m	0.400	ng/ul	0.00
17) Chrysene-d12	21.214	240	14850m	0.400	ng/ul	0.00
23) Perylene-d12	23.424	264	15900m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	38184	5.528	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.977	152	6603	0.247	ng/ul	0.00
18) Fluoranthene-d10	19.036	212	11847	0.265	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
Data File : BN032514.D
Acq On : 05 Jul 2024 18:53
Operator : MA/JU
Sample : PB161679BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK679

Manual IntegrationsAPPROVED

Quant Time: Jul 05 23:28:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

