

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
 Data File : BN032503.D
 Acq On : 05 Jul 2024 10:46
 Operator : MA/JU
 Sample : P2961-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GE0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/08/2024
 Supervised By :mohammad ahmed 07/08/2024

Quant Time: Jul 05 11:13:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.595	152	4429	0.400	ng/ul	0.00
4) Naphthalene-d8	10.371	136	12531	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.244	164	7107	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.999	188	13088m	0.400	ng/ul	0.00
17) Chrysene-d12	21.214	240	11835m	0.400	ng/ul	0.00
23) Perylene-d12	23.430	264	12514m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	24688	5.015	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.971	152	6722	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.041	212	14456	0.406	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.415	128	1223	0.037	ng/ul#	72
19) Fluoranthene	19.069	202	912	0.020	ng/ul#	58
21) Benzo(a)anthracene	21.203	228	1582	0.037	ng/ul#	47
22) Chrysene	21.252	228	2084	0.044	ng/ul#	60

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070524\
Data File : BN032503.D
Acq On : 05 Jul 2024 10:46
Operator : MA/JU
Sample : P2961-05
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GE0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024


Quant Time: Jul 05 11:13:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

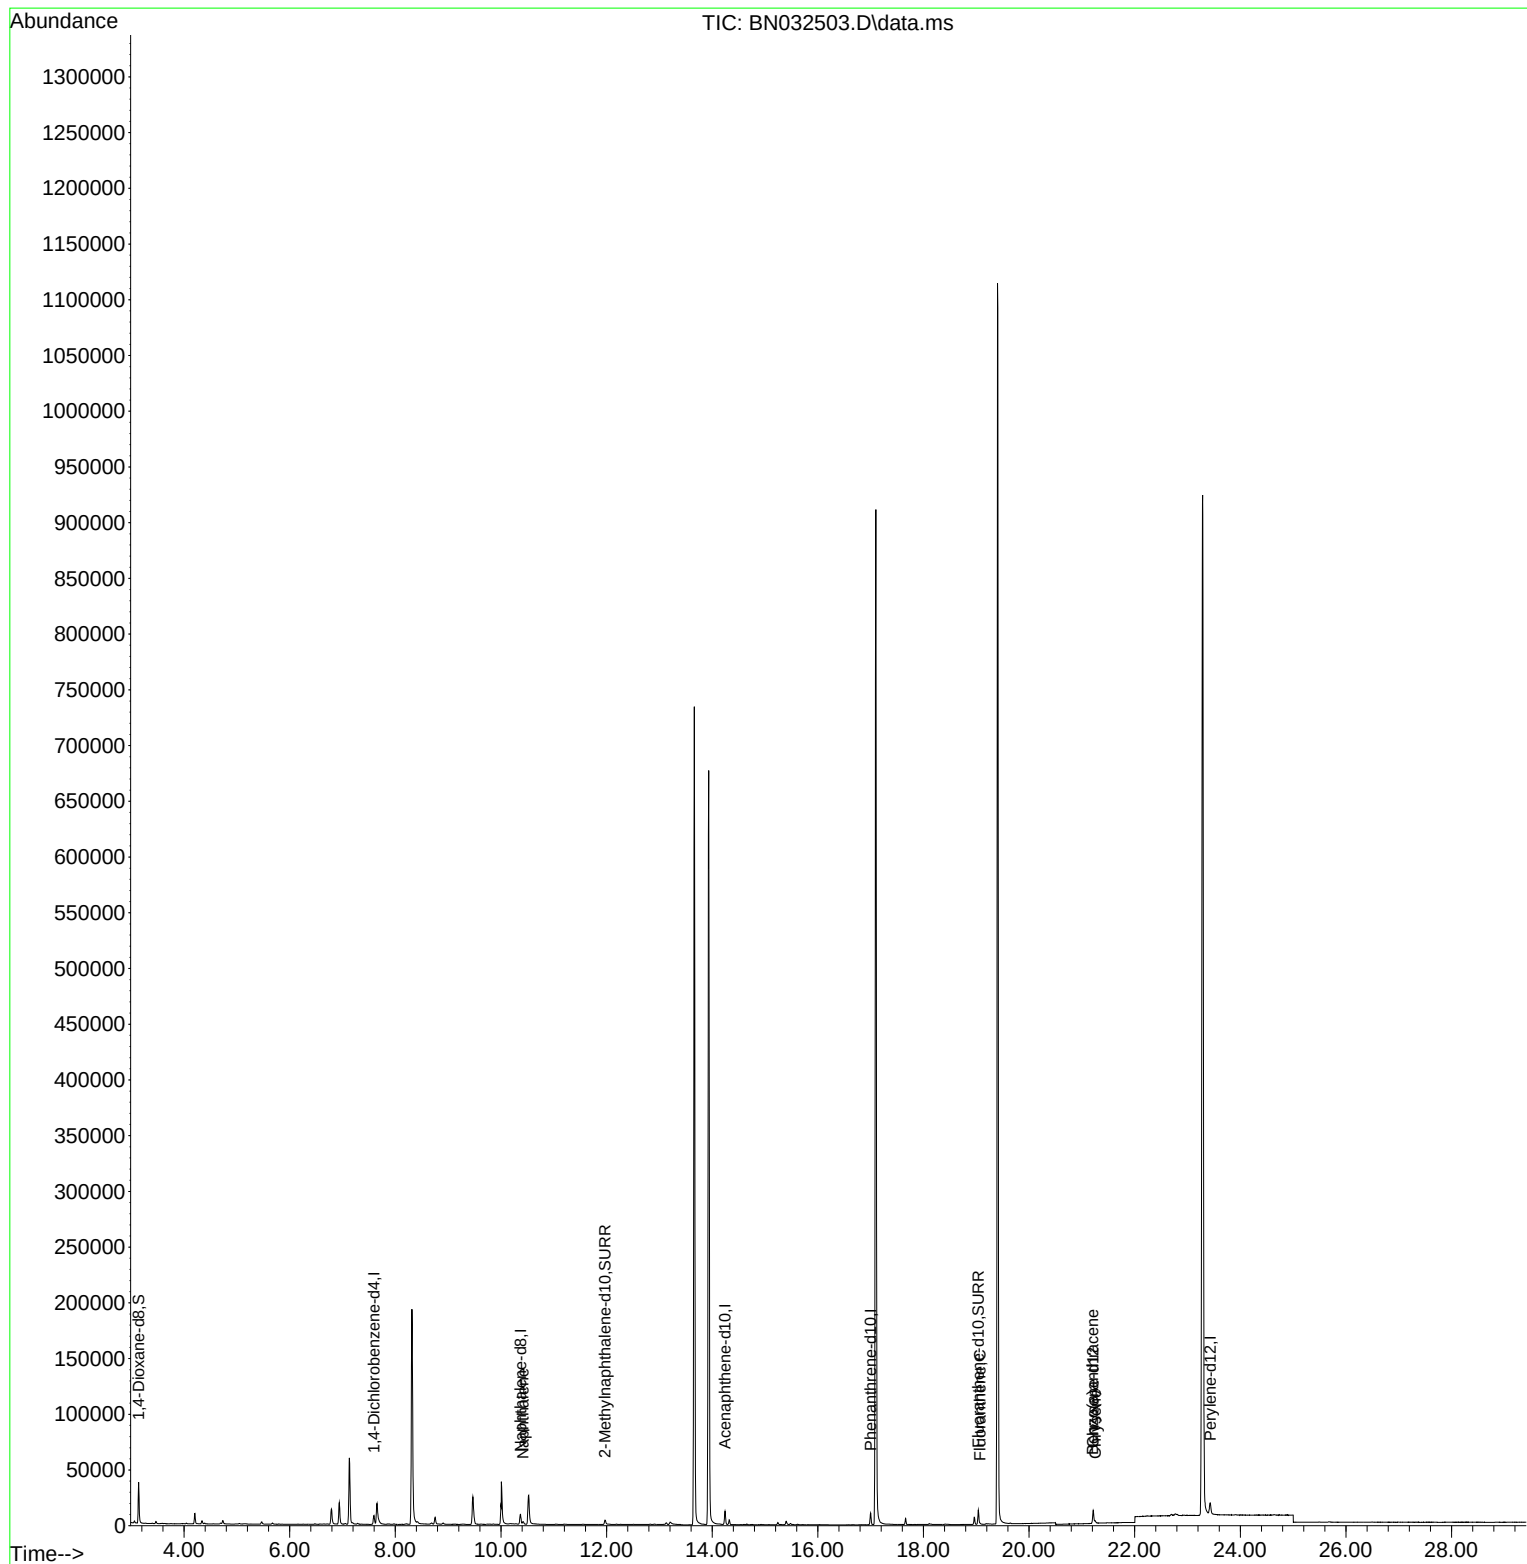

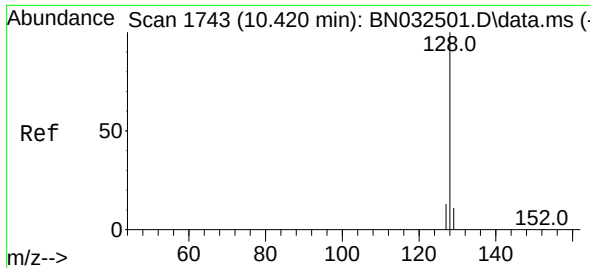

#5
Naphthalene
Concen: 0.037 ng/ul
RT: 10.415 min Scan# 1742
Delta R.T. -0.016 min
Lab File: BN032503.D
Acq: 05 Jul 2024 10:46




Instrument :
BNA_N
ClientSampleId :
E1GE0

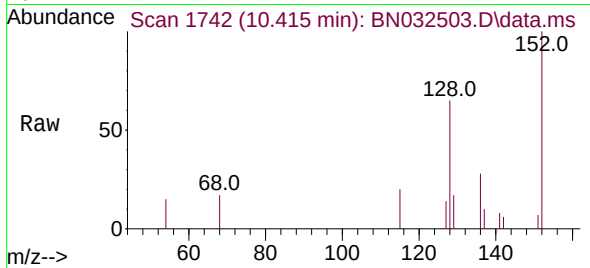

Tgt Ion:128 Resp: 122
Ion Ratio Lower Upper
128 100
129 26.4 9.2 13.8#
127 21.2 10.8 16.2#




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

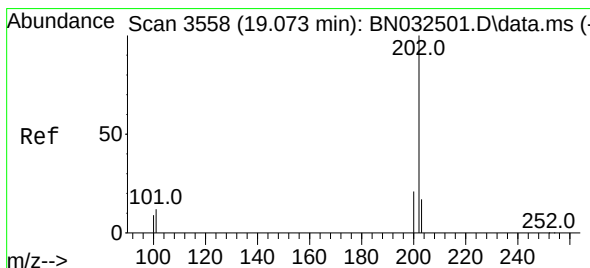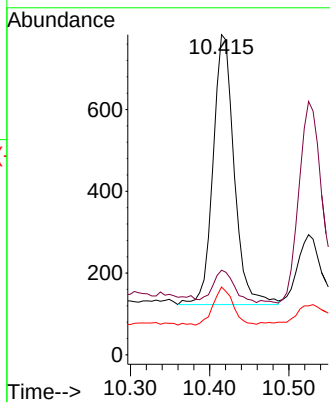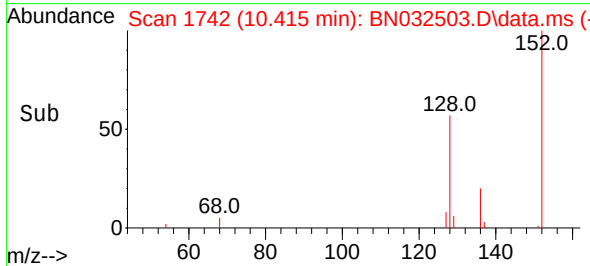

#19
Fluoranthene
Concen: 0.020 ng/ul
RT: 19.069 min Scan# 3557
Delta R.T. -0.005 min
Lab File: BN032503.D
Acq: 05 Jul 2024 10:46


Tgt Ion:202 Resp: 912
Ion Ratio Lower Upper
202 100
101 29.0 8.8 13.2#
100 20.5 6.4 9.6#

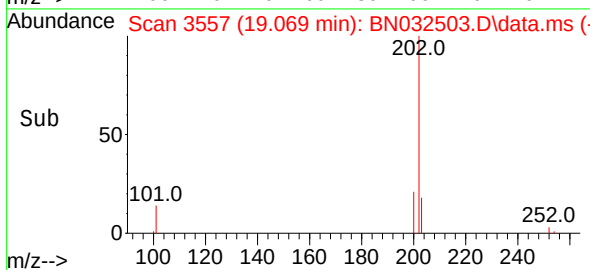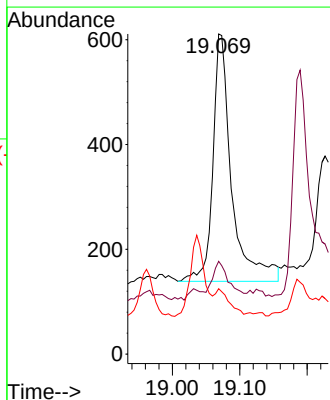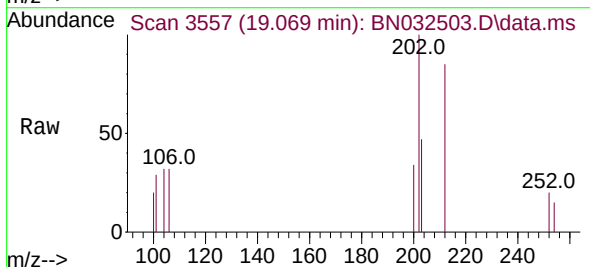

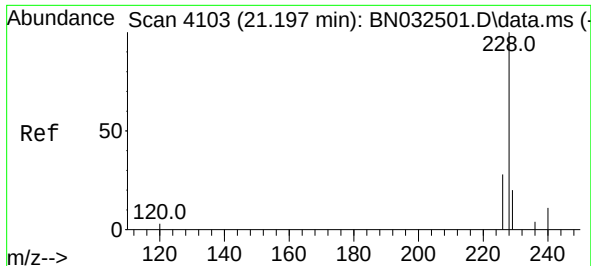

#21
Benzo(a)anthracene
Concen: 0.037 ng/ul
RT: 21.203 min Scan# 4105
Delta R.T. 0.012 min
Lab File: BN032503.D
Acq: 05 Jul 2024 10:46




Instrument :
BNA_N
ClientSampleId :
E1GE0

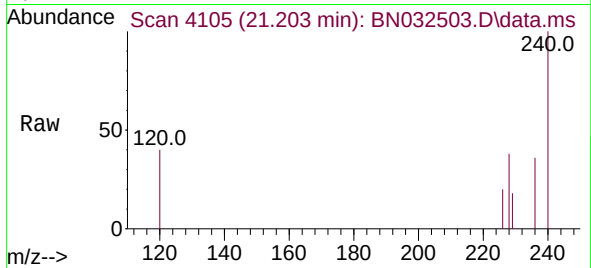

Tgt Ion:228 Resp: 1582
Ion Ratio Lower Upper
228 100
229 46.1 15.7 23.5#
226 53.0 21.8 32.8#

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

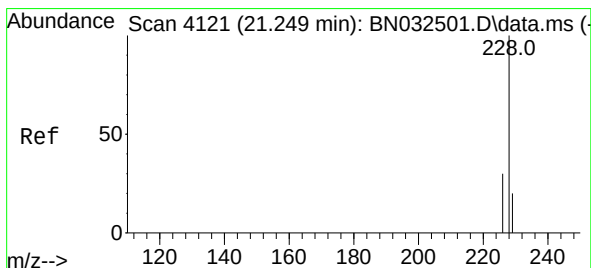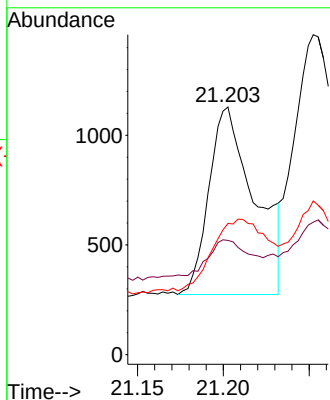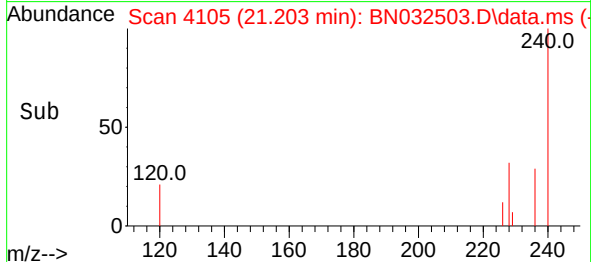

#22
Chrysene
Concen: 0.044 ng/ul
RT: 21.252 min Scan# 4122
Delta R.T. 0.009 min
Lab File: BN032503.D
Acq: 05 Jul 2024 10:46

Tgt Ion:228 Resp: 2084
Ion Ratio Lower Upper
228 100
226 48.0 23.6 35.4#
229 41.4 15.7 23.5#

