


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070620\  
 Data File : BN011096.D  
 Acq On : 06 Jul 2020 08:08  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN063020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jul 06 10:52:12 2020

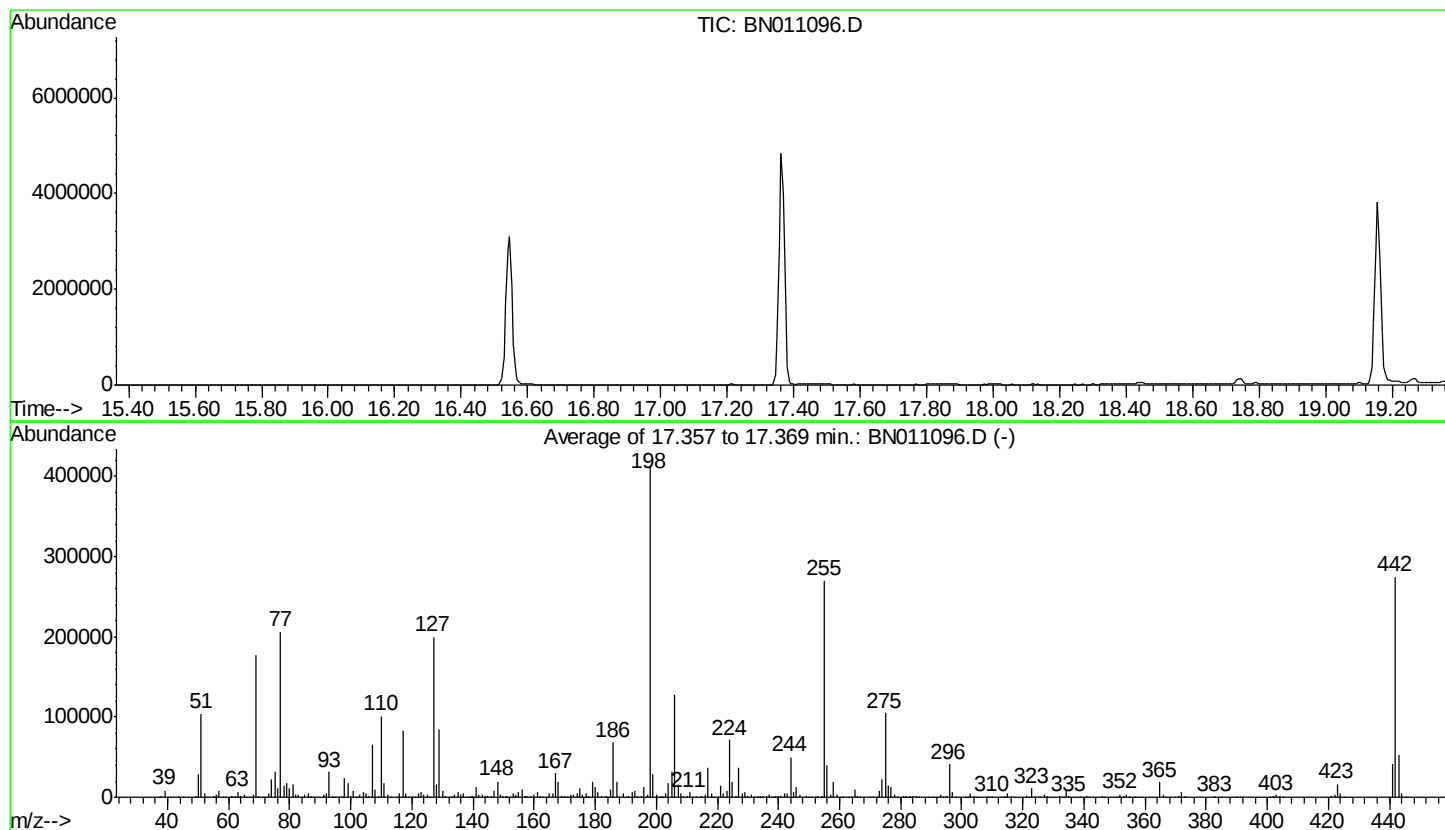

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 25.2      | 104050  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 2997    | PASS             |
| 69          | 198          | 0.00         | 100          | 43.0      | 177813  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 1131    | PASS             |
| 127         | 198          | 10           | 80           | 48.4      | 200320  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.8       | 3259    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 413504  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 28056   | PASS             |
| 275         | 198          | 10           | 60           | 25.4      | 104984  | PASS             |
| 365         | 198          | 1            | 100          | 4.6       | 19113   | PASS             |
| 441         | 198          | 0.01         | 100          | 10.2      | 42146   | PASS             |
| 442         | 198          | 50           | 100          | 66.5      | 275114  | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 52728   | PASS             |