
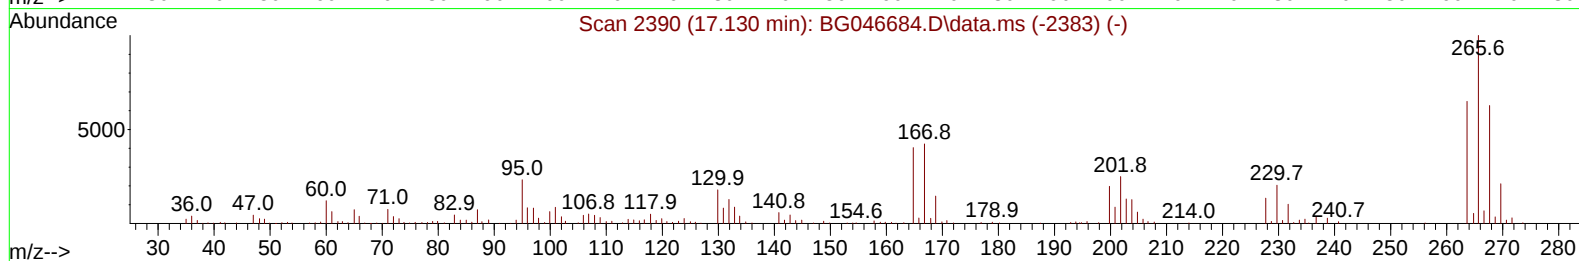
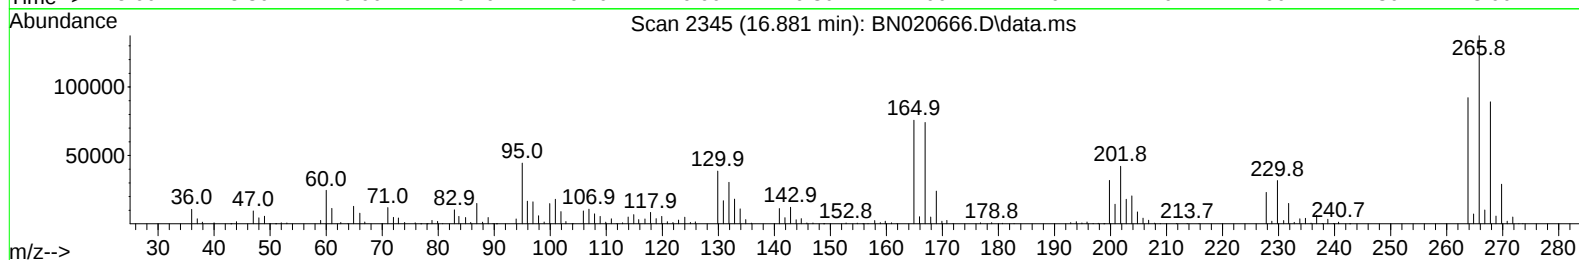


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070622\
Data File : BN020666.D
Acq On : 06 Jul 2022 13:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 01:03:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 01:03:39 2022
Response via : Initial Calibration

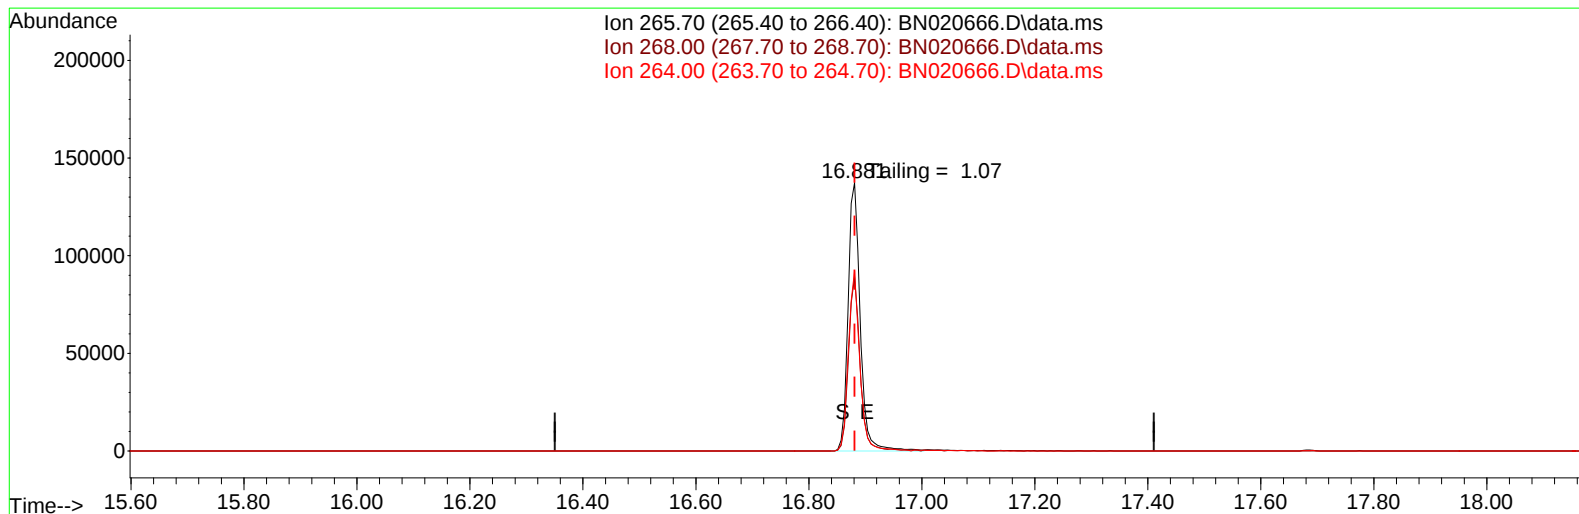

TIC: BN020666.D\data.ms

(70) Pentachlorophenol (C)




16.881min (0.000) 15799.79 ng

response 205456

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.93
264.00	61.60	67.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070622\
Data File : BN020666.D
Acq On : 06 Jul 2022 13:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 01:03:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 01:03:39 2022
Response via : Initial Calibration

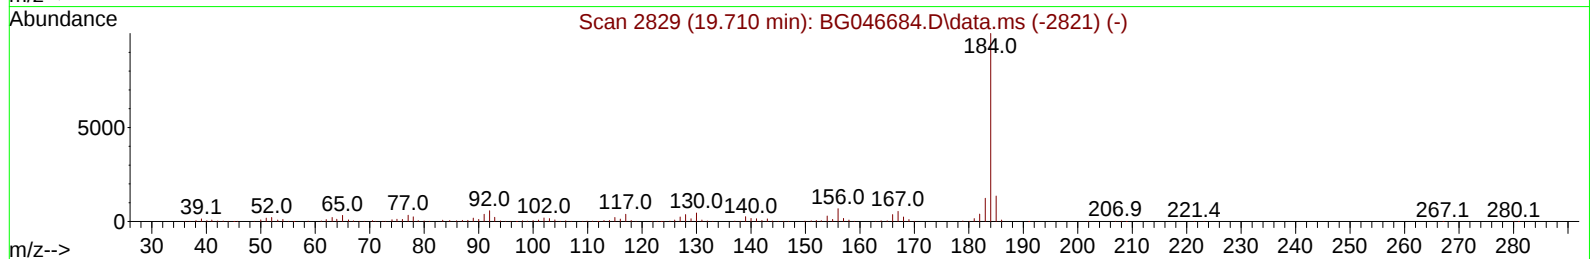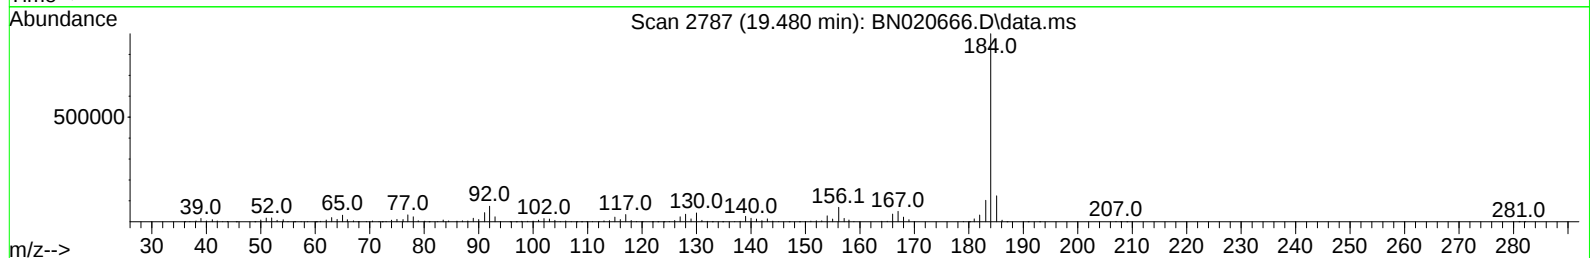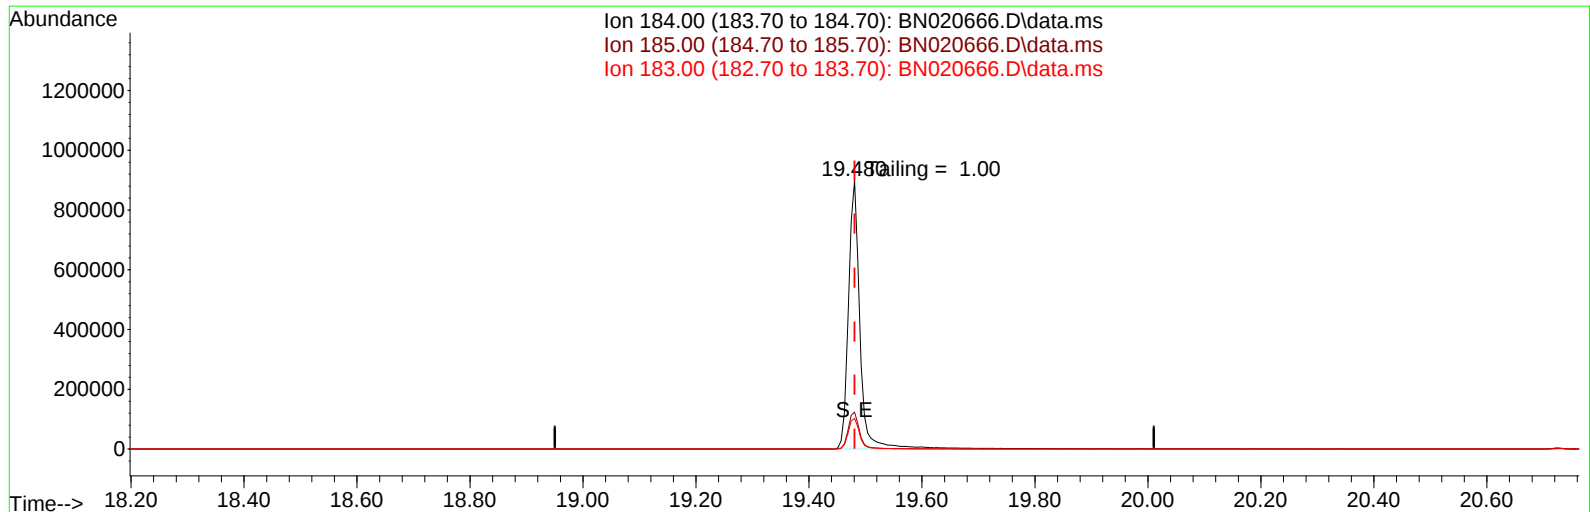

TIC: BN020666.D\data.ms

(77) Benzidine

19.480min (0.000) 0.00 ng

response 1280003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	11.42
0.00	0.00	0.00