

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070622\
 Data File : BN020672.D
 Acq On : 06 Jul 2022 18:06
 Operator : CG/JU
 Sample : N3591-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 OW-01B-64-69-070522

Quant Time: Jul 06 23:48:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 02 03:10:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.826	152	4066	0.400	ng	0.00
7) Naphthalene-d8	10.626	136	12058	0.400	ng	# 0.00
13) Acenaphthene-d10	14.474	164	6580	0.400	ng	0.00
19) Phenanthrene-d10	17.226	188	12711	0.400	ng	# 0.00
29) Chrysene-d12	21.431	240	8454	0.400	ng	0.00
35) Perylene-d12	23.788	264	5986	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.421	112	941	0.083	ng	0.00
5) Phenol-d6	7.053	99	545	0.040	ng	0.02
8) Nitrobenzene-d5	9.003	82	1973	0.202	ng	0.01
11) 2-Methylnaphthalene-d10	12.227	152	5578	0.270	ng	0.00
14) 2,4,6-Tribromophenol	15.974	330	501	0.202	ng	0.00
15) 2-Fluorobiphenyl	13.105	172	7363	0.271	ng	0.00
27) Fluoranthene-d10	19.265	212	11755	0.311	ng	0.00
31) Terphenyl-d14	19.868	244	9868	0.488	ng	0.00
Target Compounds						
9) Naphthalene	10.680	128	999	0.028	ng	# 78
30) Pyrene	19.666	202	1057	0.030	ng	97
34) Bis(2-ethylhexyl)phtha...	21.351	149	1609	0.095	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070622\
Data File : BN020672.D
Acq On : 06 Jul 2022 18:06
Operator : CG/JU
Sample : N3591-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
OW-01B-64-69-070522


Quant Time: Jul 06 23:48:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 03:10:12 2022
Response via : Initial Calibration

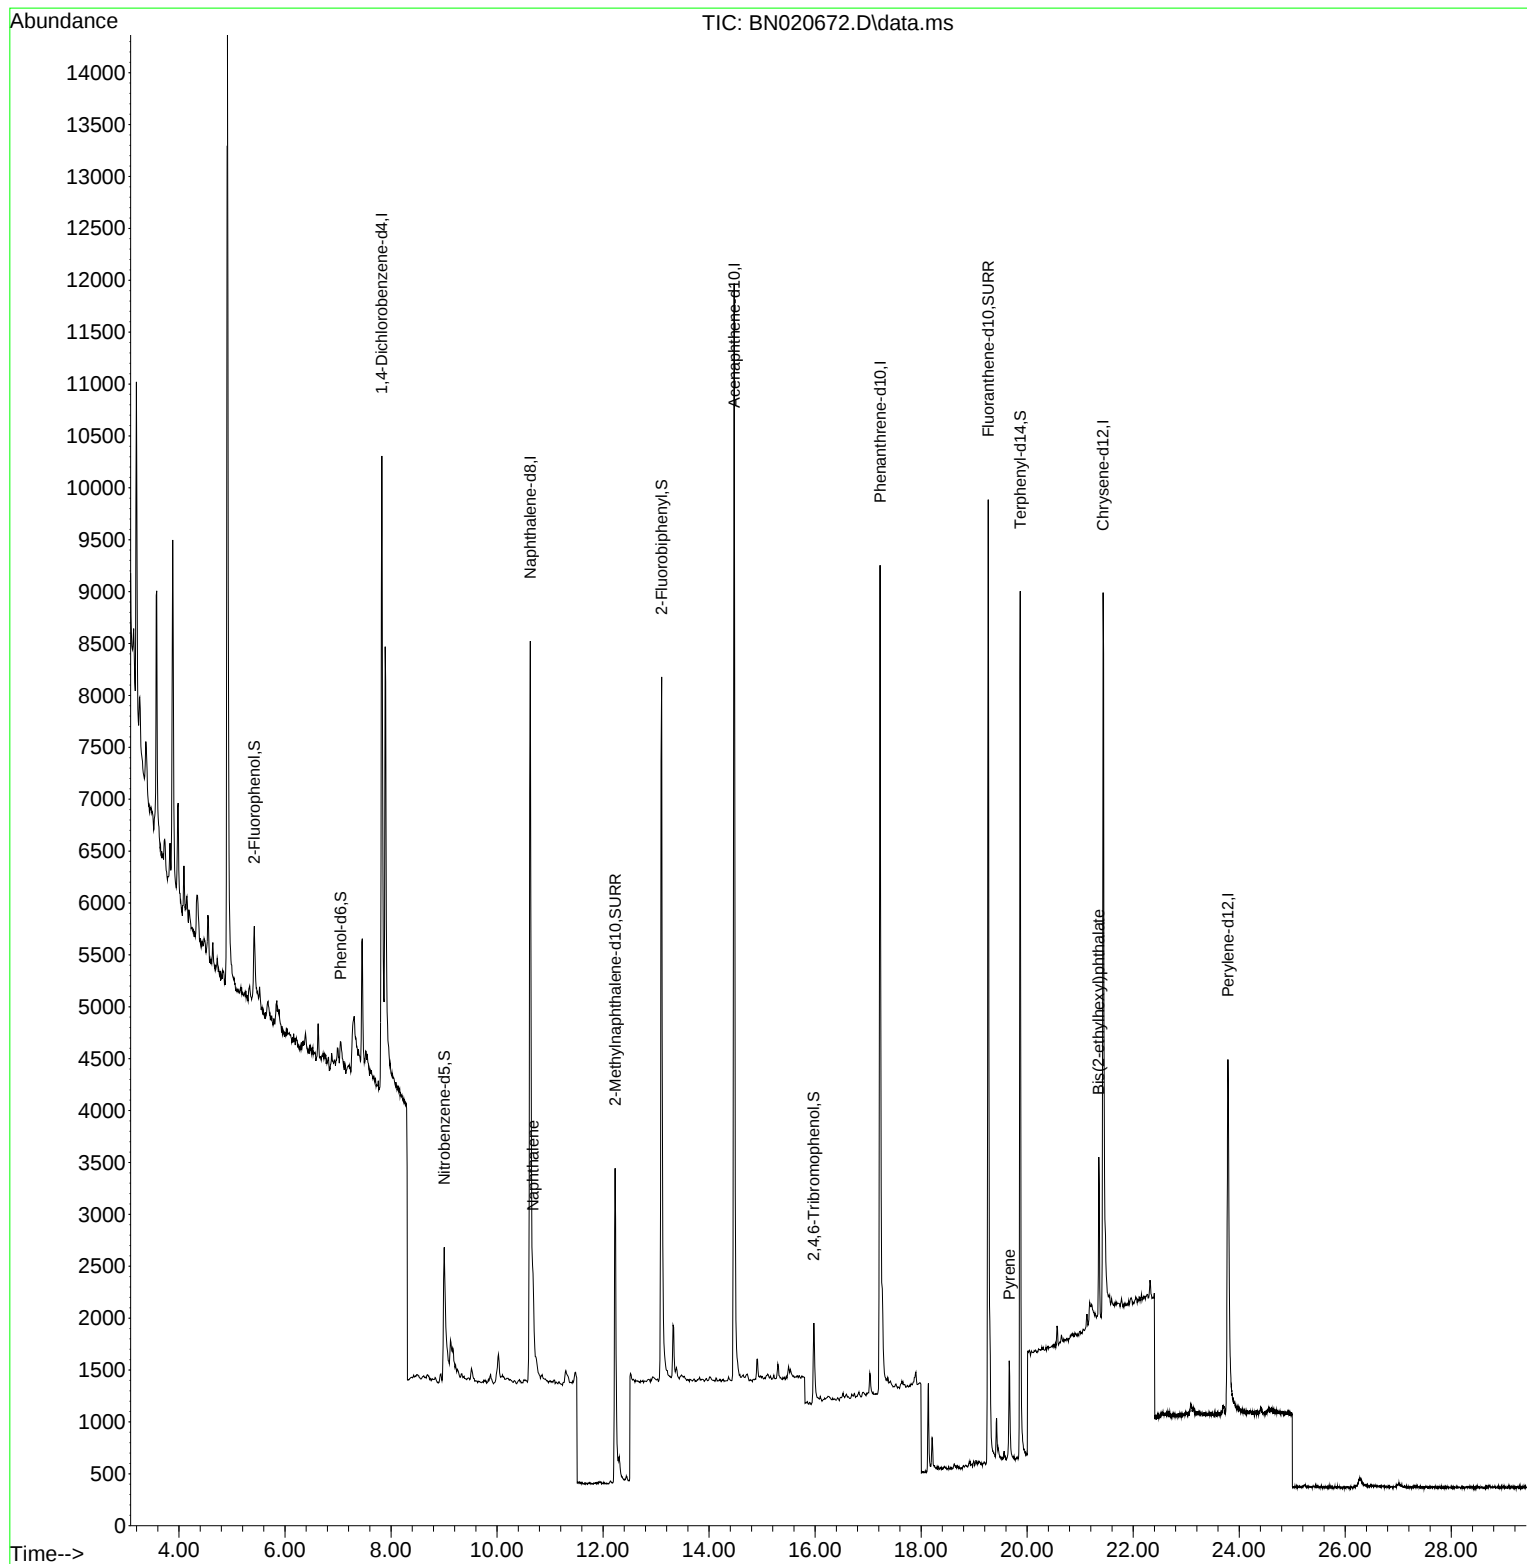






#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.826 min Scan# 61
Delta R.T. 0.001 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06

Instrument :
BNA_N
ClientSampleId :
OW-01B-64-69-070522



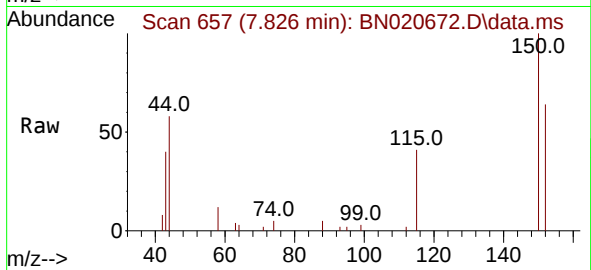


Tgt Ion:152 Resp: 4066
Ion Ratio Lower Upper
152 100
150 157.1 127.9 191.9
115 63.8 51.4 77.2

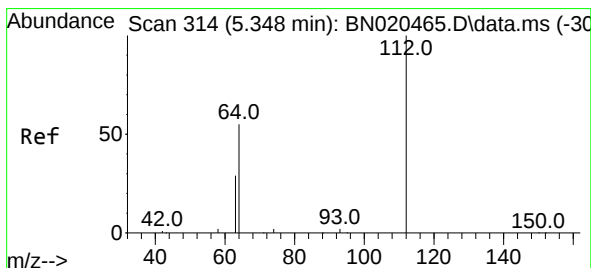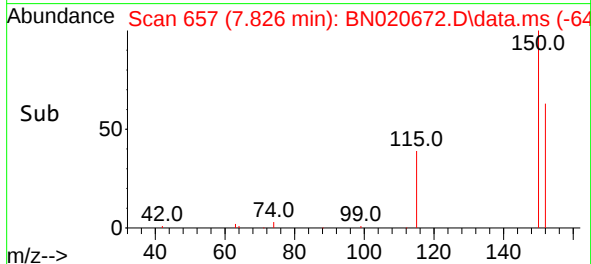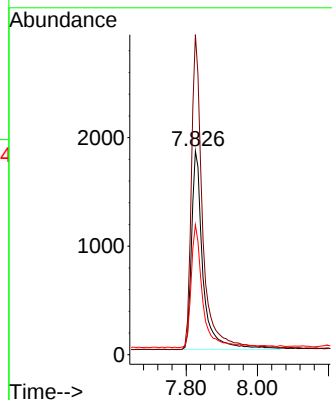

#4
2-Fluorophenol
Concen: 0.083 ng
RT: 5.421 min Scan# 324
Delta R.T. 0.007 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06

Tgt Ion:112 Resp: 941
Ion Ratio Lower Upper
112 100
64 66.4 49.1 73.7
63 37.3 26.3 39.5



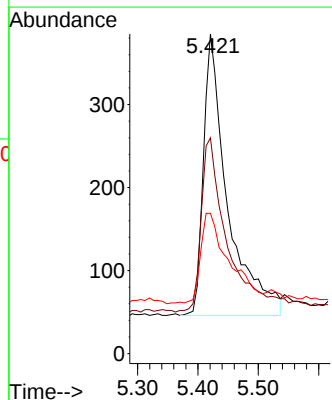





#5
Phenol-d6
Concen: 0.040 ng
RT: 7.053 min Scan# 511
Delta R.T. 0.022 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06




Instrument :
BNA_N
ClientSampleId :
OW-01B-64-69-070522

Tgt Ion: 99 Resp: 545
Ion Ratio Lower Upper
99 100
42 22.6 19.3 28.9
71 25.1 27.5 41.3#

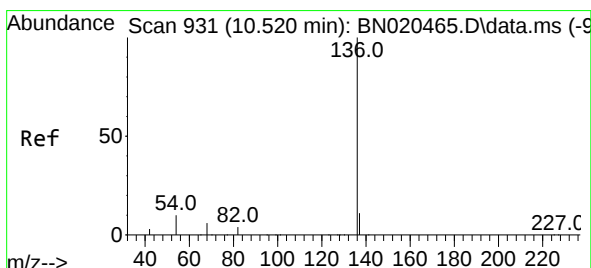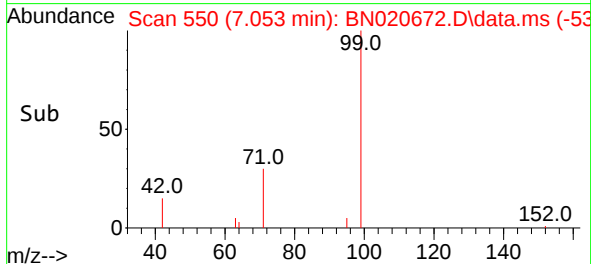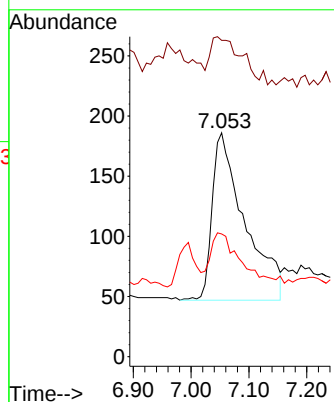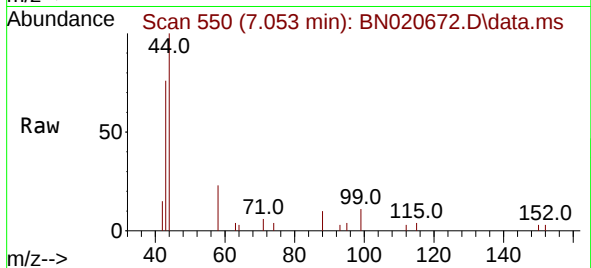

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.626 min Scan# 941
Delta R.T. 0.000 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06

Tgt Ion: 136 Resp: 12058
Ion Ratio Lower Upper
136 100
137 11.6 9.0 13.6
54 10.2 6.2 9.2#
68 6.8 4.4 6.6#



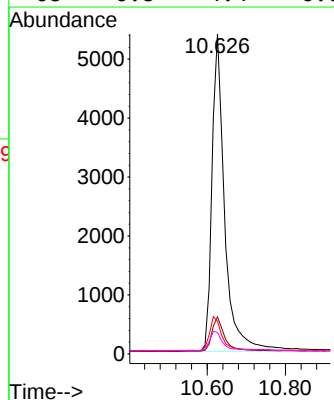





#8
 Nitrobenzene-d5
 Concen: 0.202 ng
 RT: 9.003 min Scan# 719
 Delta R.T. 0.011 min
 Lab File: BN020672.D
 Acq: 06 Jul 2022 18:06




Instrument :
 BNA_N
 ClientSampleId :
 OW-01B-64-69-070522

Tgt Ion: 82 Resp: 1973
 Ion Ratio Lower Upper
 82 100
 128 42.0 35.0 52.6
 54 61.4 46.2 69.4

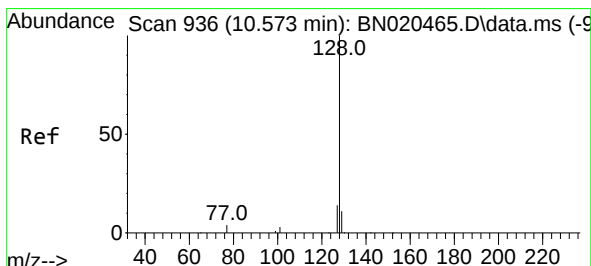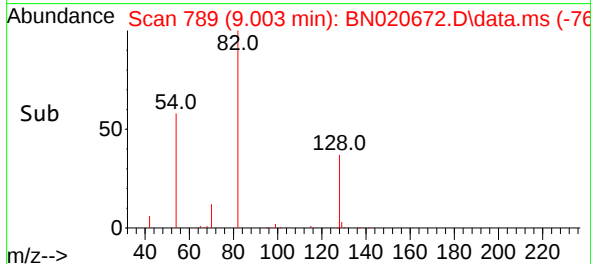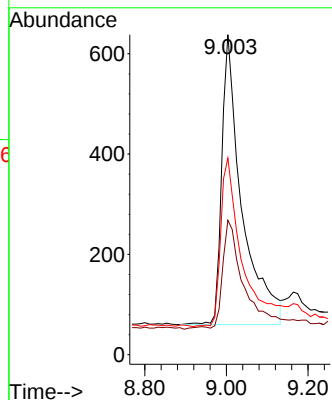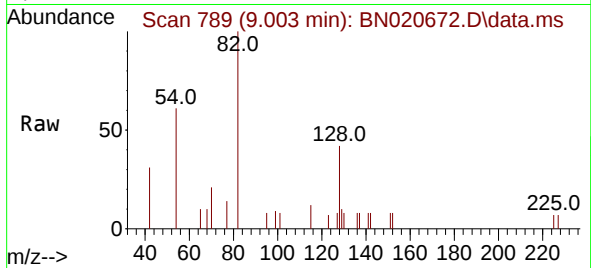

#9
 Naphthalene
 Concen: 0.028 ng
 RT: 10.680 min Scan# 946
 Delta R.T. 0.000 min
 Lab File: BN020672.D
 Acq: 06 Jul 2022 18:06

Tgt Ion: 128 Resp: 999
 Ion Ratio Lower Upper
 128 100
 129 20.8 8.9 13.3#
 127 20.8 10.8 16.2#


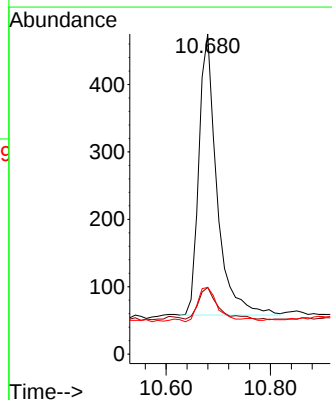





#11
2-Methylnaphthalene-d10
Concen: 0.270 ng
RT: 12.227 min Scan# 1185
Delta R.T. 0.000 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06




Instrument :
BNA_N
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion:152 Resp: 5578
Ion Ratio Lower Upper
152 100
151 19.8 16.2 24.4

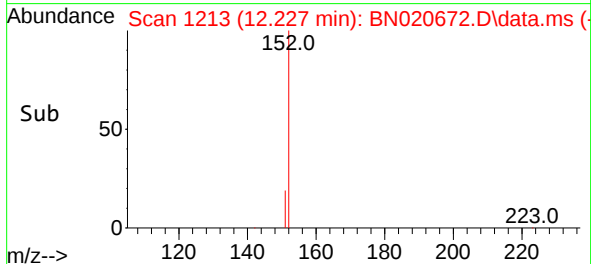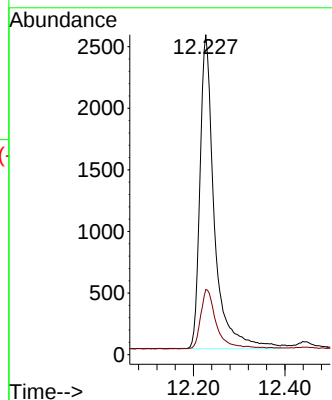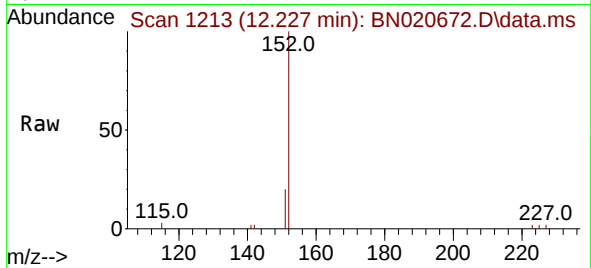

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.474 min Scan# 1471
Delta R.T. 0.000 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06


Tgt Ion:164 Resp: 6580
Ion Ratio Lower Upper
164 100
162 103.5 82.1 123.1
160 48.6 38.6 58.0

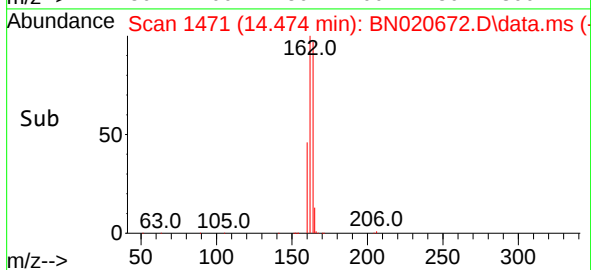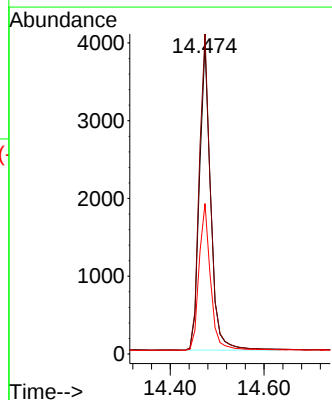



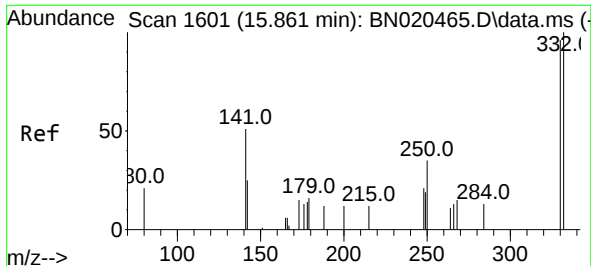


#14
2,4,6-Tribromophenol
Concen: 0.202 ng
RT: 15.974 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06

Instrument :
BNA_N
ClientSampleId :
OW-01B-64-69-070522



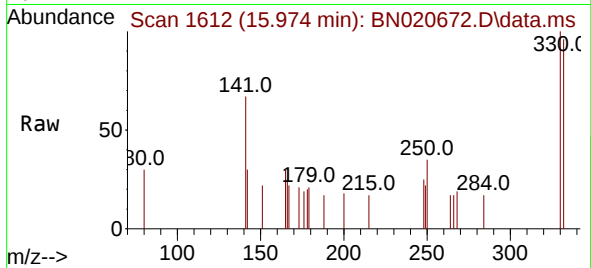


Tgt Ion:330 Resp: 501
Ion Ratio Lower Upper
330 100
332 95.4 77.6 116.4
141 56.9 41.0 61.4

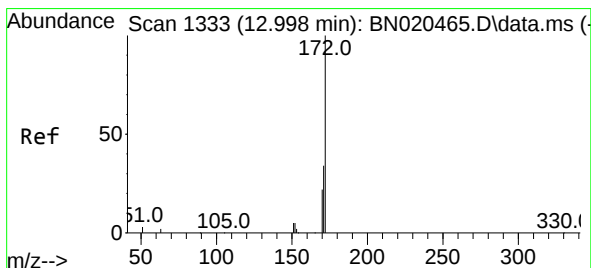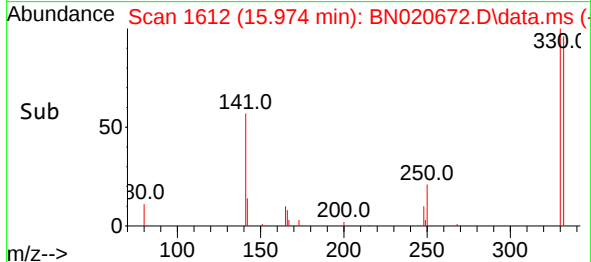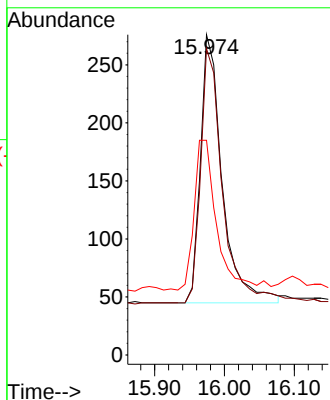

#15
2-Fluorobiphenyl
Concen: 0.271 ng
RT: 13.105 min Scan# 1343
Delta R.T. 0.000 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06

Tgt Ion:172 Resp: 7363
Ion Ratio Lower Upper
172 100
171 33.8 27.2 40.8
170 23.5 18.2 27.4



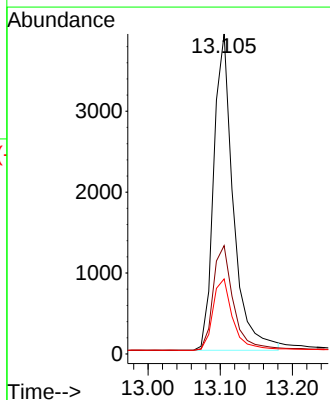
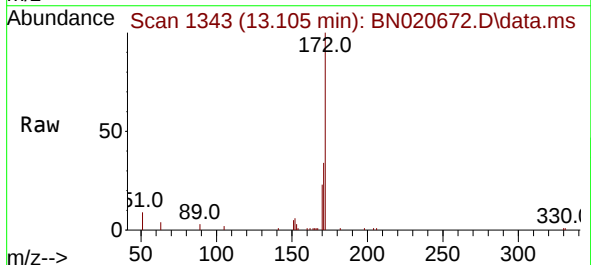




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.226 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06




Instrument :
BNA_N
ClientSampleId :
OW-01B-64-69-070522


Tgt Ion:188 Resp: 12711
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.0 7.4 11.2#

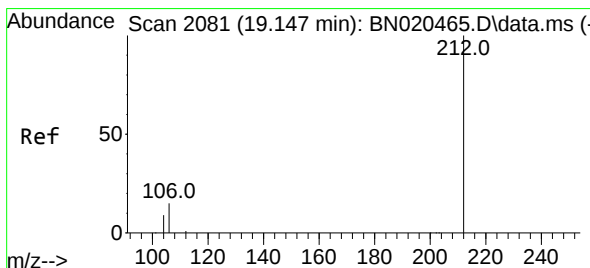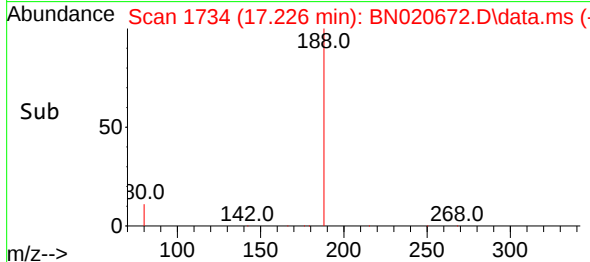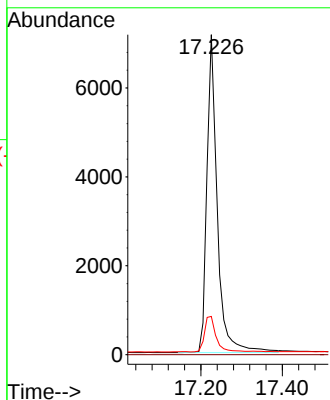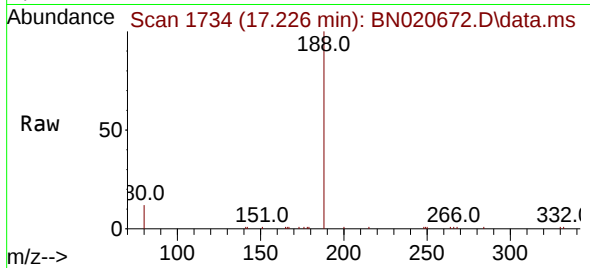

#27
Fluoranthene-d10
Concen: 0.311 ng
RT: 19.265 min Scan# 2109
Delta R.T. -0.004 min
Lab File: BN020672.D
Acq: 06 Jul 2022 18:06

Tgt Ion:212 Resp: 11755
Ion Ratio Lower Upper
212 100
106 16.0 12.6 19.0
104 9.3 7.2 10.8

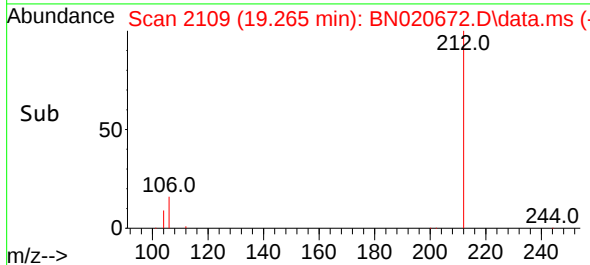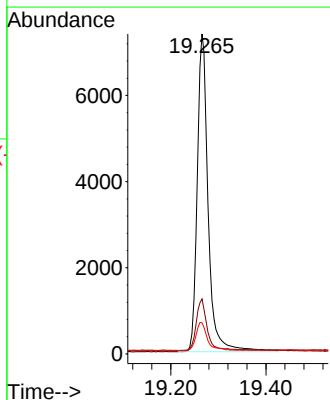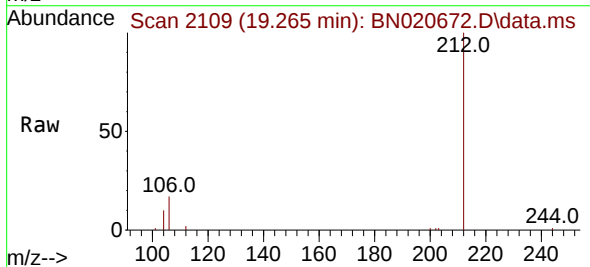

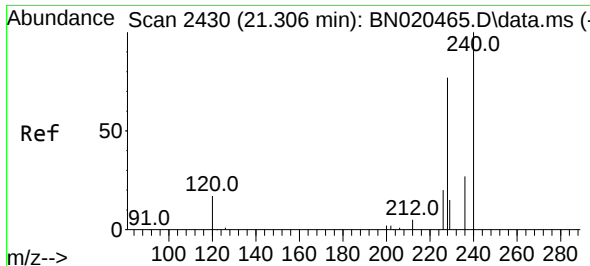

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.431 min Scan# 2444

Delta R.T. 0.000 min

Lab File: BN020672.D

Acq: 06 Jul 2022 18:06

Instrument :

BNA_N

ClientSampleId :

OW-01B-64-69-070522





Tgt Ion:240 Resp: 8454

Ion Ratio Lower Upper

240 100

120 19.3 14.6 21.8

236 28.0 22.6 33.8

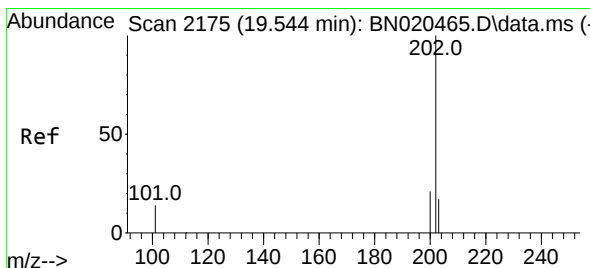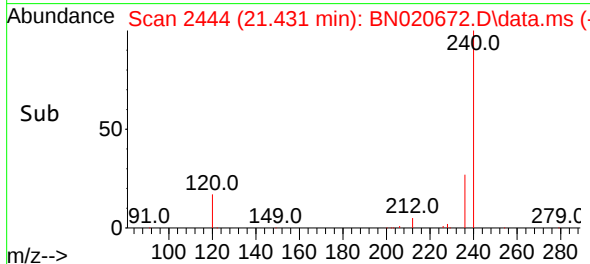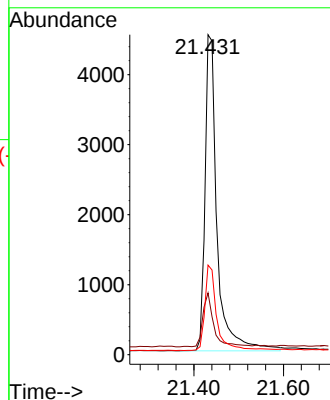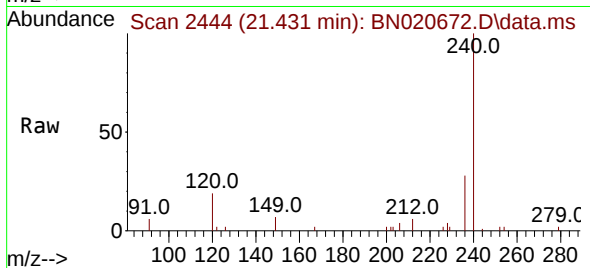

#30

Pyrene

Concen: 0.030 ng

RT: 19.666 min Scan# 2204

Delta R.T. 0.004 min

Lab File: BN020672.D

Acq: 06 Jul 2022 18:06




Tgt Ion:202 Resp: 1057

Ion Ratio Lower Upper

202 100

200 20.6 16.6 25.0


203 20.2 14.2 21.2

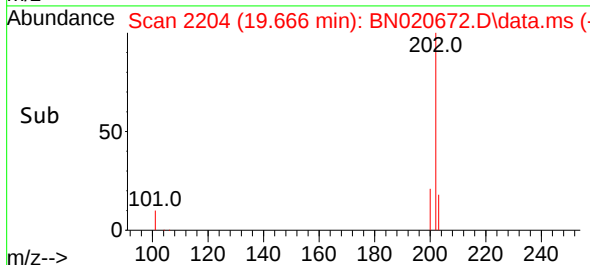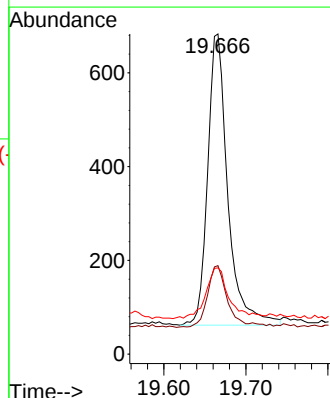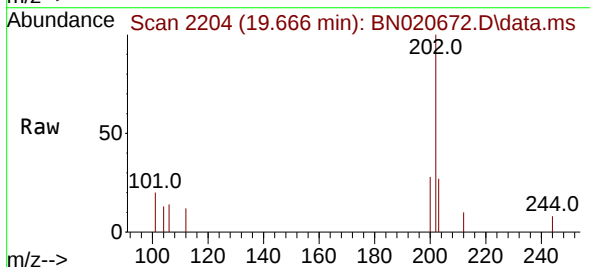






#31
 Terphenyl-d14
 Concen: 0.488 ng
 RT: 19.868 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN020672.D
 Acq: 06 Jul 2022 18:06

Instrument :
 BNA_N
 ClientSampleId :
 OW-01B-64-69-070522

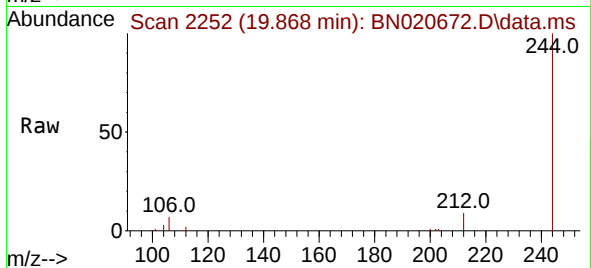

Tgt Ion:244 Resp: 9868




Ion	Ratio	Lower	Upper
244	100		
212	9.2	7.1	10.7
122	0.0	0.0	0.0

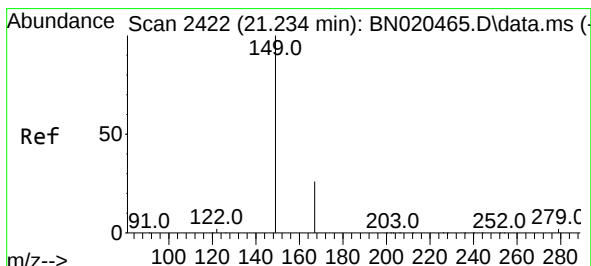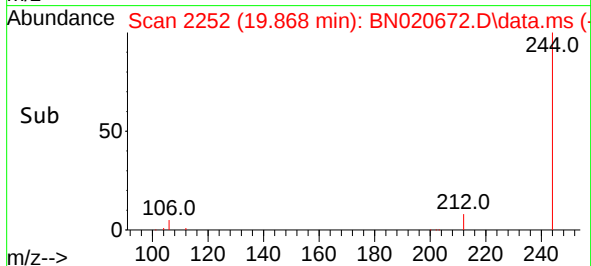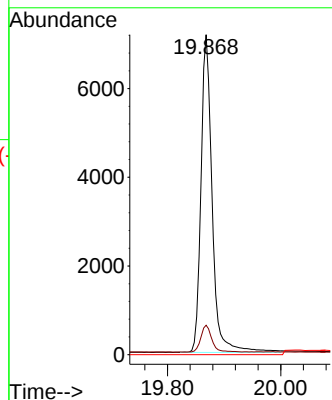


#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.095 ng
 RT: 21.351 min Scan# 2435
 Delta R.T. 0.000 min
 Lab File: BN020672.D
 Acq: 06 Jul 2022 18:06

Tgt Ion:149 Resp: 1609


Ion	Ratio	Lower	Upper
149	100		
167	24.7	21.7	32.5
279	3.0	2.2	3.2

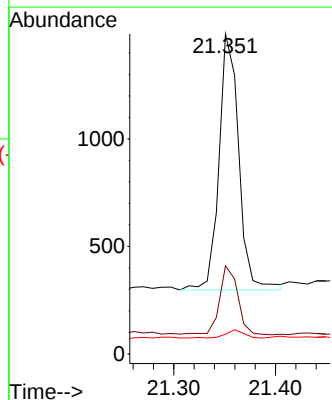

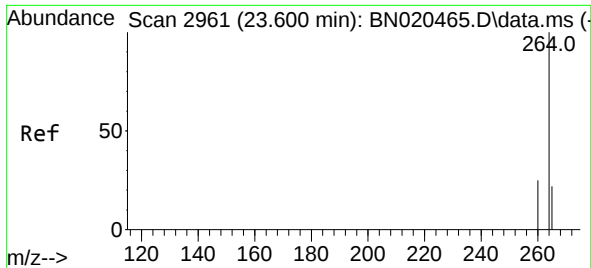

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.788 min Scan# 30
 Delta R.T. -0.003 min
 Lab File: BN020672.D
 Acq: 06 Jul 2022 18:06

Instrument :
 BNA_N
 ClientSampleId :
 OW-01B-64-69-070522

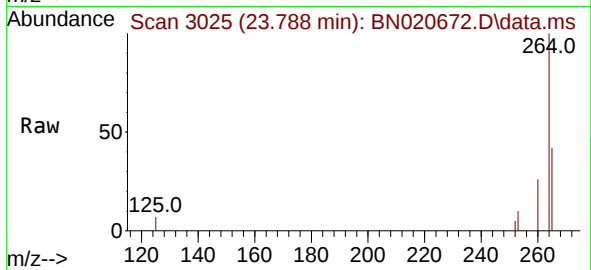

Tgt Ion:264 Resp: 5986
 Ion Ratio Lower Upper
 264 100
 260 26.2 20.9 31.3
 265 41.5 28.0 42.0

