
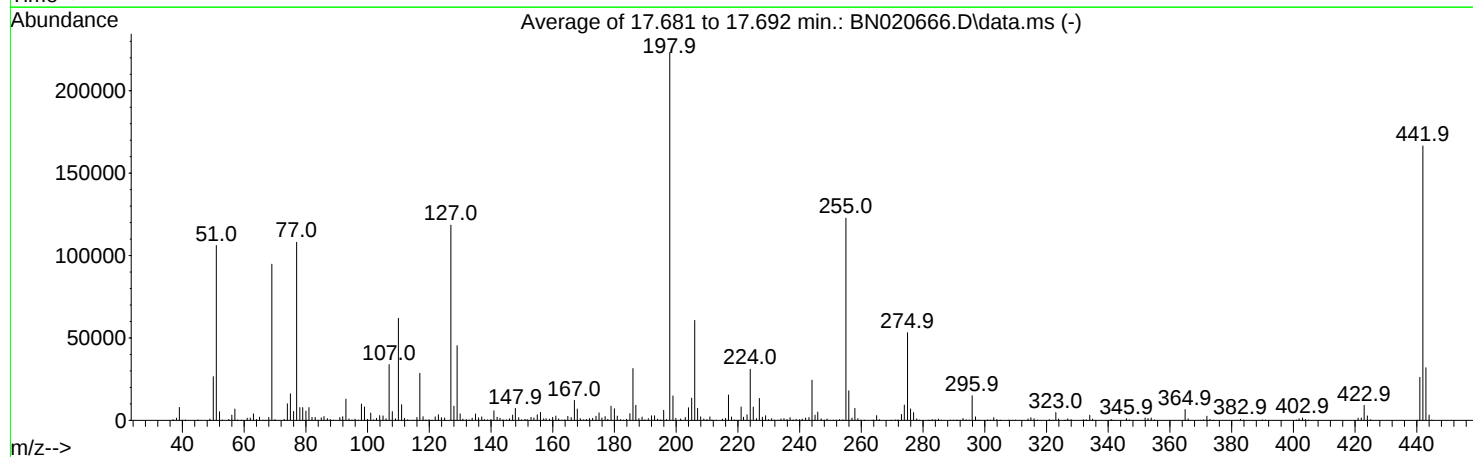


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070622\
Data File : BN020666.D
Acq On : 06 Jul 2022 13:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jul 02 03:10:12 2022

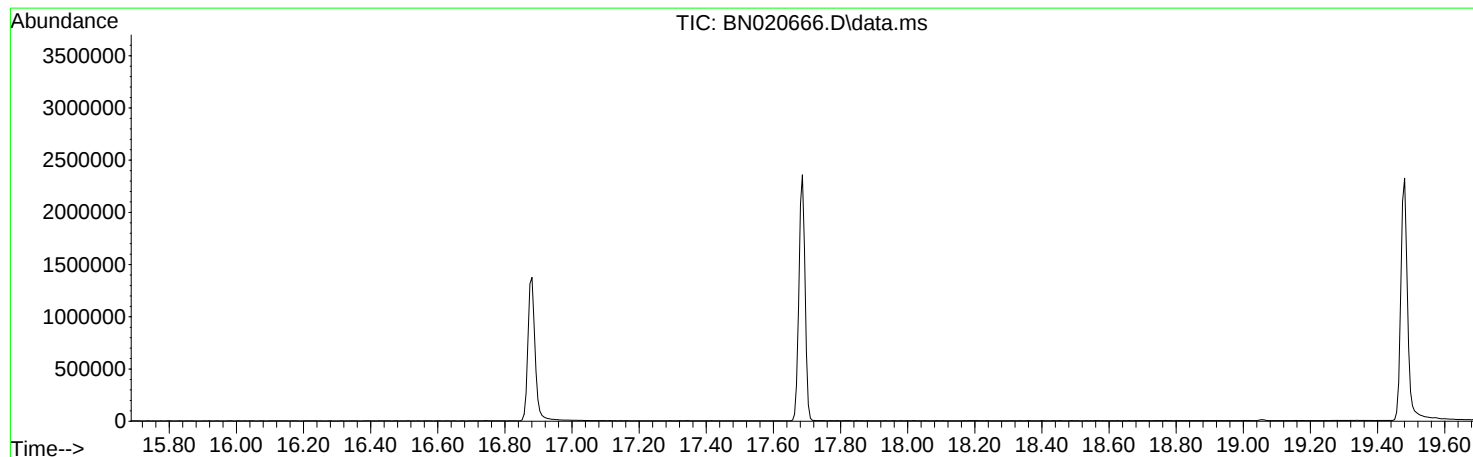




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	47.6	106157	PASS
68	69	0.00	2	2.0	1849	PASS
69	198	0.00	100	42.4	94752	PASS
70	69	0.00	2	0.5	480	PASS
127	198	10	80	53.1	118467	PASS
197	198	0.00	2	0.2	511	PASS
198	198	100	100	100.0	223211	PASS
199	198	5	9	6.7	14907	PASS
275	198	10	60	23.8	53160	PASS
365	198	1	100	3.0	6590	PASS
441	198	0.01	100	11.7	26115	PASS
442	442	50	100	100.0	166541	PASS
443	442	15	24	19.2	31928	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070622\
Data File : BN020666.D
Acq On : 06 Jul 2022 13:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 07 01:03:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 01:03:39 2022
Response via : Initial Calibration

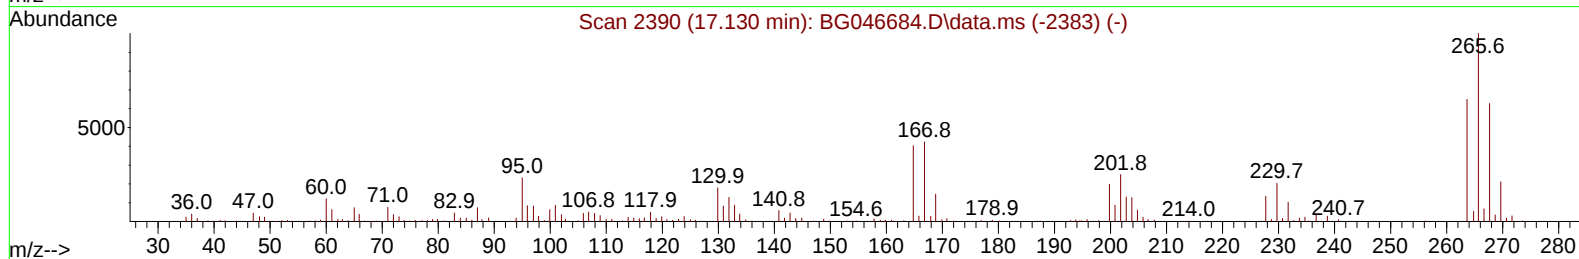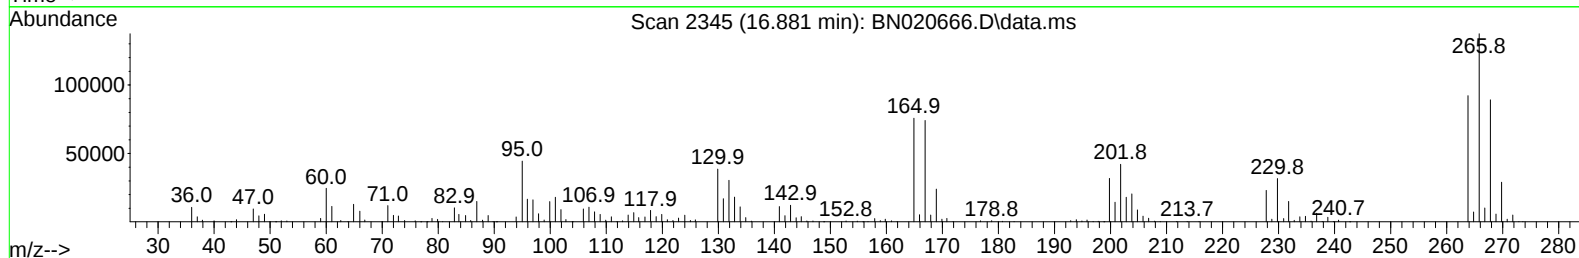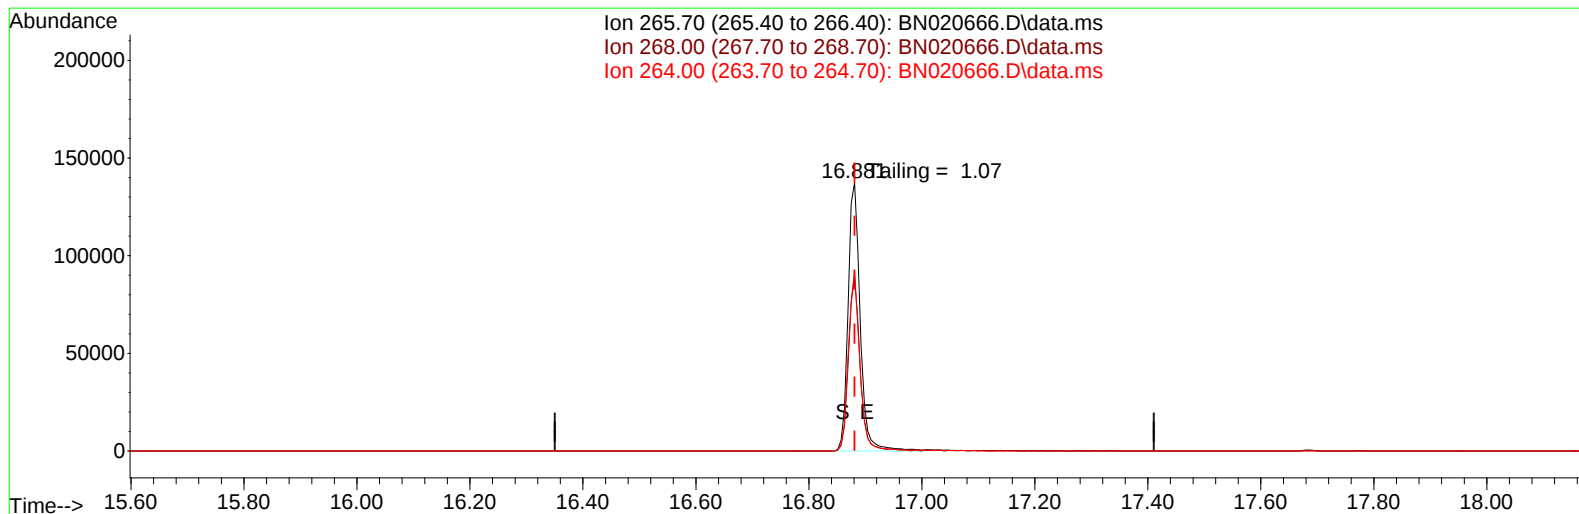

TIC: BN020666.D\data.ms

(70) Pentachlorophenol (C)

16.881min (0.000) 15799.79 ng




response 205456

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.93
264.00	61.60	67.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070622\
Data File : BN020666.D
Acq On : 06 Jul 2022 13:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 07 01:03:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 01:03:39 2022
Response via : Initial Calibration

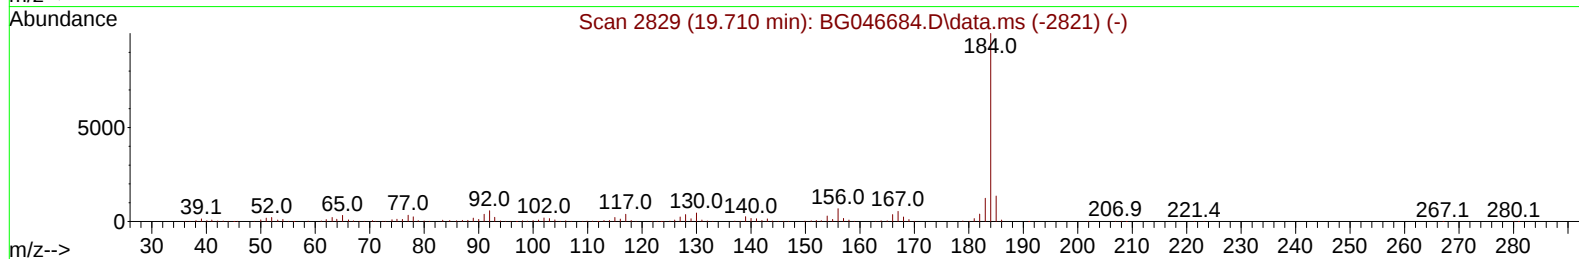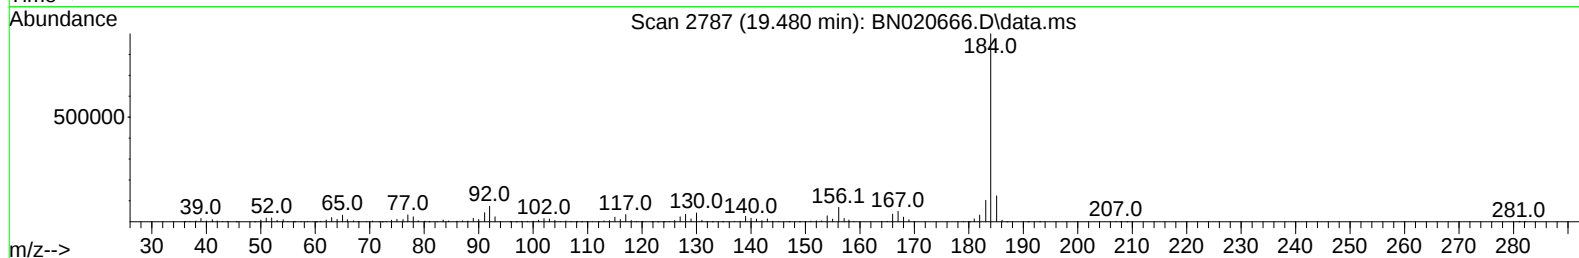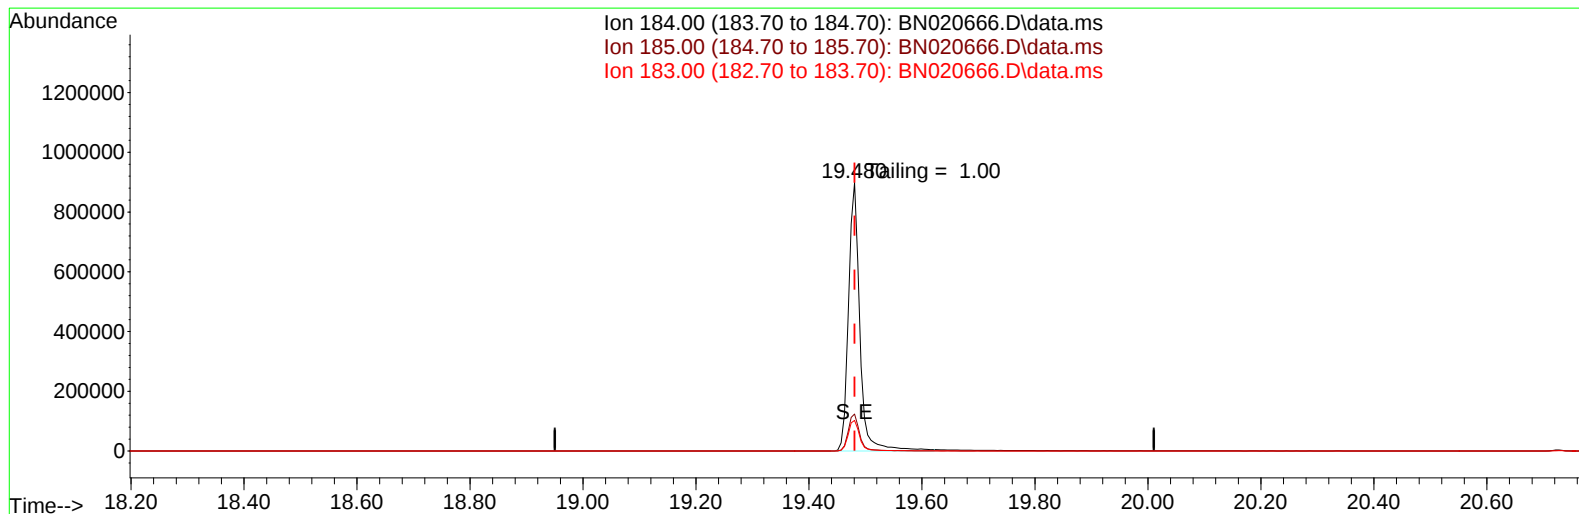

TIC: BN020666.D\data.ms

(77) Benzidine

19.480min (0.000) 0.00 ng

response 1280003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/6/2022	BNA_N	<u>BN020666.D</u>
Compound Name	Response	Retention Time
DDT	755745	20.727
DDD	13285	20.286
DDE	1720	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15005	770750	1.95

Instrument :
BNA_N
ClientSampleId :
DFTPP