


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070720\
 Data File : BN011107.D
 Acq On : 07 Jul 2020 08:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 07 10:47:09 2020

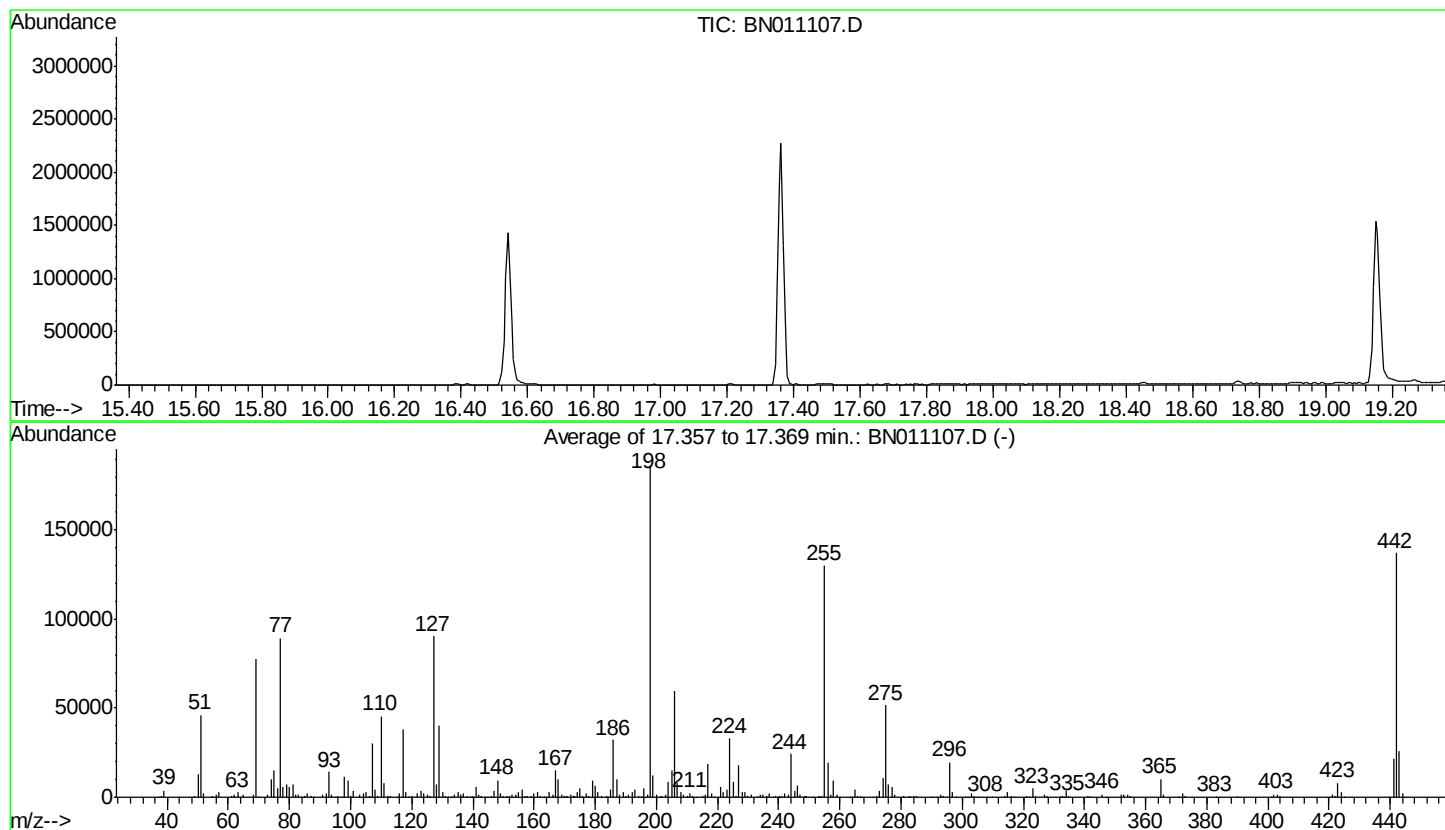

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	46101	PASS
68	69	0.00	2	1.9	1471	PASS
69	198	0.00	100	41.7	77640	PASS
70	69	0.00	2	0.5	367	PASS
127	198	10	80	48.6	90498	PASS
197	198	0.00	2	1.0	1813	PASS
198	198	100	100	100.0	186208	PASS
199	198	5	9	6.6	12357	PASS
275	198	10	60	27.7	51573	PASS
365	198	1	100	5.6	10377	PASS
441	198	0.01	100	11.7	21845	PASS
442	198	50	100	73.6	136965	PASS
443	442	15	24	19.1	26144	PASS