
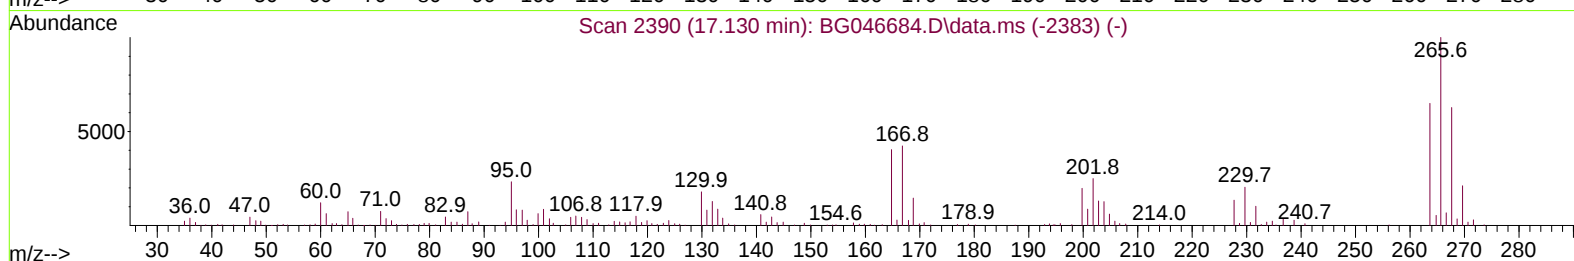
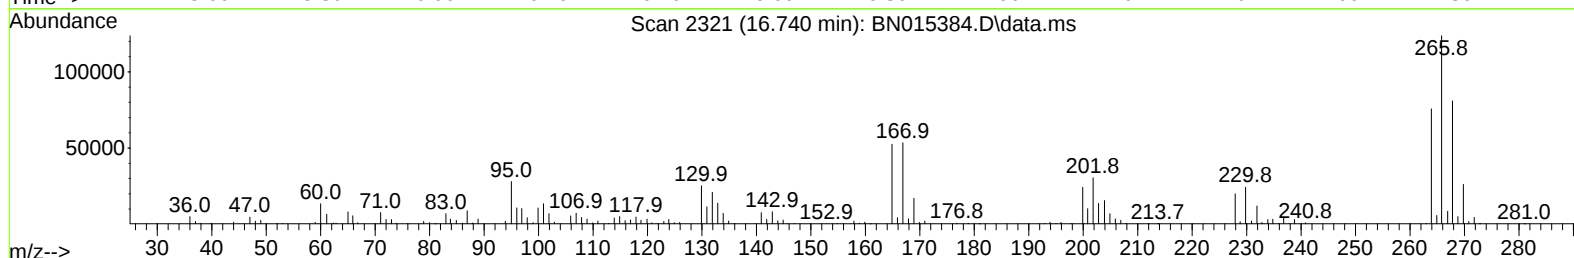


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\  
Data File : BN015384.D  
Acq On    : 07 Jul 2021  22:41  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 08 06:53:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

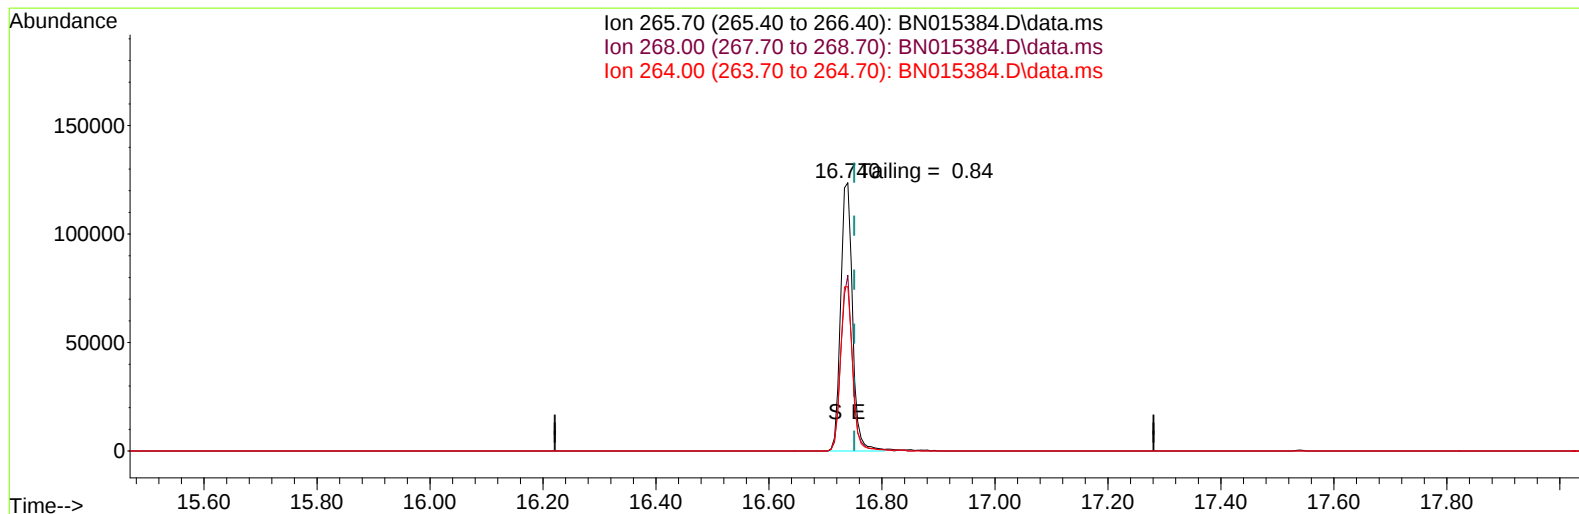

TIC: BN015384.D\data.ms

(70) Pentachlorophenol (C)




16.740min (-0.012) 23133.36 ng

response **180274**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.44
264.00	61.60	61.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
Data File : BN015384.D
Acq On : 07 Jul 2021 22:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 06:53:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

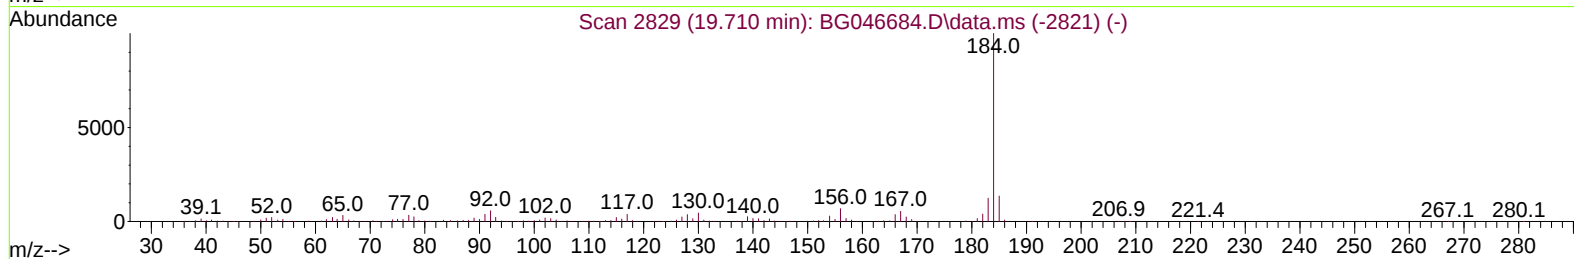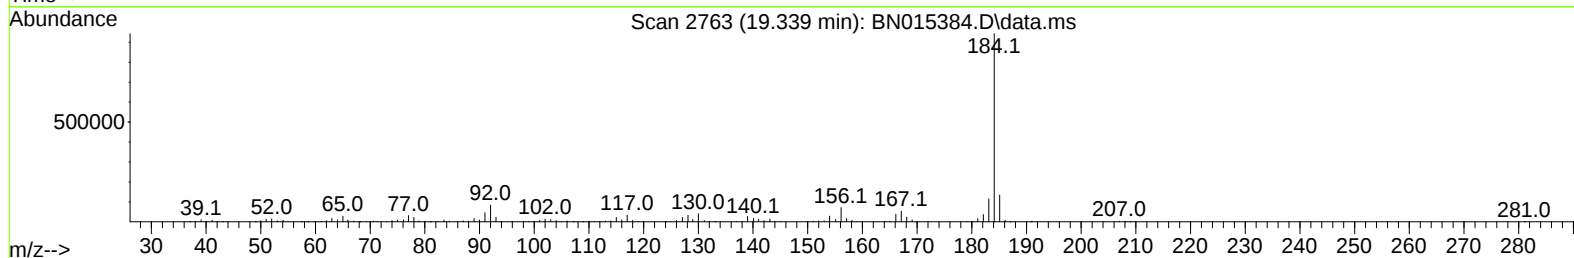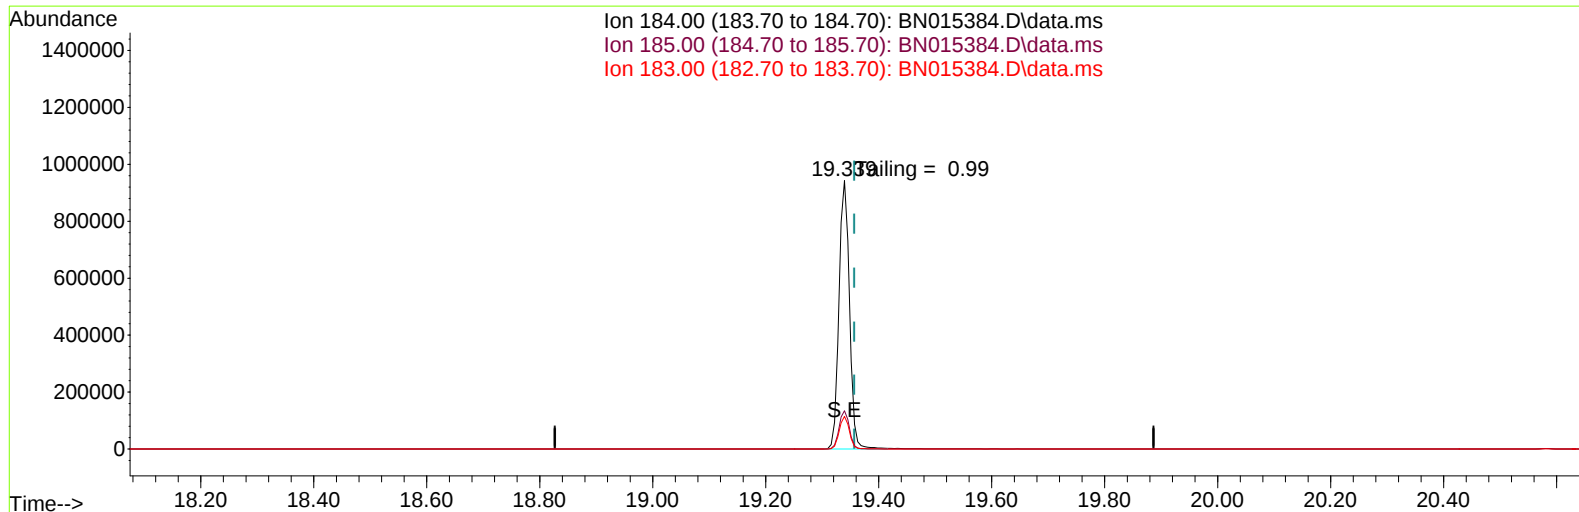

TIC: BN015384.D\data.ms

(77) Benzidine

19.339min (-0.017) 0.00 ng

response 1212357

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.26
183.00	13.20	12.20
0.00	0.00	0.00