

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
 Data File : BN015388.D
 Acq On : 08 Jul 2021 01:44
 Operator : CG/JU
 Sample : M2939-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-04-07-12-070221

Quant Time: Jul 08 06:45:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 11:11:38 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.725	152	19776	0.400	ng	# 0.00
7) Naphthalene-d8	10.483	136	88190	0.400	ng	# 0.00
13) Acenaphthene-d10	14.332	164	48135	0.400	ng	0.00
19) Phenanthrene-d10	17.078	188	97877	0.400	ng	0.00
29) Chrysene-d12	21.280	240	89192	0.400	ng	#-0.01
35) Perylene-d12	23.522	264	84042	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.346	112	6896	0.137	ng	0.00
5) Phenol-d6	6.895	99	4842	0.076	ng	0.00
8) Nitrobenzene-d5	8.860	82	22666	0.459	ng	0.00
11) 2-Methylnaphthalene-d10	12.078	152	52134	0.357	ng	0.00
14) 2,4,6-Tribromophenol	15.829	330	5801	0.499	ng	0.00
15) 2-Fluorobiphenyl	12.962	172	70989	0.363	ng	0.00
27) Fluoranthene-d10	19.122	212	124967	0.432	ng	0.00
31) Terphenyl-d14	19.723	244	97189	0.466	ng	0.00
Target Compounds						
23) Atrazine	16.543	200	148	0.175	ng	# 54
24) Pentachlorophenol	16.725	266	567	0.291	ng	# 61
34) Bis(2-ethylhexyl)phtha...	21.206	149	44426	0.549	ng	# 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
Data File : BN015388.D
Acq On : 08 Jul 2021 01:44
Operator : CG/JU
Sample : M2939-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW-04-07-12-070221

Quant Time: Jul 08 06:45:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 07 11:11:38 2021
Response via : Initial Calibration




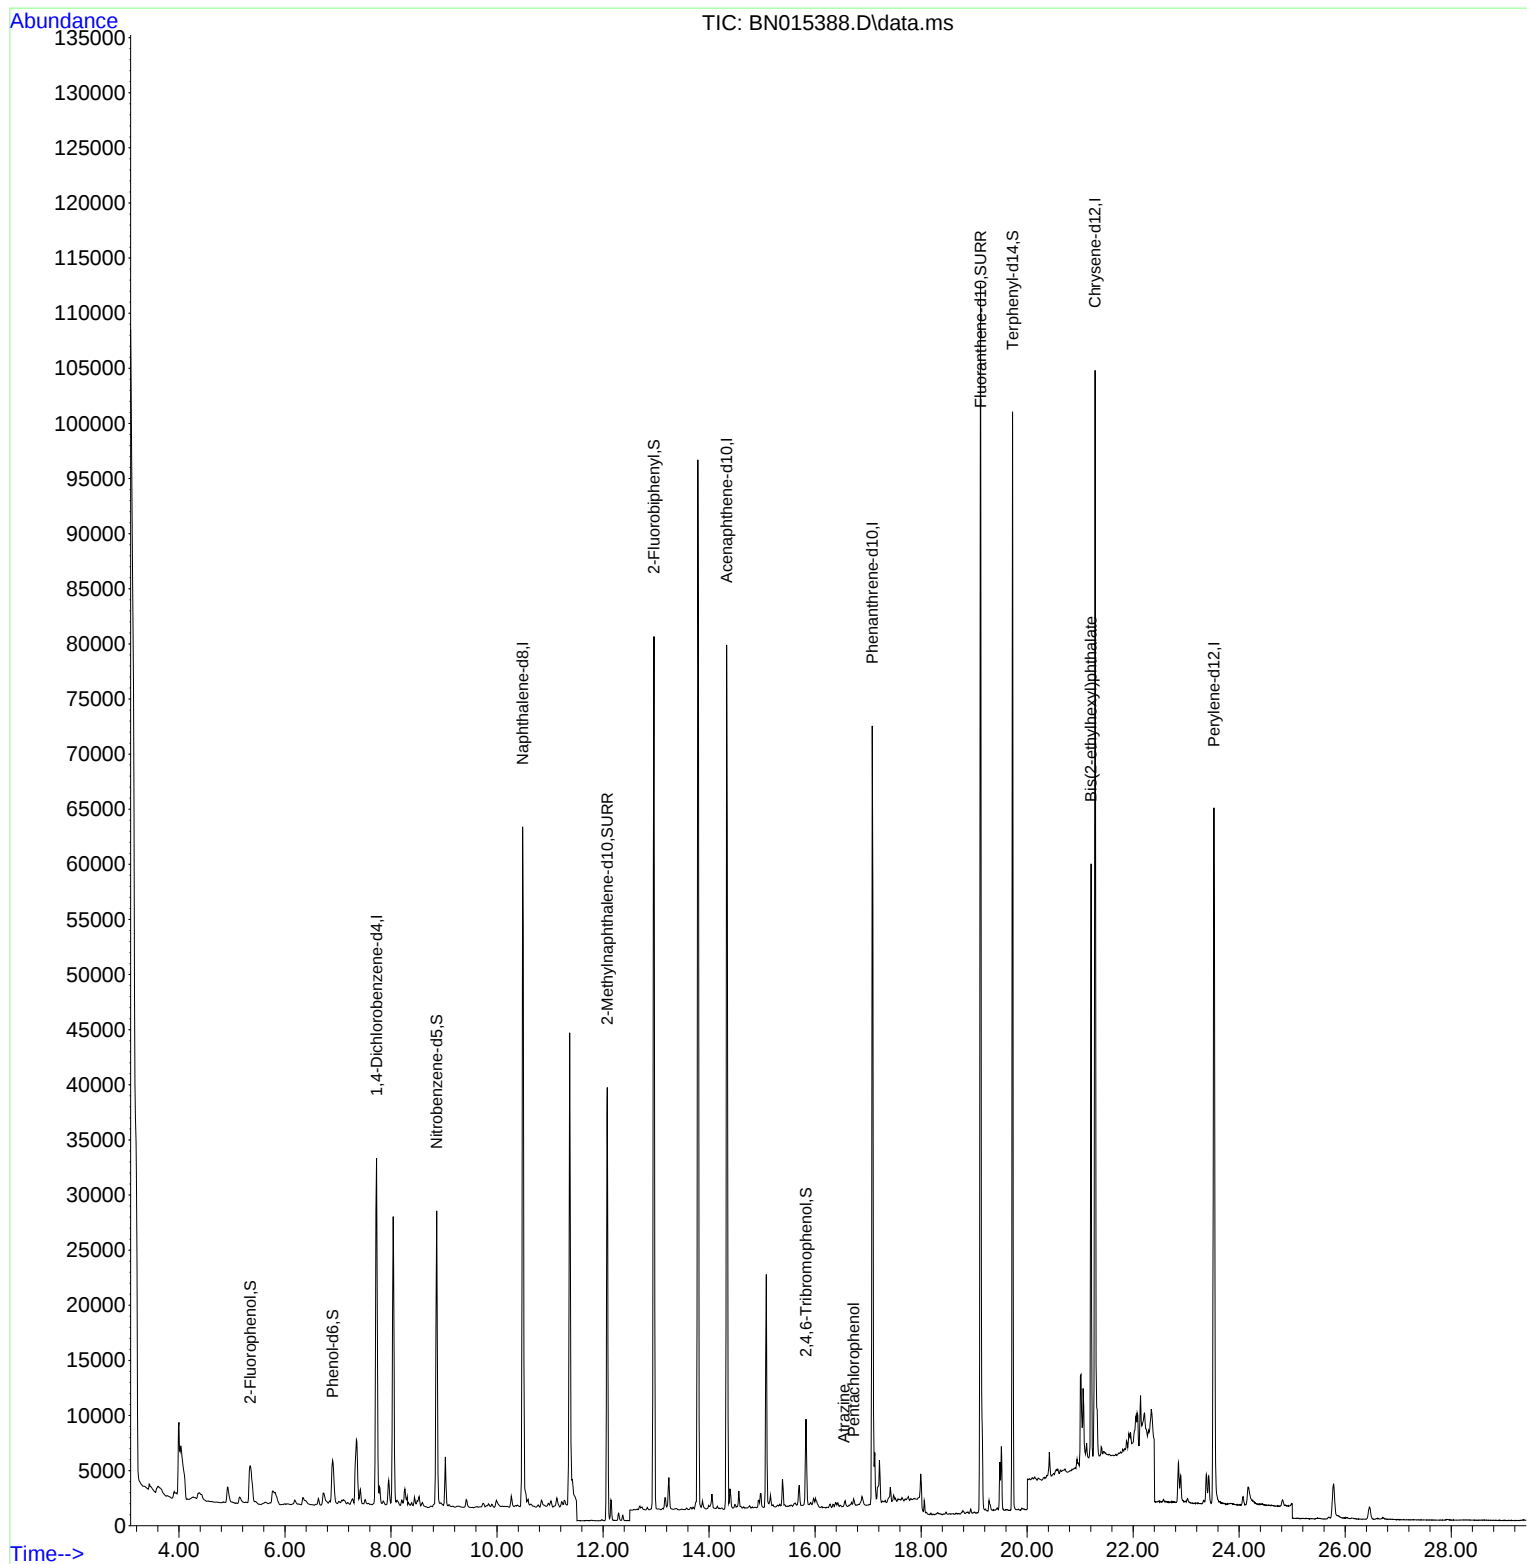


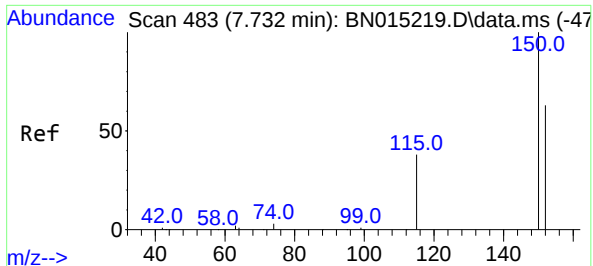

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.725 min Scan# 504
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44




Instrument :
BNA_N
ClientSampleId :
MW-04-07-12-070221


Tgt Ion:152 Resp: 19776
Ion Ratio Lower Upper
152 100
150 155.1 119.0 178.6
115 59.9 62.2 93.4#

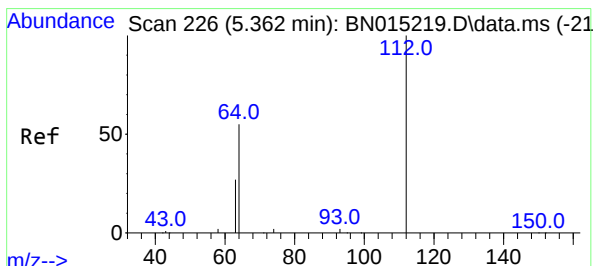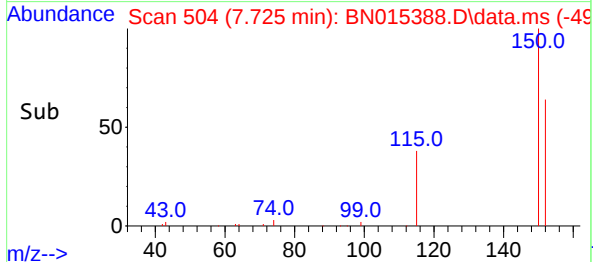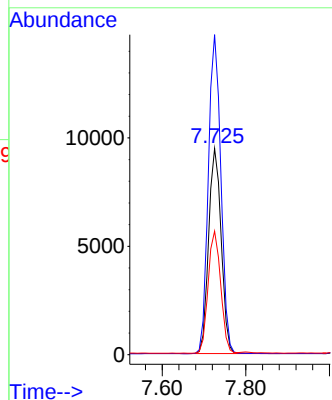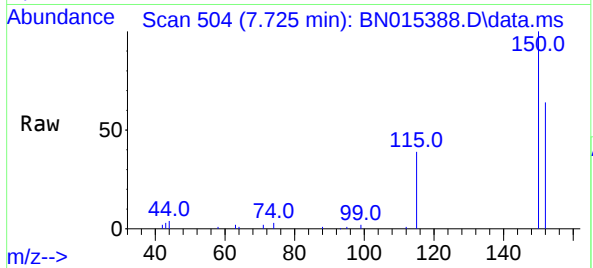

#4
2-Fluorophenol
Concen: 0.137 ng
RT: 5.346 min Scan# 246
Delta R.T. 0.009 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44

Tgt Ion:112 Resp: 6896
Ion Ratio Lower Upper
112 100
64 56.4 39.0 58.6
63 28.5 20.6 30.8


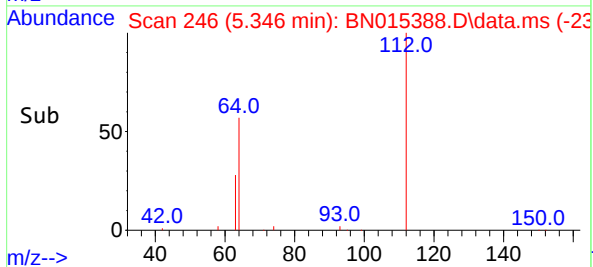
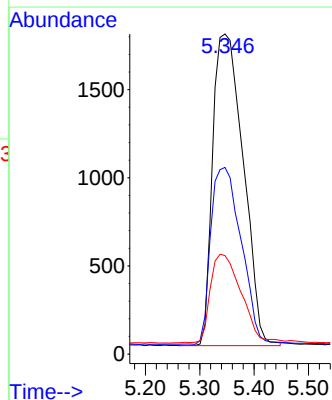
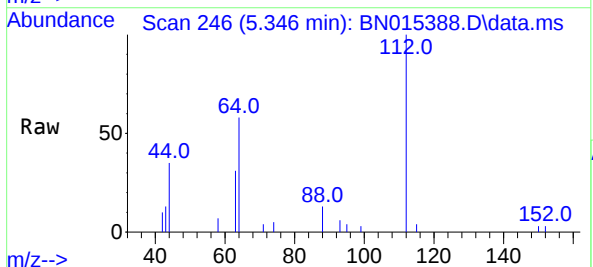




#5
Phenol-d6
Concen: 0.076 ng
RT: 6.895 min Scan# 414
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44




Instrument :
BNA_N
ClientSampleId :
MW-04-07-12-070221


Tgt Ion: 99 Resp: 4842
Ion Ratio Lower Upper
99 100
42 22.1 8.9 13.3#
71 35.7 35.6 53.4

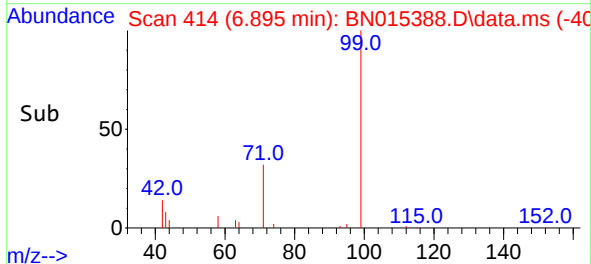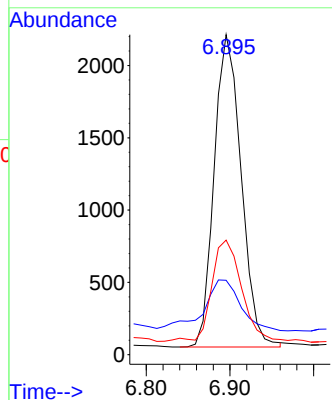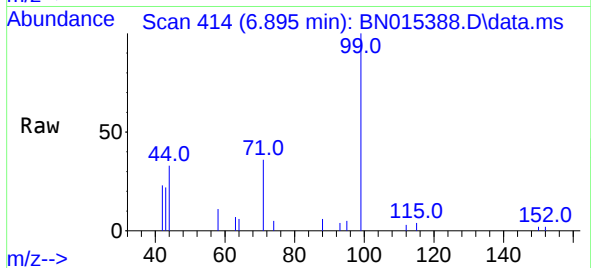

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.483 min Scan# 739
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44

Tgt Ion: 136 Resp: 88190
Ion Ratio Lower Upper
136 100
137 11.0 9.8 14.8
54 9.1 5.4 8.2#
68 7.4 4.9 7.3#


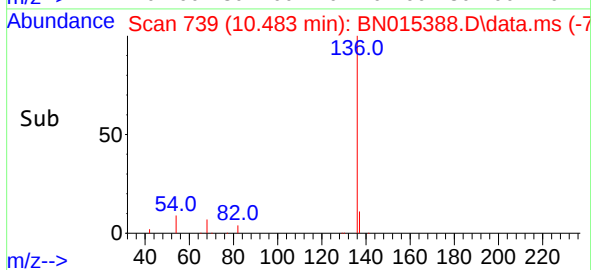
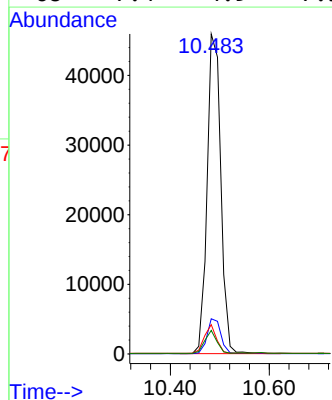
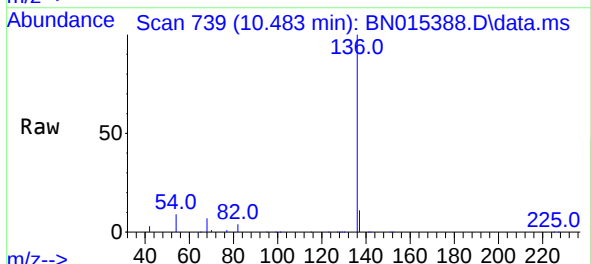




#8
Nitrobenzene-d5
Concen: 0.459 ng
RT: 8.860 min Scan# 611
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44




Instrument :
BNA_N
ClientSampleId :
MW-04-07-12-070221


Tgt Ion: 82 Resp: 22666
Ion Ratio Lower Upper
82 100
128 40.4 31.6 47.4
54 48.5 29.0 43.4#

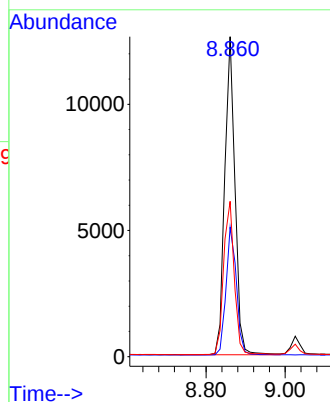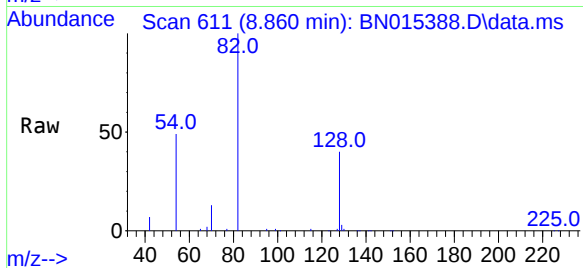

#11
2-Methylnaphthalene-d10
Concen: 0.357 ng
RT: 12.078 min Scan# 948
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44

Tgt Ion: 152 Resp: 52134
Ion Ratio Lower Upper
152 100
151 20.3 16.7 25.1


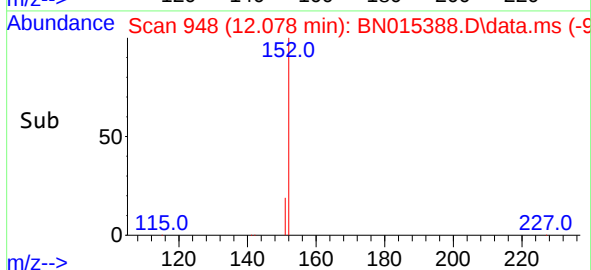
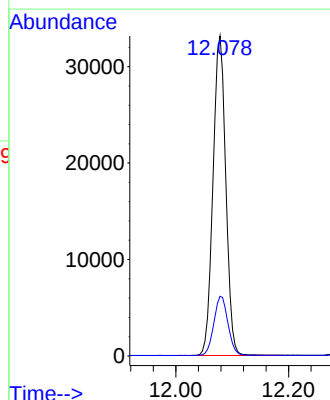
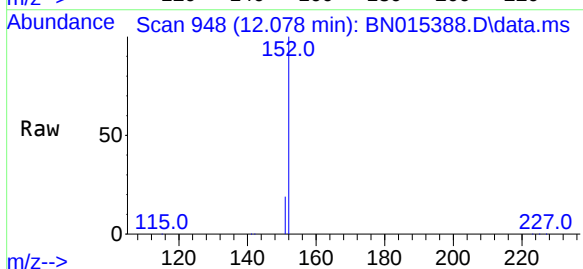




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44




Instrument :
BNA_N
ClientSampleId :
MW-04-07-12-070221


Tgt Ion:164 Resp: 48135
Ion Ratio Lower Upper
164 100
162 103.7 83.8 125.6
160 48.1 37.4 56.0

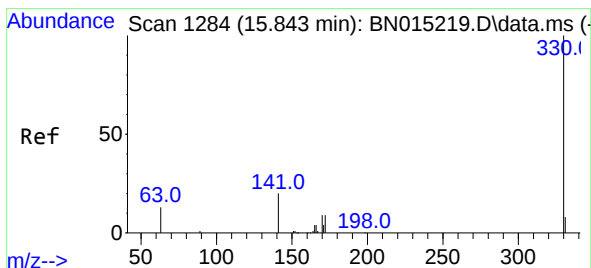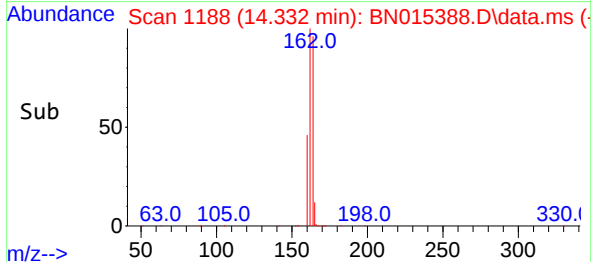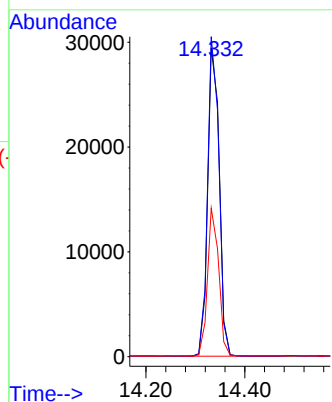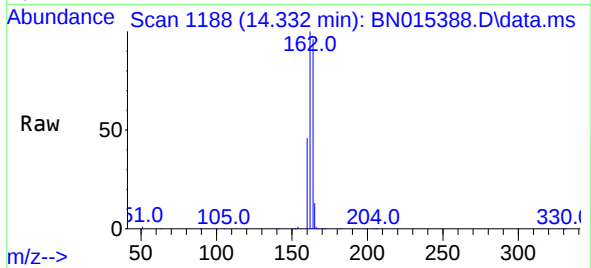

#14
2,4,6-Tribromophenol
Concen: 0.499 ng
RT: 15.829 min Scan# 1306
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44

Tgt Ion:330 Resp: 5801
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 37.1 22.4 33.6#


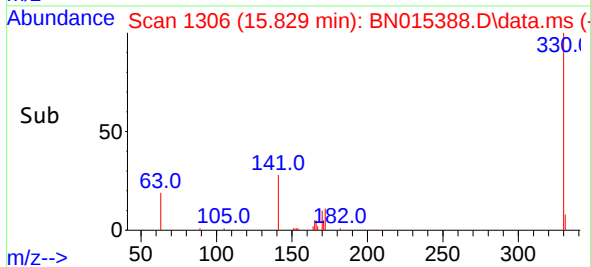
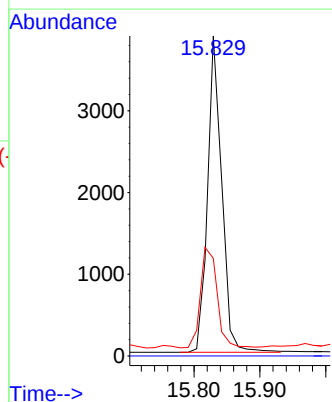
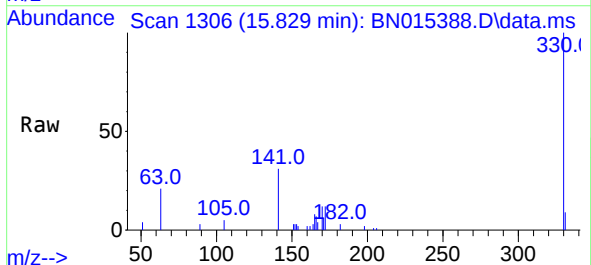




#15
2-Fluorobiphenyl
Concen: 0.363 ng
RT: 12.962 min Scan# 1080
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44




Instrument :
BNA_N
ClientSampleId :
MW-04-07-12-070221


Tgt Ion:	172	Resp:	70989
Ion	Ratio	Lower	Upper
172	100		
171	33.9	30.6	45.8
170	22.0	20.2	30.4

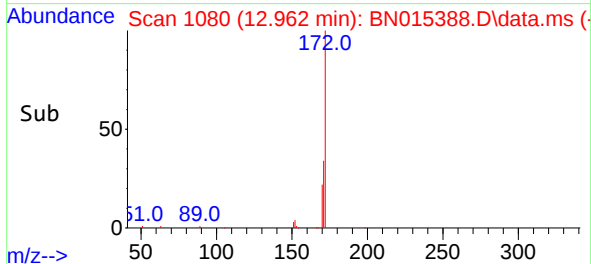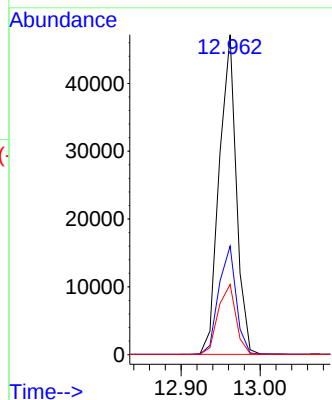

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.078 min Scan# 1408
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44

Tgt Ion:	188	Resp:	97877
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.5	9.0	13.4


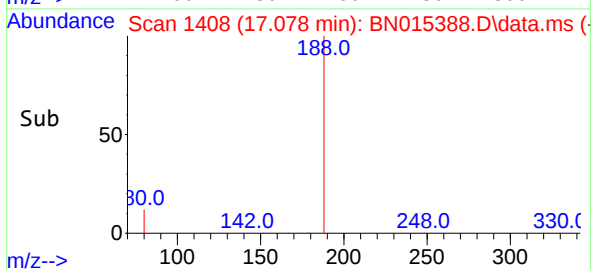
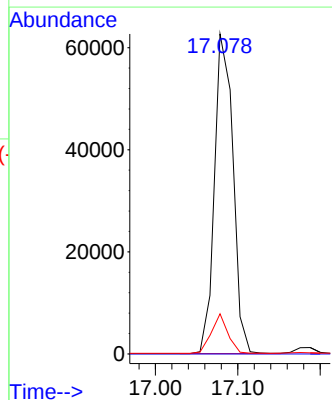
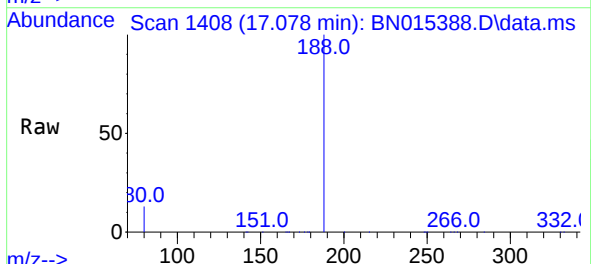




#23
Atrazine
Concen: 0.175 ng
RT: 16.543 min Scan# 1364
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44




Instrument :
BNA_N
ClientSampleId :
MW-04-07-12-070221


Tgt Ion:200 Resp: 148
Ion Ratio Lower Upper
200 100
173 75.6 21.7 32.5#
215 69.9 43.1 64.7#

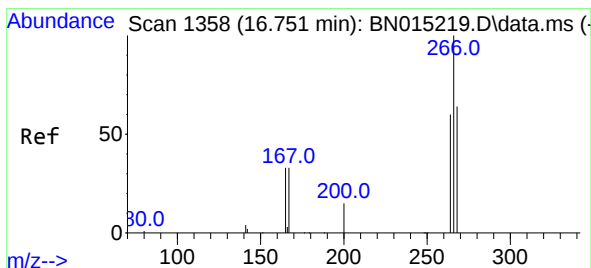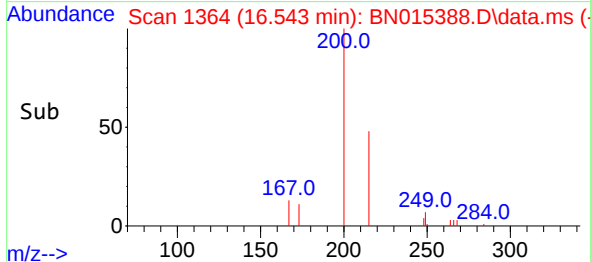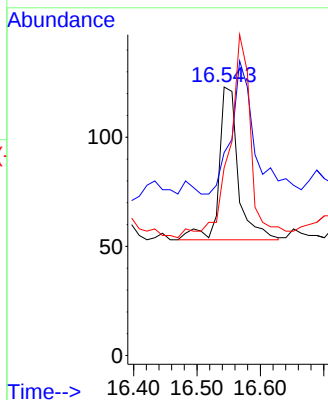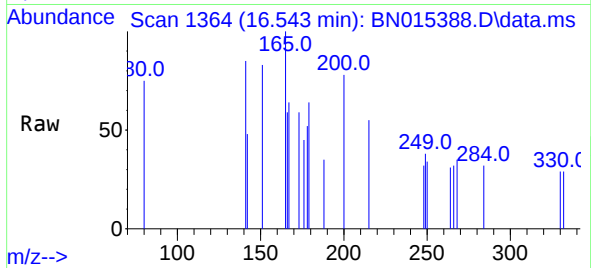

#24
Pentachlorophenol
Concen: 0.291 ng
RT: 16.725 min Scan# 1379
Delta R.T. -0.012 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44

Tgt Ion:266 Resp: 567
Ion Ratio Lower Upper
266 100
264 33.2 51.0 76.4#
268 33.2 50.6 76.0#


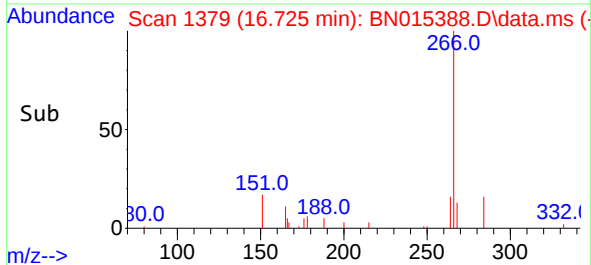
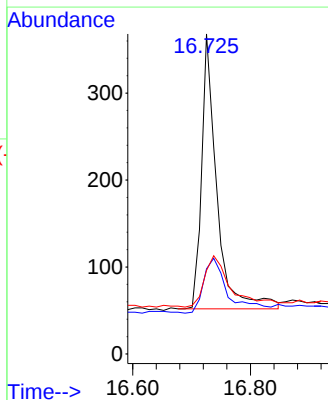
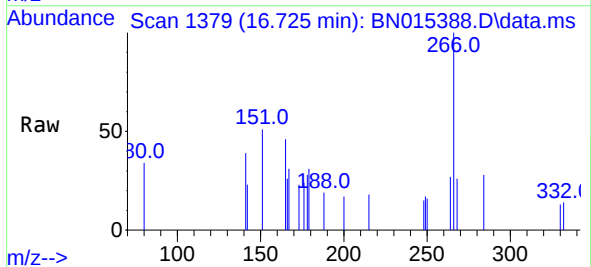




#27
Fluoranthene-d10
Concen: 0.432 ng
RT: 19.122 min Scan# 1708
Delta R.T. 0.000 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44




Instrument :
BNA_N
ClientSampleId :
MW-04-07-12-070221


Tgt Ion:212 Resp: 124967
Ion Ratio Lower Upper
212 100
106 14.1 7.0 10.6#
104 7.9 4.1 6.1#

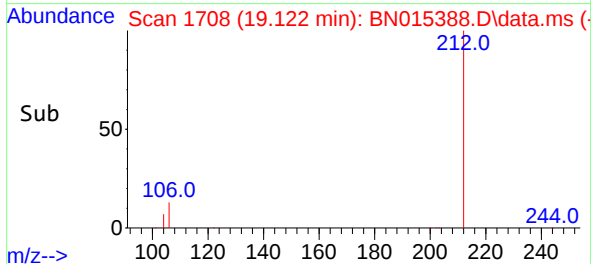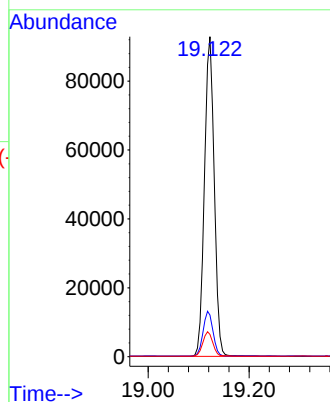

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.280 min Scan# 2006
Delta R.T. -0.011 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44

Tgt Ion:240 Resp: 89192
Ion Ratio Lower Upper
240 100
120 11.9 4.2 6.4#
236 26.7 21.4 32.2


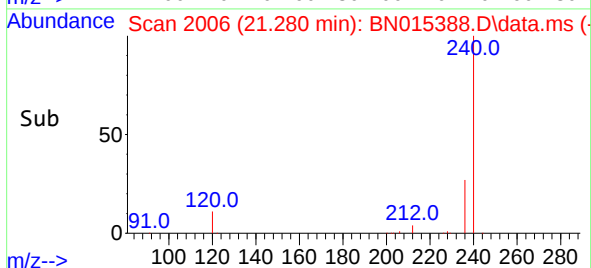
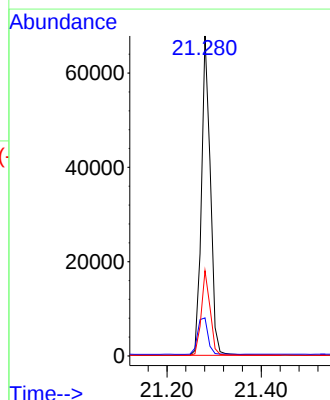
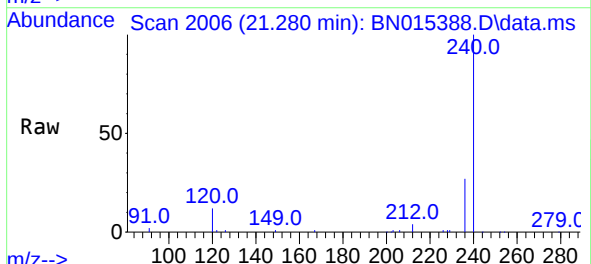




#31
 Terphenyl-d14
 Concen: 0.466 ng
 RT: 19.723 min Scan# 1829
 Delta R.T. -0.005 min
 Lab File: BN015388.D
 Acq: 08 Jul 2021 01:44




Instrument :
 BNA_N
 ClientSampleId :
 MW-04-07-12-070221


Tgt Ion:244	Resp:	97189
Ion Ratio	Lower	Upper
244	100	
212	7.8	6.3 9.5
122	13.8	6.2 9.2#

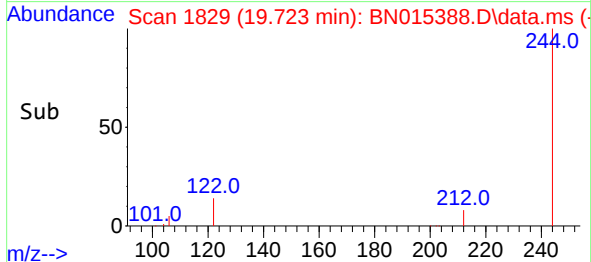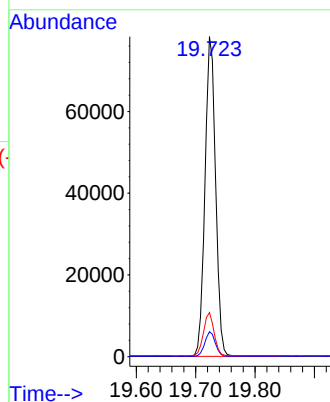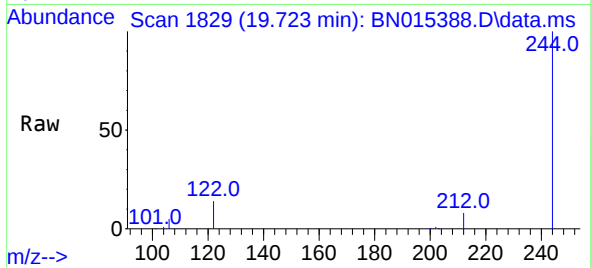

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.549 ng
 RT: 21.206 min Scan# 1999
 Delta R.T. 0.000 min
 Lab File: BN015388.D
 Acq: 08 Jul 2021 01:44

Tgt Ion:149	Resp:	44426
Ion Ratio	Lower	Upper
149	100	
167	28.2	28.9 43.3#
279	3.6	4.9 7.3#

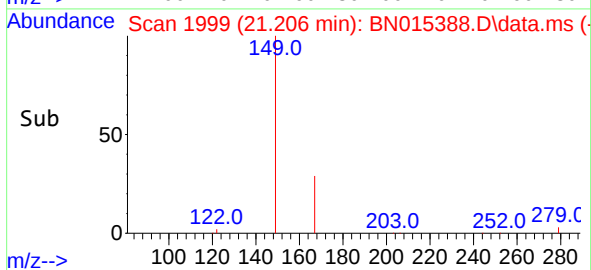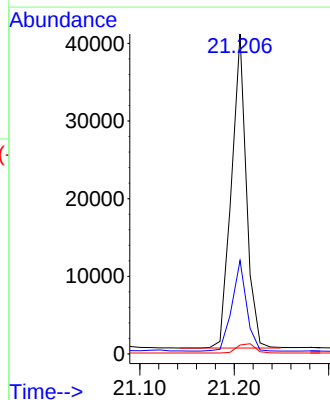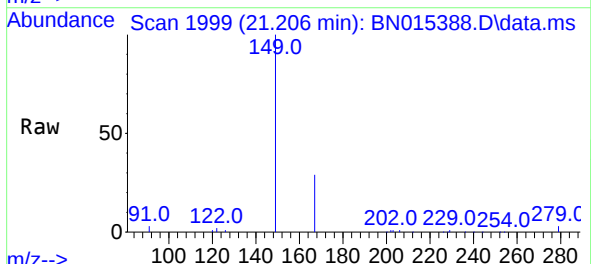

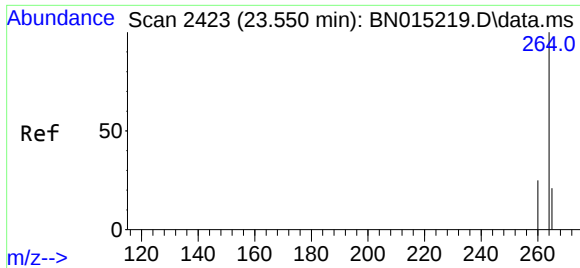

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.522 min Scan# 2438
Delta R.T. -0.007 min
Lab File: BN015388.D
Acq: 08 Jul 2021 01:44

Instrument :
BNA_N
ClientSampleId :
MW-04-07-12-070221

Tgt Ion:264	Resp:	84042
Ion	Ratio	Lower Upper
264	100	
260	24.8	20.6 31.0
265	22.6	21.4 32.2

