

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
 Data File : BN015395.D
 Acq On : 08 Jul 2021 05:57
 Operator : CG/JU
 Sample : M2953-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-11B-070621-FD

Manual Integrations
 APPROVED

mohammad
 7/8/2021 9:14:31 AM

Quant Time: Jul 08 06:57:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 11:11:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.725	152	20215	0.400	ng	# 0.00
7) Naphthalene-d8	10.483	136	92616	0.400	ng	# 0.00
13) Acenaphthene-d10	14.332	164	52262	0.400	ng	0.00
19) Phenanthrene-d10	17.078	188	104897	0.400	ng	0.00
29) Chrysene-d12	21.280	240	94086	0.400	ng	#-0.01
35) Perylene-d12	23.525	264	92458	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.365	112	3606	0.070	ng	0.03
5) Phenol-d6	6.905	99	2452	0.038	ng	0.00
8) Nitrobenzene-d5	8.860	82	24900	0.480	ng	0.00
11) 2-Methylnaphthalene-d10	12.078	152	51553	0.336	ng	0.00
14) 2,4,6-Tribromophenol	15.829	330	4347	0.413	ng	0.00
15) 2-Fluorobiphenyl	12.962	172	69412	0.327	ng	0.00
27) Fluoranthene-d10	19.122	212	112352	0.363	ng	0.00
31) Terphenyl-d14	19.723	244	87783	0.399	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.355	88	285908m	30.167	ng	Qvalue
24) Pentachlorophenol	16.725	266	2882	0.467	ng	# 35
34) Bis(2-ethylhexyl)phtha...	21.206	149	94657	0.916	ng	# 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
Data File : BN015395.D
Acq On : 08 Jul 2021 05:57
Operator : CG/JU
Sample : M2953-03
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
MW-11B-070621-FD

Manual Integrations
APPROVED

mohammad
7/8/2021 9:14:31 AM

Quant Time: Jul 08 06:57:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 07 11:11:38 2021
Response via : Initial Calibration

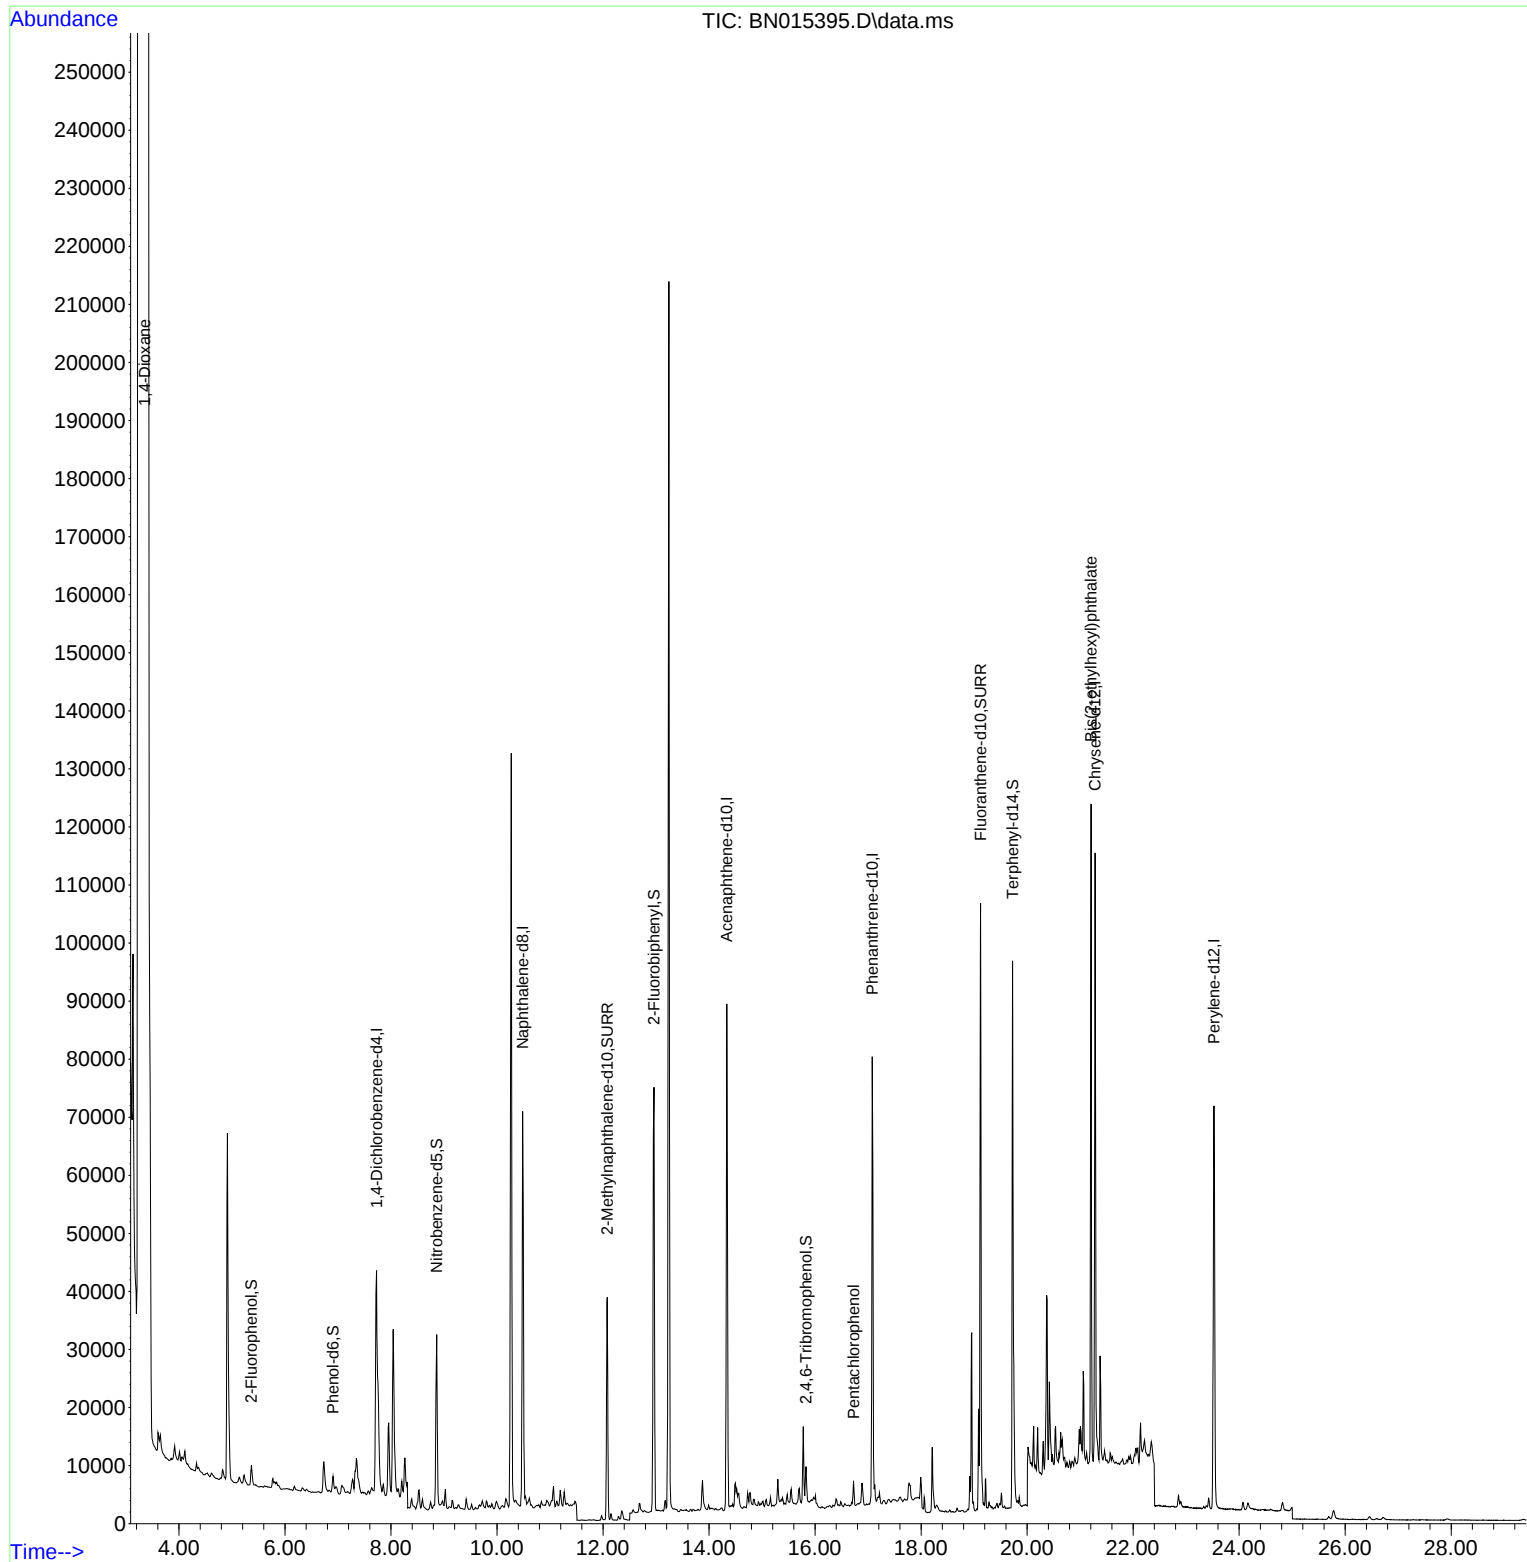

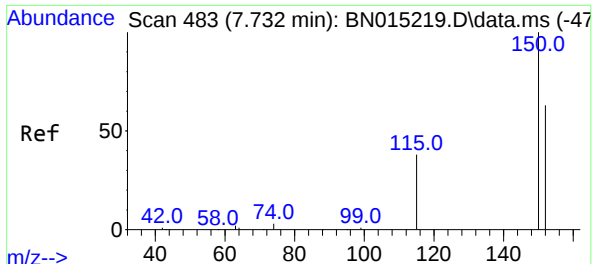





#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.725 min Scan# 504
Delta R.T. 0.000 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57

Tgt Ion: 152 Resp: 20215
Ion Ratio Lower Upper
152 100
150 155.2 119.0 178.6
115 59.1 62.2 93.4#

Instrument :
BNA_N
ClientSampleId :
MW-11B-070621-FD




Manual Integrations
APPROVED


mohammad
7/8/2021 9:14:31 AM

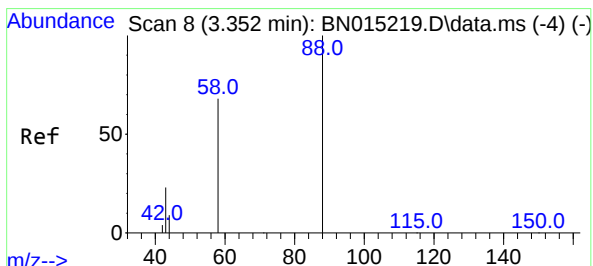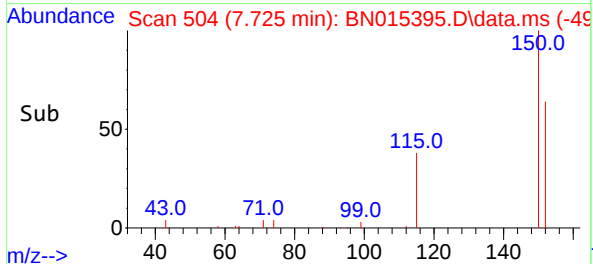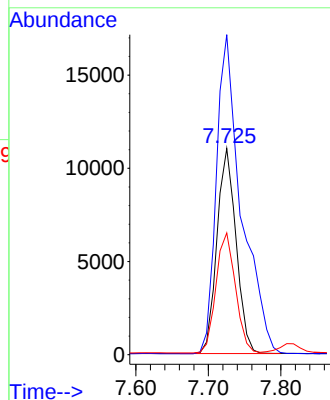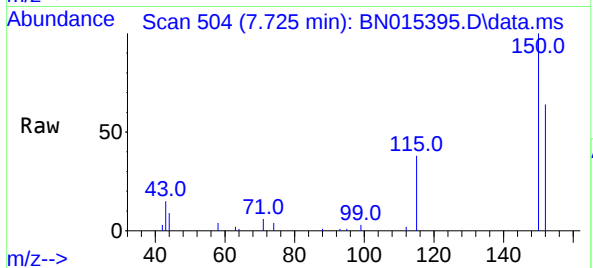

#2
1,4-Dioxane
Concen: 30.167 ng m
RT: 3.355 min Scan# 30
Delta R.T. 0.009 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57

Tgt Ion: 88 Resp: 285908
Ion Ratio Lower Upper
88 100
43 55.1 12.9 19.3#
58 135.6 38.1 57.1#

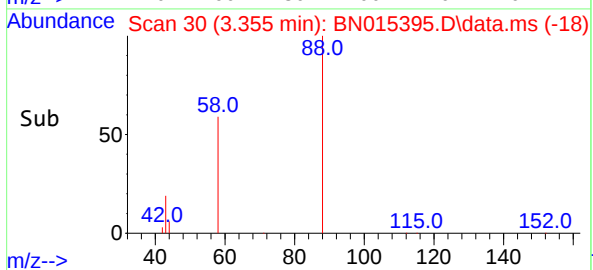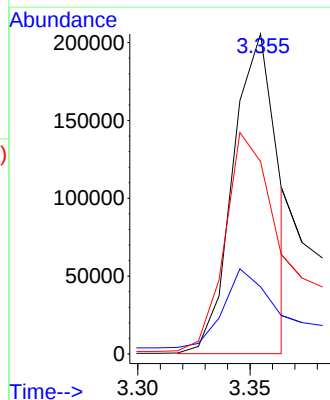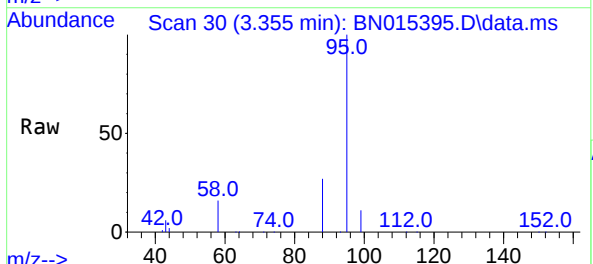

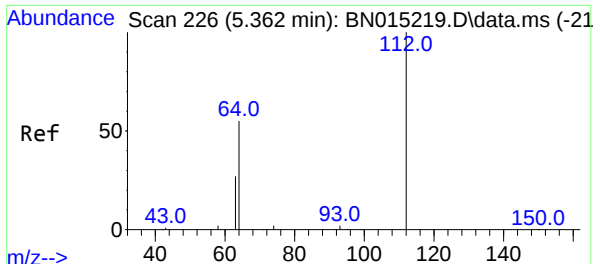





#4
2-Fluorophenol
Concen: 0.070 ng
RT: 5.365 min Scan# 248
Delta R.T. 0.028 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57

Tgt Ion:	112	Resp:	3606
Ion	Ratio	Lower	Upper
112	100		
64	54.3	39.0	58.6
63	31.0	20.6	30.8#

Instrument :
BNA_N
ClientSampleId :
MW-11B-070621-FD




Manual Integrations
APPROVED


mohammad
7/8/2021 9:14:31 AM

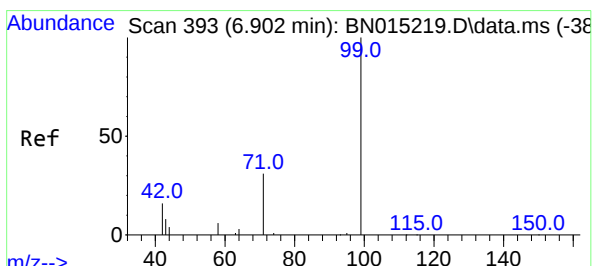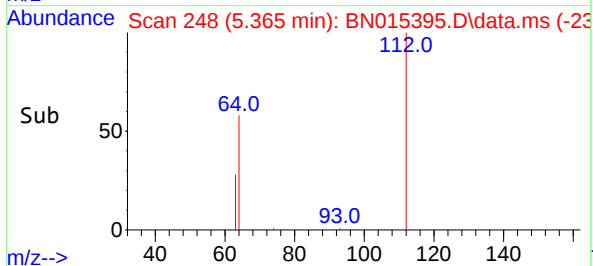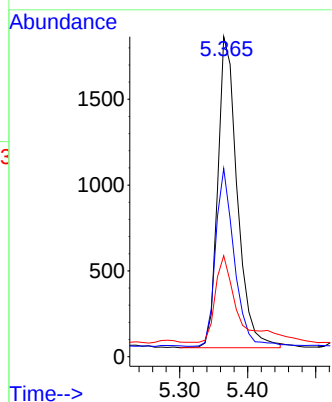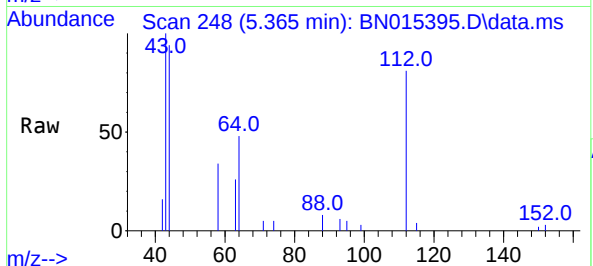

#5
Phenol-d6
Concen: 0.038 ng
RT: 6.905 min Scan# 415
Delta R.T. 0.009 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57


Tgt Ion:	99	Resp:	2452
Ion	Ratio	Lower	Upper
99	100		
42	16.2	8.9	13.3#
71	49.0	35.6	53.4

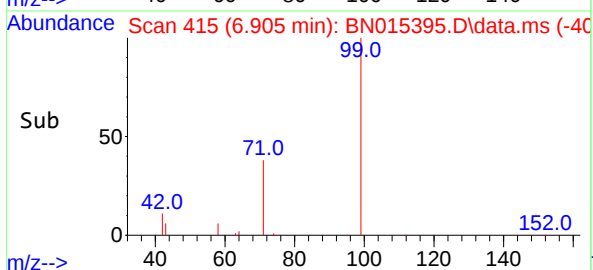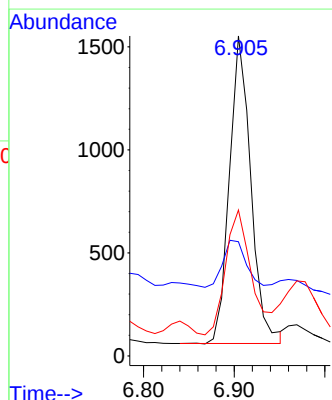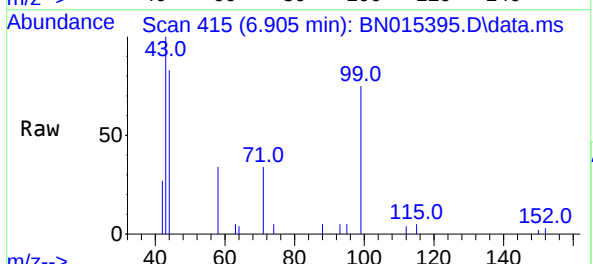

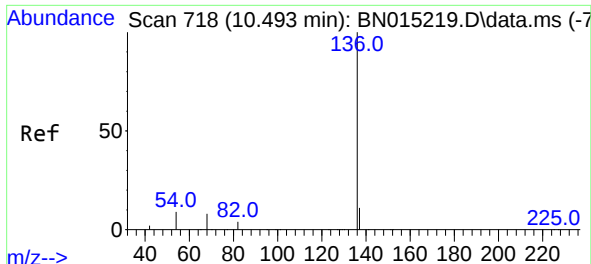

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.483 min Scan# 739
Delta R.T. -0.000 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57



Instrument :
BNA_N
ClientSampleId :
MW-11B-070621-FD

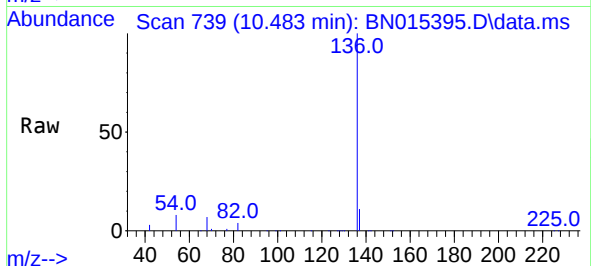


Tgt Ion:	136	Resp:	92616
Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.8	14.8
54	8.5	5.4	8.2#
68	6.9	4.9	7.3

Manual Integrations
APPROVED



mohammad
7/8/2021 9:14:31 AM

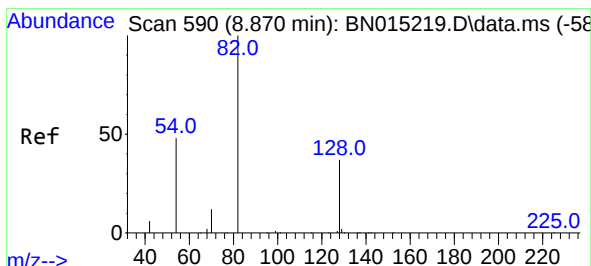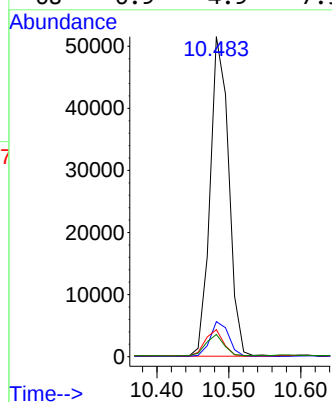


#8
Nitrobenzene-d5
Concen: 0.480 ng
RT: 8.860 min Scan# 611
Delta R.T. -0.000 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57

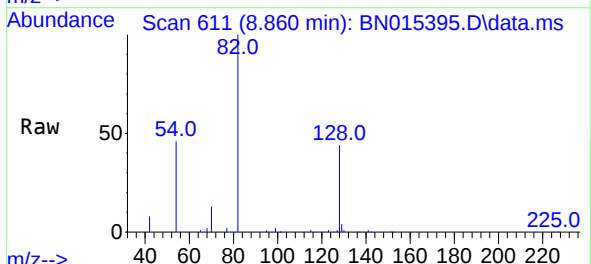

Tgt Ion:	82	Resp:	24900
Ion	Ratio	Lower	Upper
82	100		
128	43.7	31.6	47.4
54	46.3	29.0	43.4#

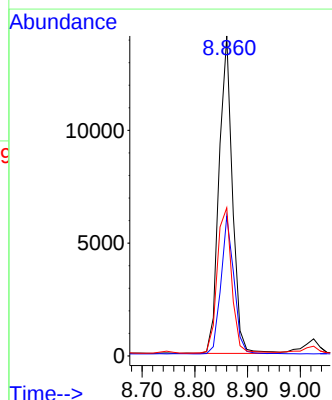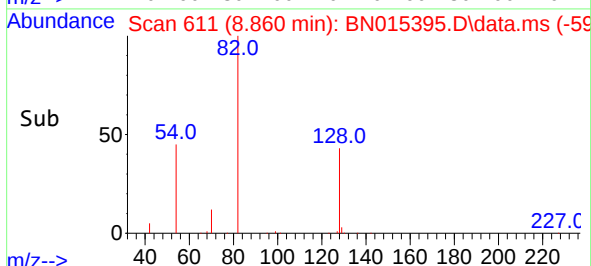

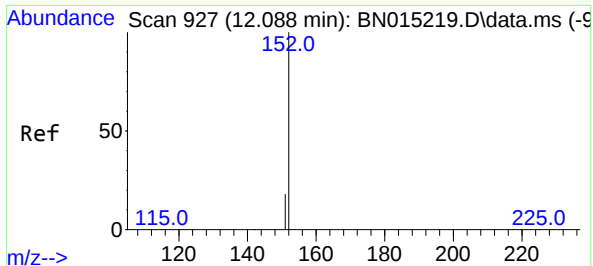





#11
2-Methylnaphthalene-d10
Concen: 0.336 ng
RT: 12.078 min Scan# 948
Delta R.T. -0.000 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57

Tgt Ion:152 Resp: 51553
Ion Ratio Lower Upper
152 100
151 20.7 16.7 25.1

Instrument :
BNA_N
ClientSampleId :
MW-11B-070621-FD




Manual Integrations
APPROVED


mohammad
7/8/2021 9:14:31 AM

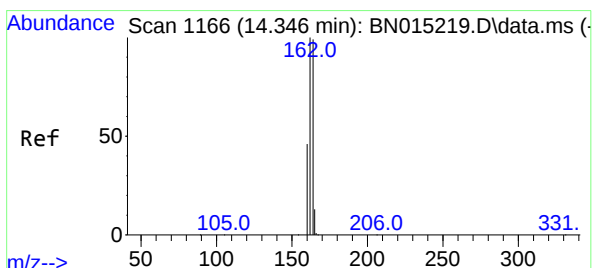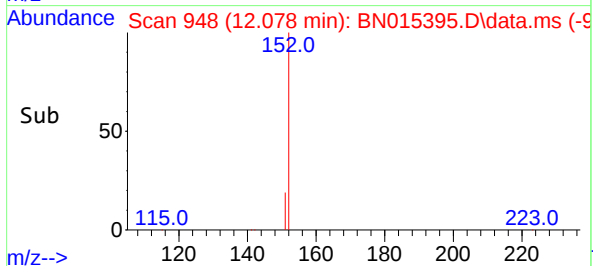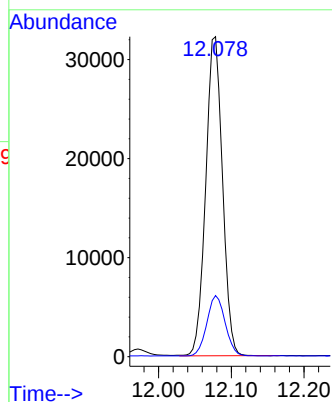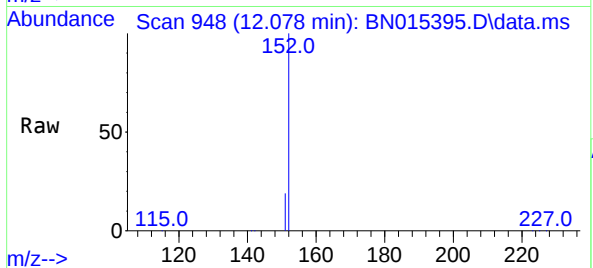

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.332 min Scan# 1188
Delta R.T. -0.000 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57


Tgt Ion:164 Resp: 52262
Ion Ratio Lower Upper
164 100
162 103.2 83.8 125.6
160 47.1 37.4 56.0

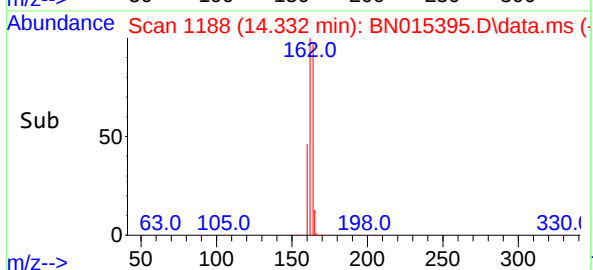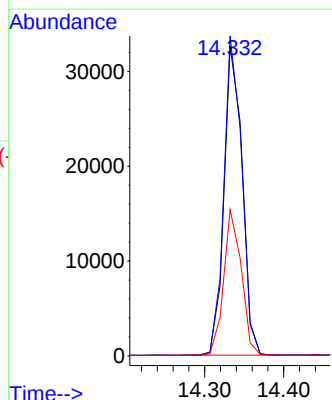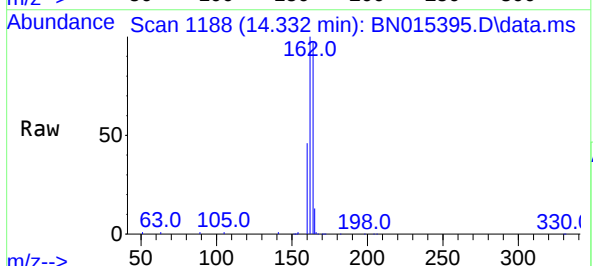

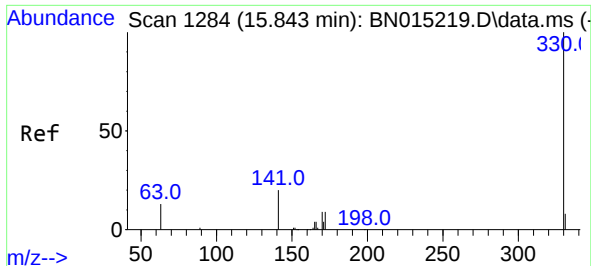

#14
2,4,6-Tribromophenol
Concen: 0.413 ng
RT: 15.829 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57




Instrument :
BNA_N
ClientSampleId :
MW-11B-070621-FD

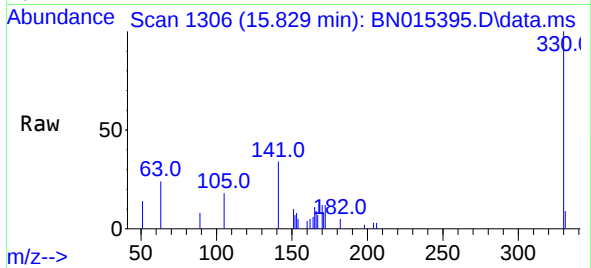

Tgt Ion:330 Resp: 4347
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 46.4 22.4 33.6#




Manual Integrations
APPROVED


mohammad
7/8/2021 9:14:31 AM

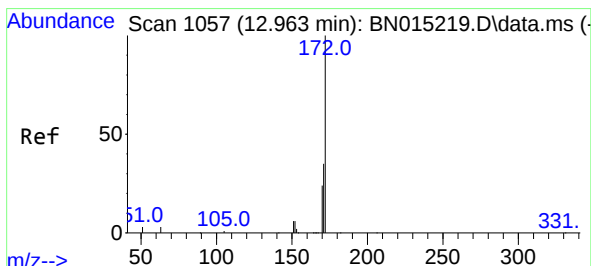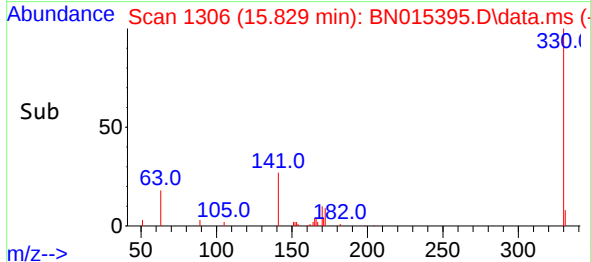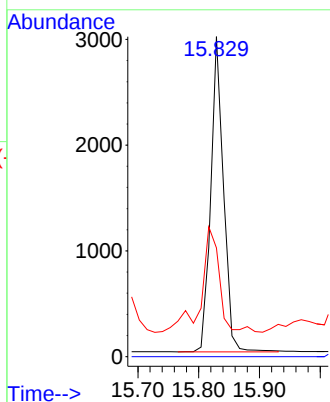

#15
2-Fluorobiphenyl
Concen: 0.327 ng
RT: 12.962 min Scan# 1080
Delta R.T. -0.000 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57

Tgt Ion:172 Resp: 69412
Ion Ratio Lower Upper
172 100
171 33.6 30.6 45.8
170 21.8 20.2 30.4

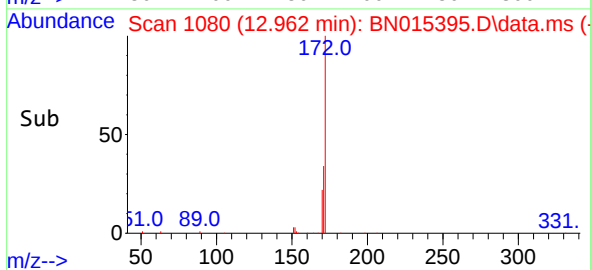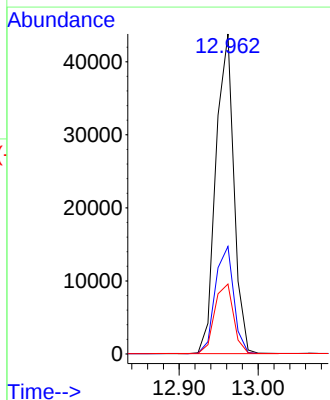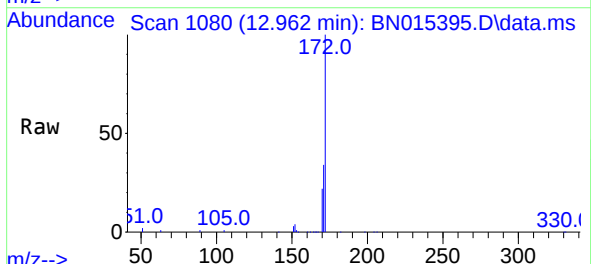

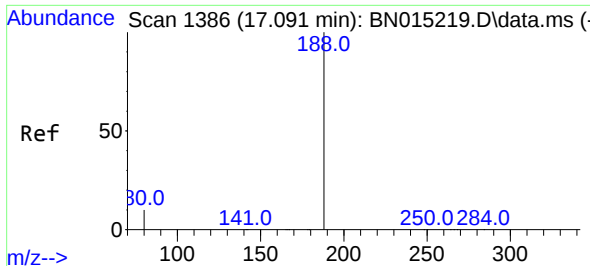





#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.078 min Scan# 1408
Delta R.T. -0.000 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57

Tgt Ion:188 Resp: 104897
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.6 9.0 13.4

Instrument :
BNA_N
ClientSampleId :
MW-11B-070621-FD




Manual Integrations
APPROVED


mohammad
7/8/2021 9:14:31 AM

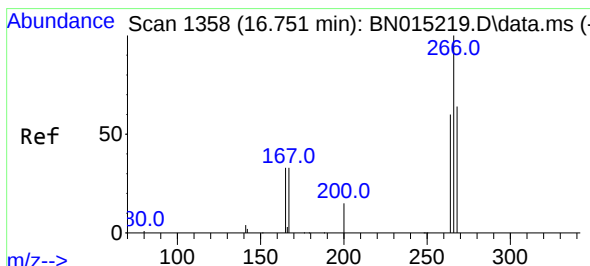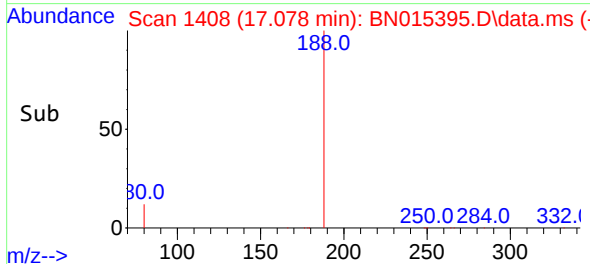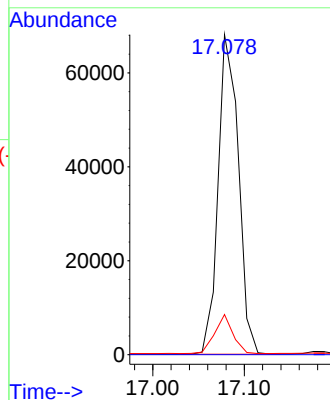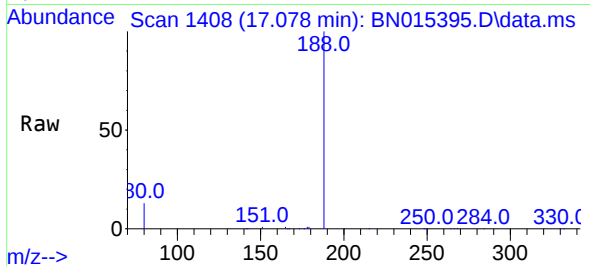

#24
Pentachlorophenol
Concen: 0.467 ng
RT: 16.725 min Scan# 1379
Delta R.T. -0.012 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57


Tgt Ion:266 Resp: 2882
Ion Ratio Lower Upper
266 100
264 13.7 51.0 76.4#
268 12.0 50.6 76.0#

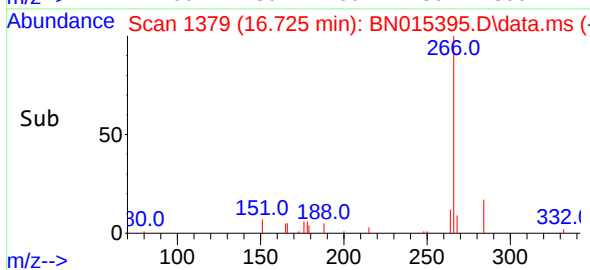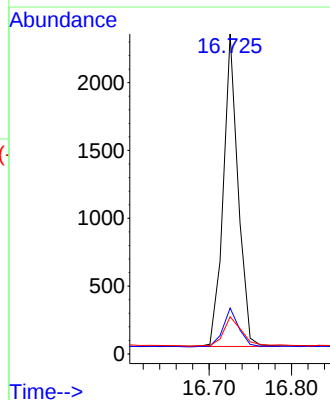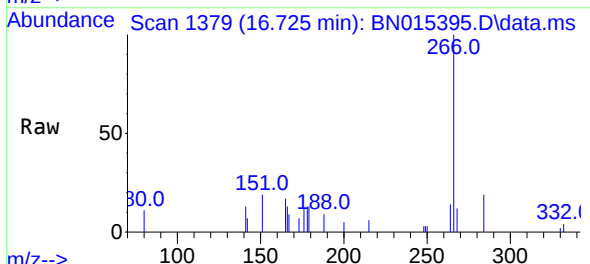

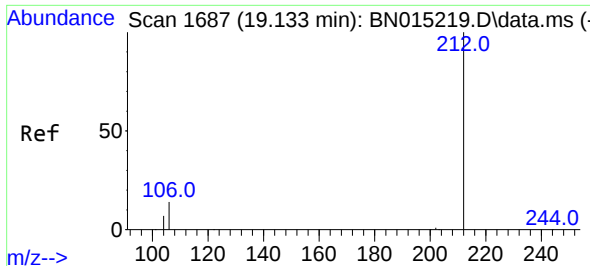

#27
Fluoranthene-d10
Concen: 0.363 ng
RT: 19.122 min Scan# 1708
Delta R.T. -0.000 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57




Instrument :
BNA_N
ClientSampleId :
MW-11B-070621-FD

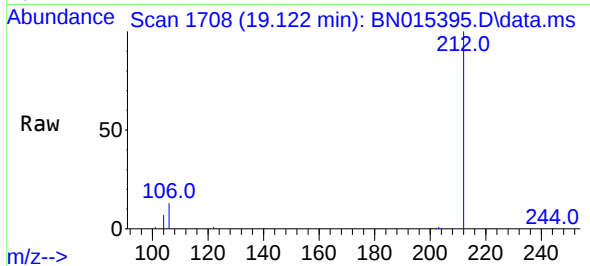


Tgt Ion:212 Resp: 112352
Ion Ratio Lower Upper
212 100
106 14.6 7.0 10.6#
104 8.0 4.1 6.1#

Manual Integrations
APPROVED



mohammad
7/8/2021 9:14:31 AM

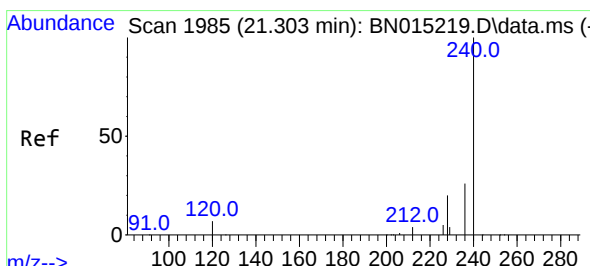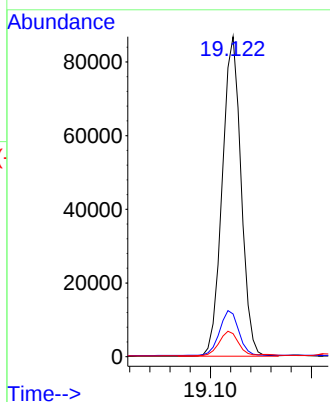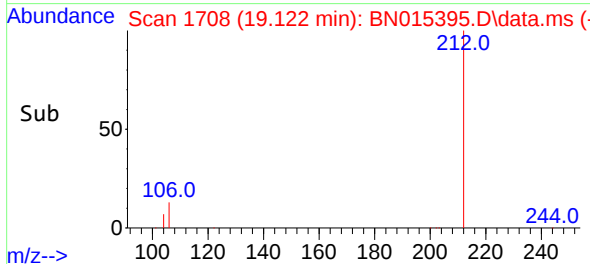


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.280 min Scan# 2006
Delta R.T. -0.011 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57

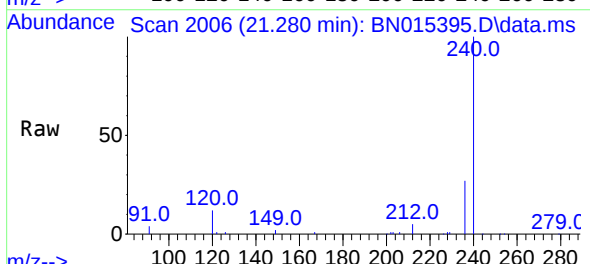


Tgt Ion:240 Resp: 94086
Ion Ratio Lower Upper
240 100
120 12.5 4.2 6.4#
236 26.7 21.4 32.2


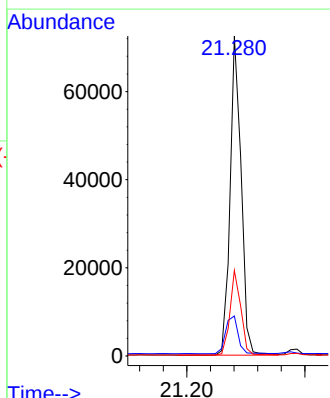
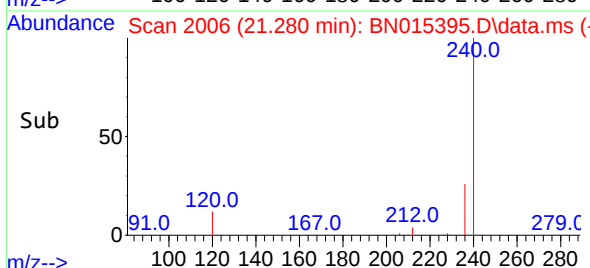


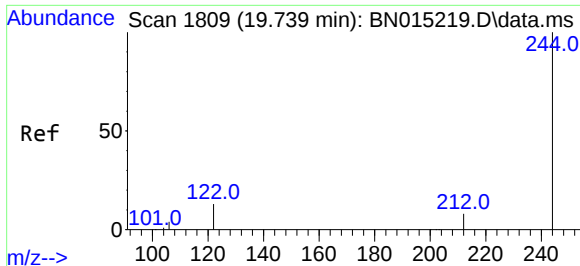


#31
 Terphenyl-d14
 Concen: 0.399 ng
 RT: 19.723 min Scan# 1829
 Delta R.T. -0.005 min
 Lab File: BN015395.D
 Acq: 08 Jul 2021 05:57

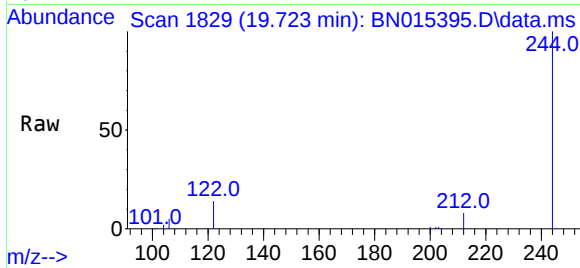



Tgt Ion:244 Resp: 87783
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.3 9.5
 122 14.1 6.2 9.2#

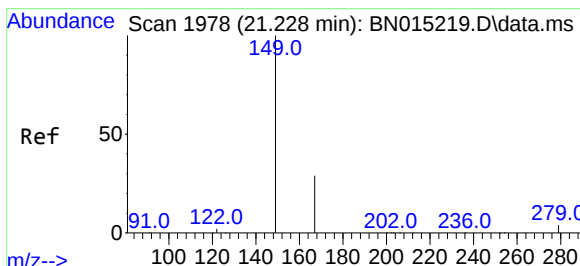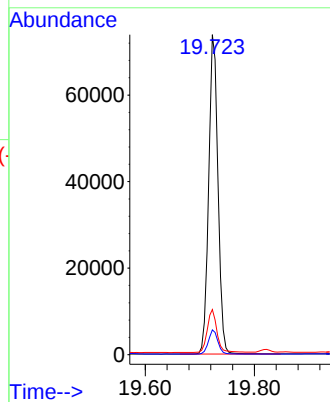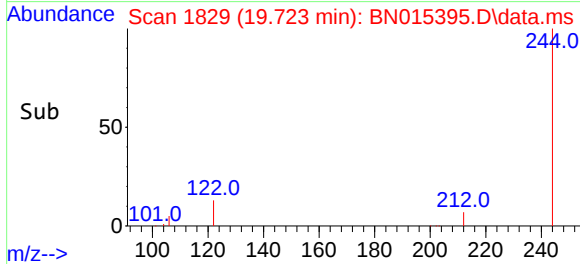

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.916 ng
 RT: 21.206 min Scan# 1999
 Delta R.T. -0.000 min
 Lab File: BN015395.D
 Acq: 08 Jul 2021 05:57

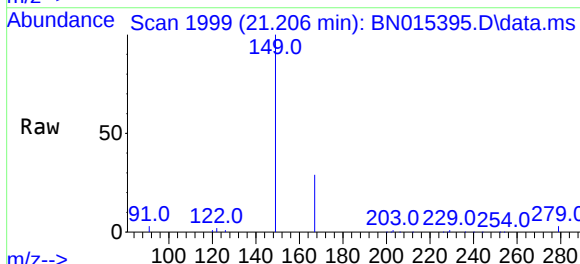


Tgt Ion:149 Resp: 94657
 Ion Ratio Lower Upper
 149 100
 167 28.2 28.9 43.3#
 279 3.7 4.9 7.3#

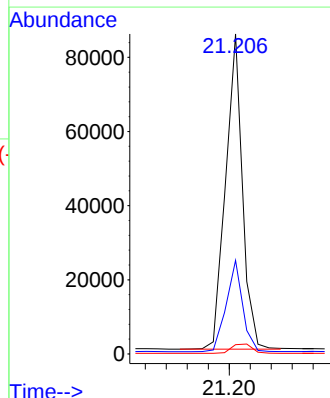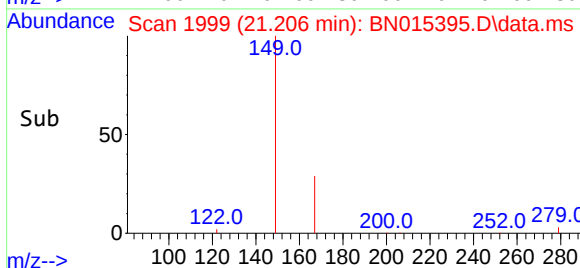


Instrument :
 BNA_N
 ClientSampleId :
 MW-11B-070621-FD

Manual Integrations
 APPROVED

mohammad
 7/8/2021 9:14:31 AM


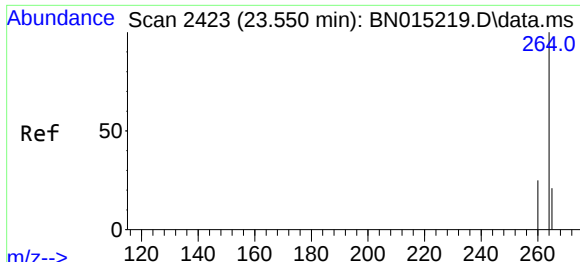


#35
Perylene-d12
Concen: 0.400 ng
RT: 23.525 min Scan# 2439
Delta R.T. -0.003 min
Lab File: BN015395.D
Acq: 08 Jul 2021 05:57

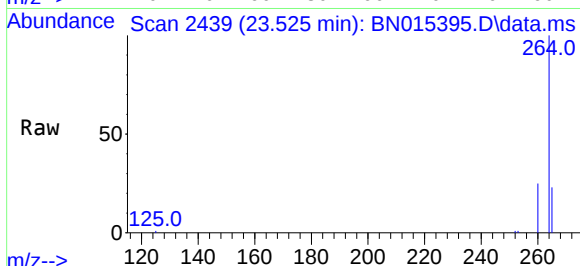

Tgt Ion: 264 Resp: 92458

Ion	Ratio	Lower	Upper
264	100		
260	24.9	20.6	31.0
265	23.2	21.4	32.2

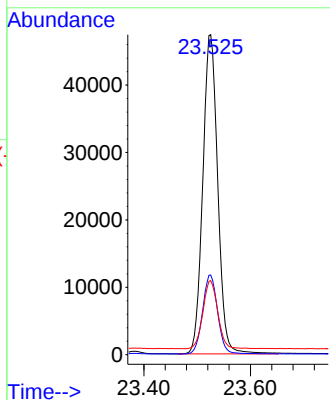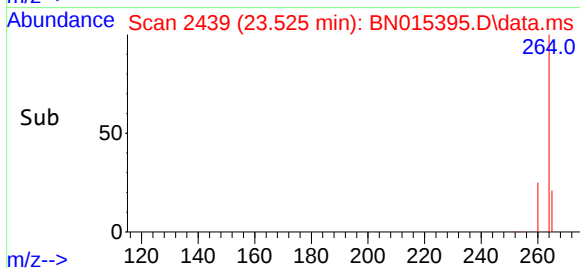

Instrument :
BNA_N
ClientSampleId :
MW-11B-070621-FD

Manual Integrations
APPROVED

mohammad
7/8/2021 9:14:31 AM