
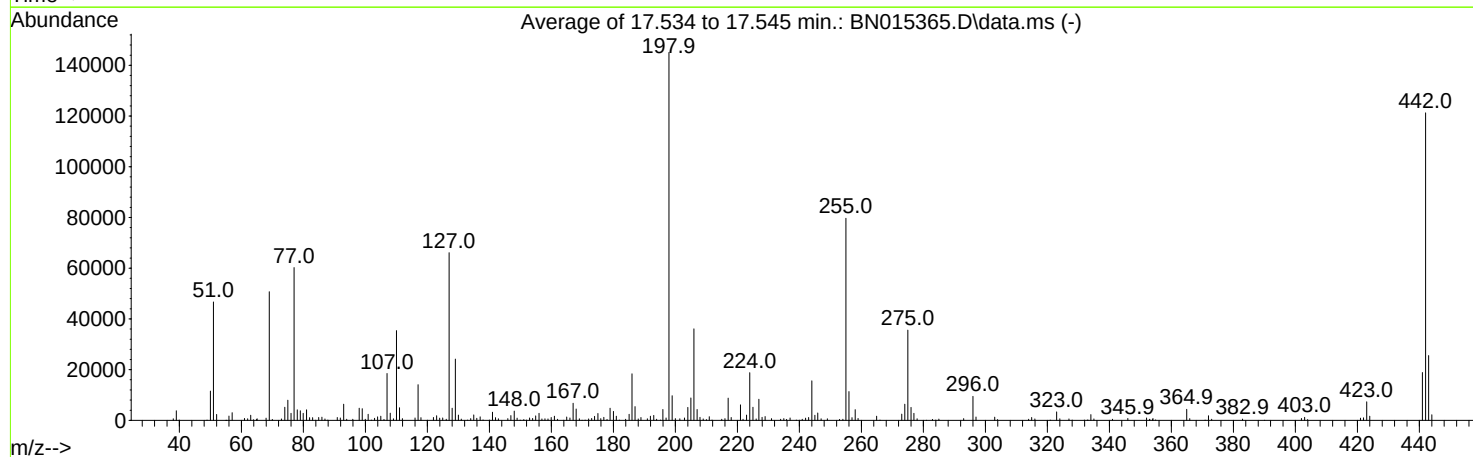


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
 Data File : BN015365.D
 Acq On : 07 Jul 2021 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 07 11:11:38 2021

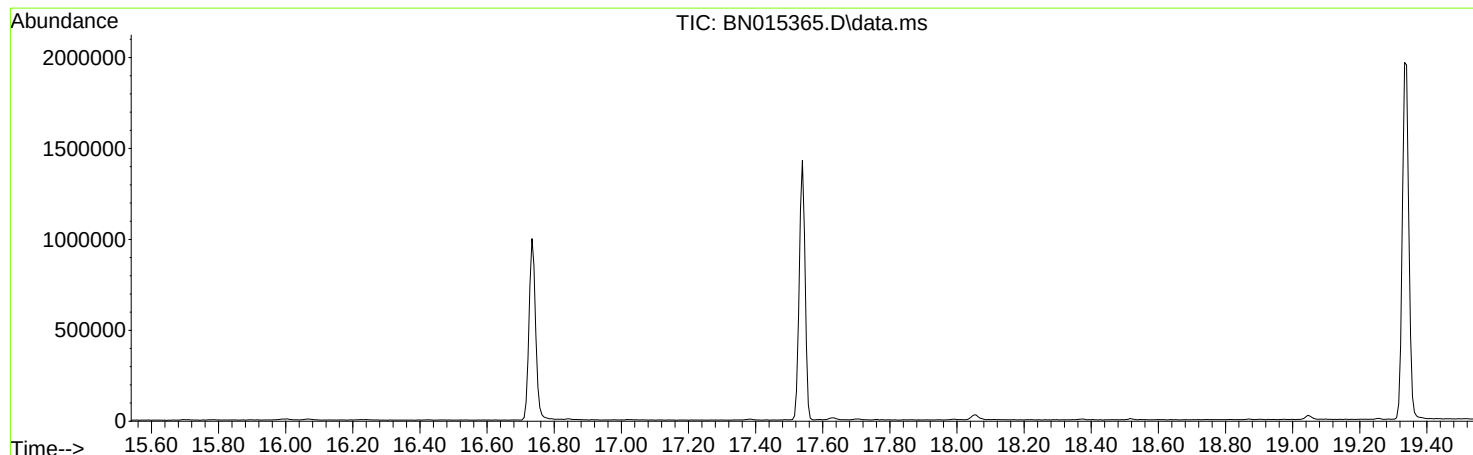

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	46667	PASS
68	69	0.00	2	1.8	903	PASS
69	198	0.00	100	35.0	50696	PASS
70	69	0.00	2	0.7	375	PASS
127	198	10	80	45.6	66104	PASS
197	198	0.00	2	0.7	945	PASS
198	198	100	100	100.0	145045	PASS
199	198	5	9	6.7	9734	PASS
275	198	10	60	24.5	35560	PASS
365	198	1	100	3.0	4372	PASS
441	198	0.01	100	13.0	18860	PASS
442	442	50	100	100.0	121261	PASS
443	442	15	24	21.1	25573	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/7/2021	BNA_N	<u>BN015365.D</u>
Compound Name	Response	Retention Time
DDT	469075	20.58
DDD	283	20.13
DDE	617	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
900	469975	0.19

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
Data File : BN015365.D
Acq On : 07 Jul 2021 09:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 07 10:52:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

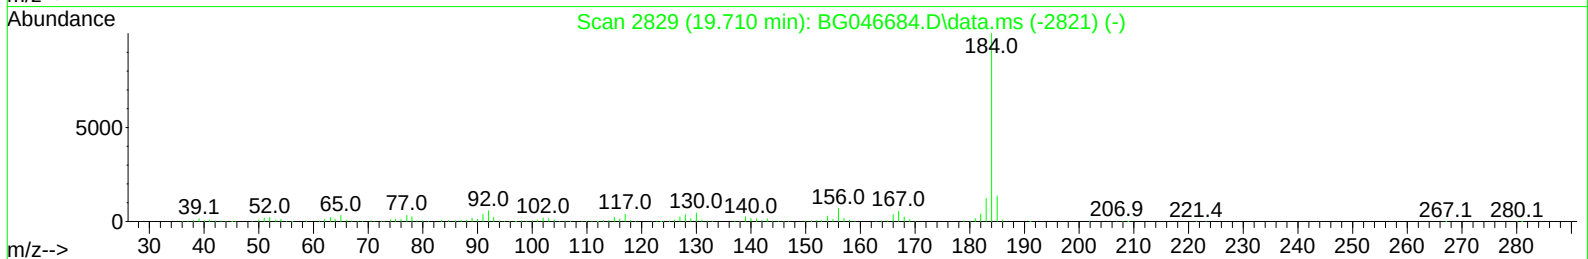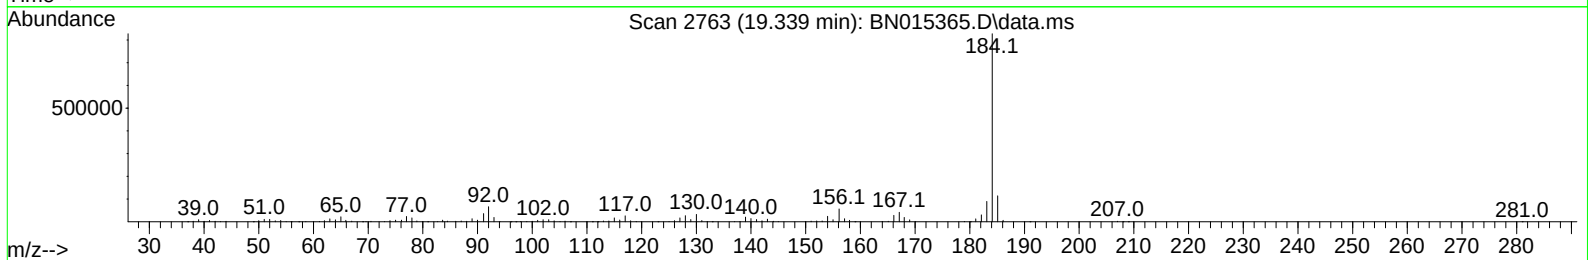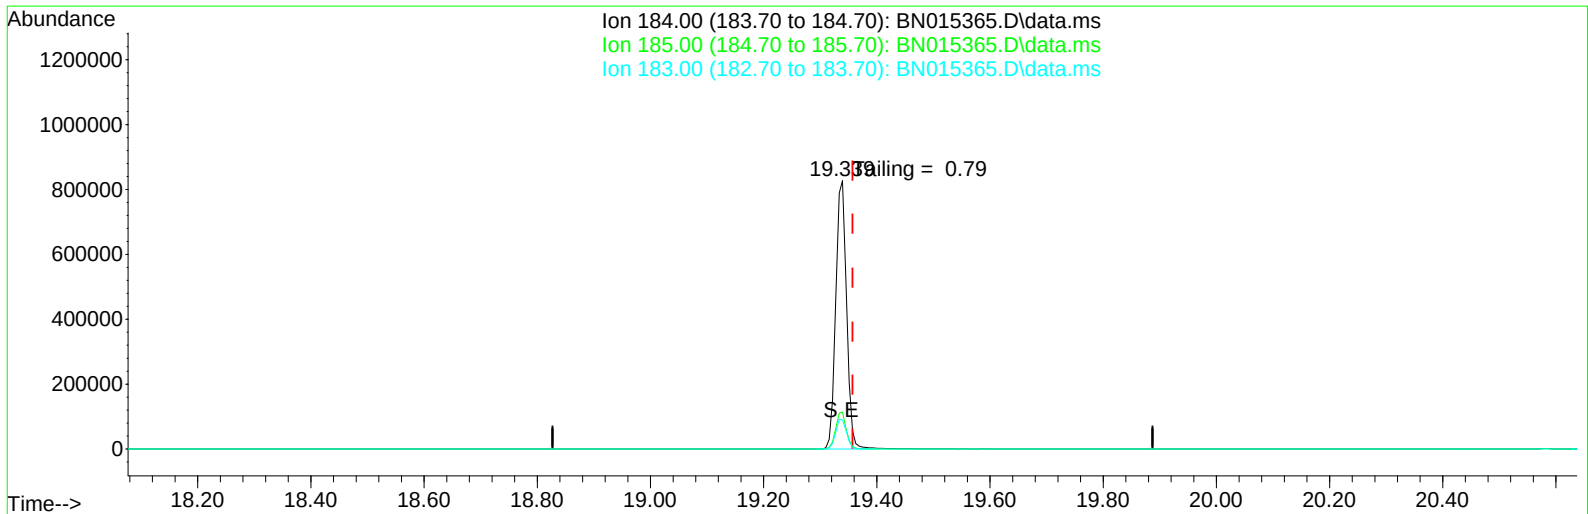

TIC: BN015365.D\data.ms

(77) Benzidine

19.339min (-0.018) 0.00 ng




response 1105844

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	10.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
 Data File : BN015365.D
 Acq On : 07 Jul 2021 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 07 10:52:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 10:10:58 2021
 Response via : Initial Calibration

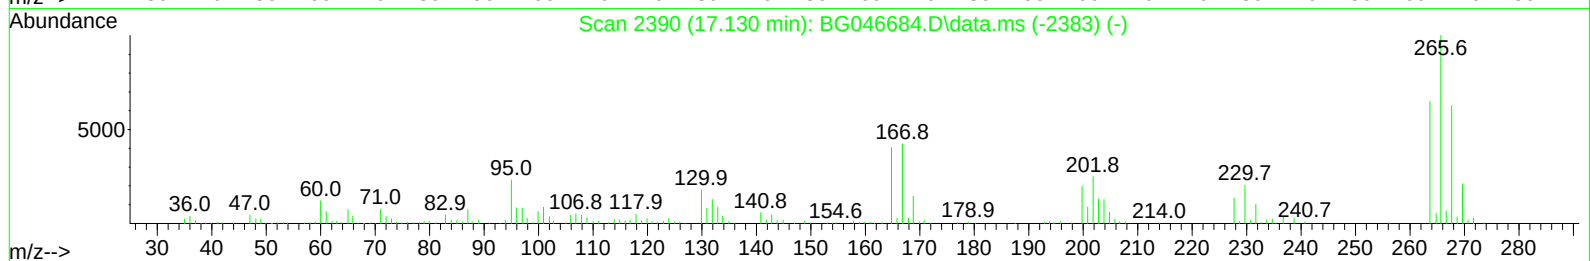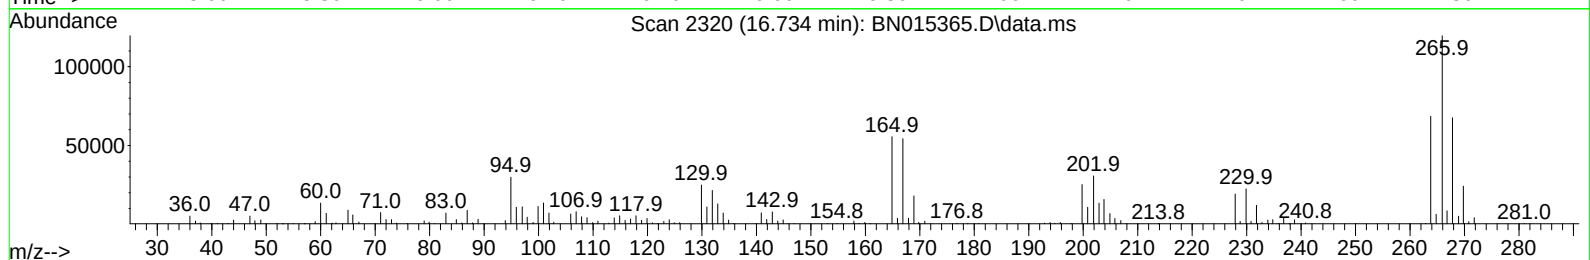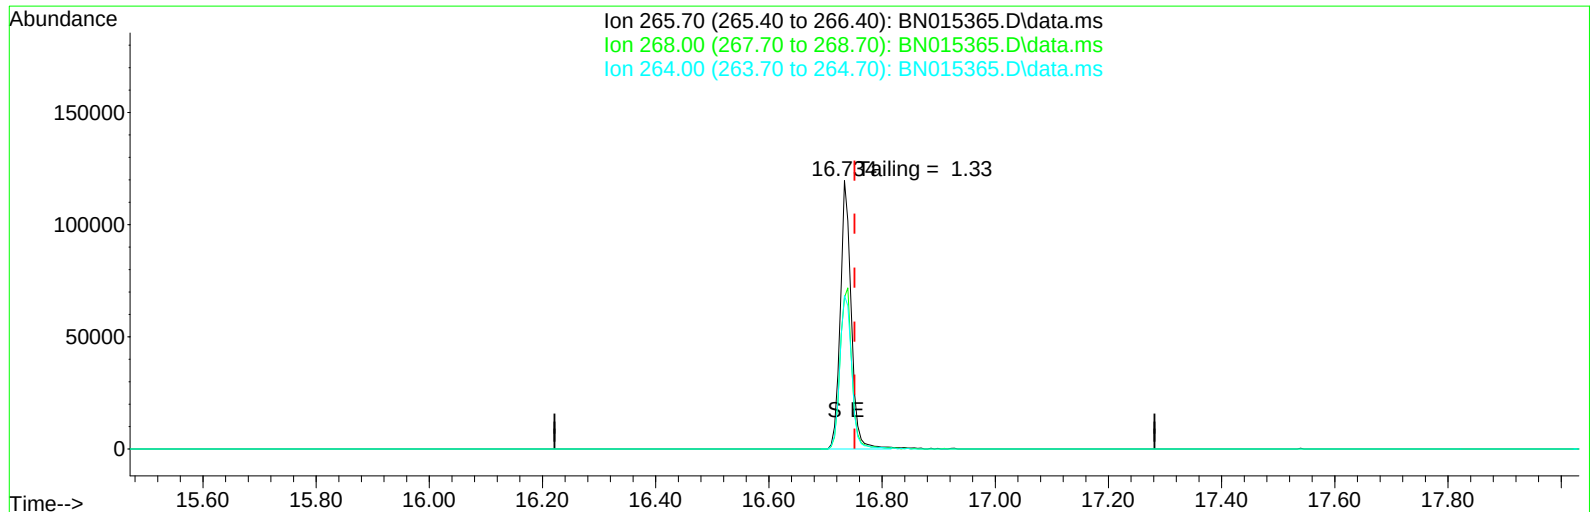

TIC: BN015365.D\data.ms

(70) Pentachlorophenol (C)

16.734min (-0.018) 27863.22 ng

response 161811

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.48
264.00	61.60	57.20
0.00	0.00	0.00