


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
 Data File : BN015384.D
 Acq On : 07 Jul 2021 22:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 07 11:11:38 2021

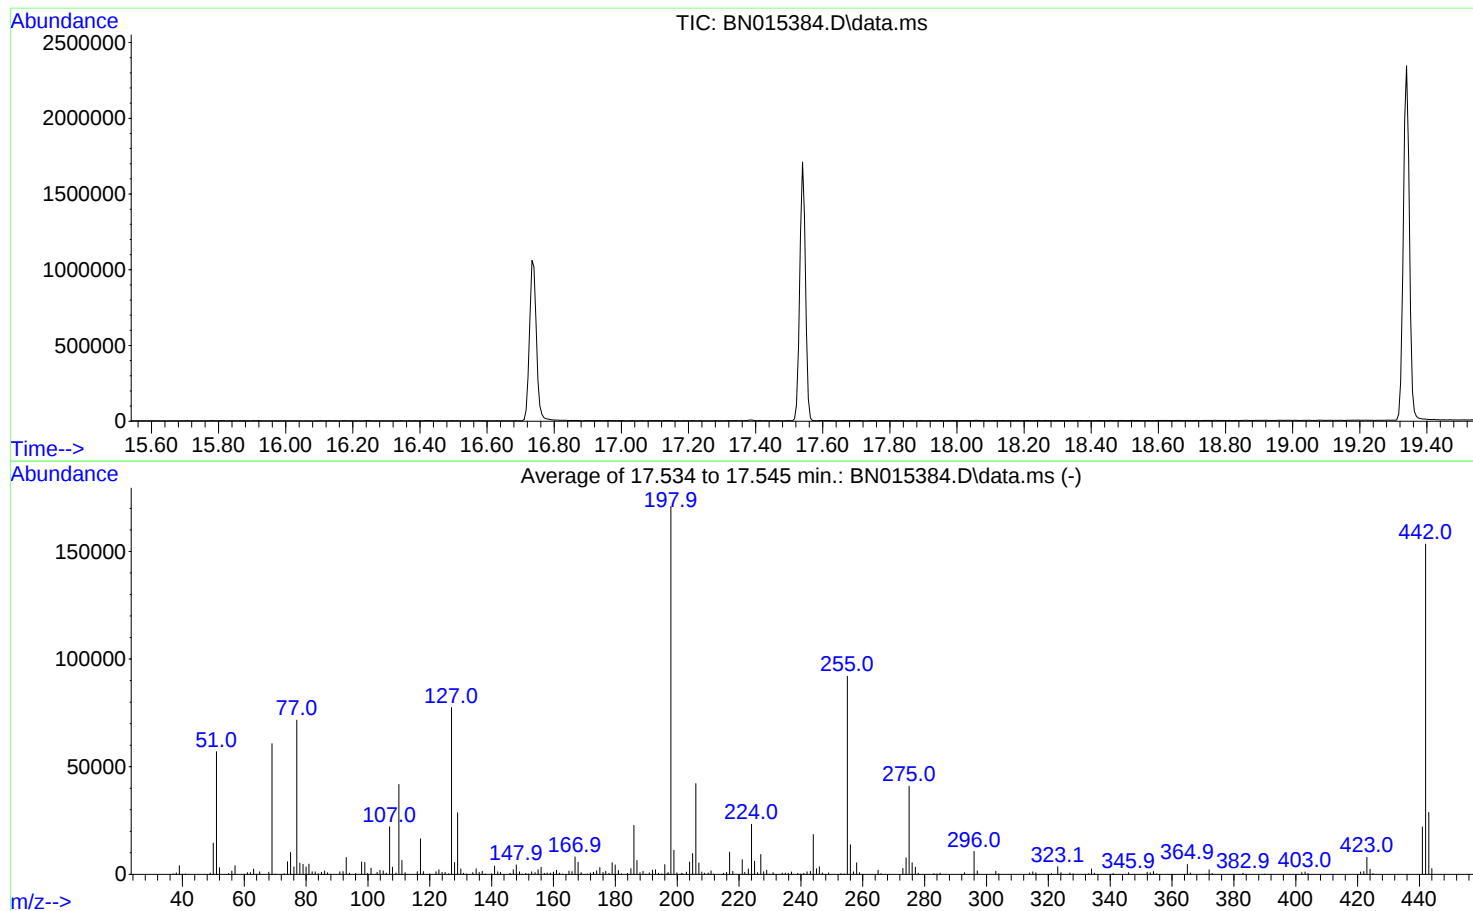




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	57016	PASS
68	69	0.00	2	1.7	1055	PASS
69	198	0.00	100	35.6	60755	PASS
70	69	0.00	2	0.2	133	PASS
127	198	10	80	45.4	77523	PASS
197	198	0.00	2	0.5	810	PASS
198	198	100	100	100.0	170859	PASS
199	198	5	9	6.6	11228	PASS
275	198	10	60	24.0	40949	PASS
365	198	1	100	2.7	4635	PASS
441	198	0.01	100	12.9	22022	PASS
442	442	50	100	100.0	153392	PASS
443	442	15	24	18.7	28757	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\  
Data File : BN015384.D  
Acq On    : 07 Jul 2021  22:41  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 08 06:53:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

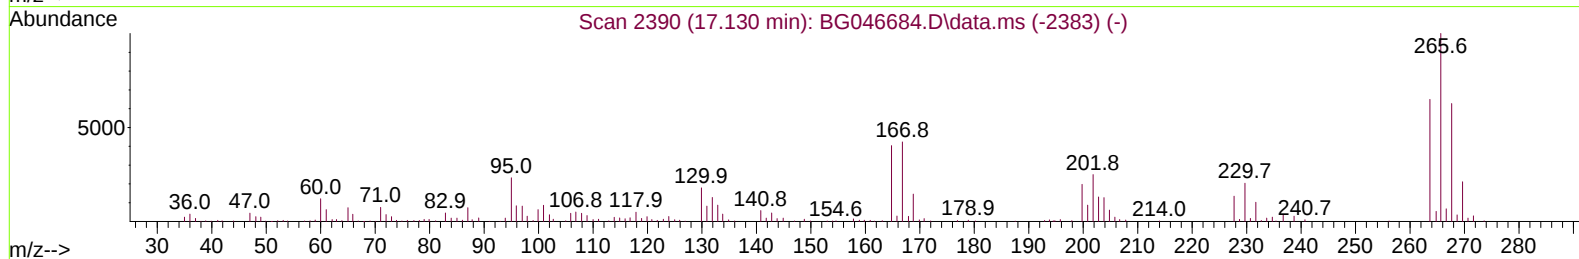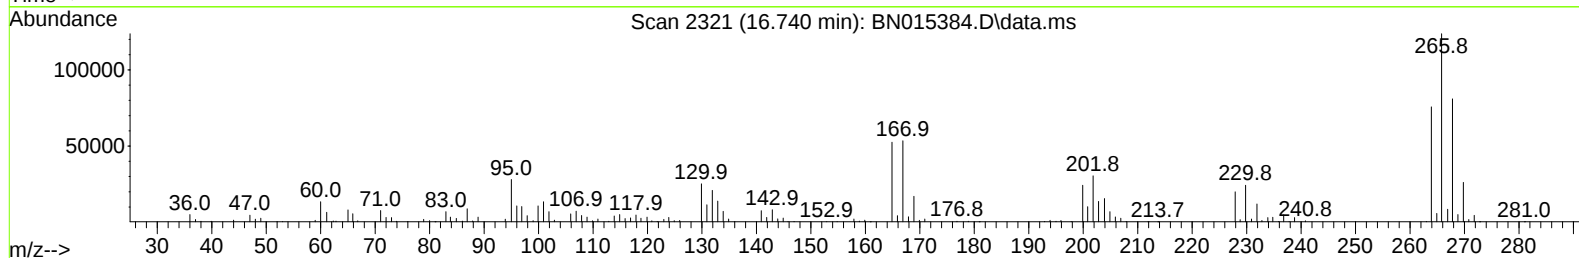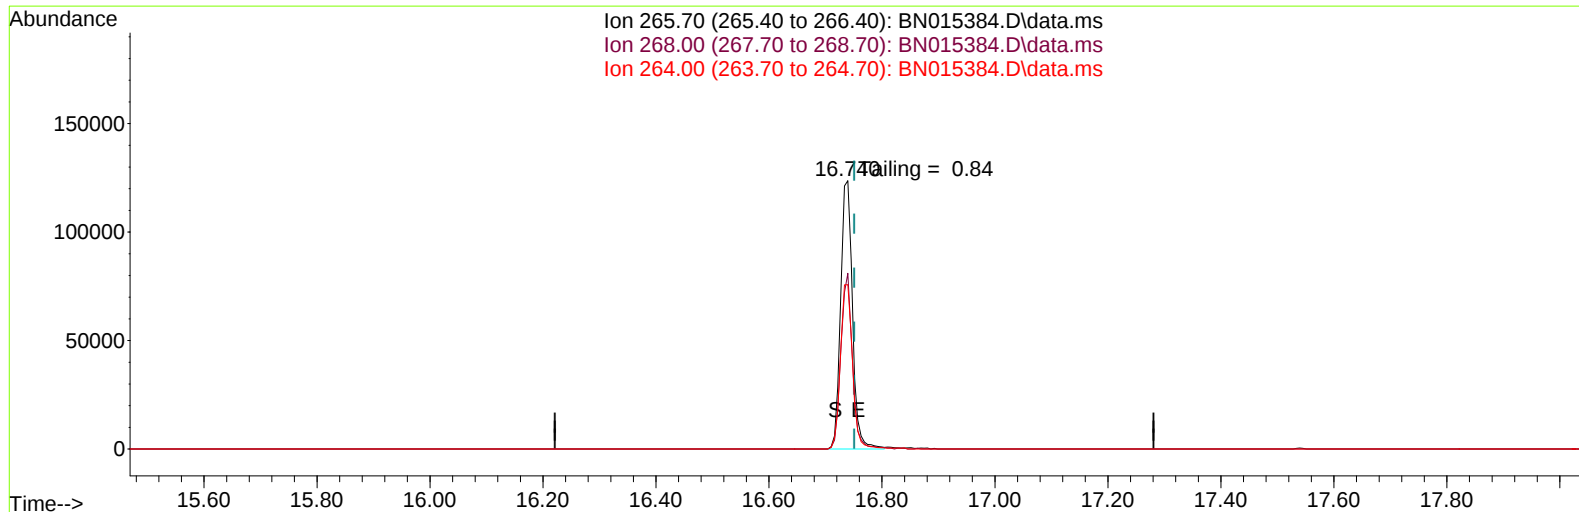

TIC: BN015384.D\data.ms

(70) Pentachlorophenol (C)

16.740min (-0.012) 23133.36 ng




response **180274**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.44
264.00	61.60	61.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070721\
Data File : BN015384.D
Acq On : 07 Jul 2021 22:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 08 06:53:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

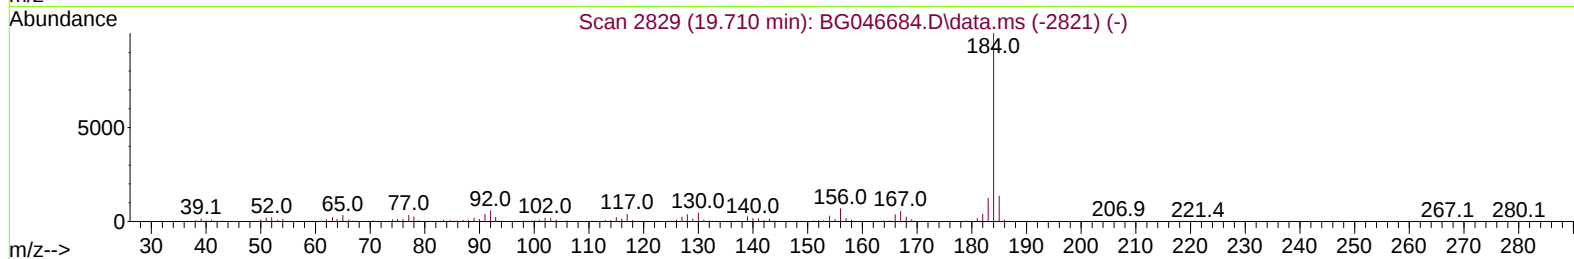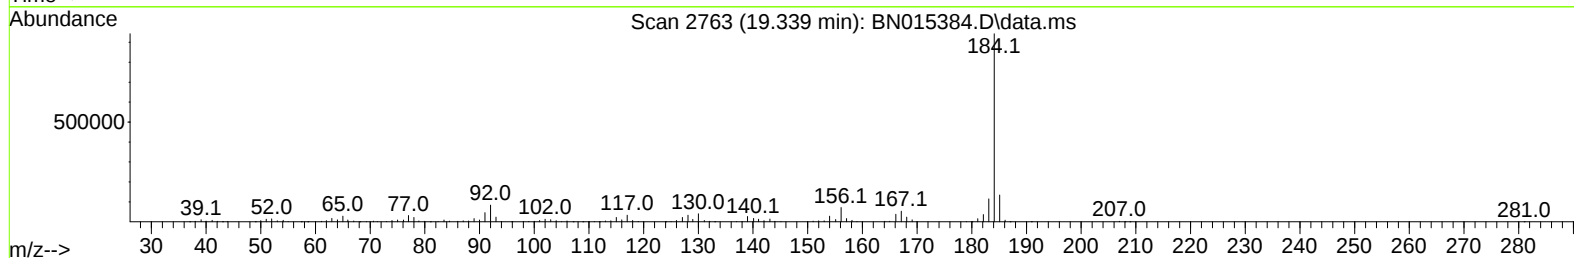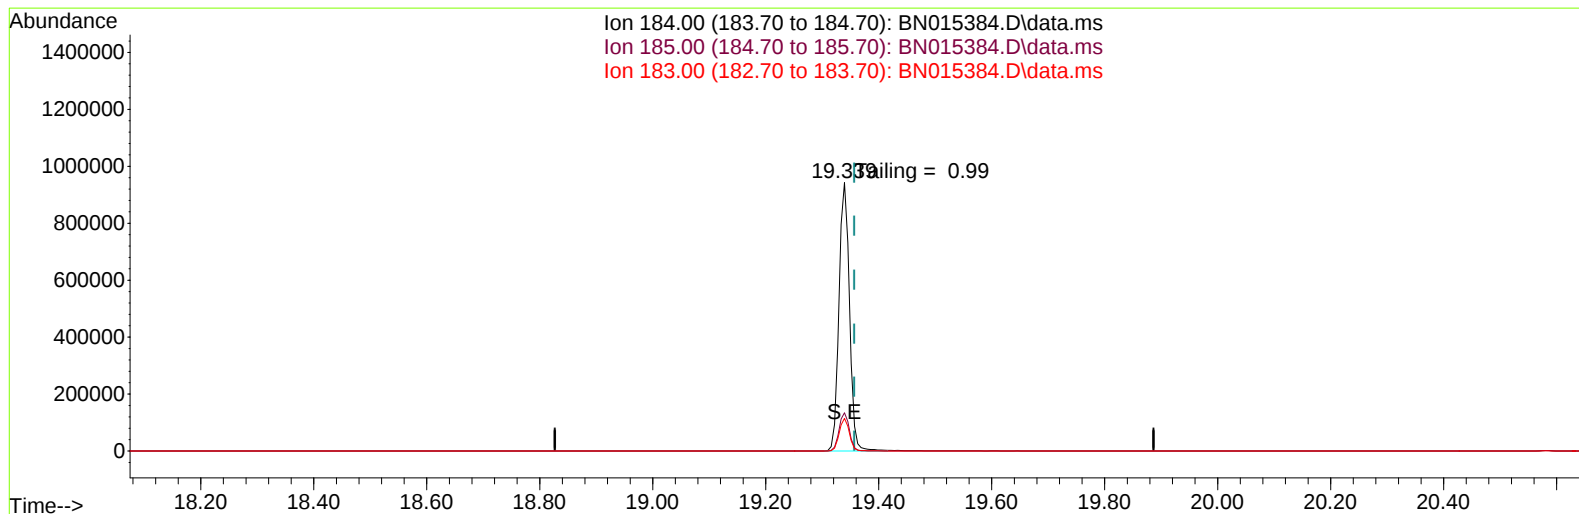

TIC: BN015384.D\data.ms

(77) Benzidine

19.339min (-0.017) 0.00 ng

response 1212357

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.26
183.00	13.20	12.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/7/2021	BNA_N	<u>BN015384.D</u>
Compound Name	Response	Retention Time
DDT	551167	20.581
DDD	2982	20.139
DDE	549	19.634
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3531	554698	0.64