

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070822\
 Data File : BN020695.D
 Acq On : 08 Jul 2022 17:06
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Jul 09 00:09:54 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 02 03:10:12 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	4542	0.400	ng	0.00
7) Naphthalene-d8	10.626	136	13916	0.400	ng	0.00
13) Acenaphthene-d10	14.474	164	7884	0.400	ng	0.00
19) Phenanthrene-d10	17.225	188	15581	0.400	ng	0.00
29) Chrysene-d12	21.431	240	9834	0.400	ng	0.00
35) Perylene-d12	23.784	264	7306	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.413	112	3376	0.268	ng	0.00
5) Phenol-d6	7.024	99	4401	0.292	ng	0.00
8) Nitrobenzene-d5	8.982	82	3608	0.320	ng	-0.01
11) 2-Methylnaphthalene-d10	12.223	152	8201	0.344	ng	0.00
14) 2,4,6-Tribromophenol	15.974	330	719	0.242	ng	0.00
15) 2-Fluorobiphenyl	13.095	172	12067	0.371	ng	-0.01
27) Fluoranthene-d10	19.265	212	14448	0.312	ng	0.00
31) Terphenyl-d14	19.872	244	9827	0.418	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.261	88	2078	0.349	ng	98
3) n-Nitrosodimethylamine	3.608	42	1524	0.281	ng	95
6) bis(2-Chloroethyl)ether	7.255	93	4086	0.315	ng	92
9) Naphthalene	10.669	128	15215	0.366	ng	100
10) Hexachlorobutadiene	10.968	225	2730	0.361	ng	# 99
12) 2-Methylnaphthalene	12.299	142	9607	0.348	ng	98
16) Acenaphthylene	14.196	152	12494	0.330	ng	98
17) Acenaphthene	14.538	154	9108	0.353	ng	95
18) Fluorene	15.521	166	11370	0.338	ng	99
20) 4,6-Dinitro-2-methylph...	15.639	198	381	0.350	ng	# 61
21) 4-Bromophenyl-phenylether	16.415	248	3348	0.370	ng	98
22) Hexachlorobenzene	16.538	284	3846	0.383	ng	97
23) Atrazine	16.692	200	2006	0.281	ng	97
24) Pentachlorophenol	16.897	266	590	0.367	ng	94
25) Phenanthrene	17.266	178	18263	0.348	ng	100
26) Anthracene	17.359	178	13883	0.306	ng	100
28) Fluoranthene	19.295	202	18498	0.323	ng	99
30) Pyrene	19.657	202	18303	0.440	ng	100
32) Benzo(a)anthracene	21.413	228	10320	0.294	ng	98
33) Chrysene	21.467	228	14494	0.373	ng	98
34) Bis(2-ethylhexyl)phtha...	21.351	149	7351	0.371	ng	98
36) Indeno(1,2,3-cd)pyrene	26.226	276	10648	0.327	ng	99
37) Benzo(b)fluoranthene	23.118	252	12238	0.435	ng	96
38) Benzo(k)fluoranthene	23.118	252	10795	0.360	ng	95
39) Benzo(a)pyrene	23.682	252	8616	0.353	ng	# 90
40) Dibenzo(a,h)anthracene	26.243	278	8460	0.324	ng	97
41) Benzo(g,h,i)perylene	26.962	276	9482	0.332	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070822\
Data File : BN020695.D
Acq On : 08 Jul 2022 17:06
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Jul 09 00:09:54 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 03:10:12 2022
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.825 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN020695.D
 Acq: 08 Jul 2022 17:06




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion: 152 Resp: 4542
 Ion Ratio Lower Upper
 152 100
 150 155.4 127.9 191.9
 115 62.9 51.4 77.2



#2
 1,4-Dioxane
 Concen: 0.349 ng
 RT: 3.261 min Scan# 25
 Delta R.T. 0.000 min
 Lab File: BN020695.D
 Acq: 08 Jul 2022 17:06

Tgt Ion: 88 Resp: 2078
 Ion Ratio Lower Upper
 88 100
 43 36.1 30.2 45.2
 58 89.8 73.0 109.6









#3
n-Nitrosodimethylamine
Concen: 0.281 ng
RT: 3.608 min Scan# 71
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 1524
Ion Ratio Lower Upper
42 100
74 99.1 84.0 126.0
44 12.8 9.8 14.8



#4
2-Fluorophenol
Concen: 0.268 ng
RT: 5.413 min Scan# 323
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion: 112 Resp: 3376
Ion Ratio Lower Upper
112 100
64 64.3 49.1 73.7
63 35.2 26.3 39.5









#5
Phenol-d6
Concen: 0.292 ng
RT: 7.024 min Scan# 54
Delta R.T. -0.007 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 4401
Ion Ratio Lower Upper
99 100
42 23.9 19.3 28.9
71 35.0 27.5 41.3



#6
bis(2-Chloroethyl)ether
Concen: 0.315 ng
RT: 7.255 min Scan# 578
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion: 93 Resp: 4086
Ion Ratio Lower Upper
93 100
63 91.9 67.4 101.0
95 36.1 26.5 39.7









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.626 min Scan# 94
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:136	Resp:	13916
Ion Ratio	Lower	Upper
136	100	
137	11.6	9.0 13.6
54	8.1	6.2 9.2
68	5.7	4.4 6.6



#8
Nitrobenzene-d5
Concen: 0.320 ng
RT: 8.982 min Scan# 787
Delta R.T. -0.011 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion: 82	Resp:	3608
Ion Ratio	Lower	Upper
82	100	
128	36.6	35.0 52.6
54	67.2	46.2 69.4









#9
Naphthalene
Concen: 0.366 ng
RT: 10.669 min Scan# 941
Delta R.T. -0.011 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:128	Resp:	15215
Ion Ratio	Lower	Upper
128	100	
129	11.3	8.9 13.3
127	13.6	10.8 16.2



#10
Hexachlorobutadiene
Concen: 0.361 ng
RT: 10.968 min Scan# 973
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:225	Resp:	2730
Ion Ratio	Lower	Upper
225	100	
223	0.0	0.0 0.0
227	64.2	50.9 76.3









#11
2-Methylnaphthalene-d10
Concen: 0.344 ng
RT: 12.223 min Scan# 1185
Delta R.T. -0.004 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 8201
Ion Ratio Lower Upper
152 100
151 20.6 16.2 24.4



#12
2-Methylnaphthalene
Concen: 0.348 ng
RT: 12.299 min Scan# 1232
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:142 Resp: 9607
Ion Ratio Lower Upper
142 100
141 87.3 71.6 107.4
115 37.8 29.8 44.8









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.474 min Scan# 1461
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:164 Resp: 7884
Ion Ratio Lower Upper
164 100
162 104.1 82.1 123.1
160 48.5 38.6 58.0



#14
2,4,6-Tribromophenol
Concen: 0.242 ng
RT: 15.974 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:330 Resp: 719
Ion Ratio Lower Upper
330 100
332 100.4 77.6 116.4
141 55.1 41.0 61.4









#15
2-Fluorobiphenyl
Concen: 0.371 ng
RT: 13.095 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172	Resp:	12067
Ion Ratio	Lower	Upper
172	100	
171	35.6	27.2 40.8
170	24.6	18.2 27.4



#16
Acenaphthylene
Concen: 0.330 ng
RT: 14.196 min Scan# 1445
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:152	Resp:	12494
Ion Ratio	Lower	Upper
152	100	
151	19.5	16.2 24.4
153	12.9	10.7 16.1









#17
Acenaphthene
Concen: 0.353 ng
RT: 14.538 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 9108
Ion Ratio Lower Upper
154 100
153 115.0 87.5 131.3
152 58.0 43.8 65.6



#18
Fluorene
Concen: 0.338 ng
RT: 15.521 min Scan# 1569
Delta R.T. -0.011 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:166 Resp: 11370
Ion Ratio Lower Upper
166 100
165 99.0 78.6 118.0
167 13.6 10.8 16.2









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.225 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:188 Resp: 15581
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.3 7.4 11.2



#20
4,6-Dinitro-2-methylphenol
Concen: 0.350 ng
RT: 15.639 min Scan# 1580
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:198 Resp: 381
Ion Ratio Lower Upper
198 100
182 31.4 12.1 18.1#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.370 ng
RT: 16.415 min Scan# 1665
Delta R.T. -0.010 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 3348
Ion Ratio Lower Upper
248 100
250 95.8 75.3 112.9
141 86.6 67.3 100.9

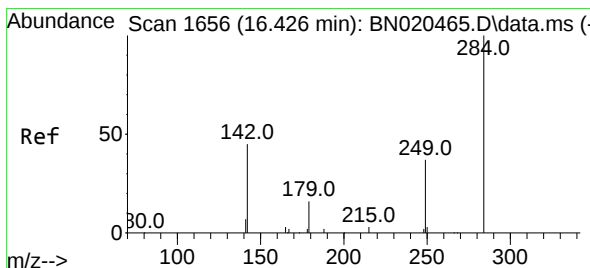

#22
Hexachlorobenzene
Concen: 0.383 ng
RT: 16.538 min Scan# 1667
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:284 Resp: 3846
Ion Ratio Lower Upper
284 100
142 47.1 35.2 52.8
249 33.6 26.6 40.0





#23

Atrazine

Concen: 0.281 ng

RT: 16.692 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN020695.D

Acq: 08 Jul 2022 17:06

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:200 Resp: 2006

Ion Ratio Lower Upper

200 100

173 32.2 23.6 35.4

215 46.6 36.6 54.8



#24

Pentachlorophenol

Concen: 0.367 ng

RT: 16.897 min Scan# 1702

Delta R.T. 0.000 min

Lab File: BN020695.D

Acq: 08 Jul 2022 17:06




Tgt Ion:266 Resp: 590


Ion Ratio Lower Upper

266 100

264 59.8 51.3 76.9

268 60.8 52.6 79.0









#25
Phenanthrene
Concen: 0.348 ng
RT: 17.266 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178 Resp: 18263
Ion Ratio Lower Upper
178 100
176 19.3 15.3 22.9
179 15.5 12.2 18.4

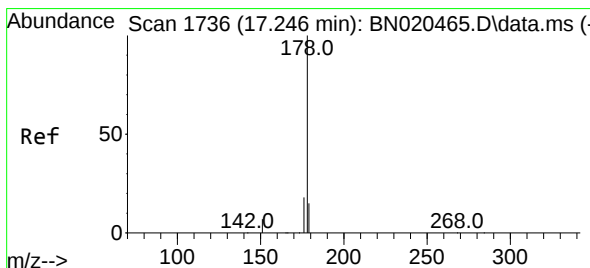

#26
Anthracene
Concen: 0.306 ng
RT: 17.359 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:178 Resp: 13883
Ion Ratio Lower Upper
178 100
176 18.7 14.9 22.3
179 15.5 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.312 ng
RT: 19.265 min Scan# 2116
Delta R.T. -0.004 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 14448
Ion Ratio Lower Upper
212 100
106 16.1 12.6 19.0
104 8.8 7.2 10.8



#28
Fluoranthene
Concen: 0.323 ng
RT: 19.295 min Scan# 2116
Delta R.T. -0.004 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:202 Resp: 18498
Ion Ratio Lower Upper
202 100
101 12.6 9.6 14.4
203 16.8 13.5 20.3









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.431 min Scan# 2430
Delta R.T. 0.000 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 9834
Ion Ratio Lower Upper
240 100
120 14.8 14.6 21.8
236 27.0 22.6 33.8



#30
Pyrene
Concen: 0.440 ng
RT: 19.657 min Scan# 2202
Delta R.T. -0.004 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06


Tgt Ion:202 Resp: 18303
Ion Ratio Lower Upper
202 100
200 20.6 16.6 25.0
203 17.5 14.2 21.2








#31
 Terphenyl-d14
 Concen: 0.418 ng
 RT: 19.872 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN020695.D
 Acq: 08 Jul 2022 17:06

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC







Tgt Ion:244 Resp: 9827
 Ion Ratio Lower Upper
 244 100
 212 9.3 7.1 10.7
 122 0.0 0.0 0.0



#32
 Benzo(a)anthracene
 Concen: 0.294 ng
 RT: 21.413 min Scan# 2442
 Delta R.T. -0.009 min
 Lab File: BN020695.D
 Acq: 08 Jul 2022 17:06

Tgt Ion:228 Resp: 10320
 Ion Ratio Lower Upper
 228 100
 226 28.1 21.2 31.8
 229 19.5 15.6 23.4





#33

Chrysene

Concen: 0.373 ng

RT: 21.467 min Scan# 2448

Delta R.T. 0.000 min

Lab File: BN020695.D

Acq: 08 Jul 2022 17:06

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:228 Resp: 14494

Ion Ratio Lower Upper

228 100

226 30.5 23.4 35.0

229 19.5 15.7 23.5



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.371 ng

RT: 21.351 min Scan# 2435

Delta R.T. 0.000 min

Lab File: BN020695.D

Acq: 08 Jul 2022 17:06




Tgt Ion:149 Resp: 7351


Ion Ratio Lower Upper

149 100

167 25.9 21.7 32.5

279 2.8 2.2 3.2





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.784 min Scan# 3024

Delta R.T. -0.006 min

Lab File: BN020695.D


Acq: 08 Jul 2022 17:06

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC






Tgt Ion:264 Resp: 7306

Ion Ratio Lower Upper

264 100

260 26.6 20.9 31.3

265 38.1 28.0 42.0

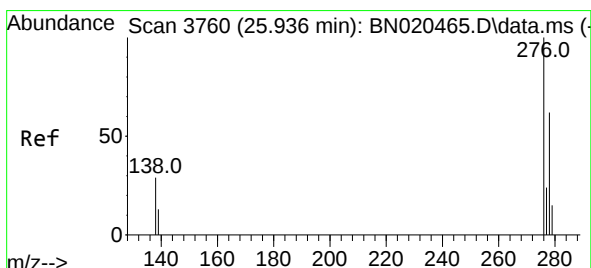

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.327 ng

RT: 26.226 min Scan# 3859

Delta R.T. 0.003 min

Lab File: BN020695.D

Acq: 08 Jul 2022 17:06




Tgt Ion:276 Resp: 10648


Ion Ratio Lower Upper

276 100

138 32.9 25.9 38.9

277 25.1 19.8 29.8









#37
Benzo(b)fluoranthene
Concen: 0.435 ng
RT: 23.118 min Scan# 21
Delta R.T. 0.044 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 12238
Ion Ratio Lower Upper
252 100
253 25.3 18.5 27.7
125 15.3 11.4 17.0



#38
Benzo(k)fluoranthene
Concen: 0.360 ng
RT: 23.118 min Scan# 2796
Delta R.T. -0.003 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06

Tgt Ion:252 Resp: 10795
Ion Ratio Lower Upper
252 100
253 25.3 18.0 27.0
125 15.3 11.0 16.4









#39
Benzo(a)pyrene
Concen: 0.353 ng
RT: 23.682 min Scan# 2926
Delta R.T. -0.003 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 8616
Ion Ratio Lower Upper
252 100
253 28.2 19.0 28.4
125 22.6 13.8 20.8#



#40
Dibenzo(a,h)anthracene
Concen: 0.324 ng
RT: 26.243 min Scan# 3865
Delta R.T. -0.003 min
Lab File: BN020695.D
Acq: 08 Jul 2022 17:06


Tgt Ion:278 Resp: 8460
Ion Ratio Lower Upper
278 100
139 24.0 18.6 28.0
279 27.2 19.7 29.5





#41
 Benzo(g,h,i)perylene
 Concen: 0.332 ng
 RT: 26.962 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BN020695.D
 Acq: 08 Jul 2022 17:06

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC



Tgt Ion:276 Resp: 9482
 Ion Ratio Lower Upper
 276 100
 277 24.6 19.5 29.3
 138 29.6 22.6 34.0

