
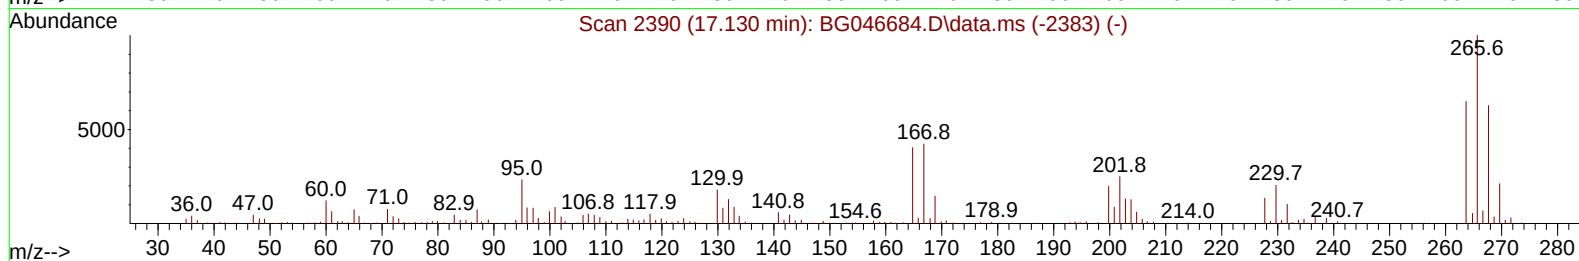
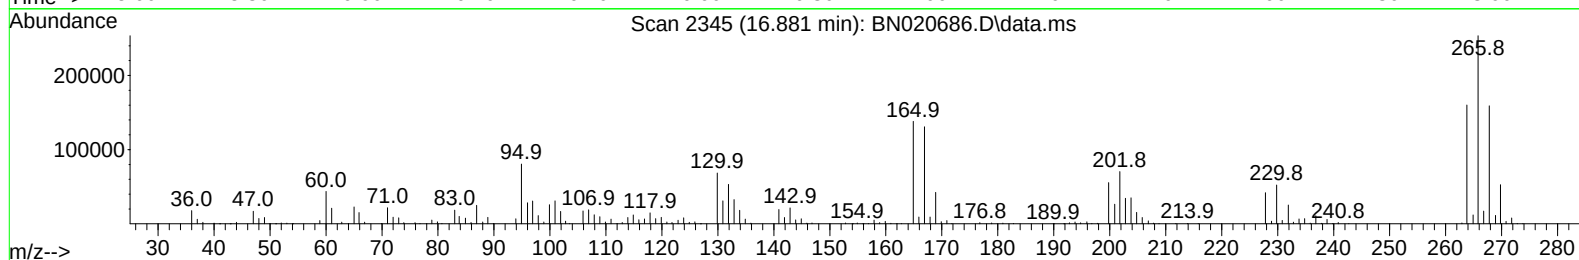


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070822\  
Data File : BN020686.D  
Acq On : 08 Jul 2022 10:00  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 01:04:11 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jul 09 01:04:06 2022  
Response via : Initial Calibration

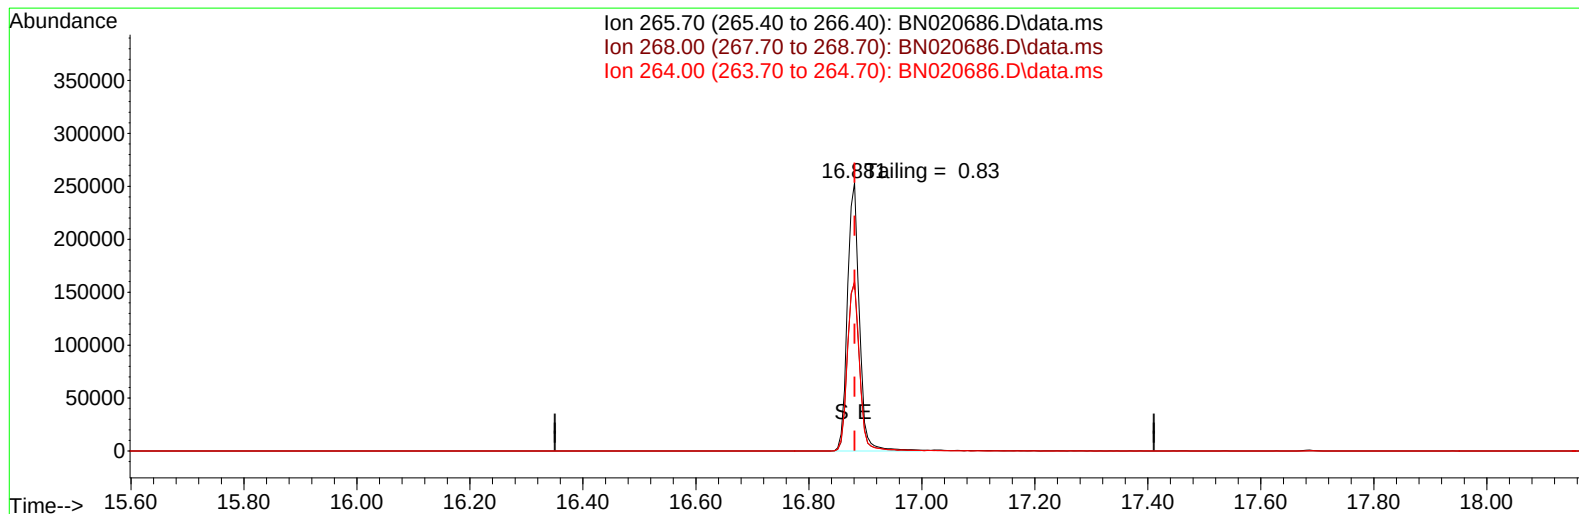

TIC: BN020686.D\data.ms

**(70) Pentachlorophenol (C)**




16.881min ( 0.000) 17249.88 ng

response 372275

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 62.79  |
| 264.00 | 61.60  | 63.19  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070822\  
Data File : BN020686.D  
Acq On : 08 Jul 2022 10:00  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 01:04:11 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jul 09 01:04:06 2022  
Response via : Initial Calibration

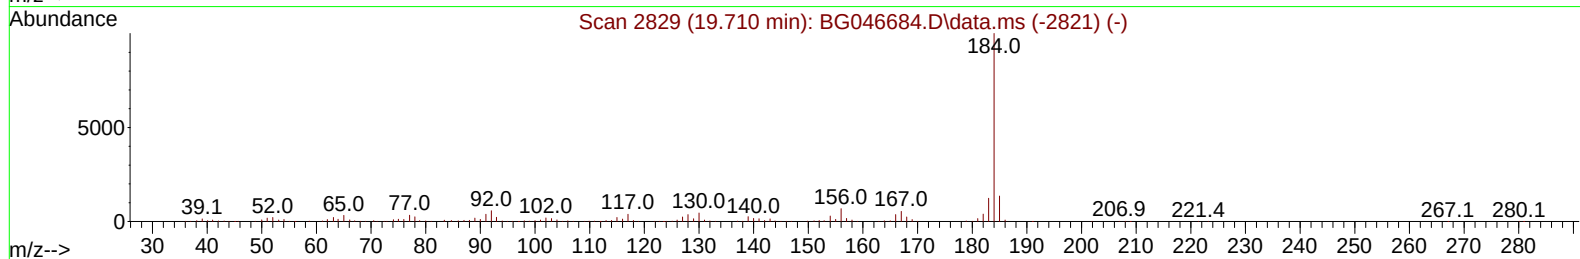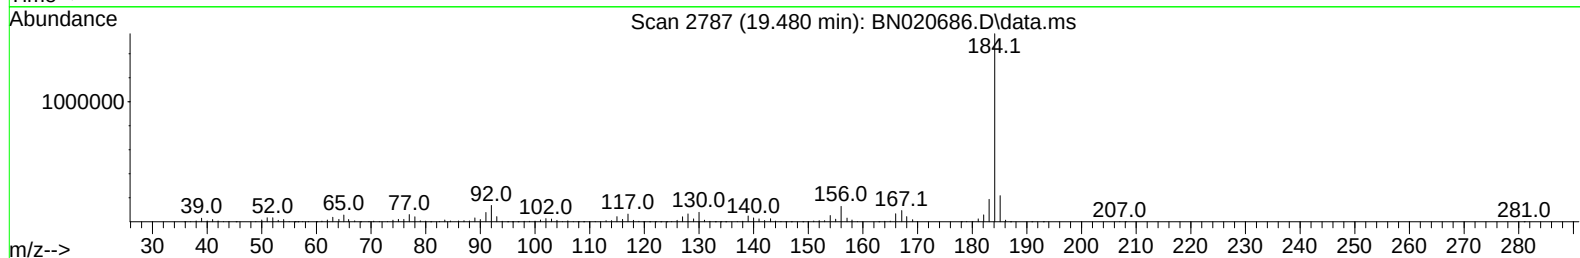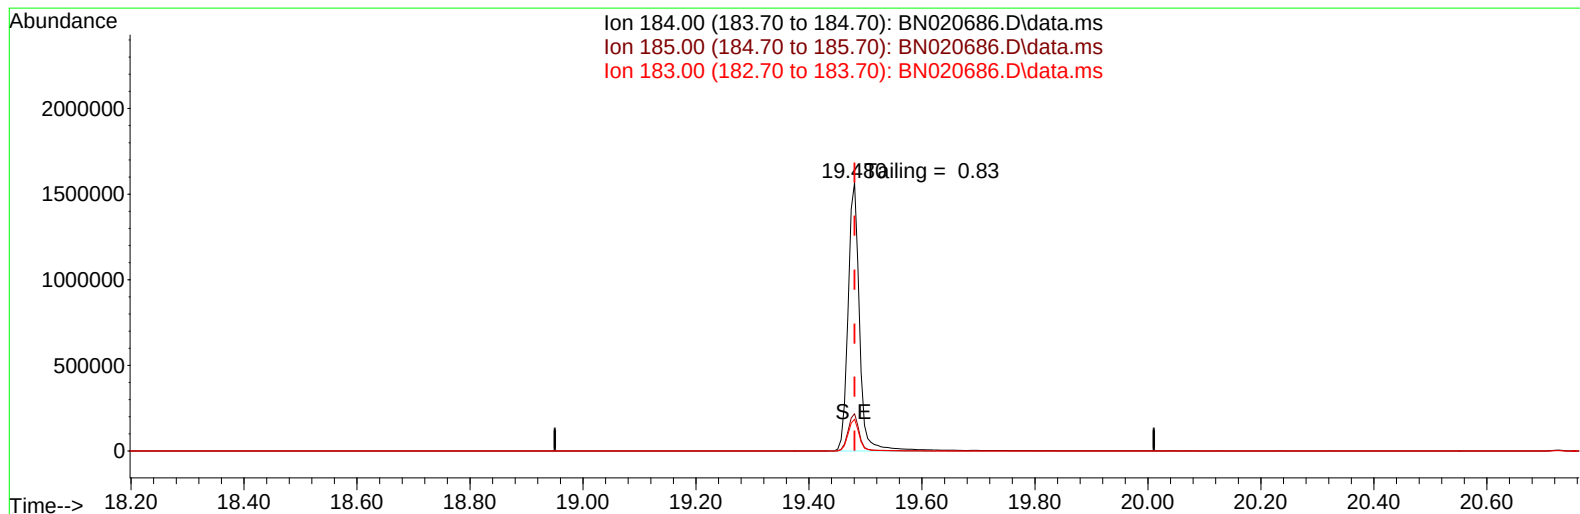

TIC: BN020686.D\data.ms

**(77) Benzidine**

19.480min ( 0.000) 0.00 ng

response 2216148

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.91  |
| 183.00 | 13.20  | 11.89  |
| 0.00   | 0.00   | 0.00   |