


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070822\
 Data File : BN020686.D
 Acq On : 08 Jul 2022 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 02 03:10:12 2022

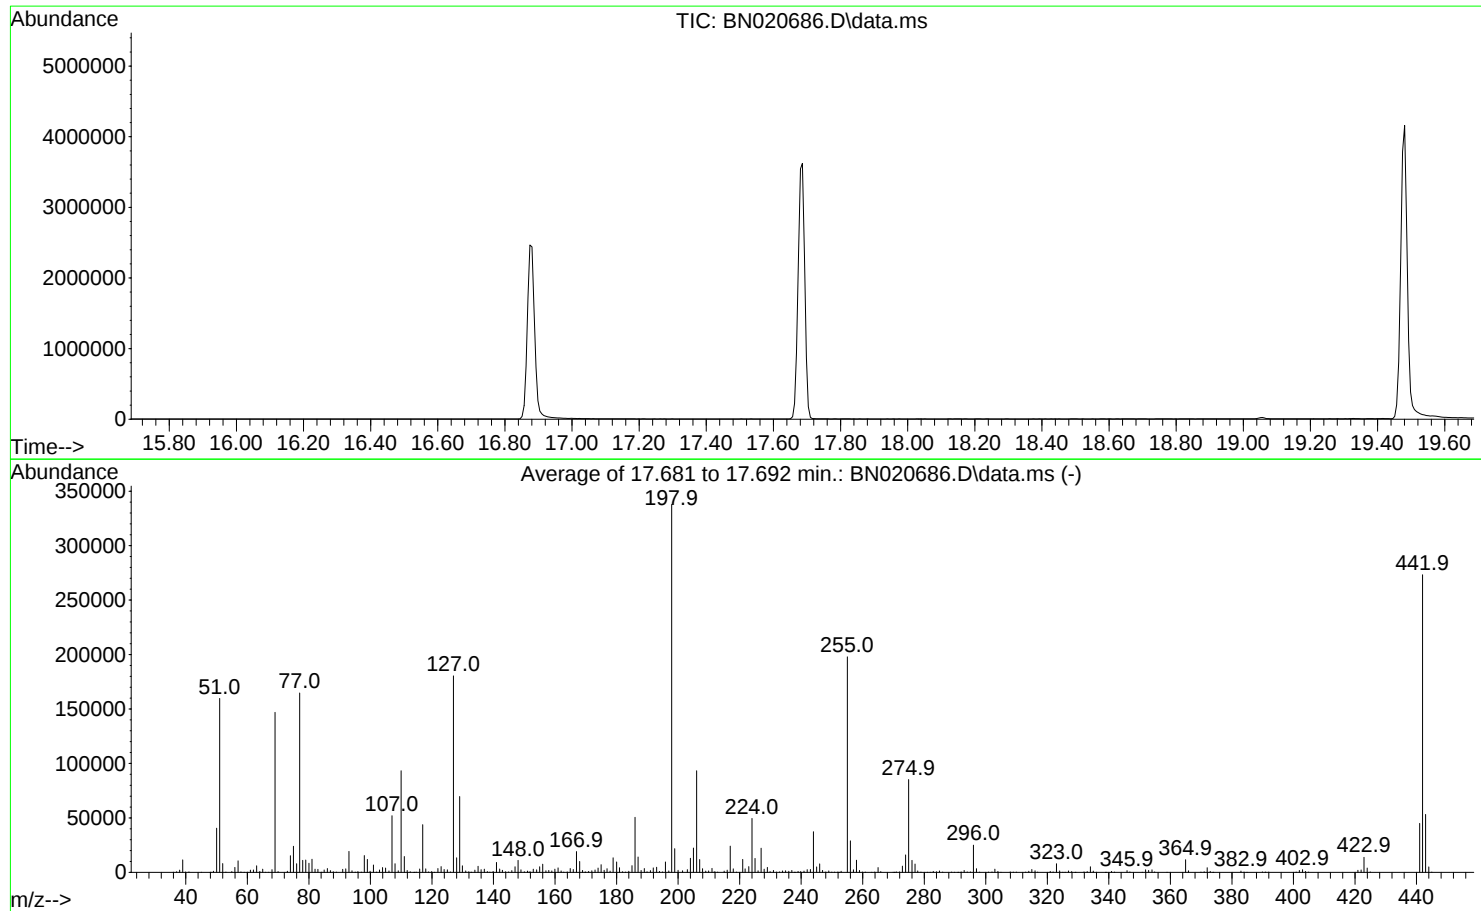




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.3	159672	PASS
68	69	0.00	2	1.7	2468	PASS
69	198	0.00	100	43.5	146864	PASS
70	69	0.00	2	0.5	764	PASS
127	198	10	80	53.4	180448	PASS
197	198	0.00	2	0.4	1373	PASS
198	198	100	100	100.0	337771	PASS
199	198	5	9	6.5	21813	PASS
275	198	10	60	25.2	85283	PASS
365	198	1	100	3.4	11610	PASS
441	198	0.01	100	13.3	44997	PASS
442	442	50	100	100.0	273301	PASS
443	442	15	24	19.4	53120	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070822\
 Data File : BN020686.D
 Acq On : 08 Jul 2022 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 09 01:04:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 09 01:04:06 2022
 Response via : Initial Calibration

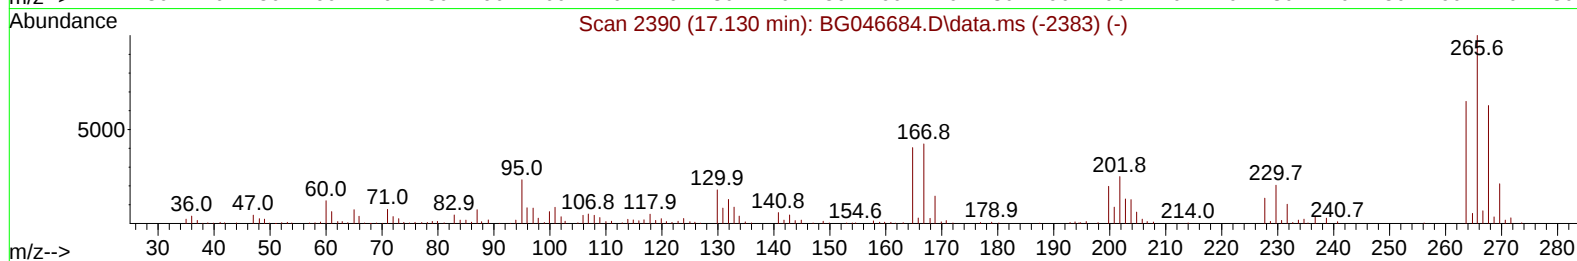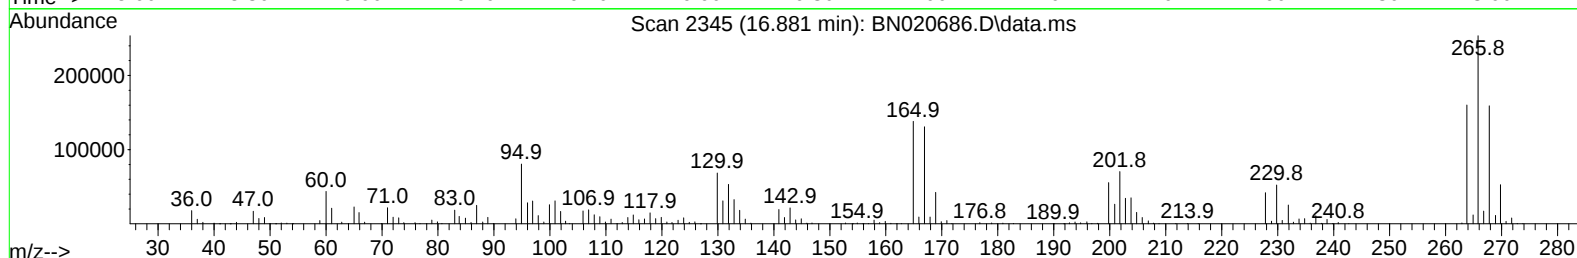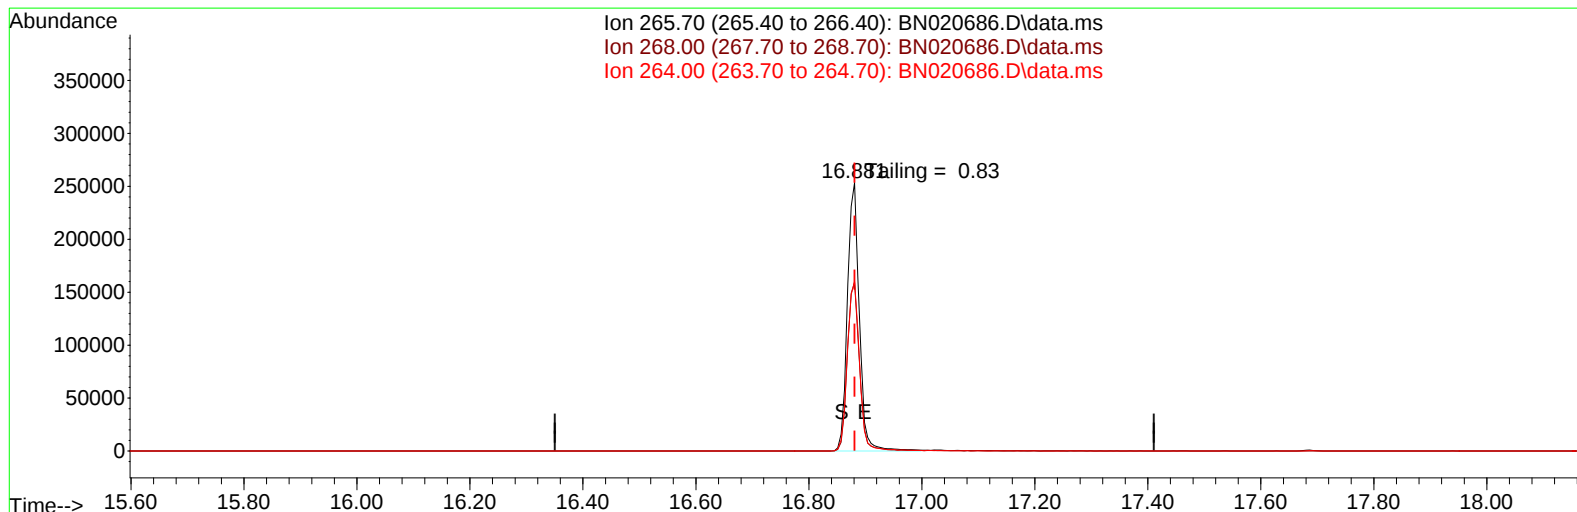

TIC: BN020686.D\data.ms

(70) Pentachlorophenol (C)

16.881min (0.000) 17249.88 ng




response 372275

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.79
264.00	61.60	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070822\
Data File : BN020686.D
Acq On : 08 Jul 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 09 01:04:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 09 01:04:06 2022
Response via : Initial Calibration

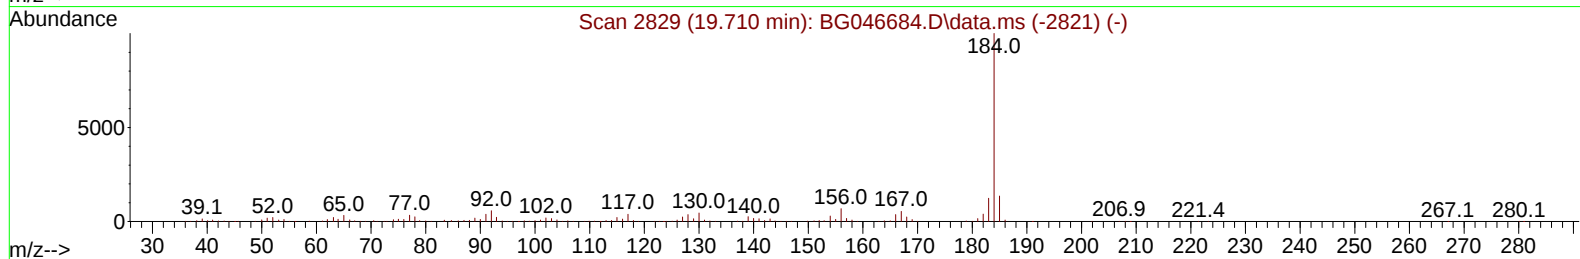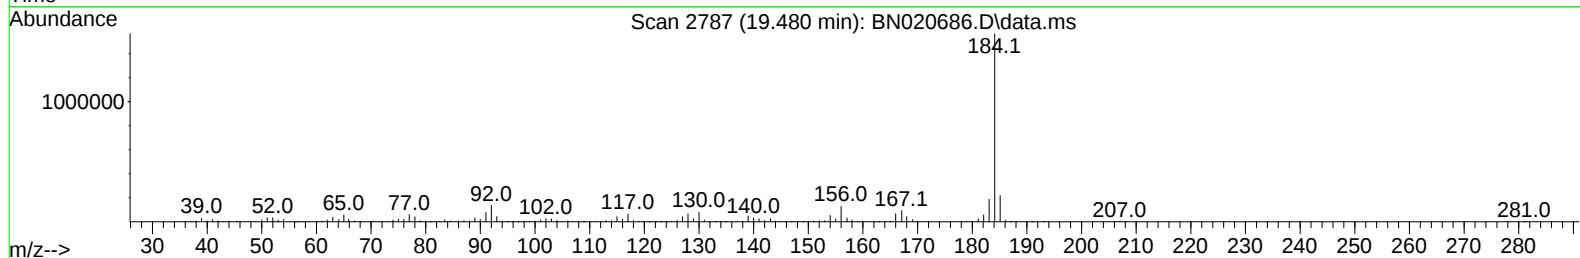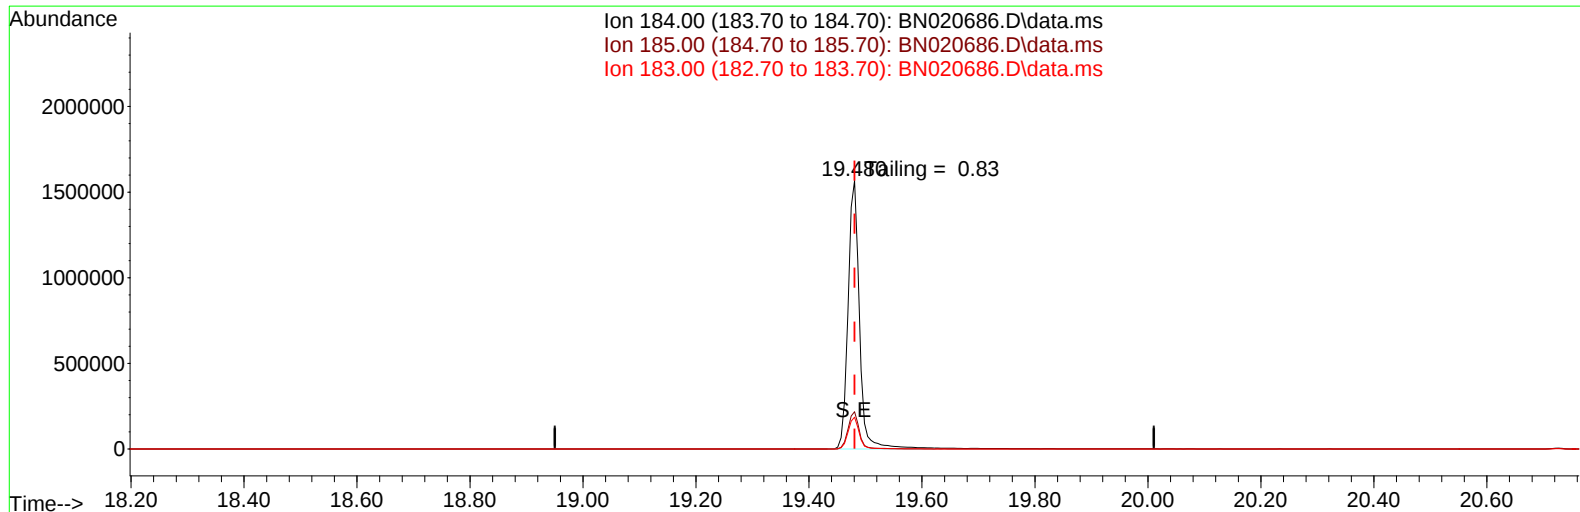

TIC: BN020686.D\data.ms

(77) Benzidine

19.480min (0.000) 0.00 ng

response 2216148

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/8/2022	BNA_N	<u>BN020686.D</u>
Compound Name	Response	Retention Time
DDT	1185642	20.727
DDD	22225	20.28
DDE	2513	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24738	1210380	2.04

Instrument :
BNA_N
ClientSampleId :
DFTPP