
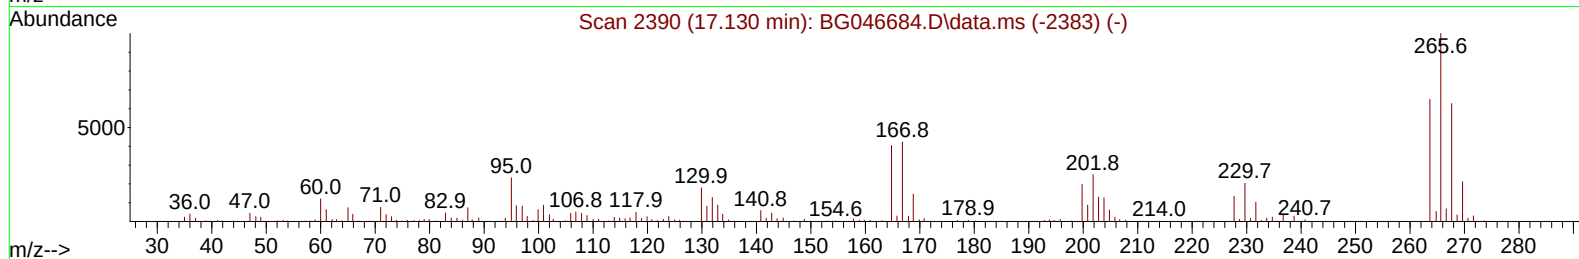
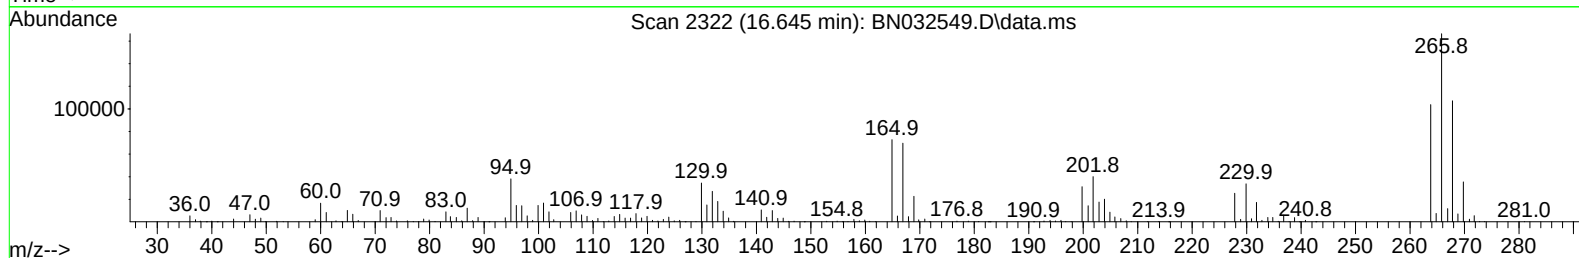


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070824\
Data File : BN032549.D
Acq On : 08 Jul 2024 10:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 11:23:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

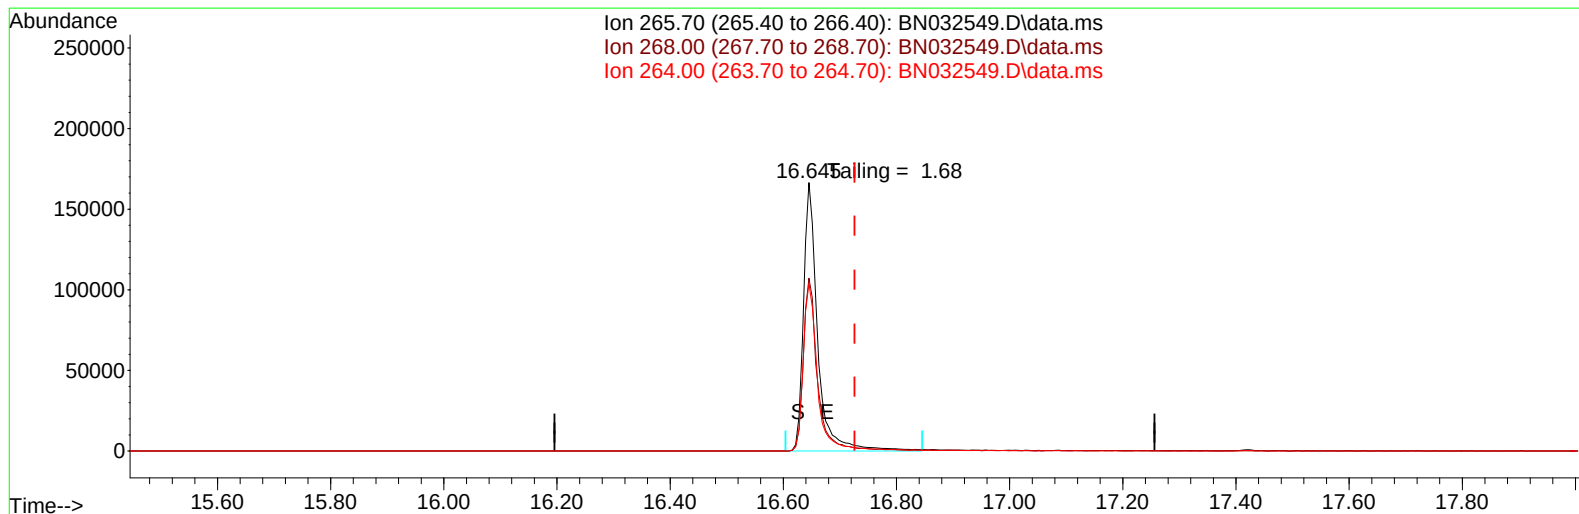

TIC: BN032549.D\data.ms

(70) Pentachlorophenol (C)




16.645min (-0.081) 22525.83 ng

response 290975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.41
264.00	61.60	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070824\
Data File : BN032549.D
Acq On : 08 Jul 2024 10:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 11:23:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

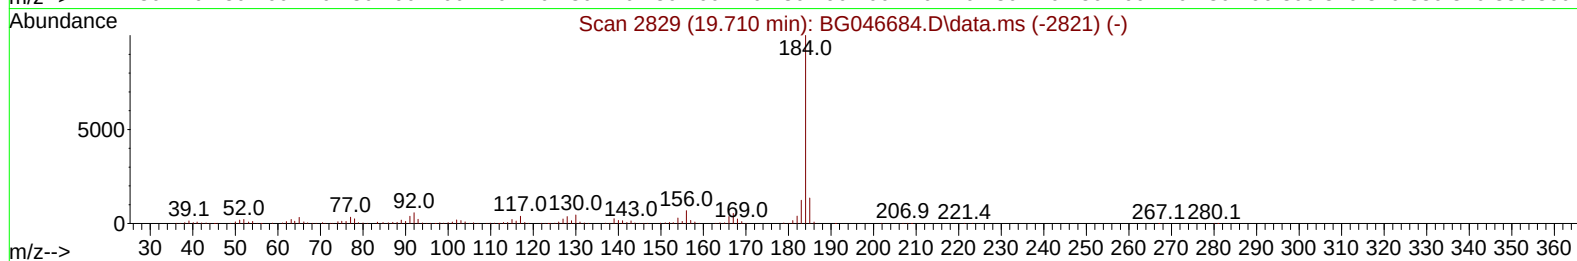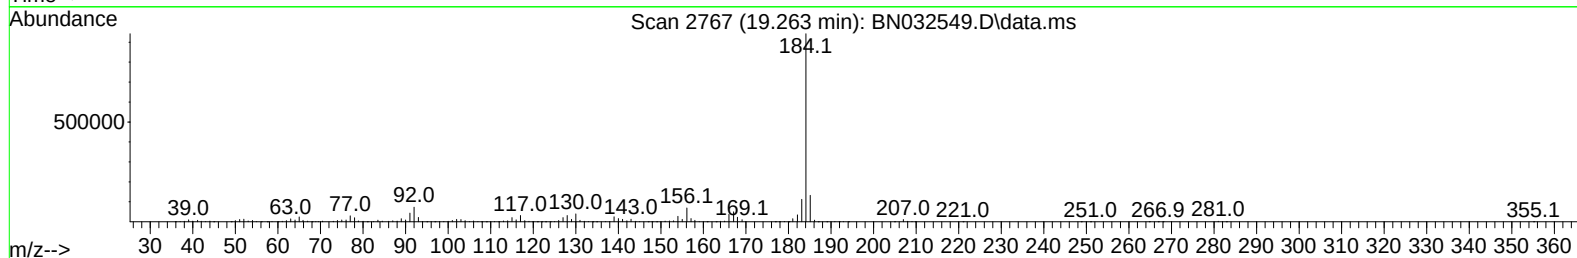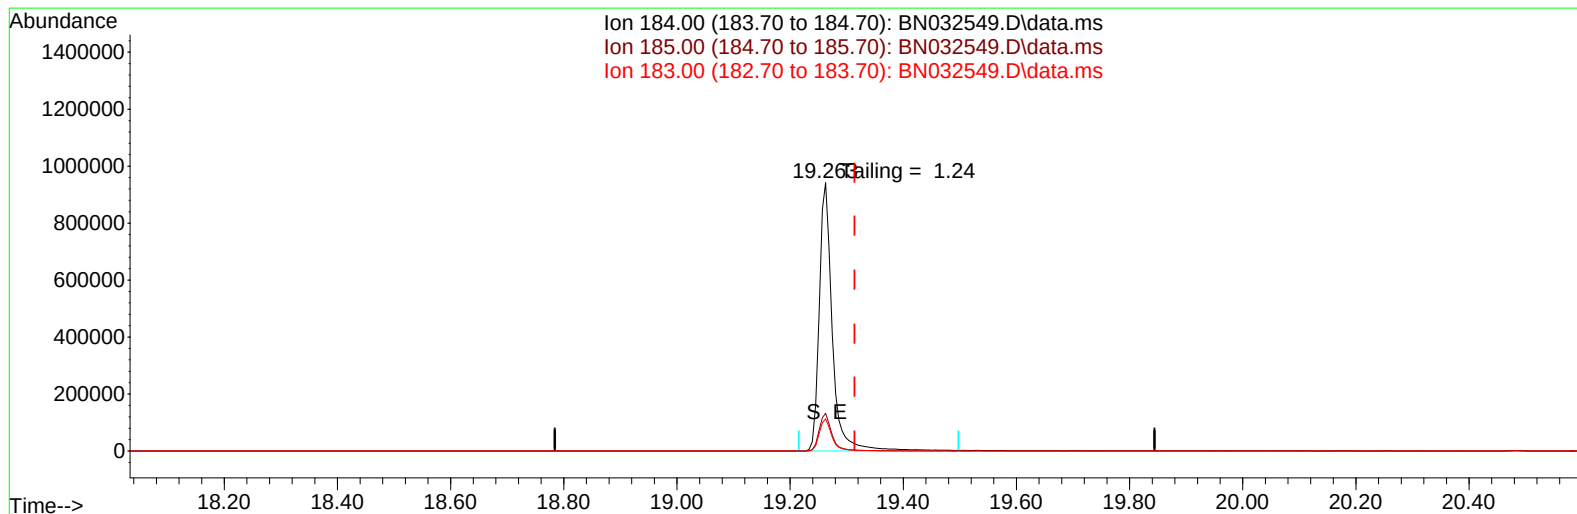

TIC: BN032549.D\data.ms

(77) Benzidine

19.263min (-0.051) 0.00 ng

response 1516228

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.97
0.00	0.00	0.00