


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070824\
Data File : BN032549.D
Acq On : 08 Jul 2024 10:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 08 15:11:21 2024

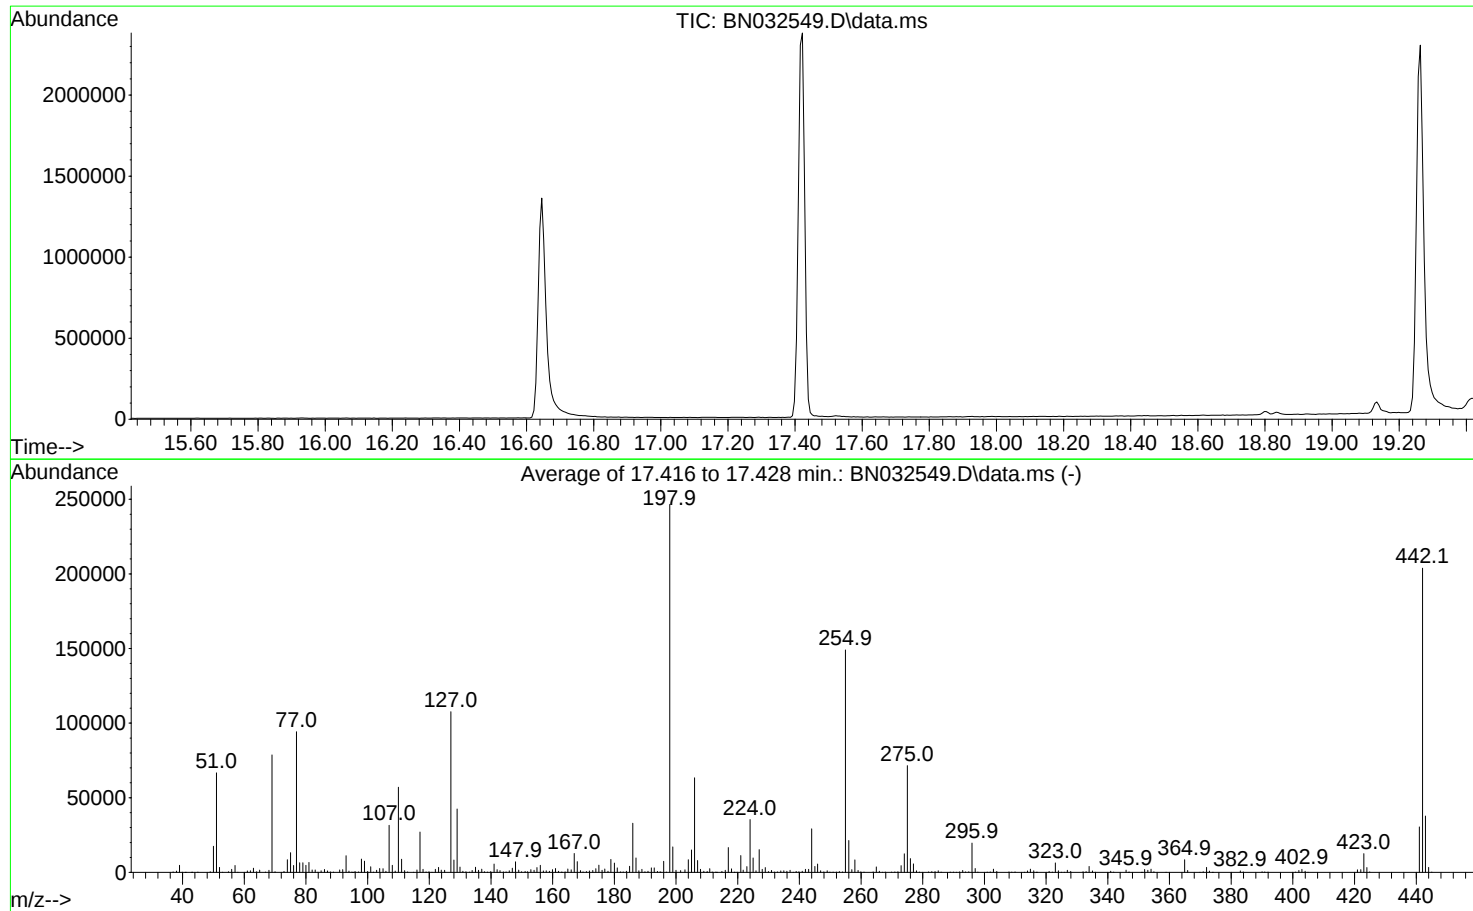




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	66712	PASS
68	69	0.00	2	1.8	1398	PASS
69	198	0.00	100	31.9	78757	PASS
70	69	0.00	2	0.6	434	PASS
127	198	10	80	43.6	107600	PASS
197	198	0.00	2	0.1	253	PASS
198	198	100	100	100.0	246507	PASS
199	198	5	9	6.9	17001	PASS
275	198	10	60	29.0	71517	PASS
365	198	1	100	3.4	8457	PASS
441	198	0.01	100	12.3	30413	PASS
442	442	50	100	100.0	203797	PASS
443	442	15	24	18.5	37701	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070824\
Data File : BN032549.D
Acq On : 08 Jul 2024 10:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 08 11:23:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

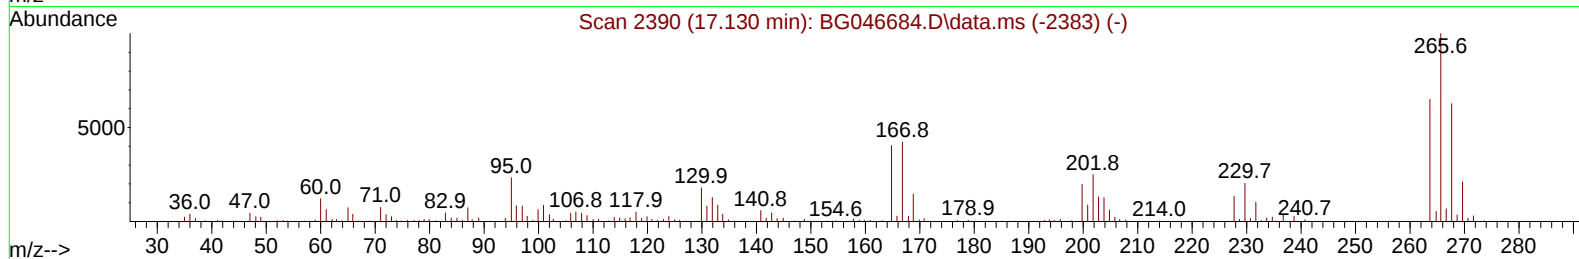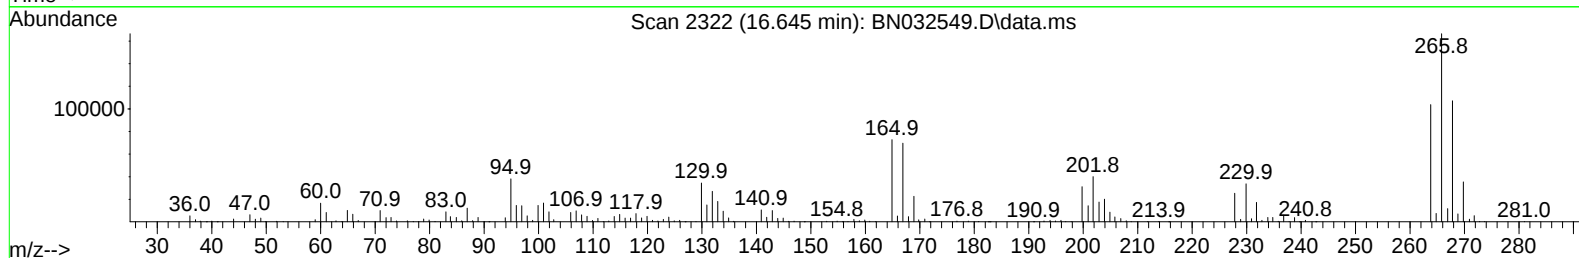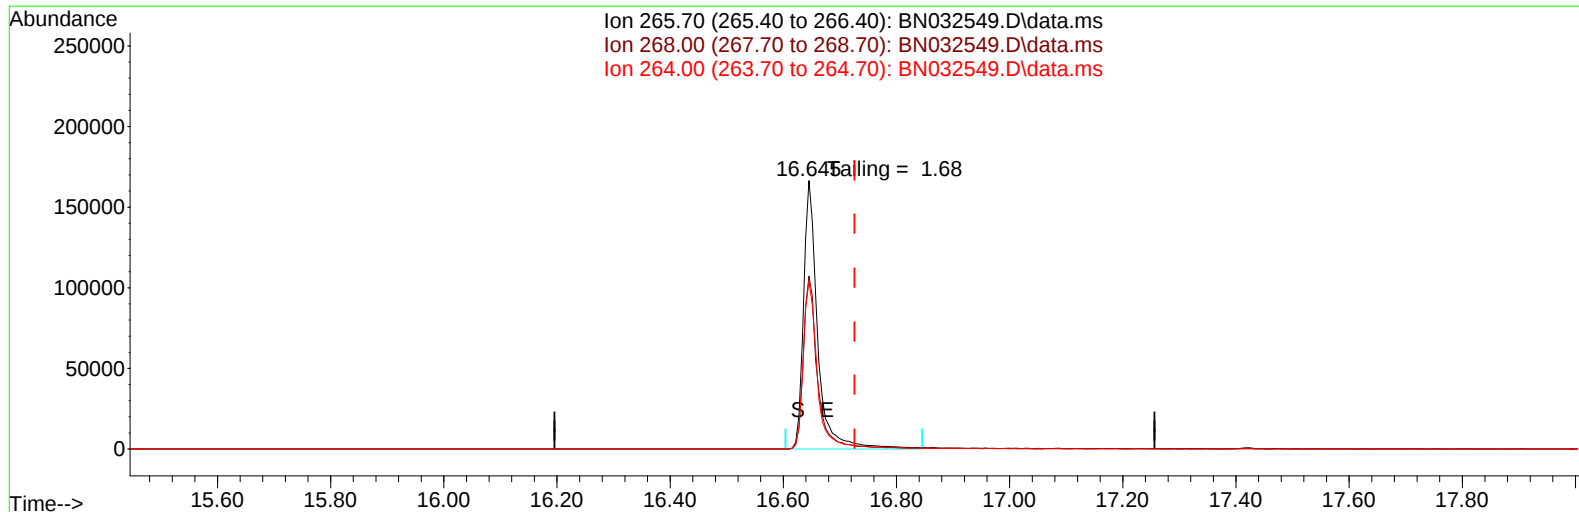

TIC: BN032549.D\data.ms

(70) Pentachlorophenol (C)

16.645min (-0.081) 22525.83 ng




response 290975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.41
264.00	61.60	62.35
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070824\  
Data File : BN032549.D  
Acq On    : 08 Jul 2024  10:04  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 08 11:23:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

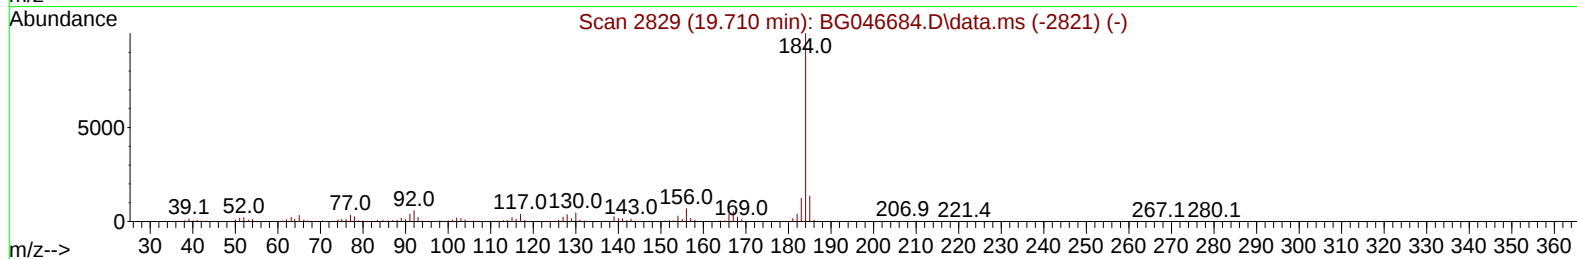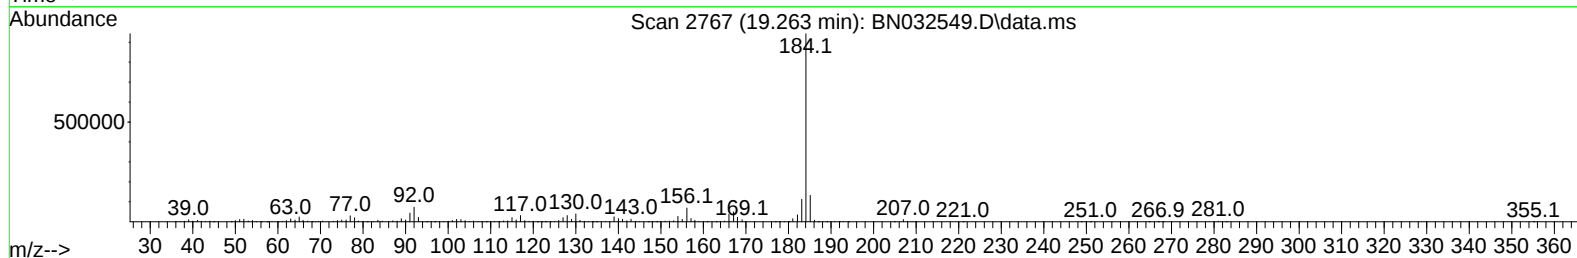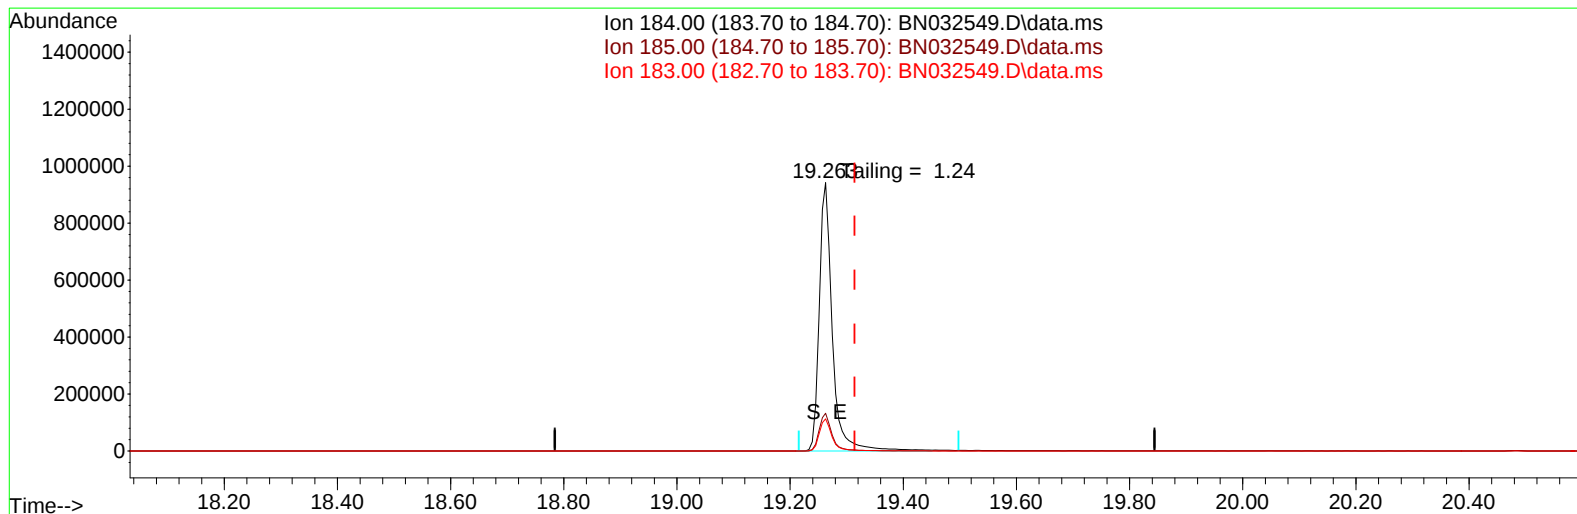

TIC: BN032549.D\data.ms

(77) Benzidine

19.263min (-0.051) 0.00 ng

response **1516228**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/8/2024	BNA_N	<u>BN0325449.D</u>
Compound Name	Response	Retention Time
DDT	397059	20.486
DDD	292723	20.045
DDE	12948	19.527
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
305671	702730	43.50

Instrument :
BNA_N
ClientSampleId :
DFTPP