


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070919\
 Data File : BN006760.D
 Acq On : 09 Jul 2019 08:06
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN070919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 09 13:11:11 2019

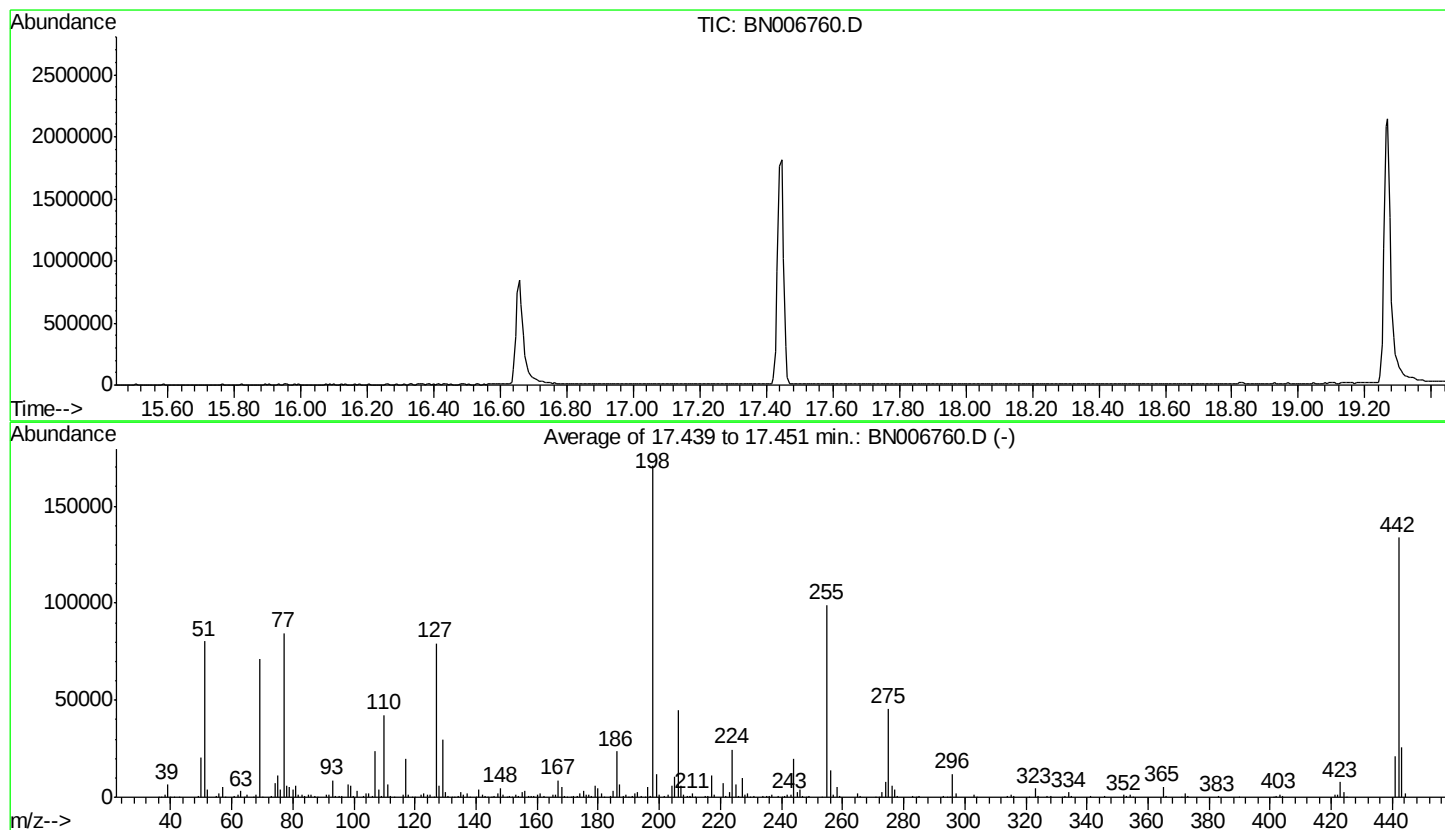

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	80469	PASS
68	69	0.00	2	1.8	1288	PASS
69	198	0.00	100	41.7	71296	PASS
70	69	0.00	2	0.4	298	PASS
127	198	10	80	46.4	79218	PASS
197	198	0.00	2	0.4	761	PASS
198	198	100	100	100.0	170866	PASS
199	198	5	9	6.9	11731	PASS
275	198	10	60	26.8	45842	PASS
365	198	1	100	3.3	5572	PASS
441	198	0.01	100	12.2	20885	PASS
442	198	50	100	78.4	133890	PASS
443	442	15	24	19.1	25573	PASS