

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
 Data File : BN032578.D
 Acq On : 09 Jul 2024 09:13
 Operator : MA/JU
 Sample : P3167-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 09 12:01:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 09 02:39:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.588	152	4525	0.400	ng	0.00
7) Naphthalene-d8	10.368	136	15344	0.400	ng	-0.01
13) Acenaphthene-d10	14.231	164	10209	0.400	ng	0.00
19) Phenanthrene-d10	17.004	188	22934	0.400	ng	0.00
29) Chrysene-d12	21.202	240	18858	0.400	ng	0.00
35) Perylene-d12	23.420	264	17183	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.226	112	919	0.080	ng	0.01
5) Phenol-d6	6.830	99	1088	0.074	ng	0.00
8) Nitrobenzene-d5	8.798	82	2952	0.258	ng	0.00
11) 2-Methylnaphthalene-d10	11.960	152	7486	0.309	ng	-0.02
14) 2,4,6-Tribromophenol	15.762	330	293	0.063	ng	0.00
15) 2-Fluorobiphenyl	12.852	172	11364	0.302	ng	-0.01
27) Fluoranthene-d10	19.035	212	15516	0.260	ng	0.00
31) Terphenyl-d14	19.630	244	14138	0.307	ng	-0.02
Target Compounds						
6) bis(2-Chloroethyl)ether	7.046	93	18	0.088	ng	# 1
12) 2-Methylnaphthalene	12.043	142	569	0.020	ng	# 80
20) 4,6-Dinitro-2-methylph...	15.471	198	4	0.198	ng	# 1
24) Pentachlorophenol	16.693	266	33	0.173	ng	# 57
34) Bis(2-ethylhexyl)phtha...	21.094	149	41558	0.981	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032578.D
Acq On : 09 Jul 2024 09:13
Operator : MA/JU
Sample : P3167-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jul 09 12:01:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 02:39:48 2024
Response via : Initial Calibration

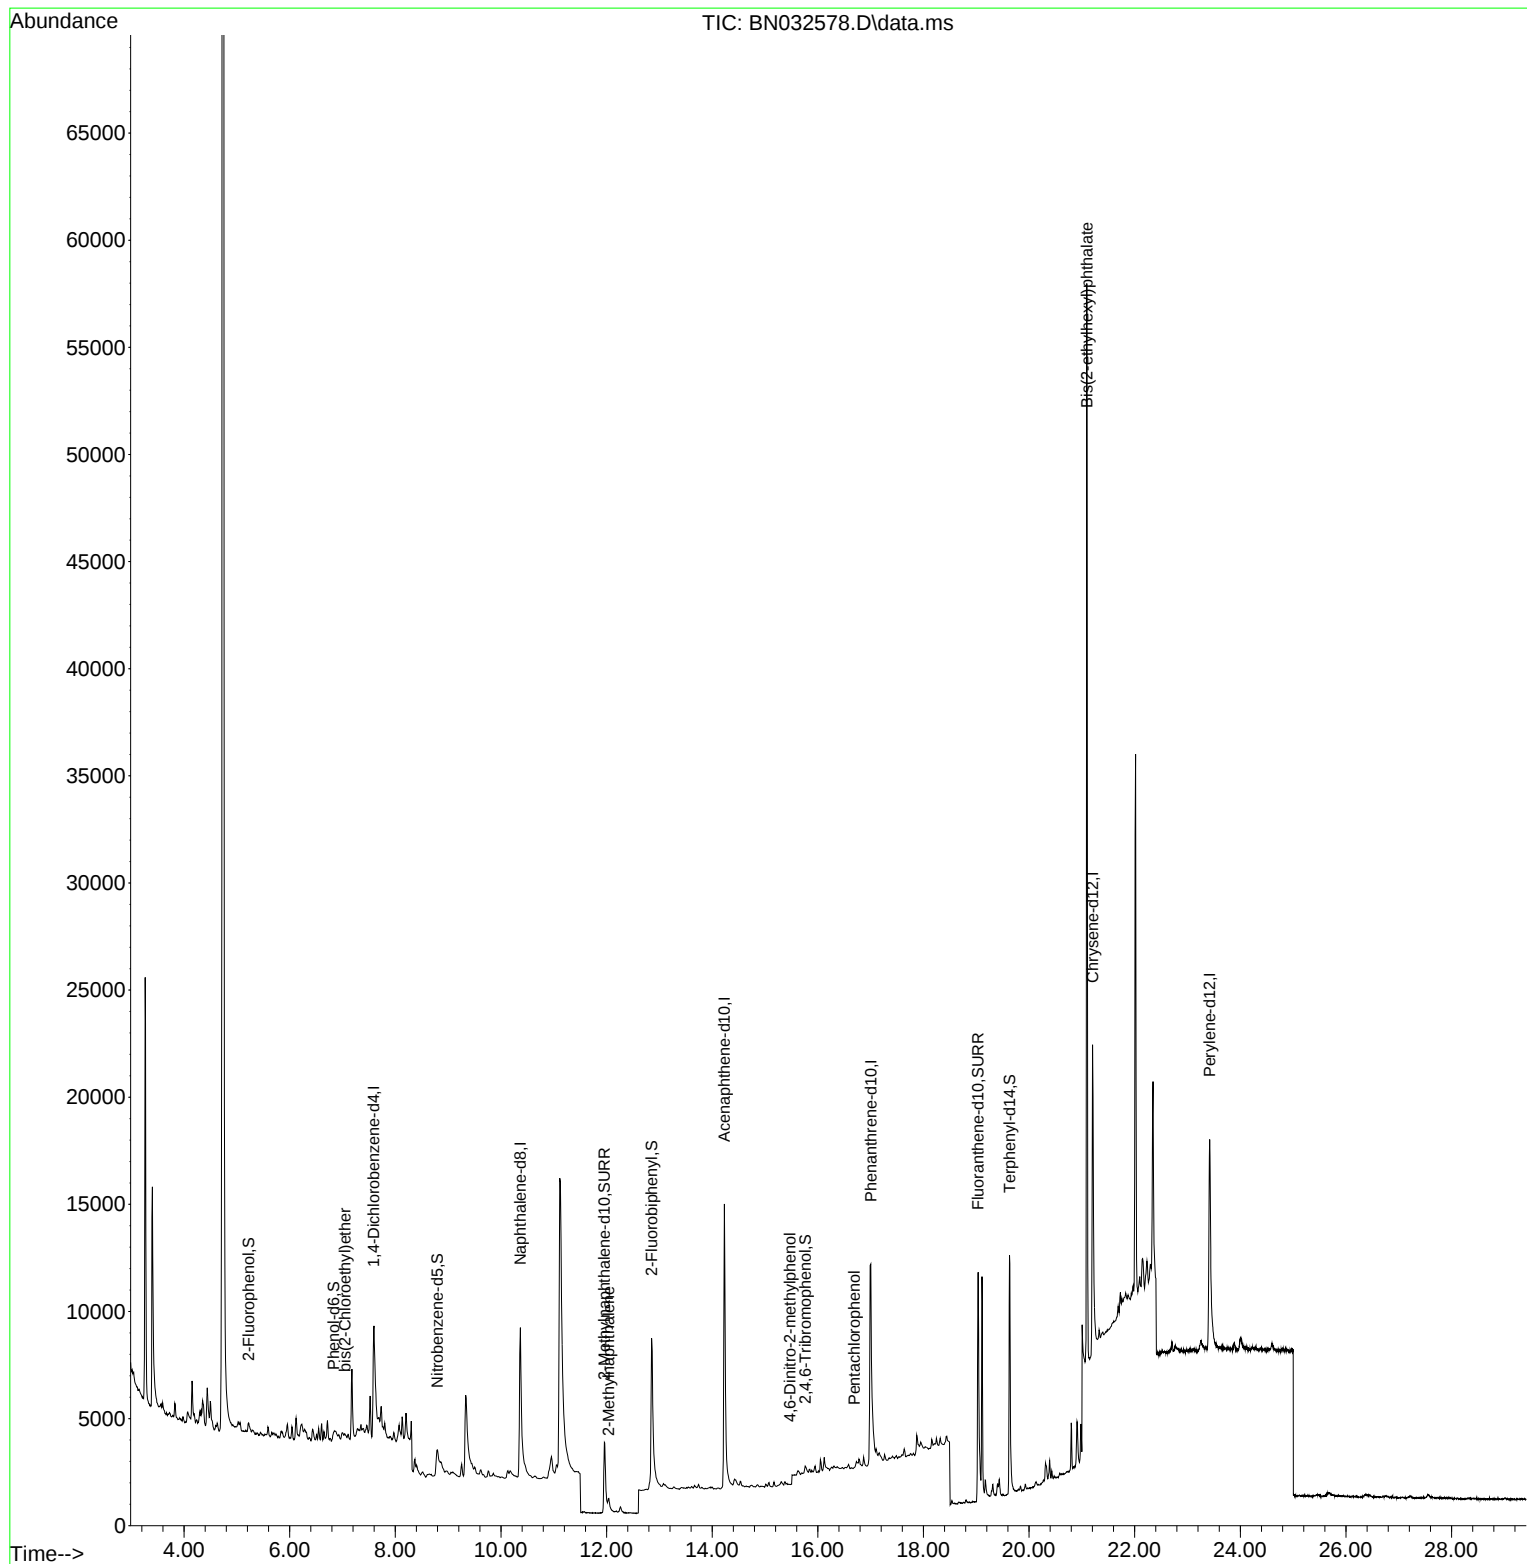






#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.588 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13

Instrument :
BNA_N
ClientSampleId :



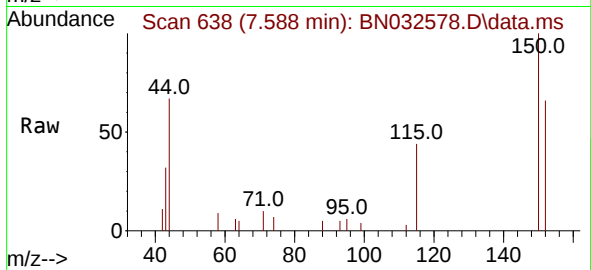



Tgt Ion:152 Resp: 4525
Ion Ratio Lower Upper
152 100
150 151.9 121.6 182.4
115 66.8 53.1 79.7

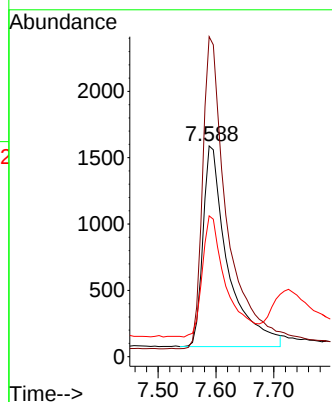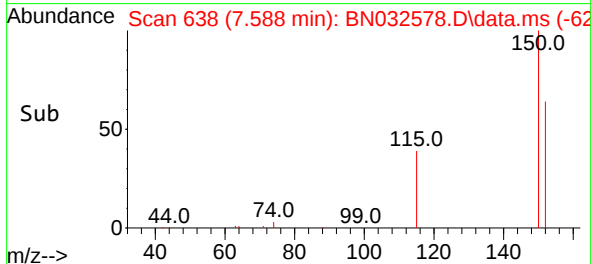

#4
2-Fluorophenol
Concen: 0.080 ng
RT: 5.226 min Scan# 311
Delta R.T. 0.014 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13

Tgt Ion:112 Resp: 919
Ion Ratio Lower Upper
112 100
64 55.6 41.2 61.8
63 26.9 21.6 32.4

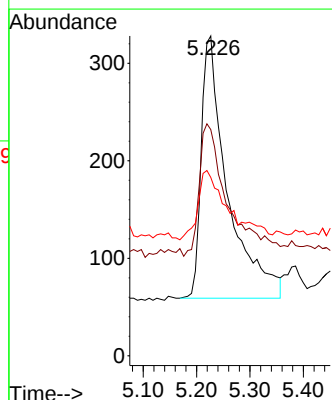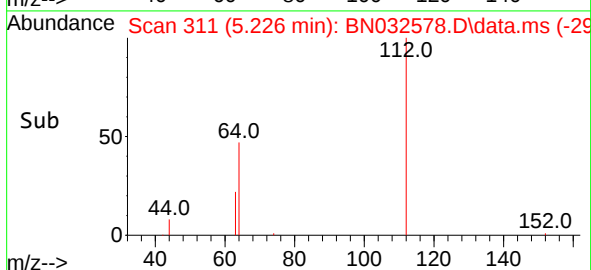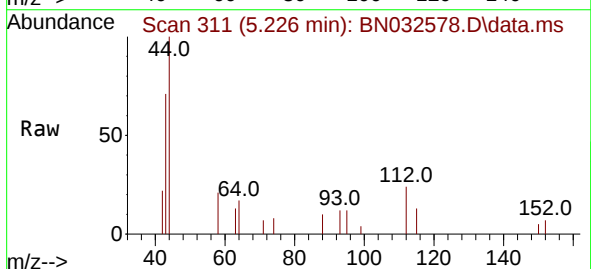

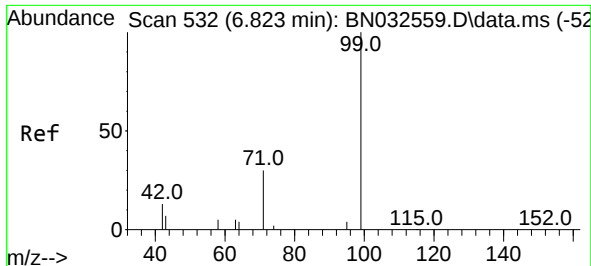

#5

Phenol-d6

Concen: 0.074 ng

RT: 6.830 min Scan# 51

Delta R.T. 0.007 min


Lab File: BN032578.D

Acq: 09 Jul 2024 09:13




Instrument :

BNA_N

ClientSampleId :



Tgt Ion:	99	Resp:	1088
Ion Ratio	Lower	Upper	
99	100		
42	17.3	10.6	16.0#
71	24.2	25.2	37.8#

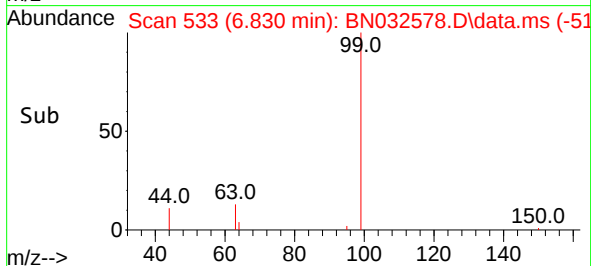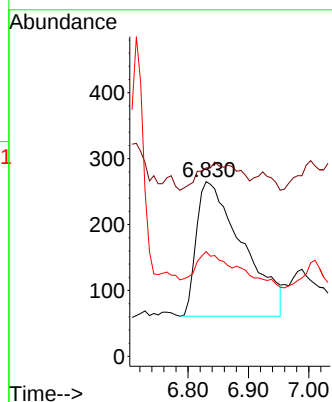

#6

bis(2-Chloroethyl)ether

Concen: 0.088 ng




RT: 7.046 min Scan# 563


Delta R.T. 0.007 min

Lab File: BN032578.D

Acq: 09 Jul 2024 09:13

Tgt Ion:	93	Resp:	18
Ion Ratio	Lower	Upper	
93	100		
63	0.0	54.1	81.1#
95	777.8	30.5	45.7#

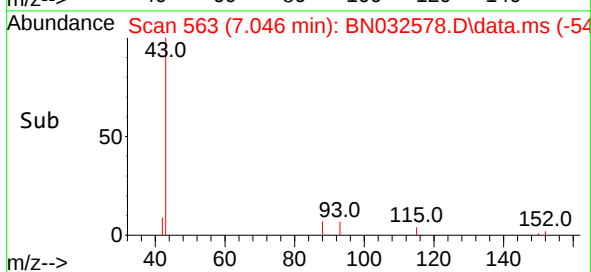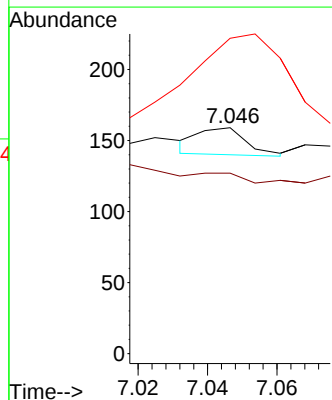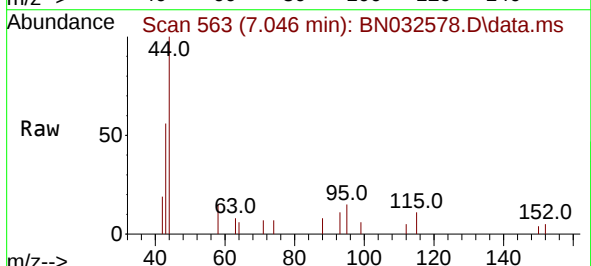



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.368 min Scan# 91

Delta R.T. -0.010 min

Lab File: BN032578.D

Acq: 09 Jul 2024 09:13

Instrument :

BNA_N

ClientSampleId :

Tgt Ion:136 Resp: 15344





Ion Ratio Lower Upper

136 100

137 12.2 10.0 15.0

54 7.7 6.6 9.8

68 7.1 5.8 8.8

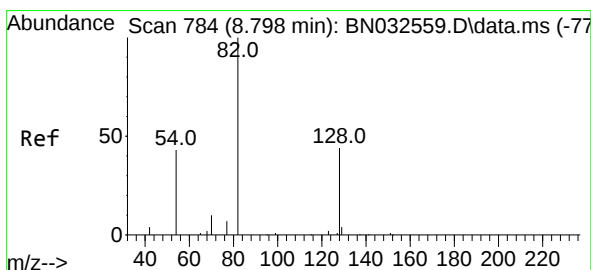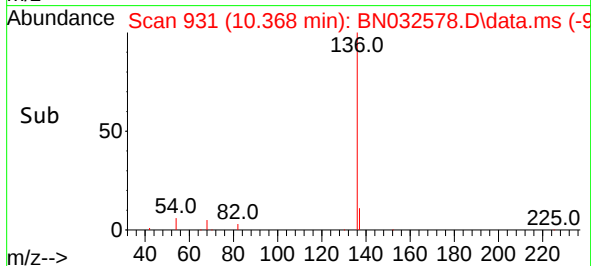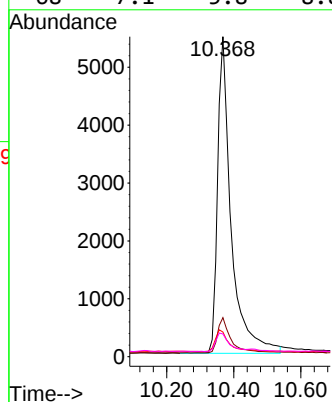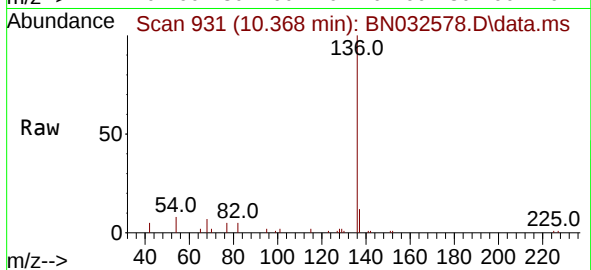

#8

Nitrobenzene-d5

Concen: 0.258 ng

RT: 8.798 min Scan# 784

Delta R.T. -0.000 min

Lab File: BN032578.D

Acq: 09 Jul 2024 09:13




Tgt Ion: 82 Resp: 2952


Ion Ratio Lower Upper

82 100

128 52.8 43.4 65.2

54 51.1 40.2 60.2

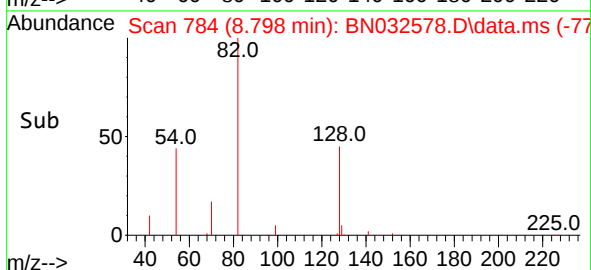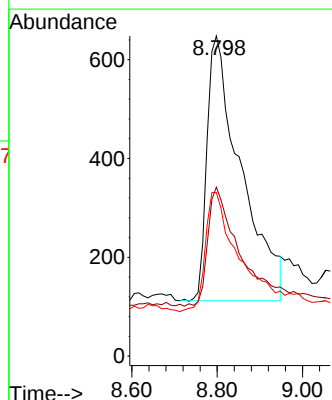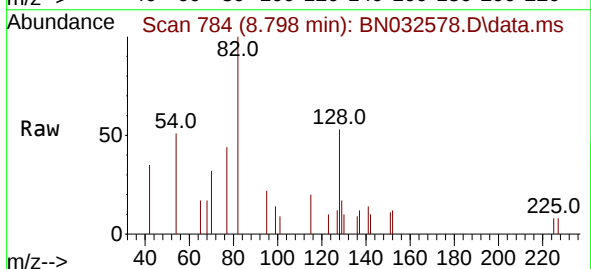

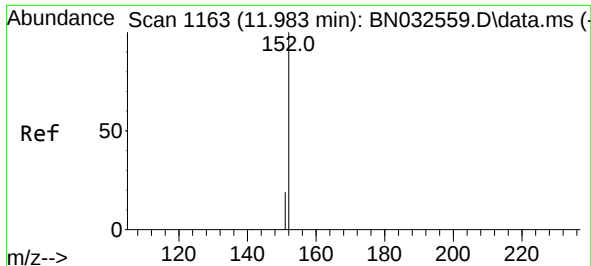

#11

2-Methylnaphthalene-d10

Concen: 0.309 ng

RT: 11.960 min Scan# 1157

Delta R.T. -0.023 min


Lab File: BN032578.D

Acq: 09 Jul 2024 09:13

Instrument :

BNA_N

ClientSampleId :






Tgt Ion:152 Resp: 7486

Ion Ratio Lower Upper

152 100

151 20.0 16.4 24.6

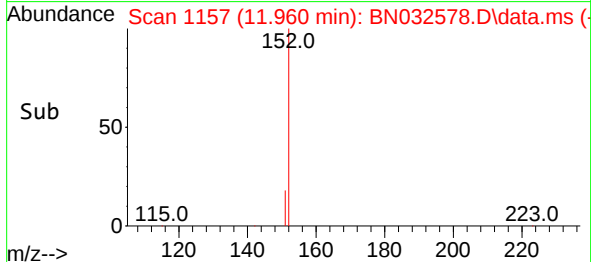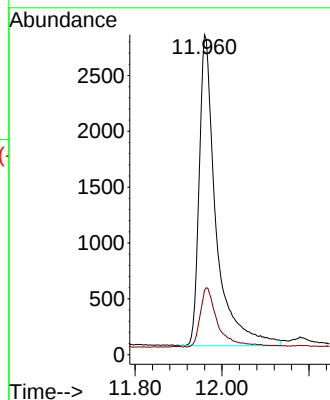

#12

2-Methylnaphthalene

Concen: 0.020 ng

RT: 12.043 min Scan# 1179

Delta R.T. -0.015 min

Lab File: BN032578.D

Acq: 09 Jul 2024 09:13




Tgt Ion:142 Resp: 569


Ion Ratio Lower Upper

142 100

141 93.5 71.0 106.6

115 71.9 30.5 45.7#


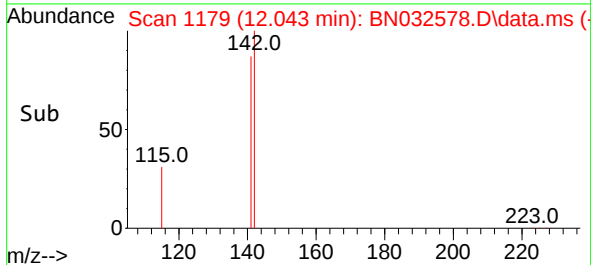
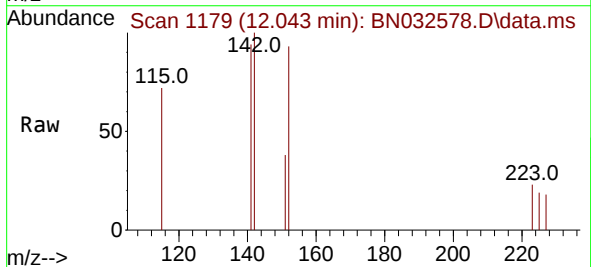
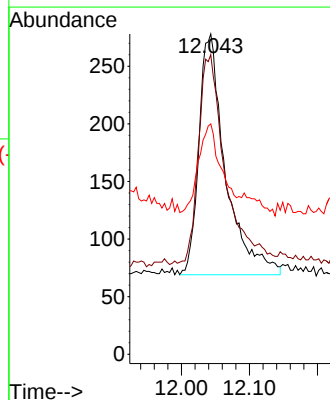


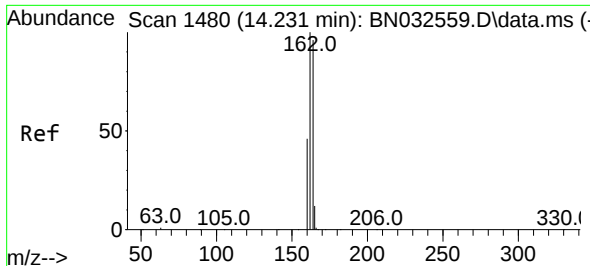

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.231 min Scan# 1480
Delta R.T. -0.000 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:164 Resp: 10209
Ion Ratio Lower Upper
164 100
162 103.9 83.2 124.8
160 48.9 38.6 57.8

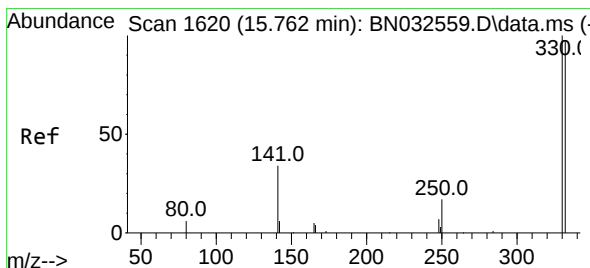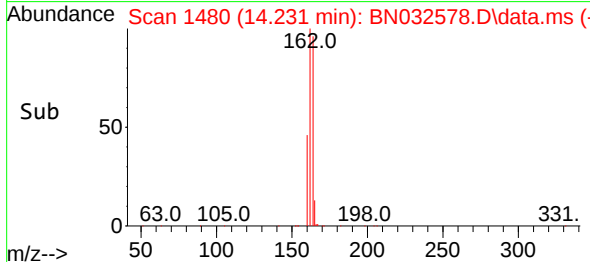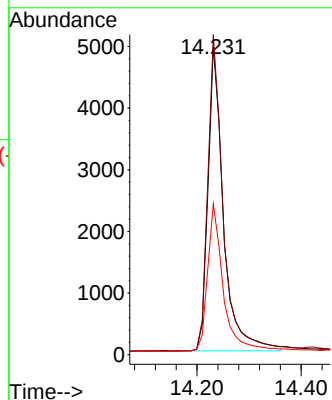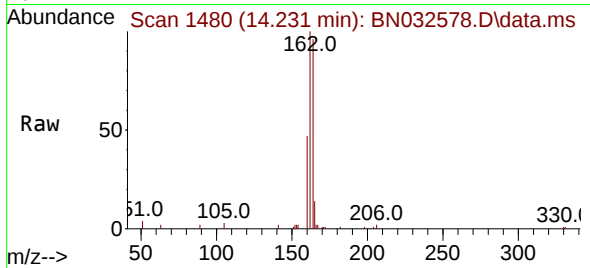

#14
2,4,6-Tribromophenol
Concen: 0.063 ng
RT: 15.762 min Scan# 1620
Delta R.T. -0.000 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13

Tgt Ion:330 Resp: 293
Ion Ratio Lower Upper
330 100
332 96.9 77.7 116.5
141 41.6 31.8 47.8


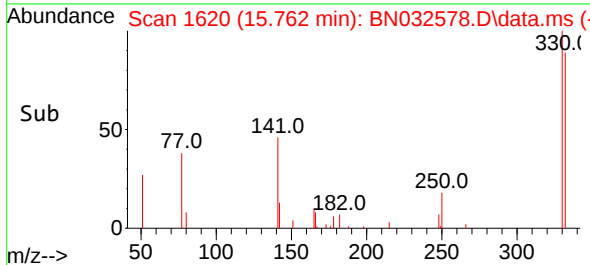
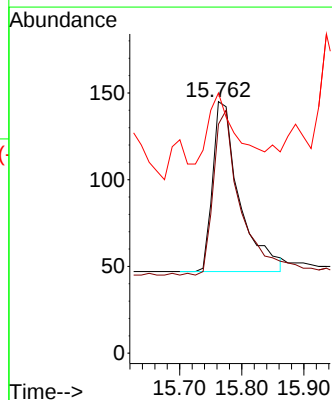
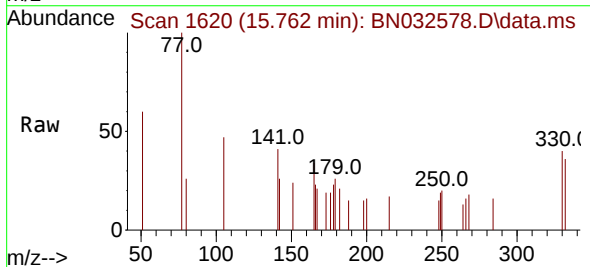


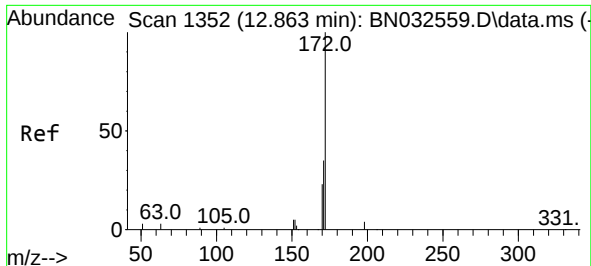

#15
2-Fluorobiphenyl
Concen: 0.302 ng
RT: 12.852 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:172 Resp: 11364
Ion Ratio Lower Upper
172 100
171 35.5 28.5 42.7
170 24.2 19.2 28.8

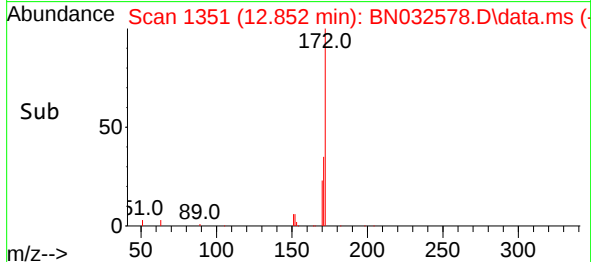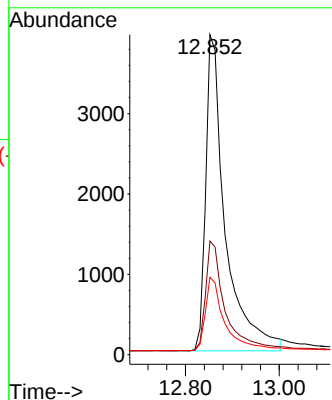

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.004 min Scan# 1720
Delta R.T. -0.000 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13

Tgt Ion:188 Resp: 22934
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.9 7.8 11.6


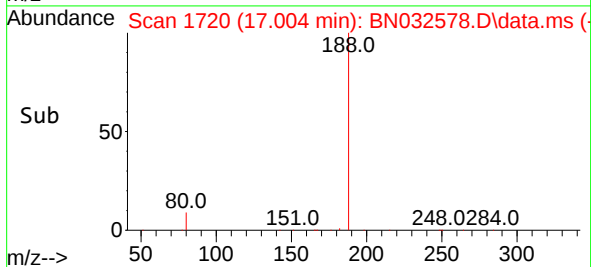
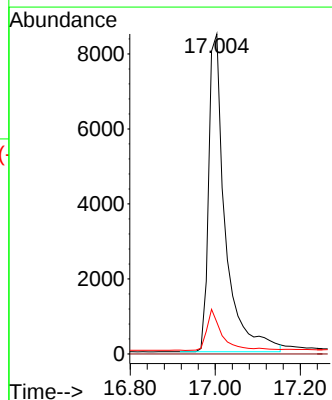
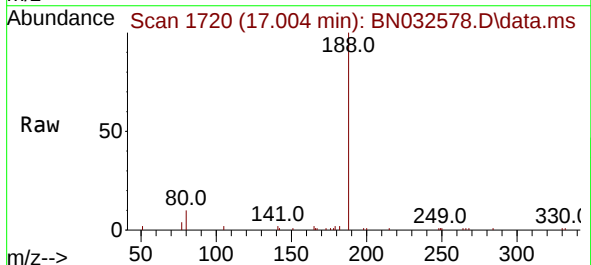


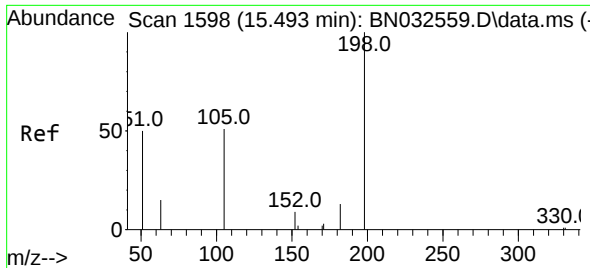

#20
4,6-Dinitro-2-methylphenol
Concen: 0.198 ng
RT: 15.471 min Scan# 1596
Delta R.T. -0.022 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:198 Resp: 4
Ion Ratio Lower Upper
198 100
51 369.8 123.4 185.2#
105 279.2 79.5 119.3#

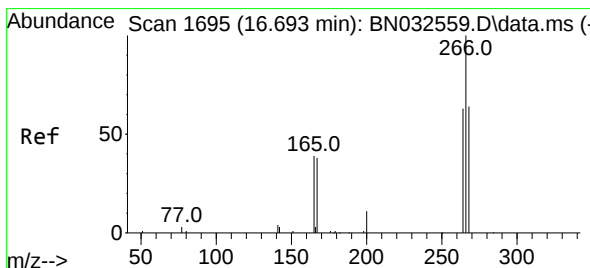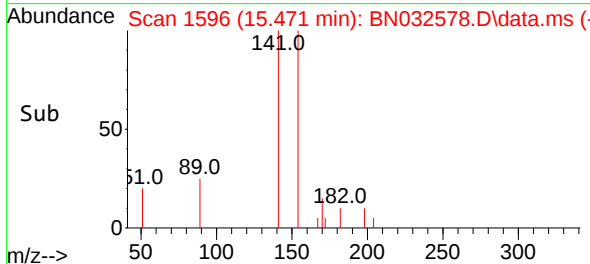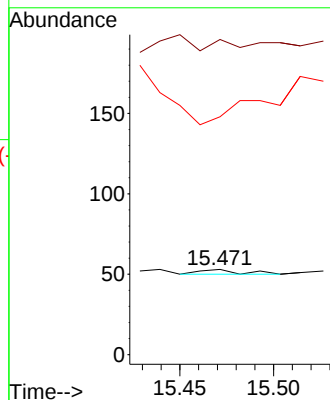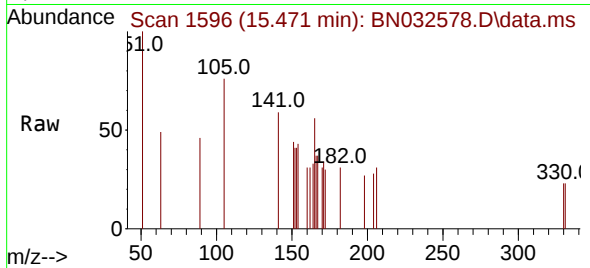

#24
Pentachlorophenol
Concen: 0.173 ng
RT: 16.693 min Scan# 1695
Delta R.T. 0.000 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13


Tgt Ion:266 Resp: 33
Ion Ratio Lower Upper
266 100
264 39.4 49.6 74.4#
268 21.2 52.2 78.2#

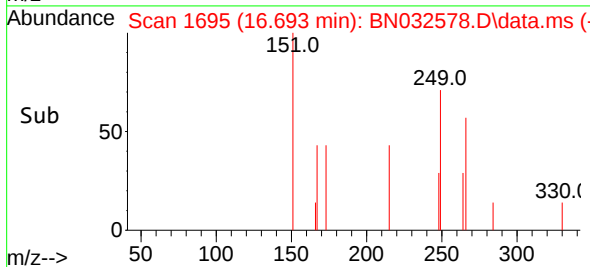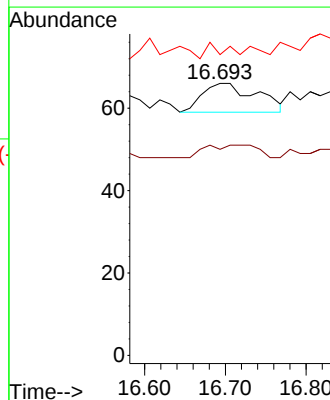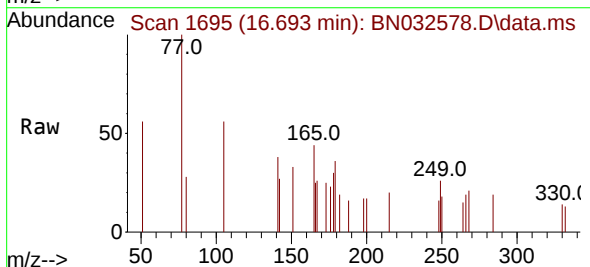






#27
Fluoranthene-d10
Concen: 0.260 ng
RT: 19.035 min Scan# 1955
Delta R.T. -0.009 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13

Instrument :
BNA_N
ClientSampleId :







Tgt Ion:212 Resp: 15516
Ion Ratio Lower Upper
212 100
106 15.2 11.8 17.8
104 8.0 6.9 10.3

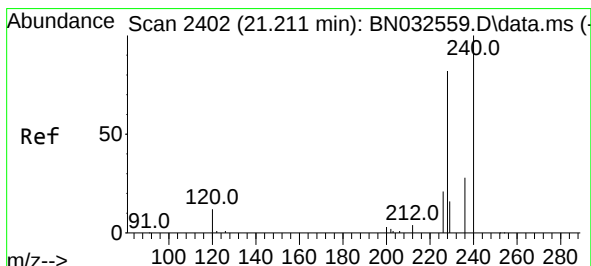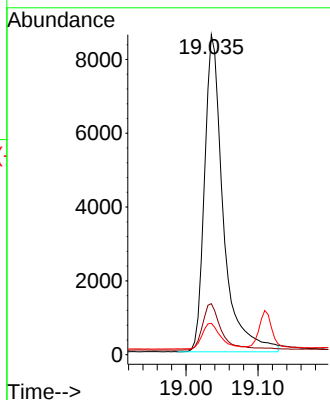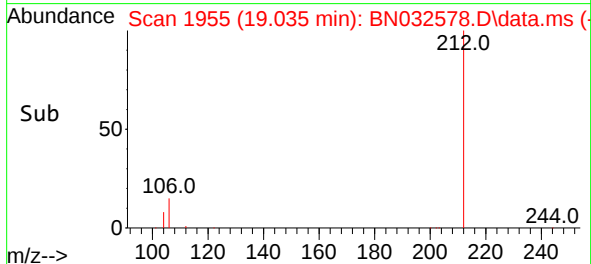

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.202 min Scan# 2401
Delta R.T. -0.009 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13


Tgt Ion:240 Resp: 18858
Ion Ratio Lower Upper
240 100
120 18.6 13.0 19.4
236 29.0 23.1 34.7

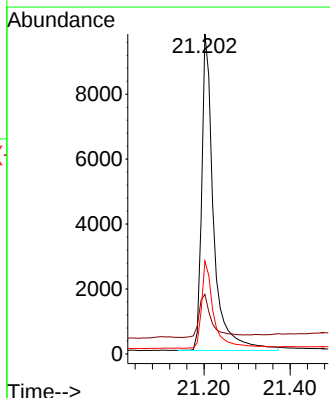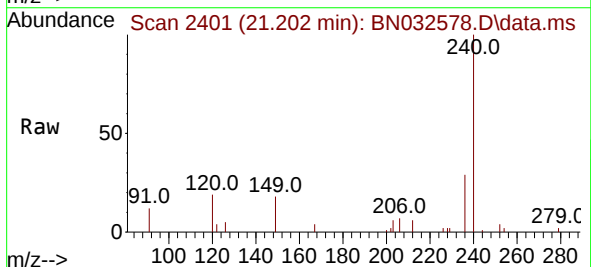






#31
Terphenyl-d14
Concen: 0.307 ng
RT: 19.630 min Scan# 2083
Delta R.T. -0.019 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13

Instrument :
BNA_N
ClientSampleId :



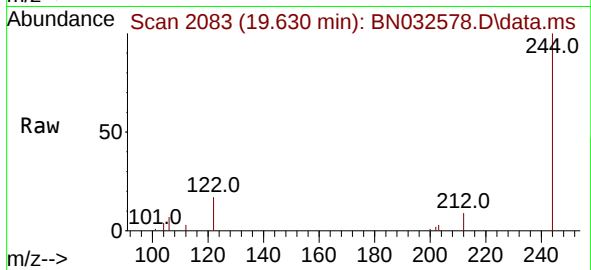



Tgt Ion:244 Resp: 14138
Ion Ratio Lower Upper
244 100
212 9.2 7.2 10.8
122 16.9 12.1 18.1

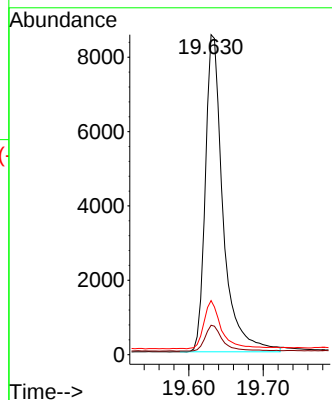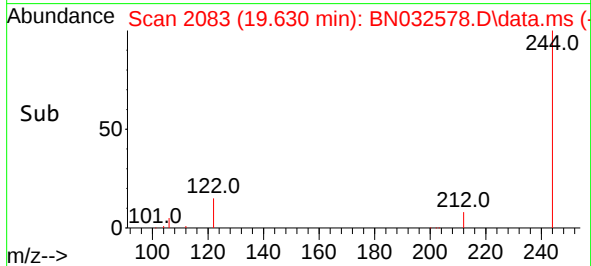

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.981 ng
RT: 21.094 min Scan# 2389
Delta R.T. -0.009 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13


Tgt Ion:149 Resp: 41558
Ion Ratio Lower Upper
149 100
167 28.1 21.6 32.4
279 3.6 3.0 4.6

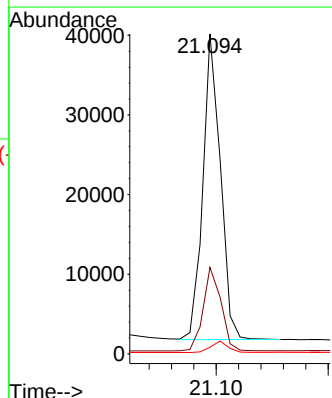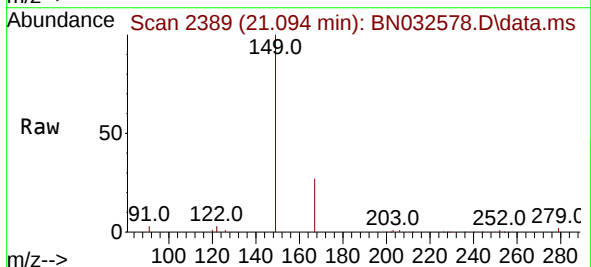

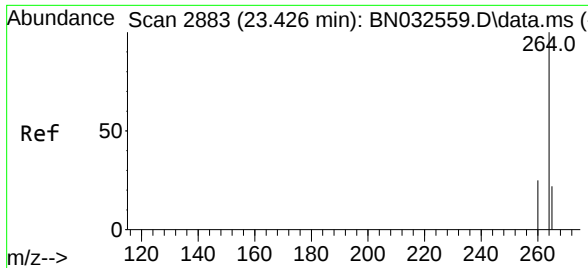

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.420 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN032578.D
Acq: 09 Jul 2024 09:13

Instrument :
BNA_N
ClientSampleId :

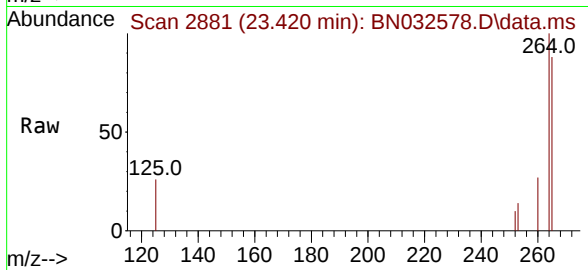

Tgt Ion:264 Resp: 17183
Ion Ratio Lower Upper
264 100
260 26.7 21.0 31.6
265 88.0 76.6 115.0

