
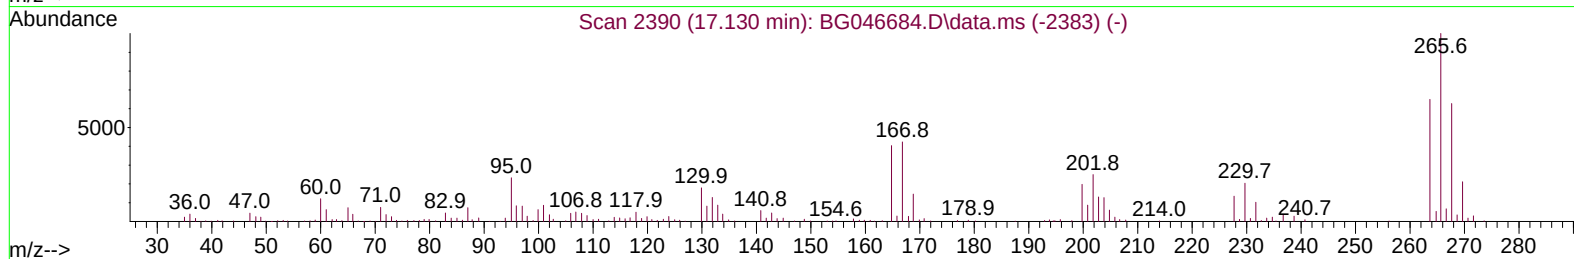
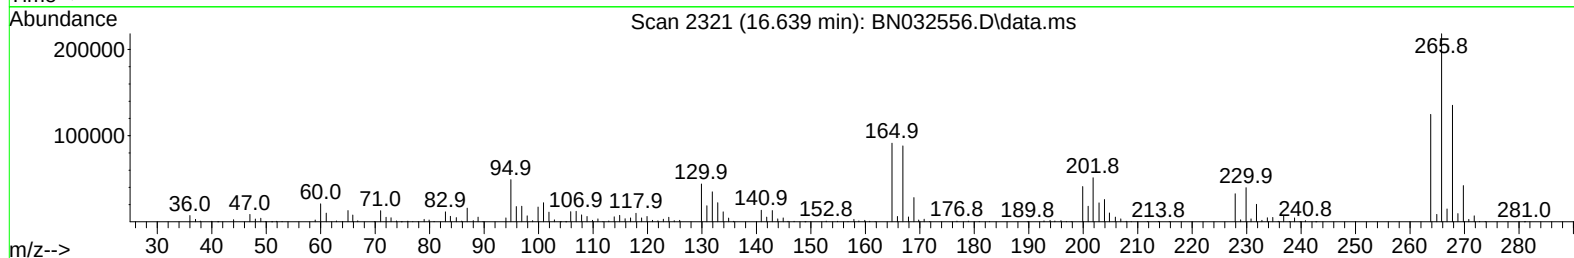


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032556.D
Acq On : 08 Jul 2024 18:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jul 09 03:02:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

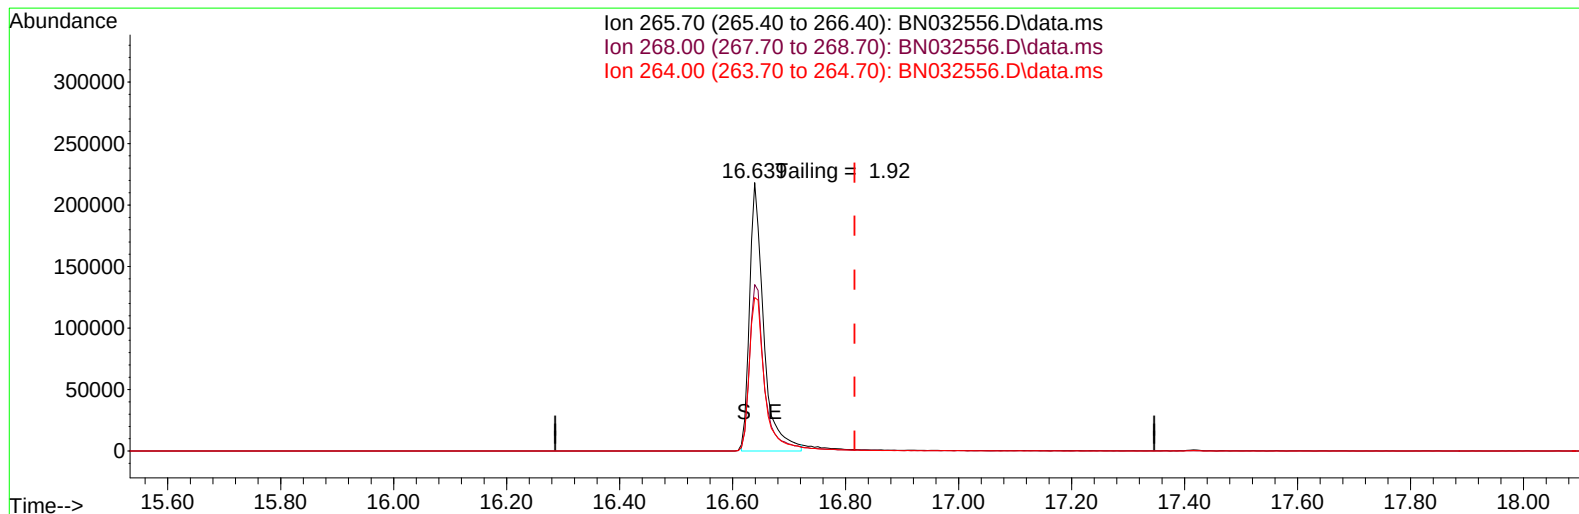

TIC: BN032556.D\data.ms

(70) Pentachlorophenol (C)




16.639min (-0.177) 24262.73 ng

response 396429

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.02
264.00	61.60	57.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032556.D
Acq On : 08 Jul 2024 18:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jul 09 03:02:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

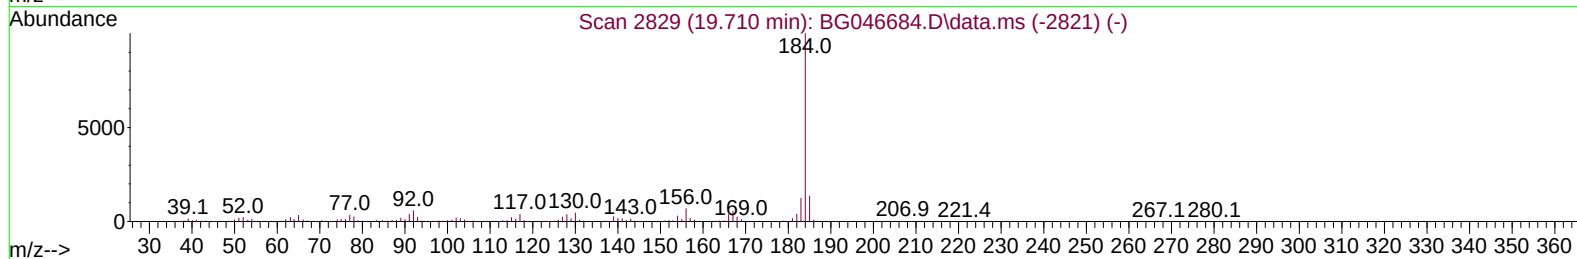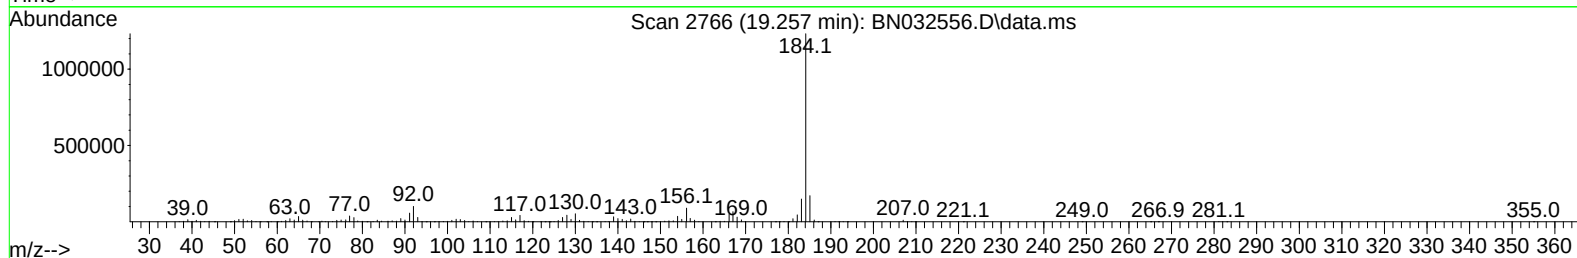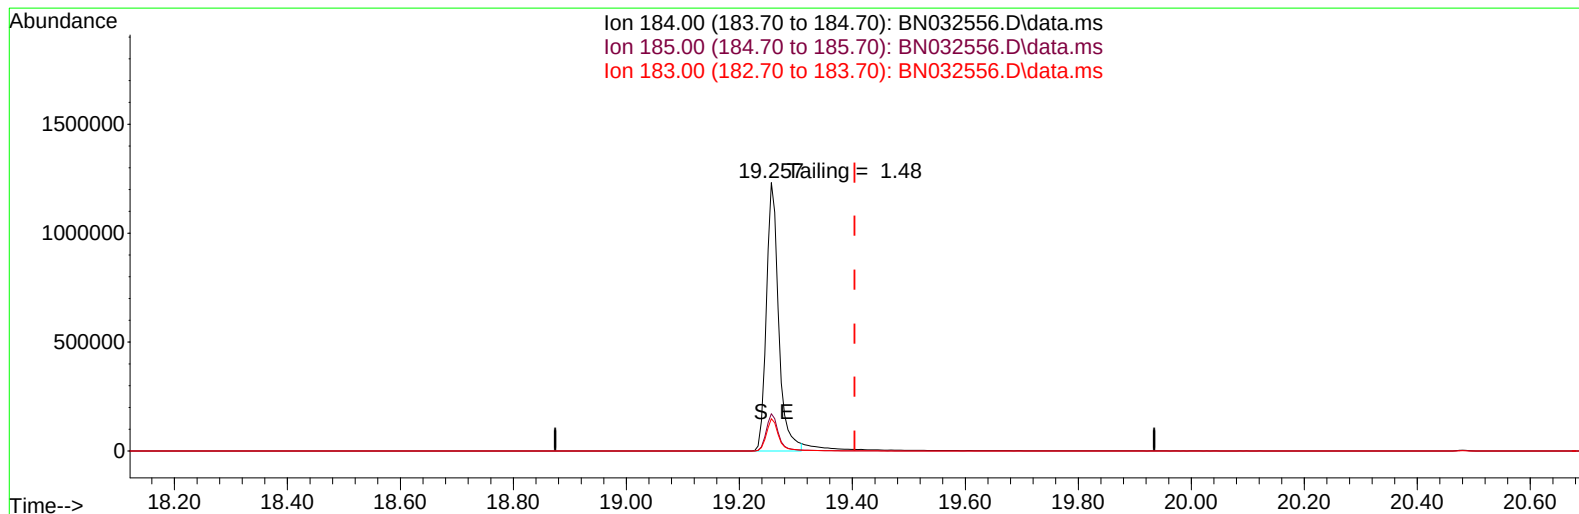

TIC: BN032556.D\data.ms

(77) Benzidine

19.257min (-0.147) 0.00 ng

response 1975287

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	12.06
0.00	0.00	0.00