

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
 Data File : BN032580.D
 Acq On : 09 Jul 2024 10:25
 Operator : MA/JU
 Sample : P3167-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 VPB196-HYD-20240703

Quant Time: Jul 09 12:02:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 09 02:39:48 2024
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/10/2024
 Supervised By :mohammad ahmed 07/11/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.588	152	4318	0.400	ng	0.00
7) Naphthalene-d8	10.389	136	13228	0.400	ng	0.01
13) Acenaphthene-d10	14.242	164	10062	0.400	ng	0.01
19) Phenanthrene-d10	17.016	188	22246	0.400	ng	0.01
29) Chrysene-d12	21.211	240	17711	0.400	ng	# 0.00
35) Perylene-d12	23.431	264	10573	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.227	112	551	0.050	ng	0.01
5) Phenol-d6	6.801	99	115	0.008	ng	-0.02
8) Nitrobenzene-d5	8.830	82	3395m	0.344	ng	0.03
11) 2-Methylnaphthalene-d10	11.990	152	74	0.004	ng	0.00
14) 2,4,6-Tribromophenol	15.775	330	1237	0.271	ng	0.01
15) 2-Fluorobiphenyl	12.874	172	11279	0.304	ng	0.01
27) Fluoranthene-d10	19.045	212	11867	0.205	ng	0.00
31) Terphenyl-d14	19.635	244	19398	0.449	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.161	88	425	0.075	ng	# 75
34) Bis(2-ethylhexyl)phtha...	21.095	149	2125	0.053	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032580.D
Acq On : 09 Jul 2024 10:25
Operator : MA/JU
Sample : P3167-08
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
VPB196-HYD-20240703

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024


Quant Time: Jul 09 12:02:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 02:39:48 2024
Response via : Initial Calibration

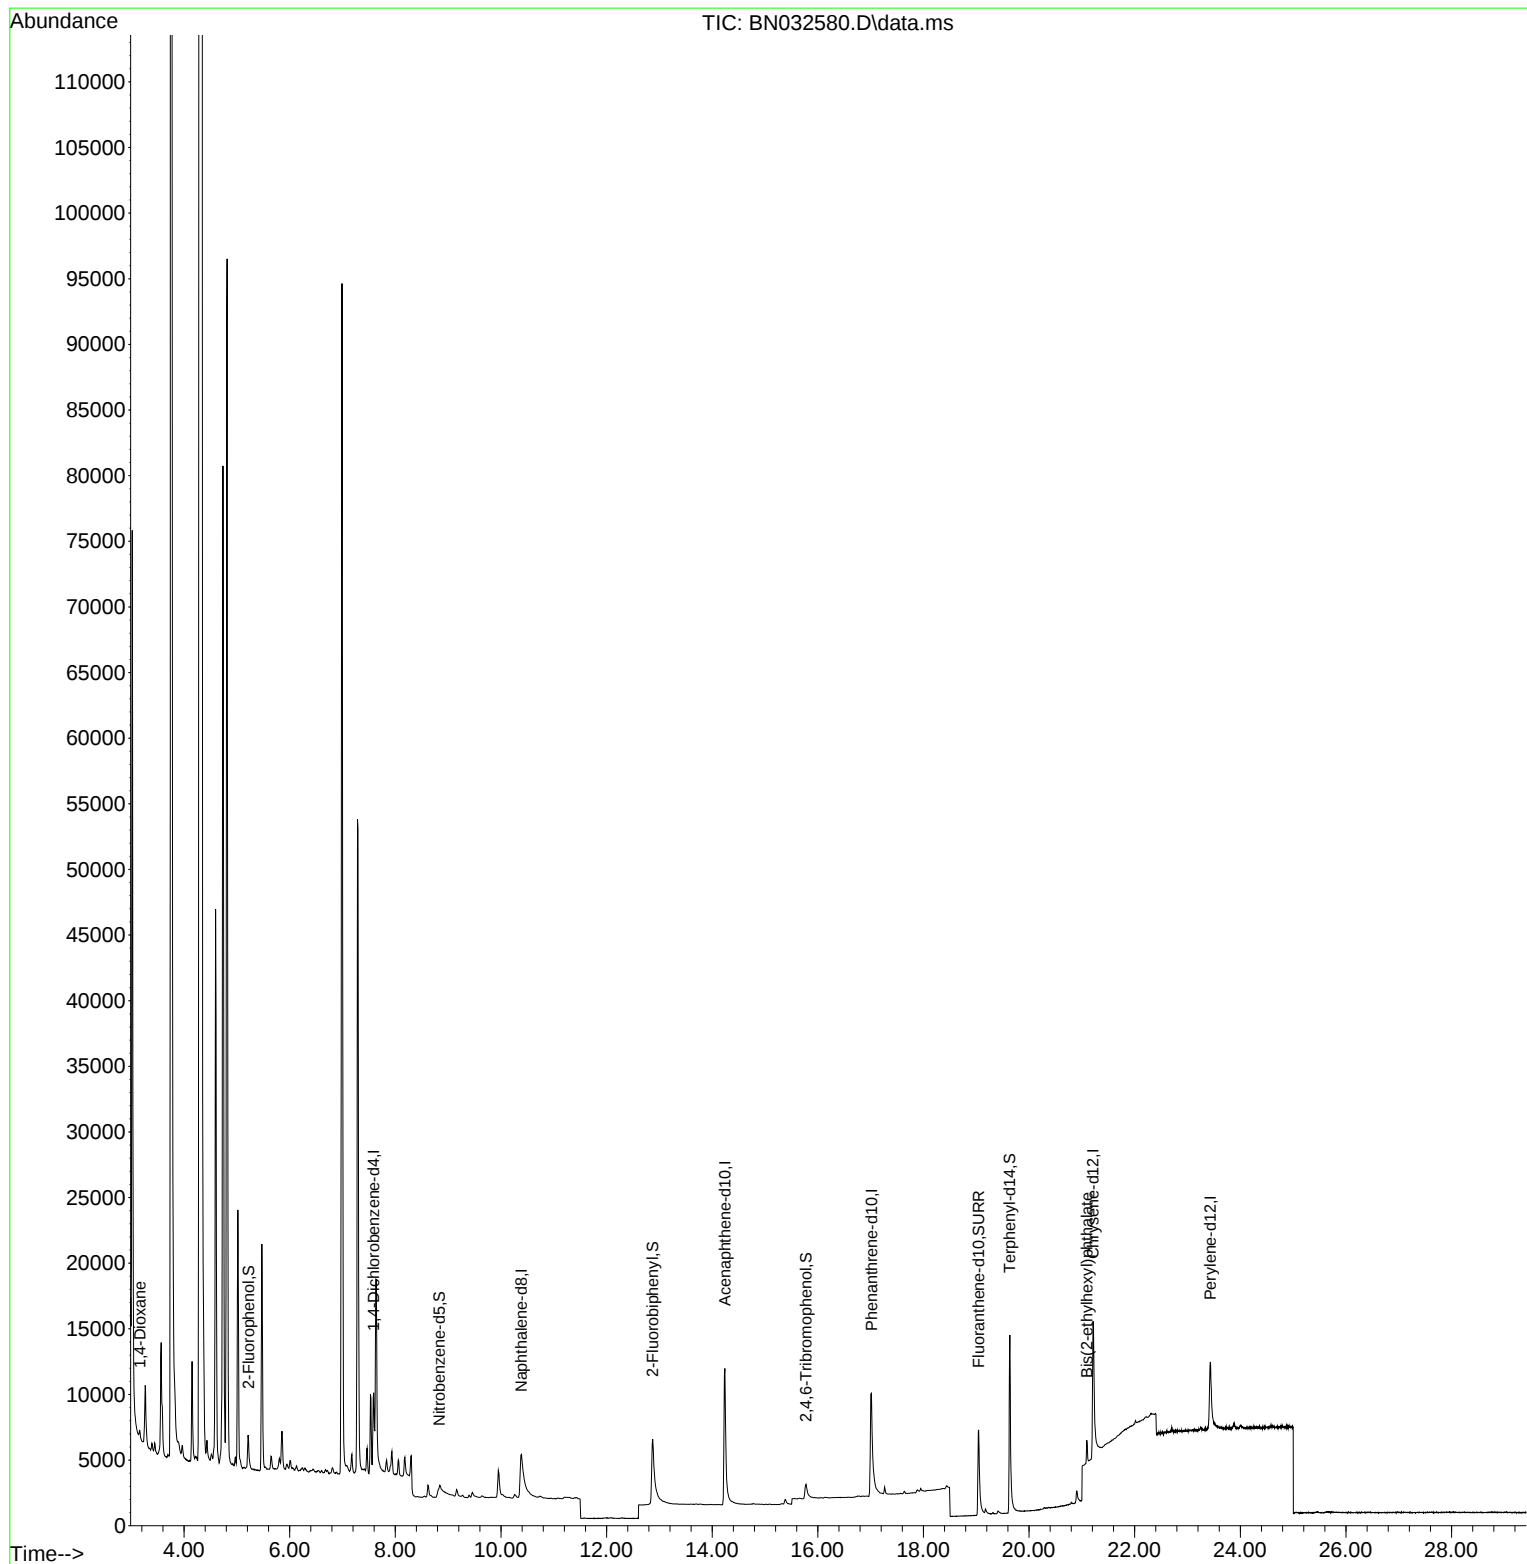



#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.588 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN032580.D
 Acq: 09 Jul 2024 10:25




Instrument :
 BNA_N
 ClientSampleId :
 VPB196-HYD-20240703



Tgt Ion:152 Resp: 4318
 Ion Ratio Lower Upper
 152 100
 150 152.0 121.6 182.4
 115 70.5 53.1 79.7




Manual Integrations
 APPROVED


Reviewed By :Jagrut Upadhyay 07/10/2024
 Supervised By :mohammad ahmed 07/11/2024

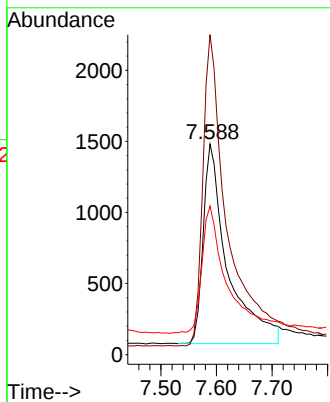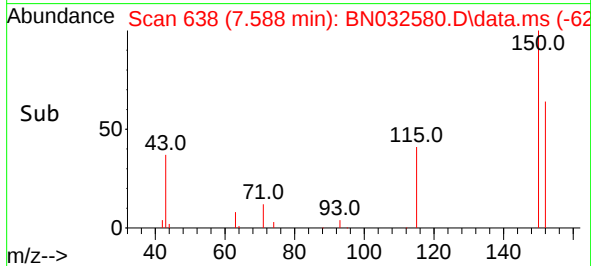

#2
 1,4-Dioxane
 Concen: 0.075 ng
 RT: 3.161 min Scan# 25
 Delta R.T. 0.000 min
 Lab File: BN032580.D
 Acq: 09 Jul 2024 10:25

Tgt Ion: 88 Resp: 425
 Ion Ratio Lower Upper
 88 100
 43 0.0 20.4 30.6#
 58 75.8 51.0 76.6

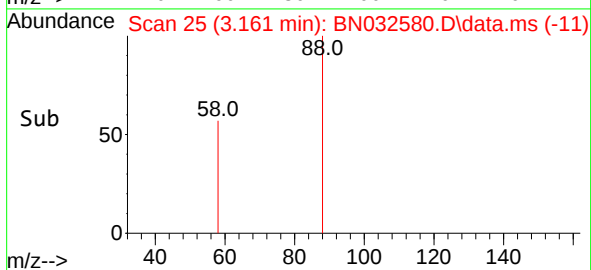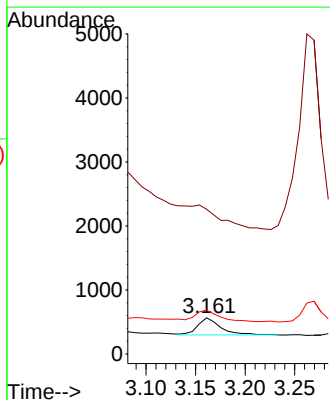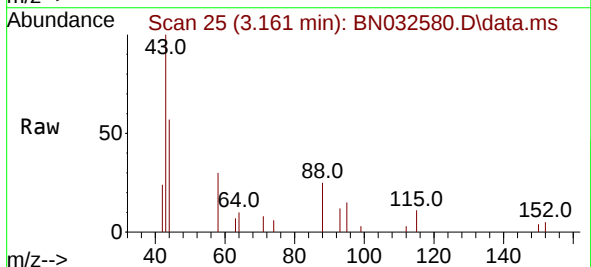







#4
2-Fluorophenol
Concen: 0.050 ng
RT: 5.227 min Scan# 311
Delta R.T. 0.015 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25

Instrument :
BNA_N
ClientSampleId :
VPB196-HYD-20240703

Tgt Ion:112 Resp: 55
Ion Ratio Lower Upper
112 100
64 48.8 41.2 61.8
63 29.0 21.6 32.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

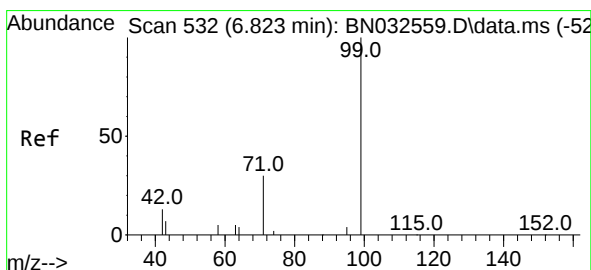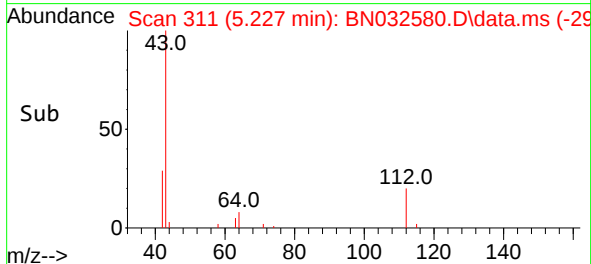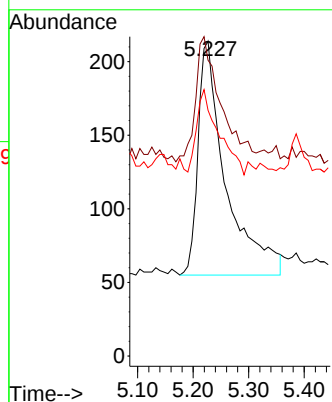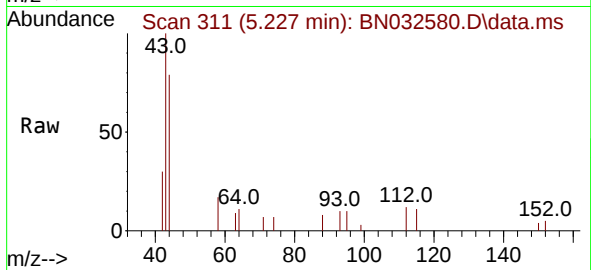

#5
Phenol-d6
Concen: 0.008 ng
RT: 6.801 min Scan# 529
Delta R.T. -0.022 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25


Tgt Ion: 99 Resp: 115
Ion Ratio Lower Upper
99 100
42 0.0 10.6 16.0#
71 0.0 25.2 37.8#

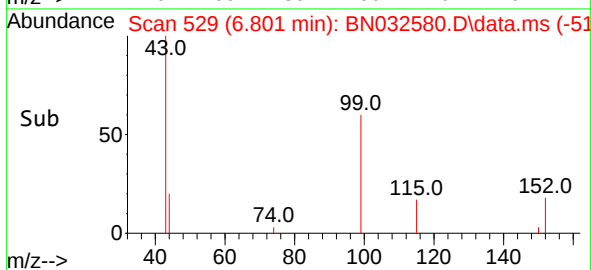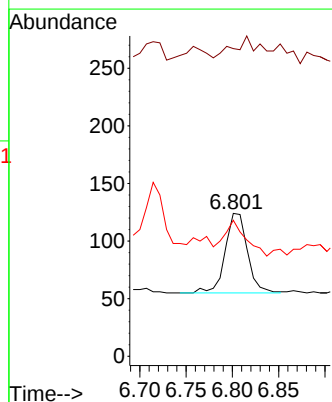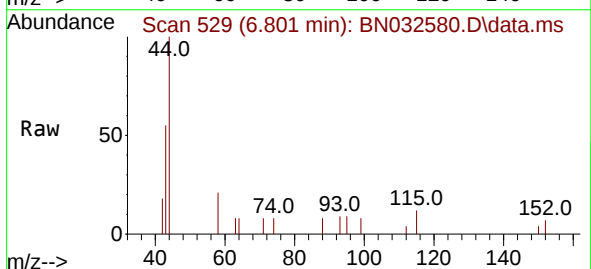

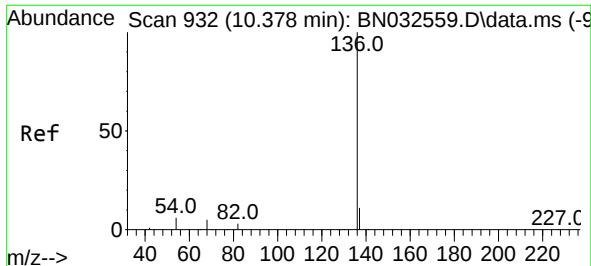

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.389 min Scan# 911
Delta R.T. 0.011 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25




Instrument :
BNA_N
ClientSampleId :
VPB196-HYD-20240703



Tgt Ion:136 Resp: 13228
Ion Ratio Lower Upper
136 100
137 13.7 10.0 15.0
54 9.6 6.6 9.8
68 8.6 5.8 8.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

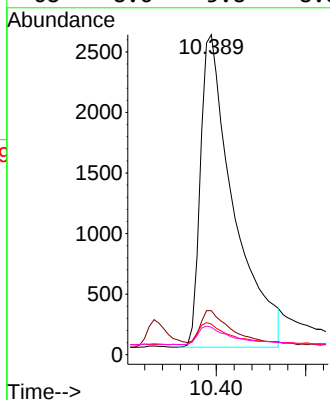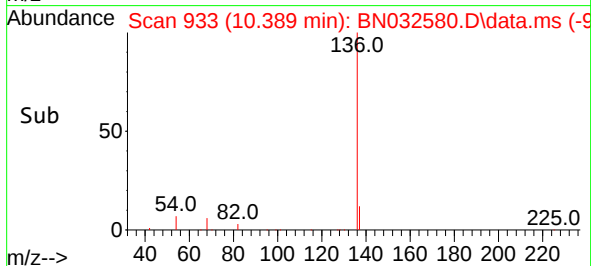

#8
Nitrobenzene-d5
Concen: 0.344 ng m
RT: 8.830 min Scan# 787
Delta R.T. 0.032 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25


Tgt Ion: 82 Resp: 3395
Ion Ratio Lower Upper
82 100
128 57.3 43.4 65.2
54 53.5 40.2 60.2

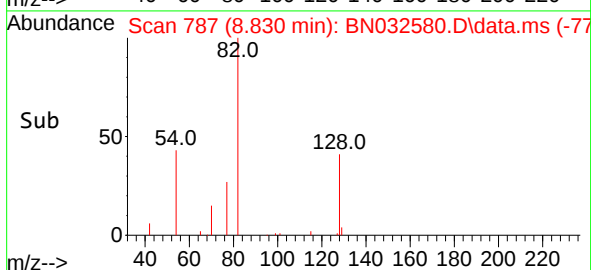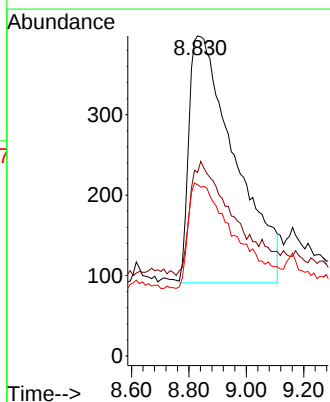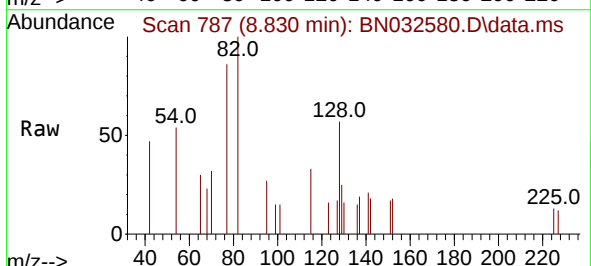

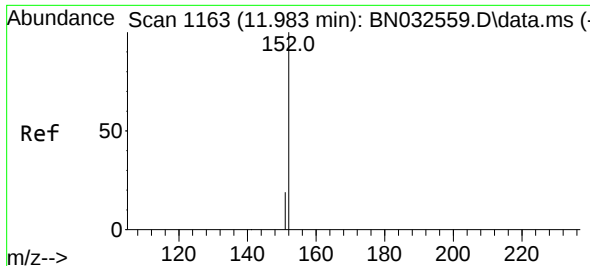

#11
2-Methylnaphthalene-d10
Concen: 0.004 ng
RT: 11.990 min Scan# 1165
Delta R.T. 0.008 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25




Instrument :
BNA_N
ClientSampleId :
VPB196-HYD-20240703

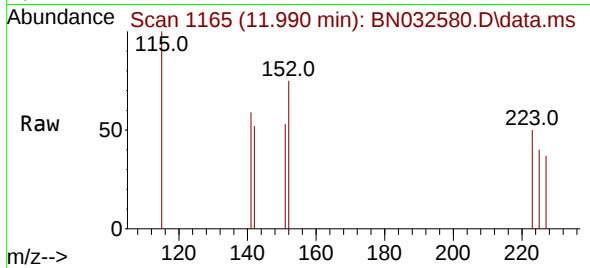


Tgt Ion:152 Resp: 74
Ion Ratio Lower Upper
152 100
151 5.4 16.4 24.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

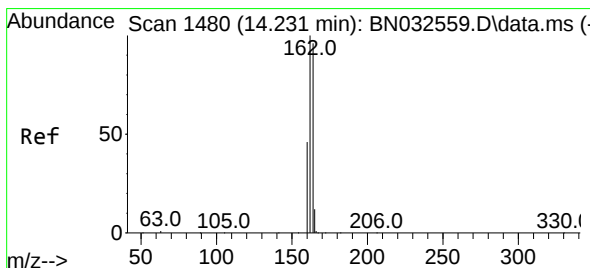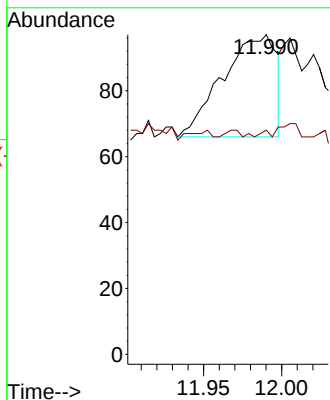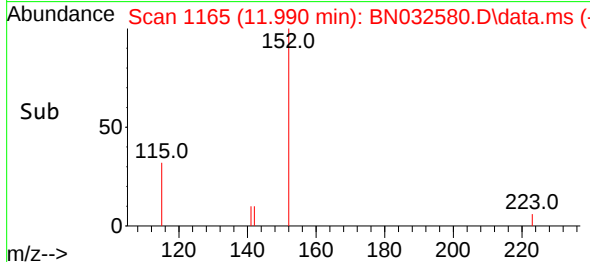


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.242 min Scan# 1481
Delta R.T. 0.011 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25

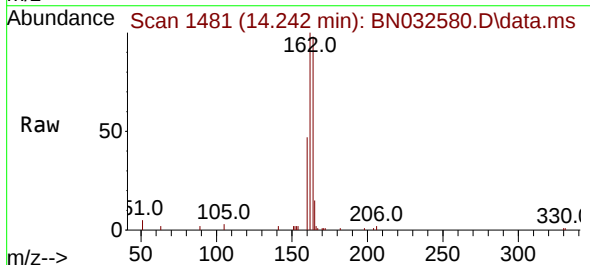


Tgt Ion:164 Resp: 10062
Ion Ratio Lower Upper
164 100
162 101.9 83.2 124.8
160 47.6 38.6 57.8

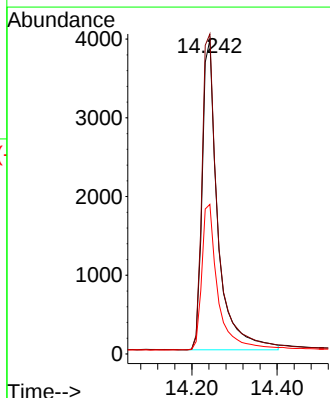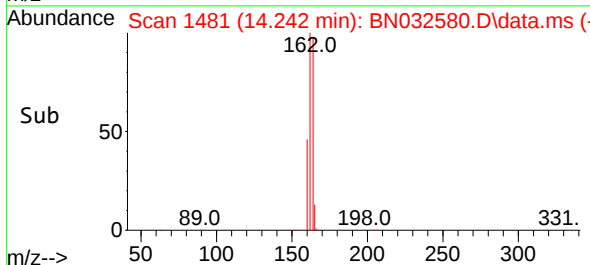

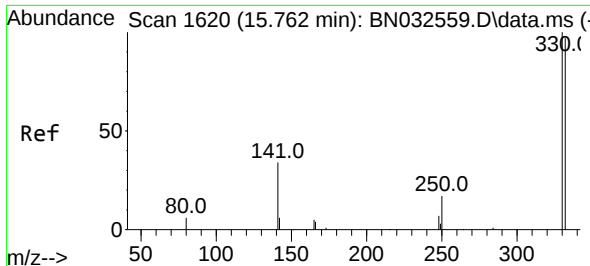

#14
2,4,6-Tribromophenol
Concen: 0.271 ng
RT: 15.775 min Scan# 1621
Delta R.T. 0.013 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25




Instrument :
BNA_N
ClientSampleId :
VPB196-HYD-20240703

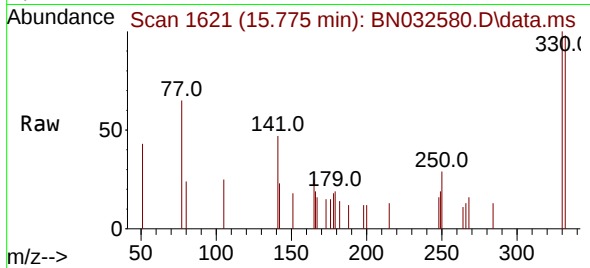


Tgt Ion: 330 Resp: 123
Ion Ratio Lower Upper
330 100
332 101.1 77.7 116.5
141 39.2 31.8 47.8

Manual Integrations
APPROVED



Reviewed By : Jagrut Upadhyay 07/10/2024
Supervised By : mohammad ahmed 07/11/2024

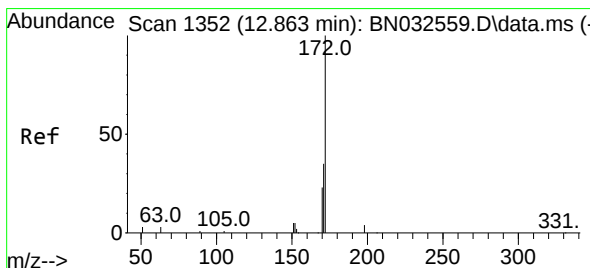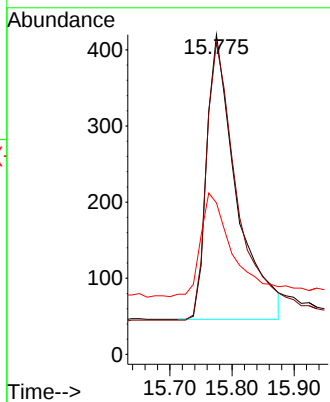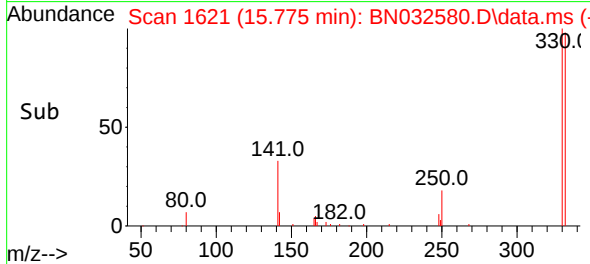


#15
2-Fluorobiphenyl
Concen: 0.304 ng
RT: 12.874 min Scan# 1353
Delta R.T. 0.011 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25

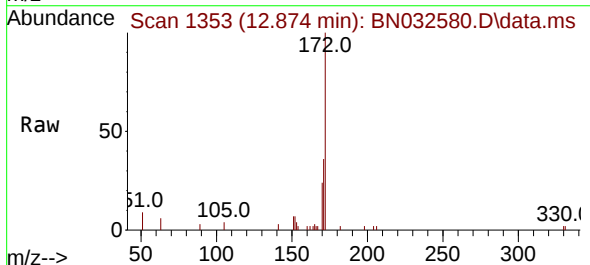


Tgt Ion: 172 Resp: 11279
Ion Ratio Lower Upper
172 100
171 35.6 28.5 42.7
170 24.4 19.2 28.8

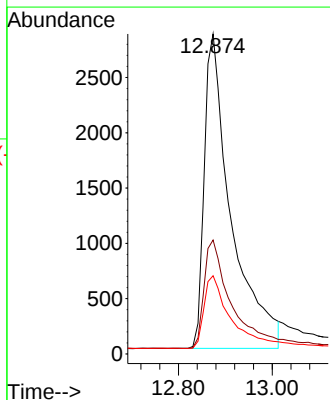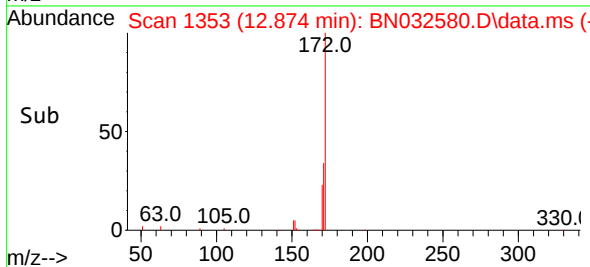

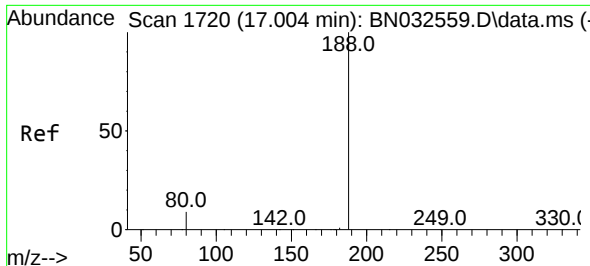

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.016 min Scan# 11
Delta R.T. 0.012 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25




Instrument :
BNA_N
ClientSampleId :
VPB196-HYD-20240703

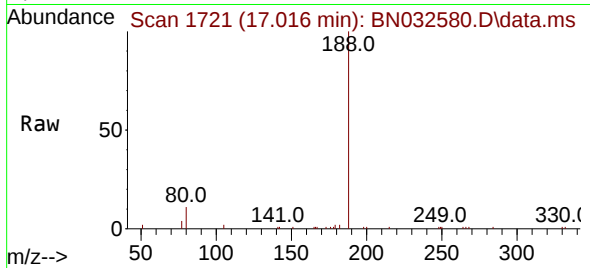


Tgt Ion:188 Resp: 22240
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.8 7.8 11.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

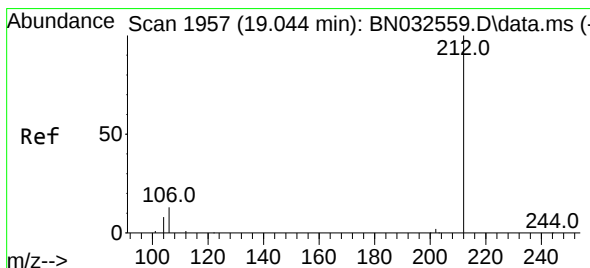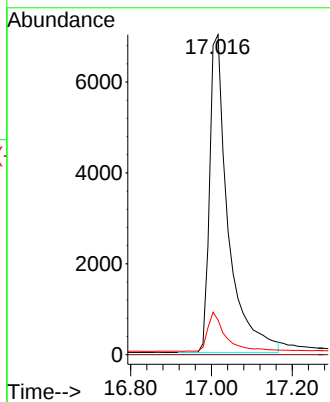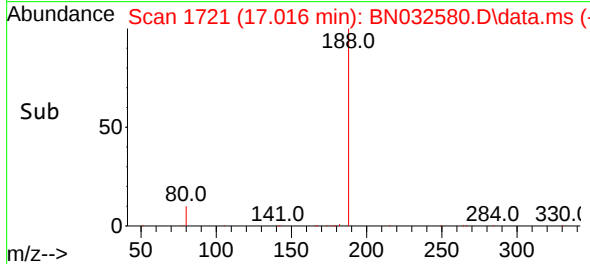


#27
Fluoranthene-d10
Concen: 0.205 ng
RT: 19.045 min Scan# 1957
Delta R.T. 0.000 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25

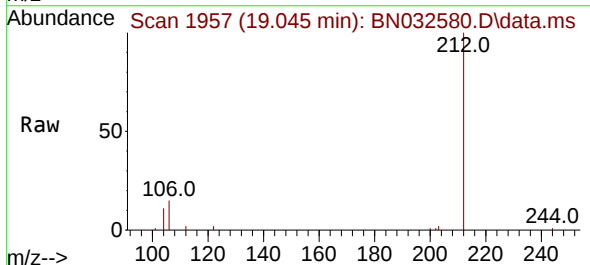


Tgt Ion:212 Resp: 11867
Ion Ratio Lower Upper
212 100
106 14.8 11.8 17.8
104 9.1 6.9 10.3

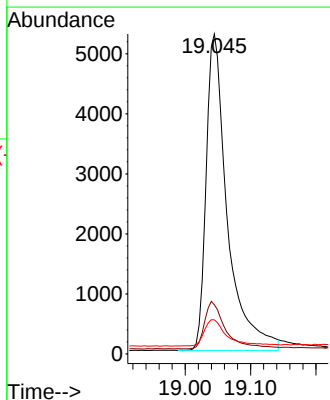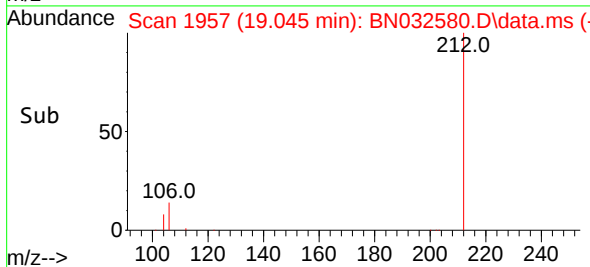



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.211 min Scan# 2402
Delta R.T. 0.000 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25




Instrument :
BNA_N
ClientSampleId :
VPB196-HYD-20240703




Tgt Ion:240 Resp: 1771
Ion Ratio Lower Upper
240 100
120 20.0 13.0 19.4
236 29.6 23.1 34.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

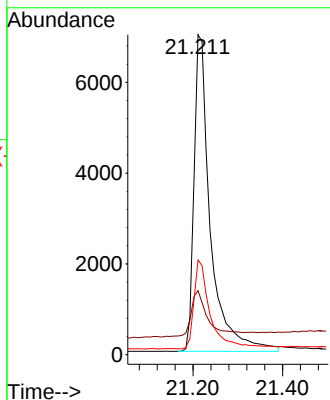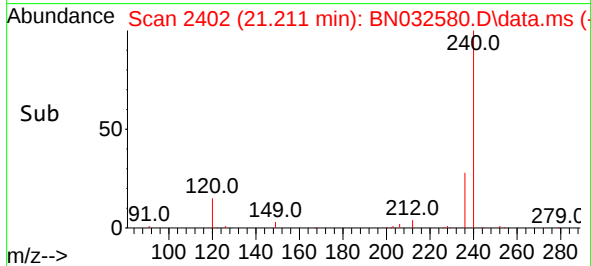


#31
Terphenyl-d14
Concen: 0.449 ng
RT: 19.635 min Scan# 2084
Delta R.T. -0.014 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25

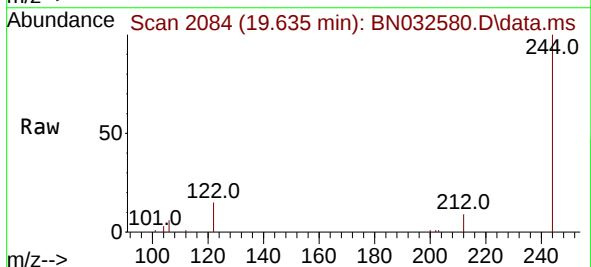


Tgt Ion:244 Resp: 19398
Ion Ratio Lower Upper
244 100
212 8.8 7.2 10.8
122 15.2 12.1 18.1

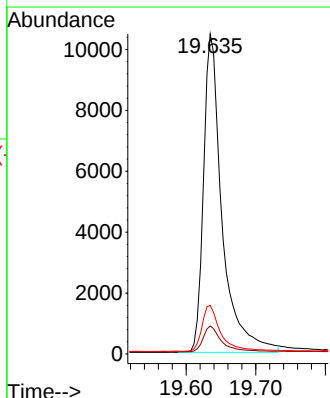

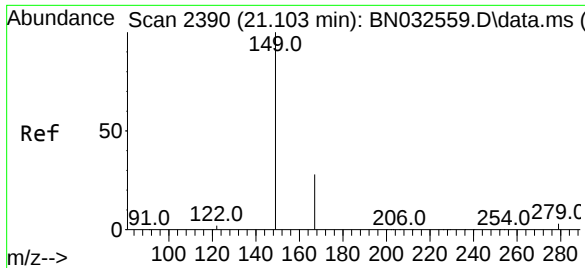

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.053 ng
RT: 21.095 min Scan# 2129
Delta R.T. -0.009 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25




Instrument :
BNA_N
ClientSampleId :
VPB196-HYD-20240703

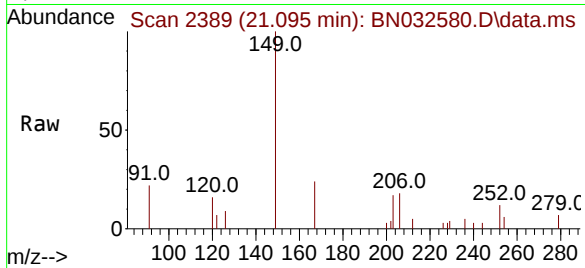

Tgt Ion:149 Resp: 2129
Ion Ratio Lower Upper
149 100
167 24.2 21.6 32.4
279 3.8 3.0 4.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

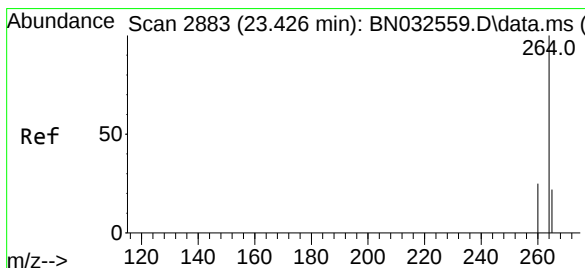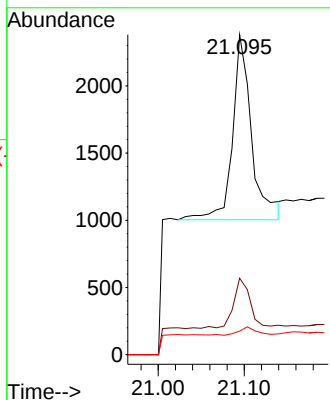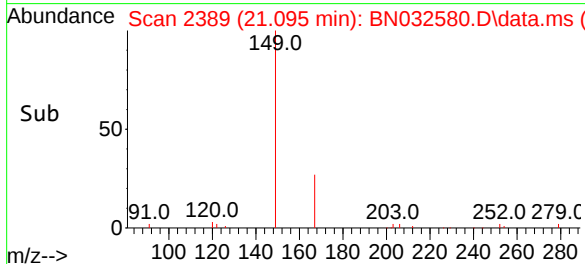

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.431 min Scan# 2885
Delta R.T. 0.006 min
Lab File: BN032580.D
Acq: 09 Jul 2024 10:25

Tgt Ion:264 Resp: 10573
Ion Ratio Lower Upper
264 100
260 27.7 21.0 31.6
265 147.2 76.6 115.0#

