

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
 Data File : BN032588.D
 Acq On : 09 Jul 2024 15:14
 Operator : MA/JU
 Sample : P3128-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-189-GW-610-612

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/10/2024
 Supervised By :mohammad ahmed 07/11/2024

Quant Time: Jul 09 15:56:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 09 02:39:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.588	152	4166	0.400	ng	0.00
7) Naphthalene-d8	10.368	136	13369	0.400	ng	-0.01
13) Acenaphthene-d10	14.231	164	8454	0.400	ng	0.00
19) Phenanthrene-d10	17.004	188	16823	0.400	ng	0.00
29) Chrysene-d12	21.211	240	14035	0.400	ng	# 0.00
35) Perylene-d12	23.429	264	14860	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.219	112	1962	0.186	ng	0.00
5) Phenol-d6	6.873	99	998	0.074	ng	0.05
8) Nitrobenzene-d5	8.809	82	2696m	0.270	ng	0.01
11) 2-Methylnaphthalene-d10	11.967	152	5688	0.269	ng	-0.02
14) 2,4,6-Tribromophenol	15.763	330	1092	0.285	ng	0.00
15) 2-Fluorobiphenyl	12.852	172	8726	0.280	ng	-0.01
27) Fluoranthene-d10	19.040	212	14899	0.340	ng	0.00
31) Terphenyl-d14	19.635	244	13247	0.387	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.161	88	25870	4.716	ng	99
34) Bis(2-ethylhexyl)phtha...	21.095	149	2979	0.094	ng	# 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032588.D
Acq On : 09 Jul 2024 15:14
Operator : MA/JU
Sample : P3128-02
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BP-VPB-189-GW-610-612

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024


Quant Time: Jul 09 15:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 02:39:48 2024
Response via : Initial Calibration

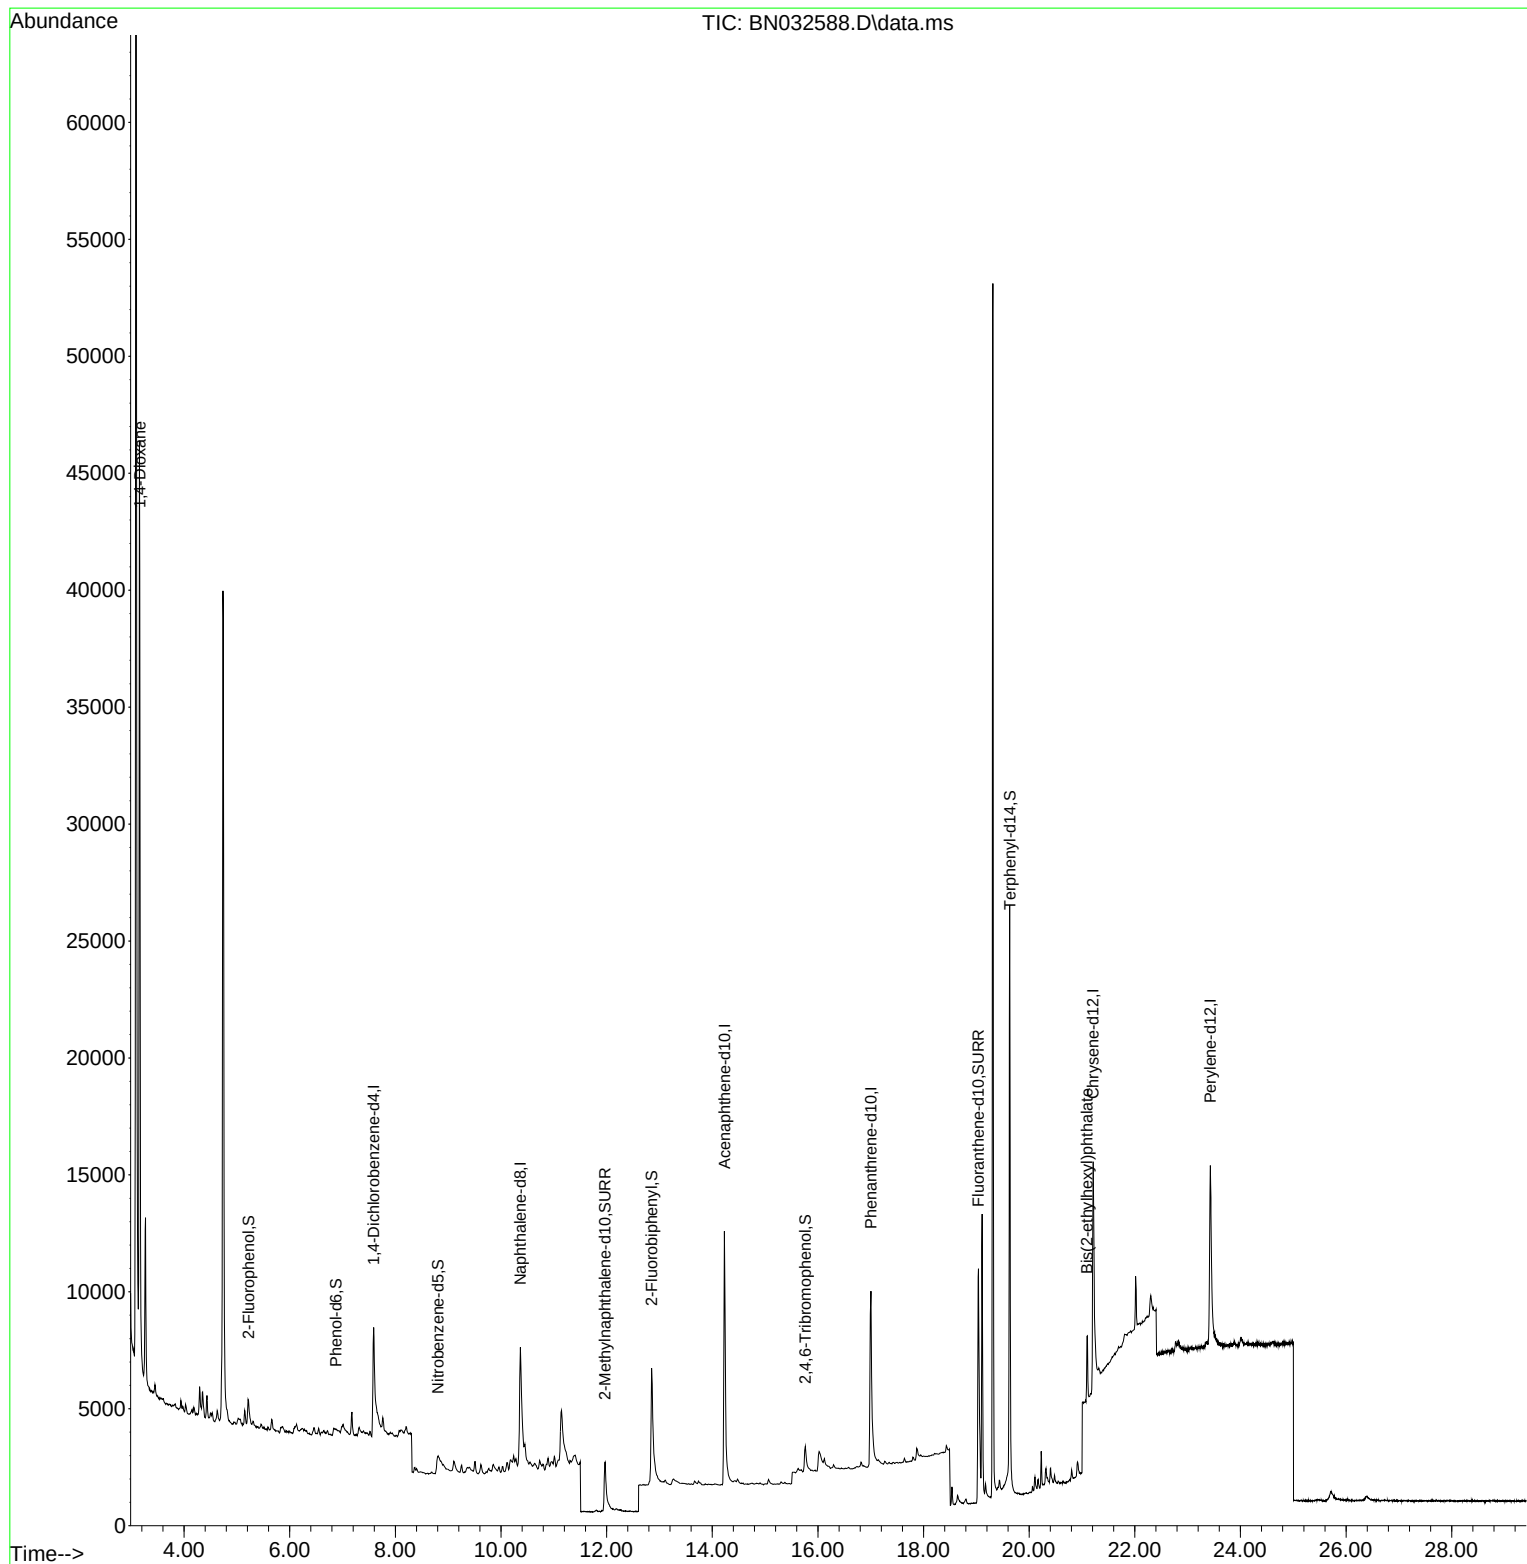

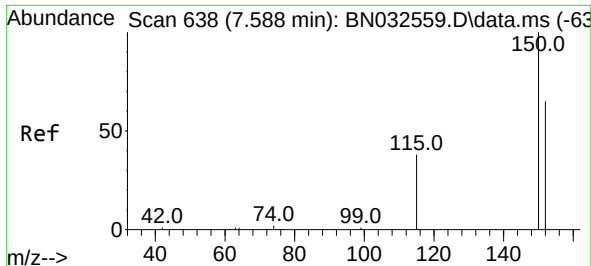

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.588 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14




Instrument :
BNA_N
ClientSampleId :
BP-VPB-189-GW-610-612

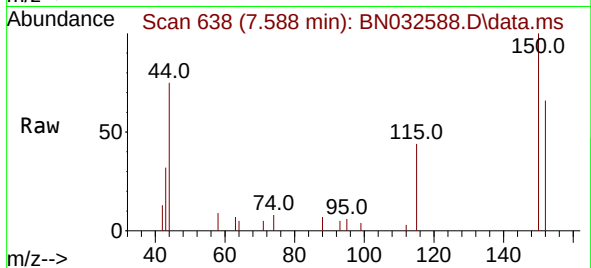


Tgt Ion:152 Resp: 416
Ion Ratio Lower Upper
152 100
150 152.2 121.6 182.4
115 67.3 53.1 79.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

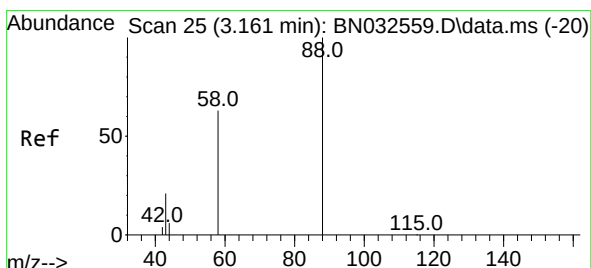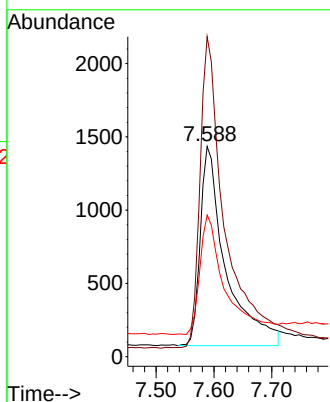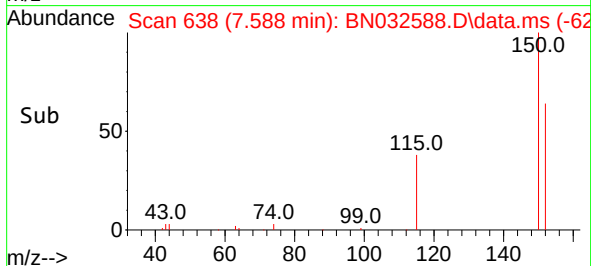


#2
1,4-Dioxane
Concen: 4.716 ng
RT: 3.161 min Scan# 25
Delta R.T. 0.000 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14

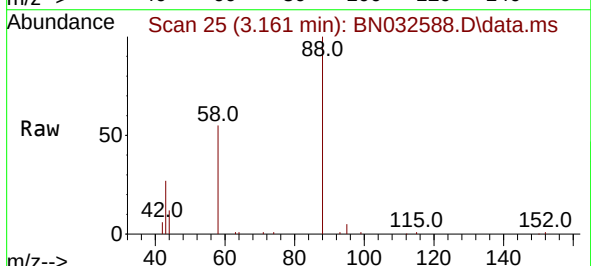


Tgt Ion: 88 Resp: 25870
Ion Ratio Lower Upper
88 100
43 24.9 20.4 30.6
58 62.7 51.0 76.6

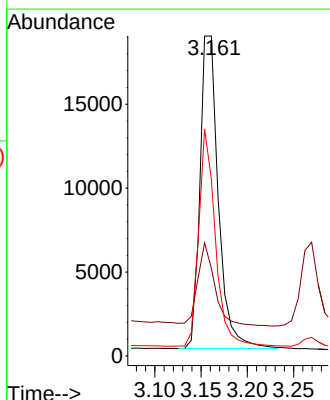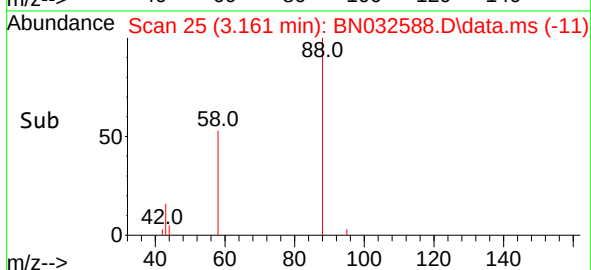

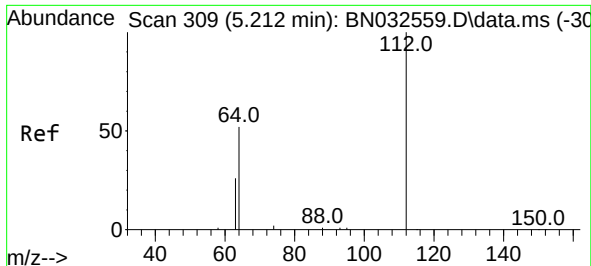

#4
2-Fluorophenol
Concen: 0.186 ng
RT: 5.219 min Scan# 310
Delta R.T. 0.007 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14




Instrument :
BNA_N
ClientSampleId :
BP-VPB-189-GW-610-612

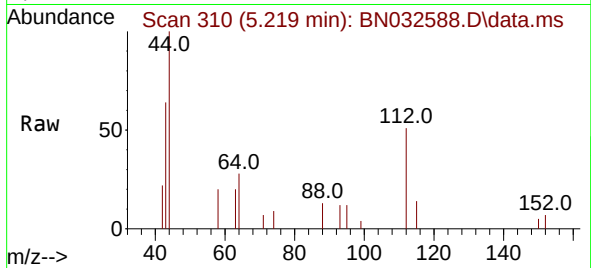

Tgt Ion:112 Resp: 196
Ion Ratio Lower Upper
112 100
64 50.2 41.2 61.8
63 26.8 21.6 32.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

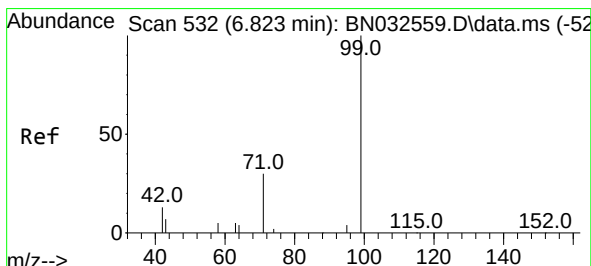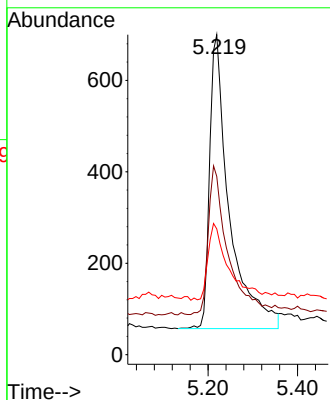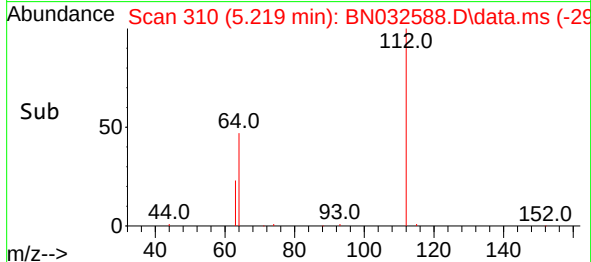

#5
Phenol-d6
Concen: 0.074 ng
RT: 6.873 min Scan# 539
Delta R.T. 0.051 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14


Tgt Ion: 99 Resp: 998
Ion Ratio Lower Upper
99 100
42 2.3 10.6 16.0#
71 0.0 25.2 37.8#

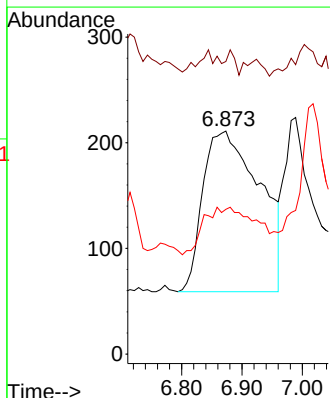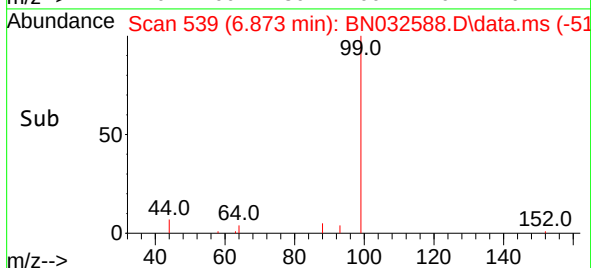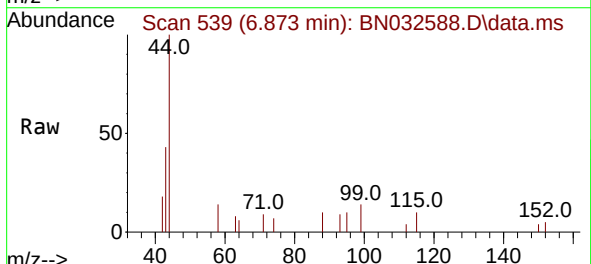

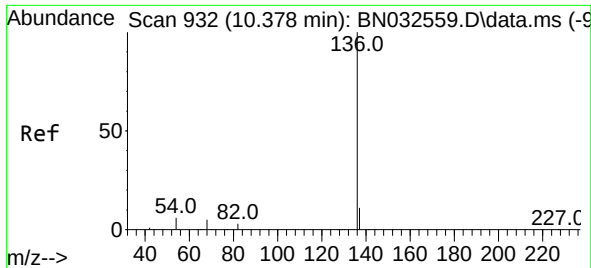

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.368 min Scan# 91
Delta R.T. -0.010 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14




Instrument :
BNA_N
ClientSampleId :
BP-VPB-189-GW-610-612

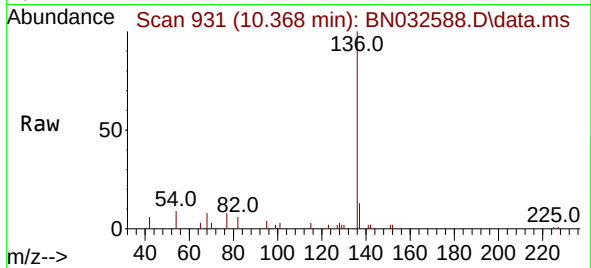

Tgt Ion:136 Resp: 1336
Ion Ratio Lower Upper
136 100
137 12.7 10.0 15.0
54 9.2 6.6 9.8
68 8.2 5.8 8.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

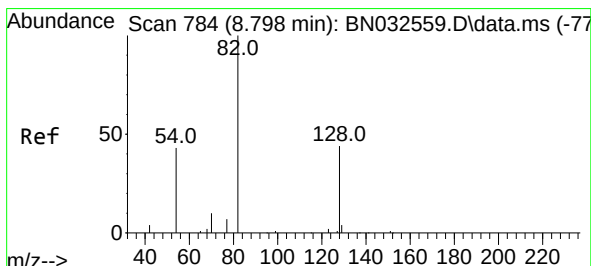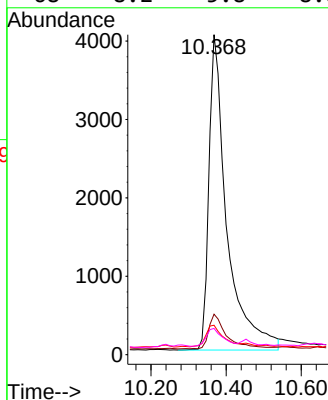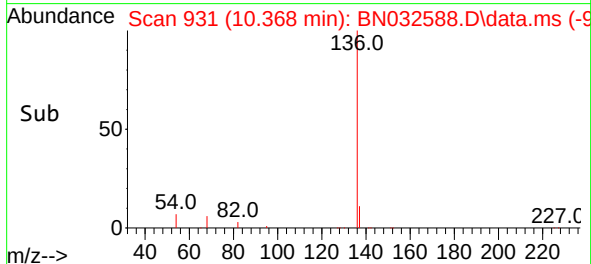

#8
Nitrobenzene-d5
Concen: 0.270 ng m
RT: 8.809 min Scan# 785
Delta R.T. 0.011 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14


Tgt Ion: 82 Resp: 2696
Ion Ratio Lower Upper
82 100
128 59.5 43.4 65.2
54 53.9 40.2 60.2

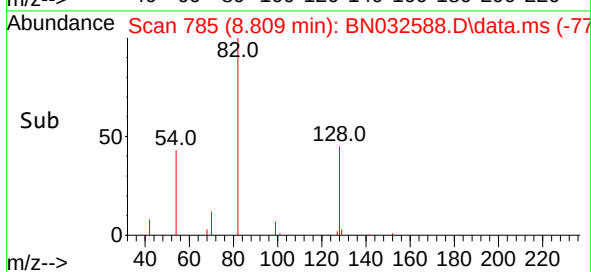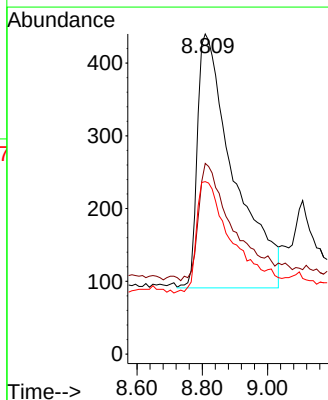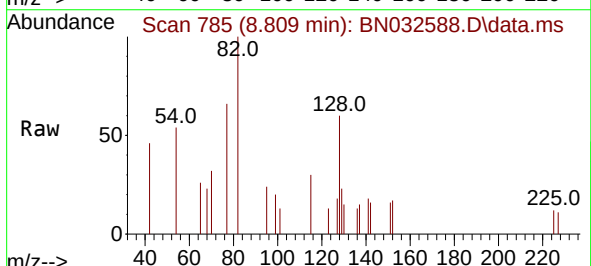

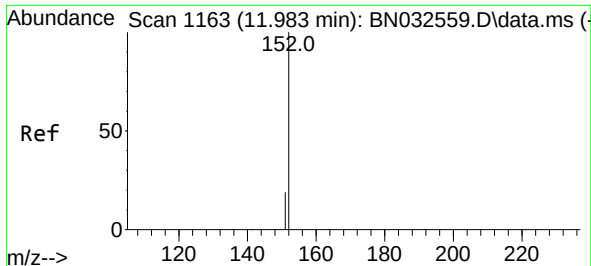

#11
2-Methylnaphthalene-d10
Concen: 0.269 ng
RT: 11.967 min Scan# 1163
Delta R.T. -0.015 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14




Instrument :
BNA_N
ClientSampleId :
BP-VPB-189-GW-610-612

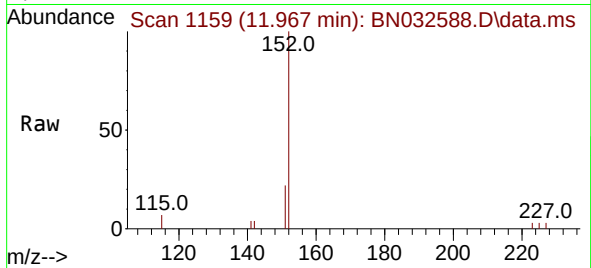


Tgt Ion:152 Resp: 568
Ion Ratio Lower Upper
152 100
151 19.1 16.4 24.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

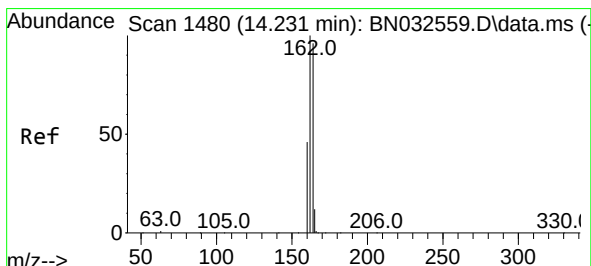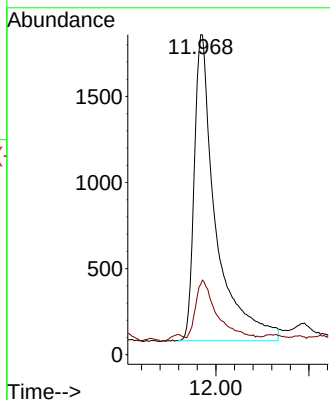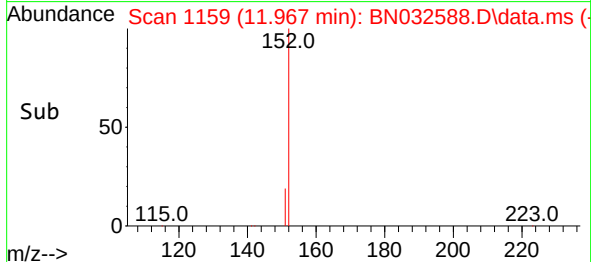


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.231 min Scan# 1480
Delta R.T. 0.000 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14

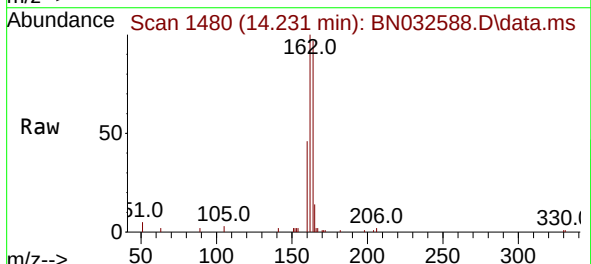


Tgt Ion:164 Resp: 8454
Ion Ratio Lower Upper
164 100
162 103.3 83.2 124.8
160 47.0 38.6 57.8

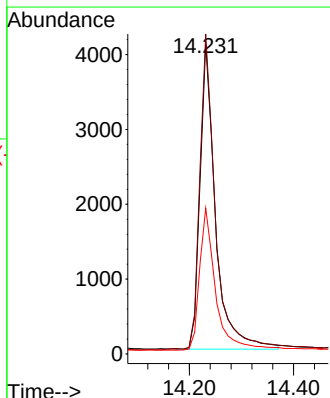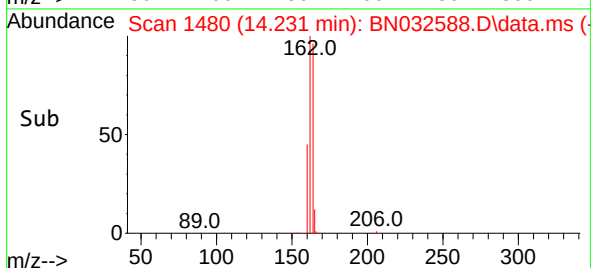

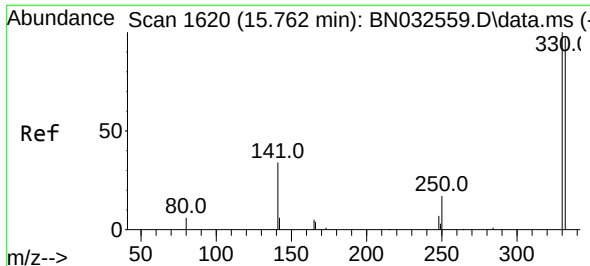

#14
2,4,6-Tribromophenol
Concen: 0.285 ng
RT: 15.763 min Scan# 1092
Delta R.T. 0.000 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14




Instrument :
BNA_N
ClientSampleId :
BP-VPB-189-GW-610-612

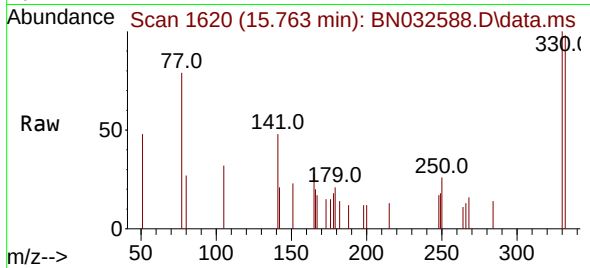


Tgt Ion:330 Resp: 1092
Ion Ratio Lower Upper
330 100
332 94.7 77.7 116.5
141 42.0 31.8 47.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

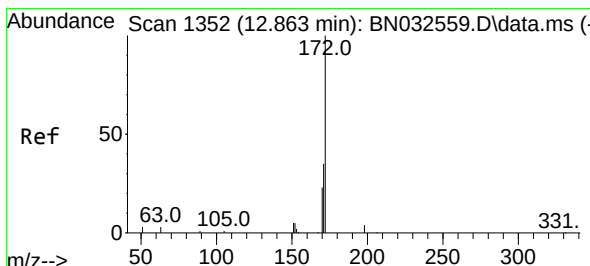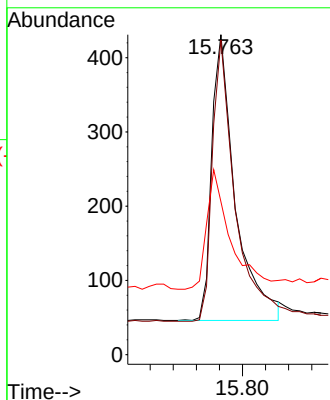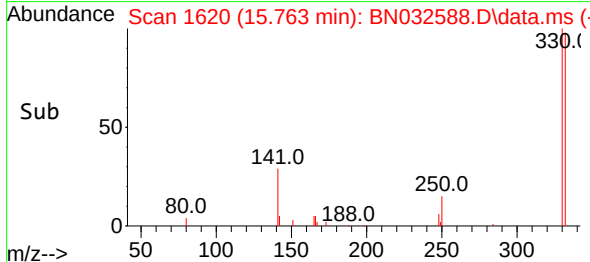


#15
2-Fluorobiphenyl
Concen: 0.280 ng
RT: 12.852 min Scan# 1351
Delta R.T. -0.011 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14

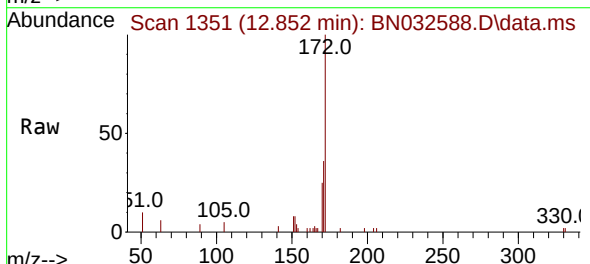


Tgt Ion:172 Resp: 8726
Ion Ratio Lower Upper
172 100
171 36.3 28.5 42.7
170 24.8 19.2 28.8

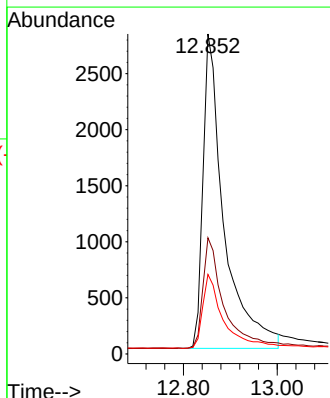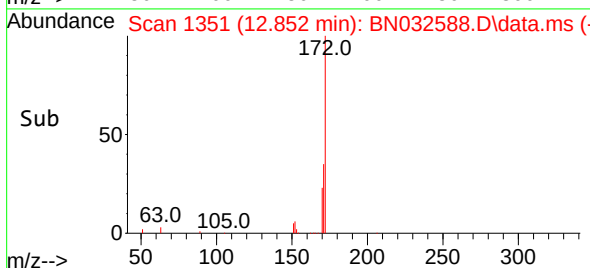

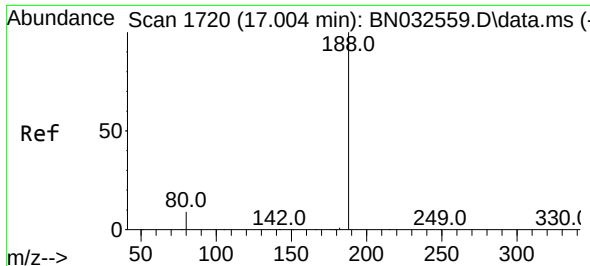

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.004 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14




Instrument :
BNA_N
ClientSampleId :
BP-VPB-189-GW-610-612

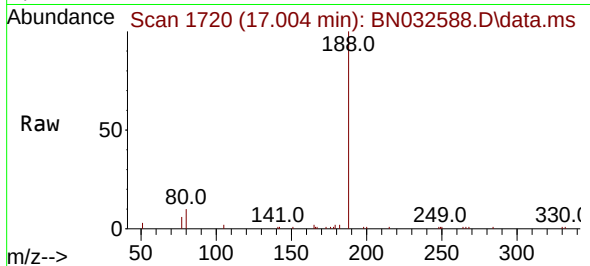


Tgt Ion:188 Resp: 1682
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.5 7.8 11.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

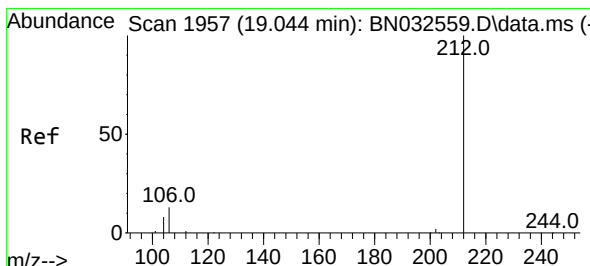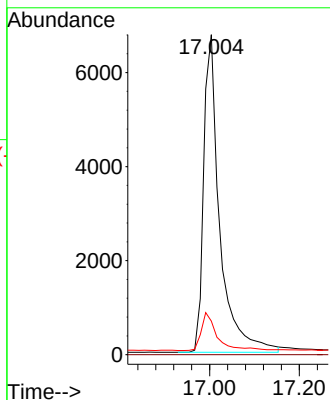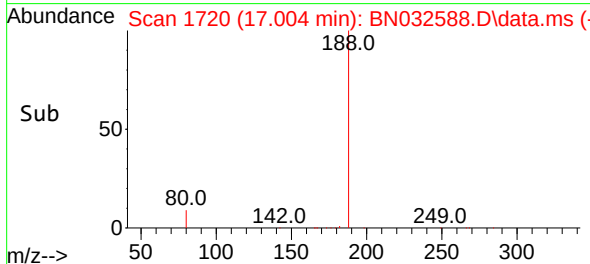


#27
Fluoranthene-d10
Concen: 0.340 ng
RT: 19.040 min Scan# 1956
Delta R.T. -0.005 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14

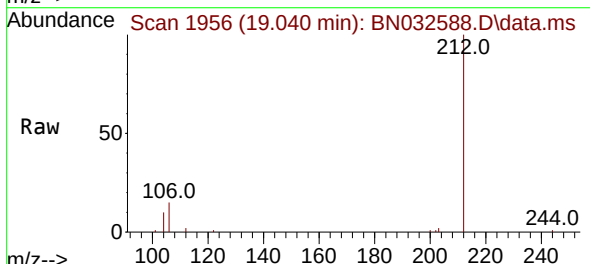


Tgt Ion:212 Resp: 14899
Ion Ratio Lower Upper
212 100
106 14.7 11.8 17.8
104 8.3 6.9 10.3

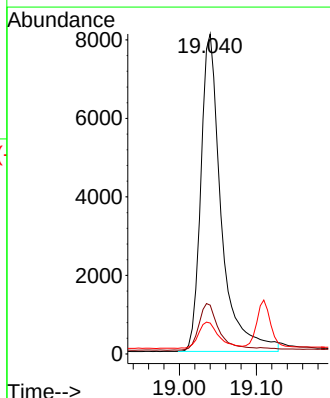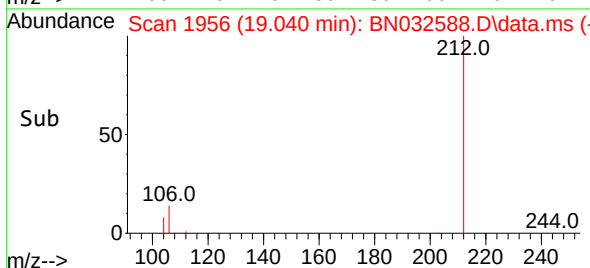

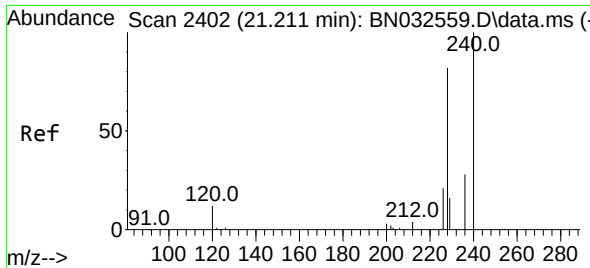

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.211 min Scan# 2402
Delta R.T. 0.000 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14




Instrument :
BNA_N
ClientSampleId :
BP-VPB-189-GW-610-612

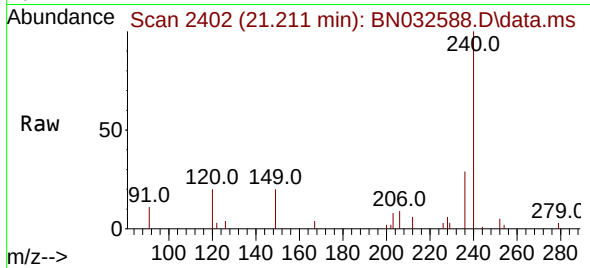

Tgt Ion:240 Resp: 14035
Ion Ratio Lower Upper
240 100
120 20.0 13.0 19.45
236 29.3 23.1 34.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

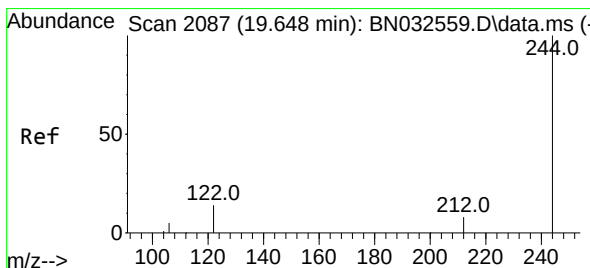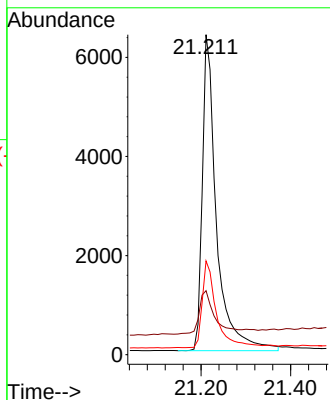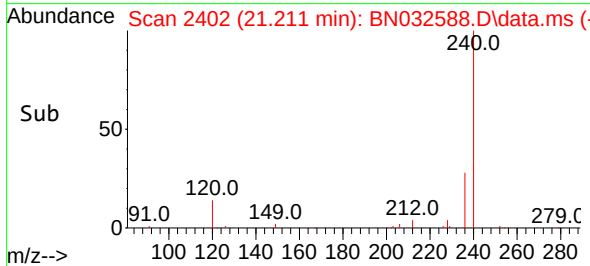

#31
Terphenyl-d14
Concen: 0.387 ng
RT: 19.635 min Scan# 2084
Delta R.T. -0.014 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14


Tgt Ion:244 Resp: 13247
Ion Ratio Lower Upper
244 100
212 19.0 7.2 10.85
122 15.1 12.1 18.1

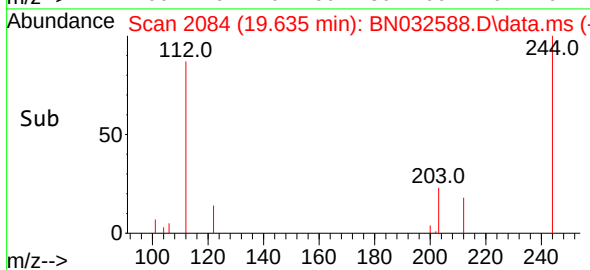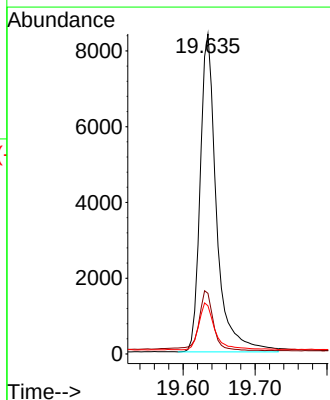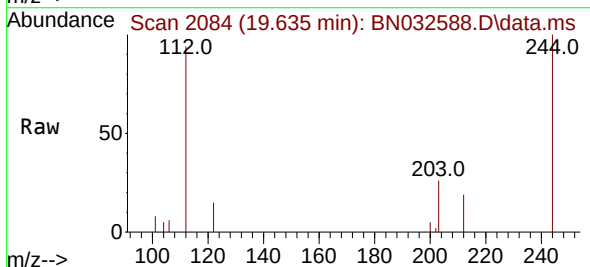

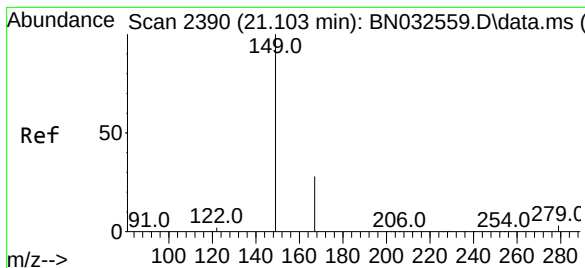

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.094 ng
RT: 21.095 min Scan# 2109
Delta R.T. -0.009 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14




Instrument :
BNA_N
ClientSampleId :
BP-VPB-189-GW-610-612

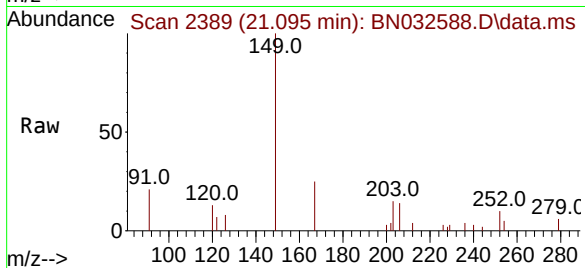

Tgt Ion:149 Resp: 2979
Ion Ratio Lower Upper
149 100
167 26.3 21.6 32.4
279 4.8 3.0 4.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/10/2024
Supervised By :mohammad ahmed 07/11/2024

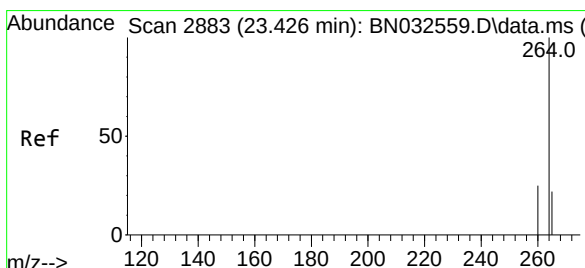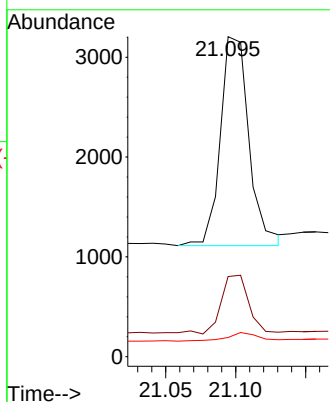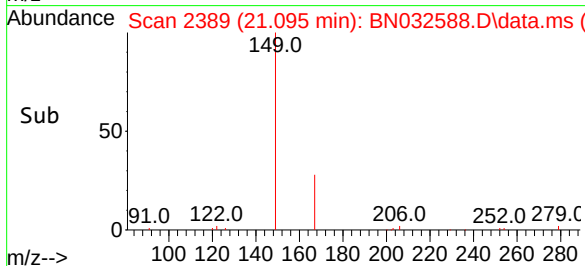

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.429 min Scan# 2884
Delta R.T. 0.003 min
Lab File: BN032588.D
Acq: 09 Jul 2024 15:14

Tgt Ion:264 Resp: 14860
Ion Ratio Lower Upper
264 100
260 26.5 21.0 31.6
265 106.2 76.6 115.0

