


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070924\  
Data File : BN032556.D  
Acq On : 08 Jul 2024 18:36  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN070924.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Jul 09 02:39:48 2024

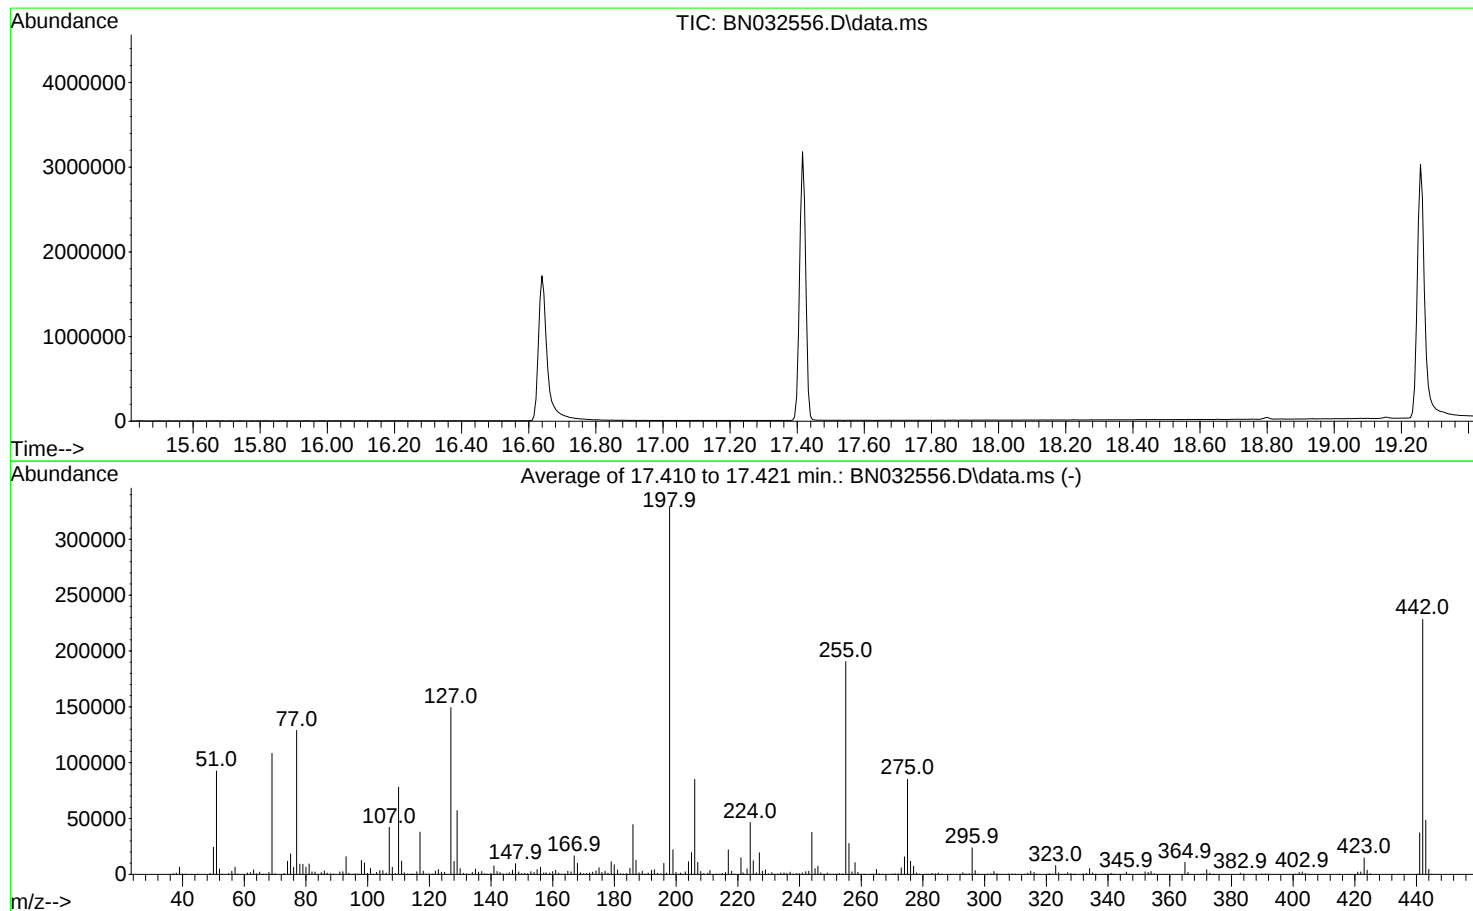




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 28.1         | 92581      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1919       | PASS                |
| 69             | 198             | 0.00            | 100             | 32.9         | 108296     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 653        | PASS                |
| 127            | 198             | 10              | 80              | 45.3         | 149248     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 1112       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 329408     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 22019      | PASS                |
| 275            | 198             | 10              | 60              | 25.8         | 85144      | PASS                |
| 365            | 198             | 1               | 100             | 3.3          | 10718      | PASS                |
| 441            | 198             | 0.01            | 100             | 11.3         | 37147      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 228459     | PASS                |
| 443            | 442             | 15              | 24              | 21.2         | 48419      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070924\  
Data File : BN032556.D  
Acq On : 08 Jul 2024 18:36  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Jul 09 03:02:26 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 20 01:44:29 2024  
Response via : Initial Calibration

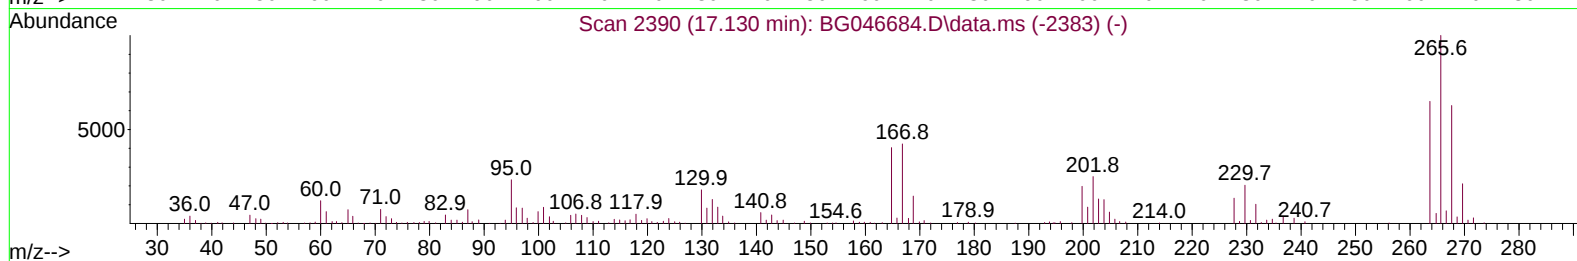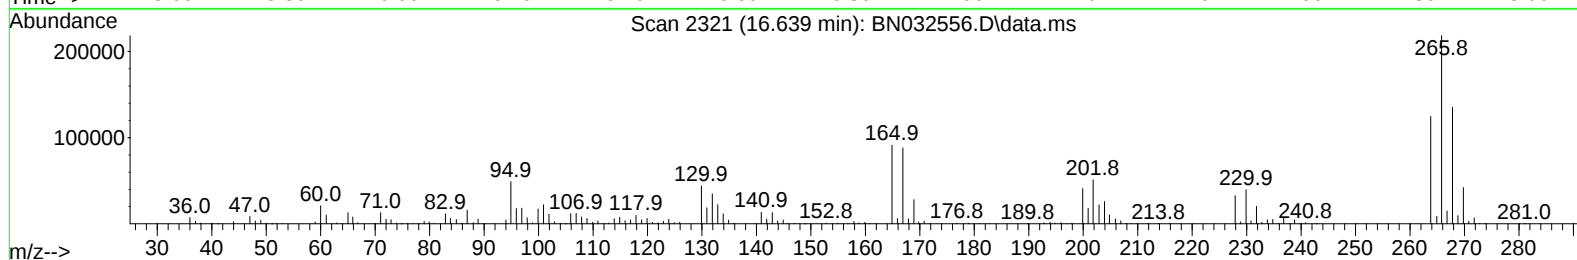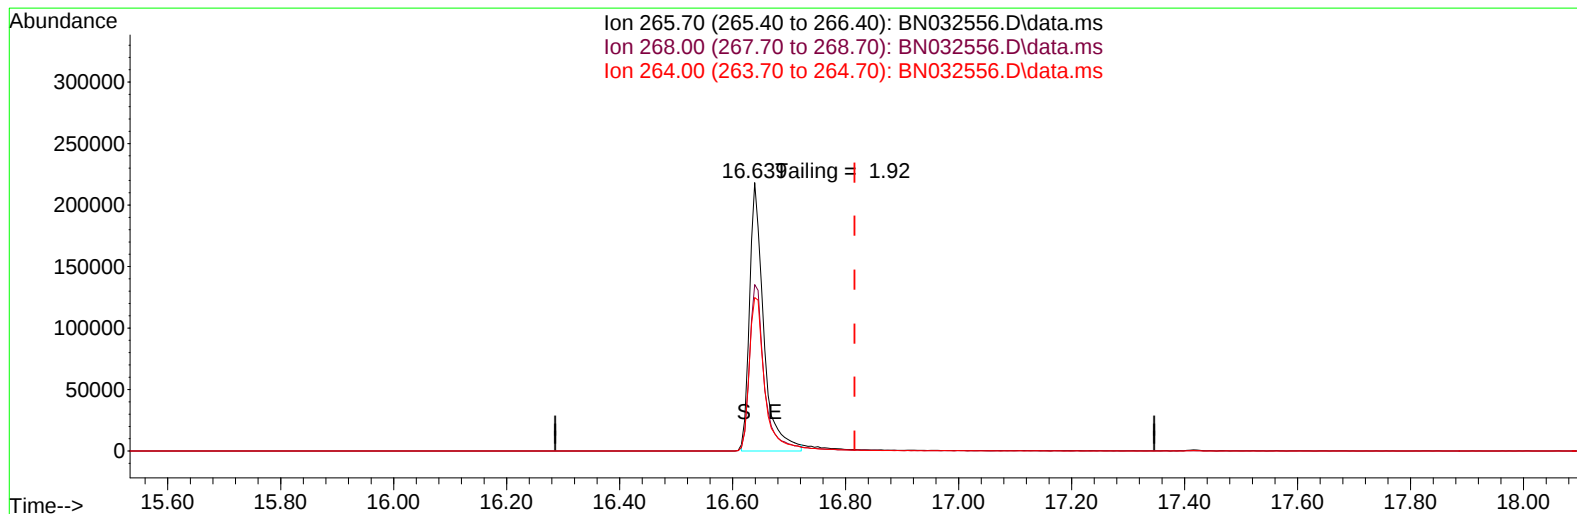

TIC: BN032556.D\data.ms

**(70) Pentachlorophenol (C)**

16.639min (-0.177) 24262.73 ng




response 396429

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 62.02  |
| 264.00 | 61.60  | 57.16  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070924\  
Data File : BN032556.D  
Acq On : 08 Jul 2024 18:36  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Jul 09 03:02:26 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 20 01:44:29 2024  
Response via : Initial Calibration

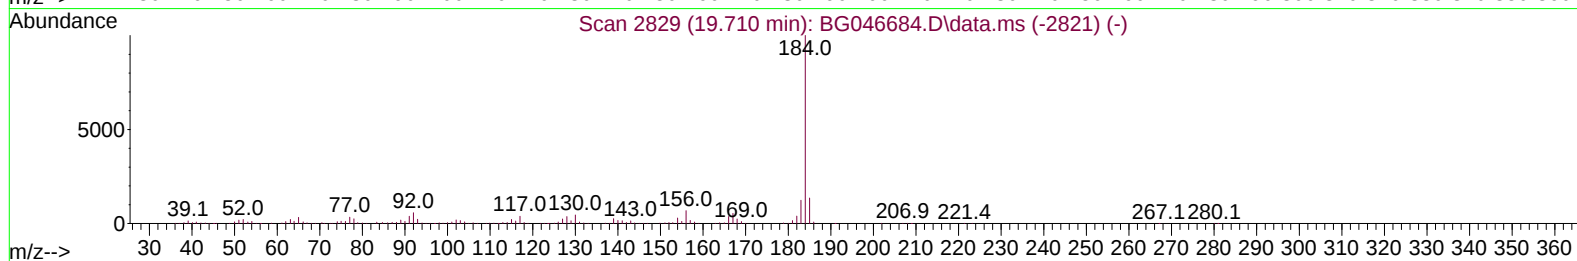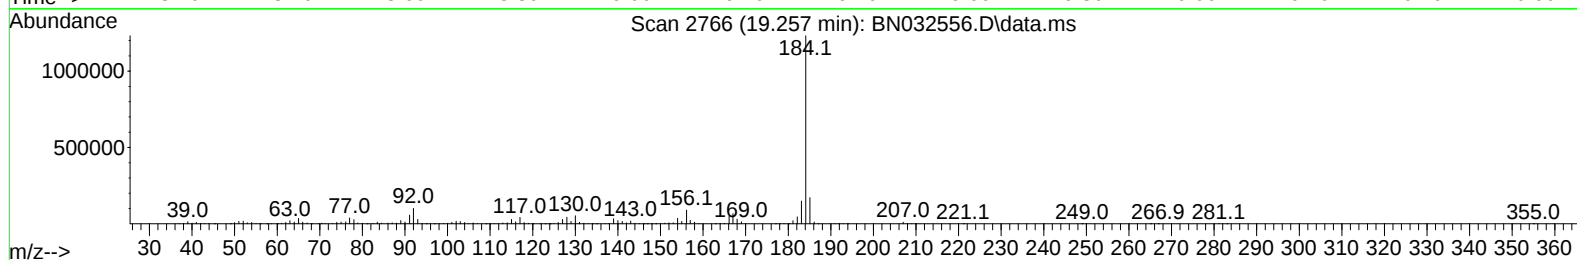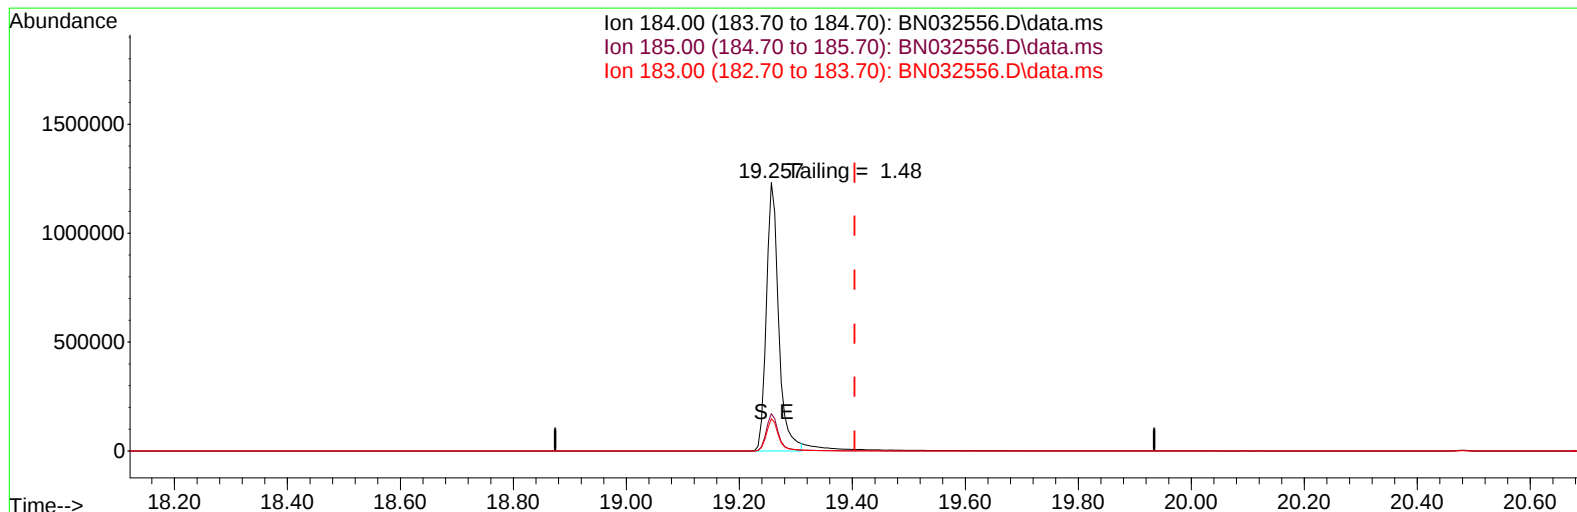

TIC: BN032556.D\data.ms

(77) Benzidine

19.257min (-0.147) 0.00 ng

response 1975287

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.89  |
| 183.00 | 13.20  | 12.06  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 7/9/2024      | BNA_N            | <u>BN032556.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1068373          | 20.48              |
| DDD           | 8762             | 20.086             |
| DDE           | 493              | 19.533             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 9255          | 1077628          | 0.86               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP