


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032574.D
Acq On : 09 Jul 2024 06:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 02:39:48 2024

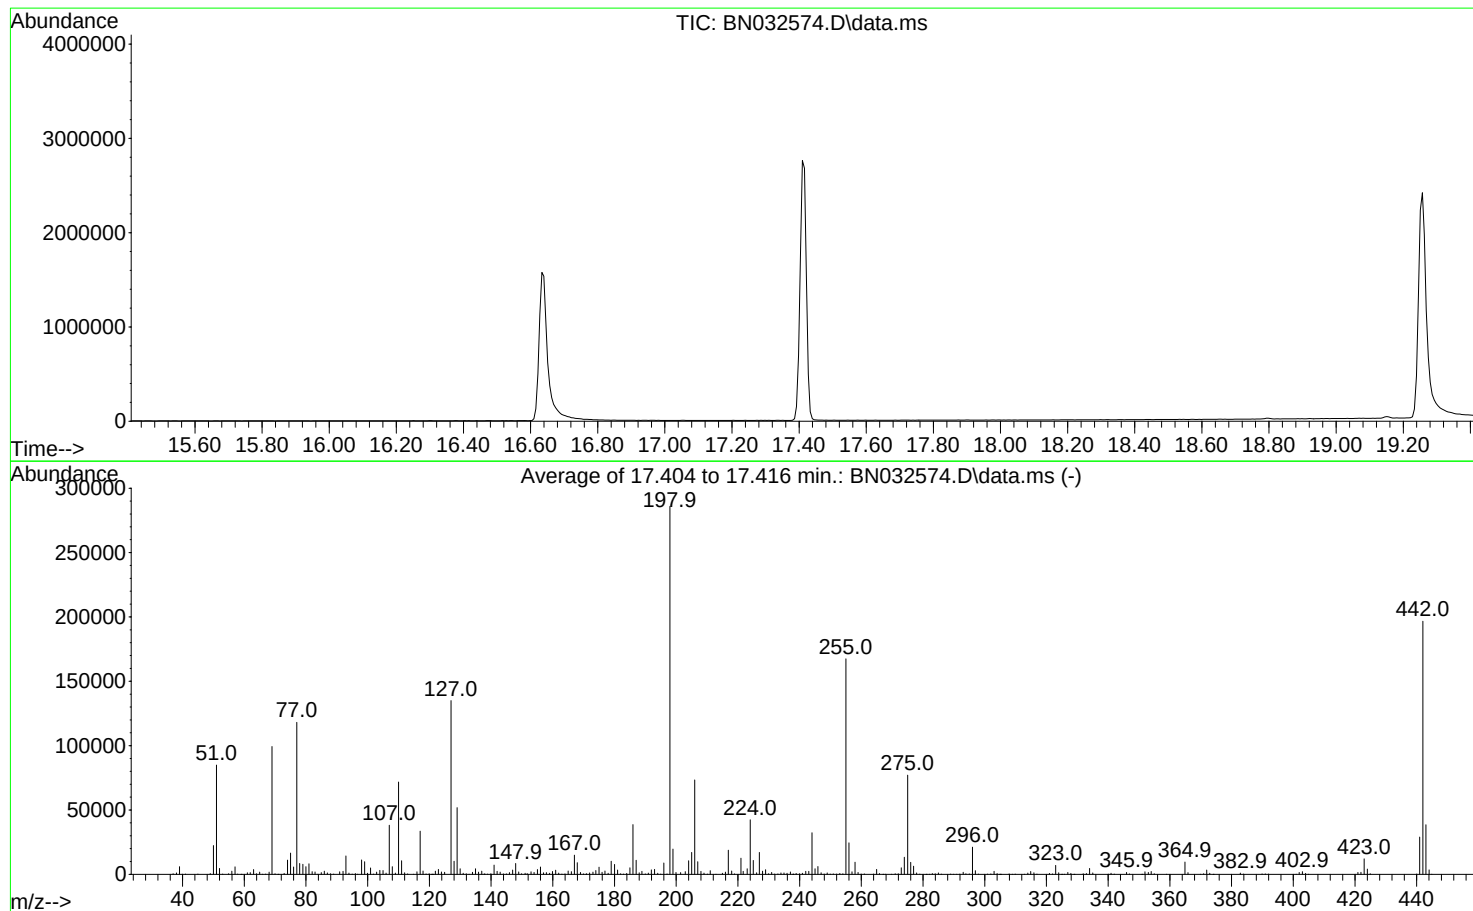




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	84957	PASS
68	69	0.00	2	1.7	1719	PASS
69	198	0.00	100	34.8	99317	PASS
70	69	0.00	2	0.6	562	PASS
127	198	10	80	47.2	134971	PASS
197	198	0.00	2	0.1	383	PASS
198	198	100	100	100.0	285803	PASS
199	198	5	9	6.9	19644	PASS
275	198	10	60	27.0	77141	PASS
365	198	1	100	3.4	9629	PASS
441	198	0.01	100	10.1	28971	PASS
442	442	50	100	100.0	196701	PASS
443	442	15	24	19.6	38603	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032574.D
Acq On : 09 Jul 2024 06:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 09 08:06:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

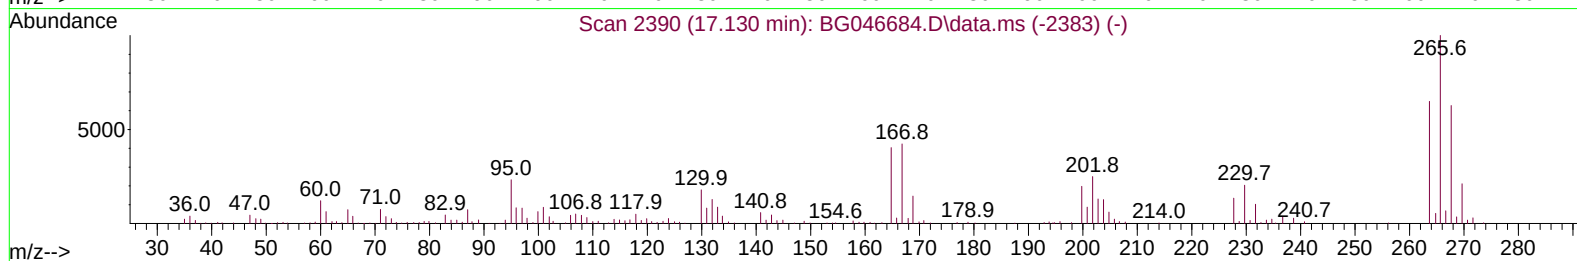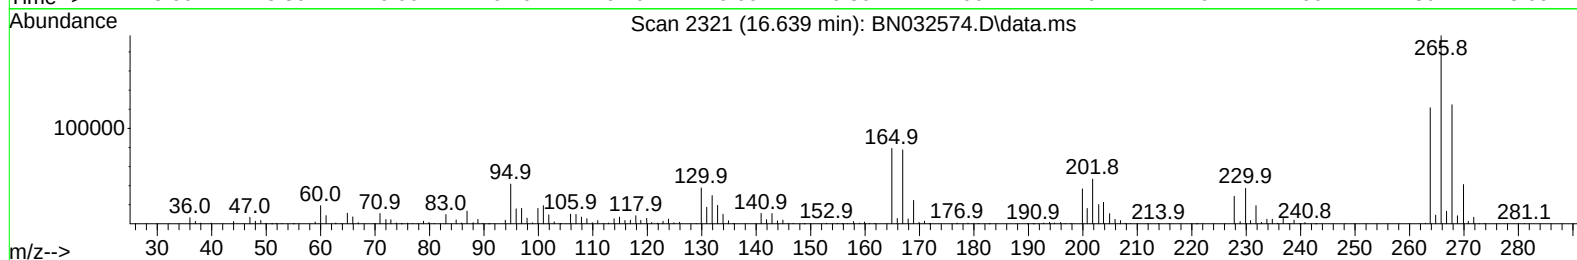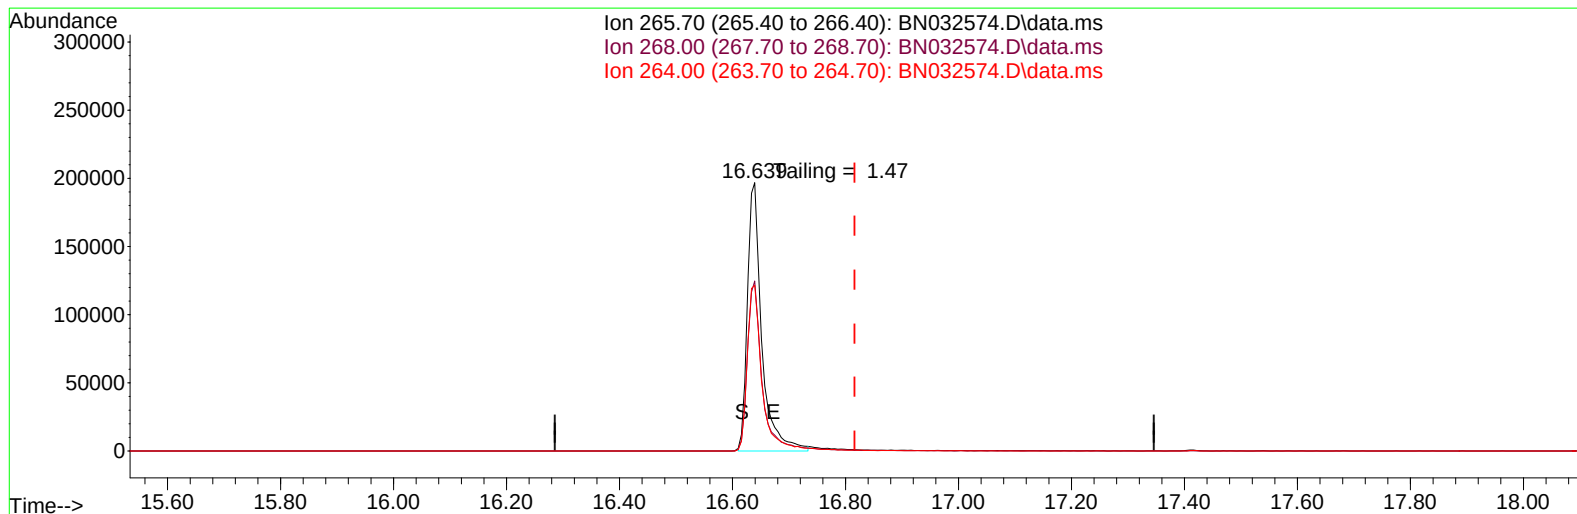

TIC: BN032574.D\data.ms

(70) Pentachlorophenol (C)

16.639min (-0.177) 23970.66 ng




response 359301

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.35
264.00	61.60	61.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032574.D
Acq On : 09 Jul 2024 06:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 09 08:06:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

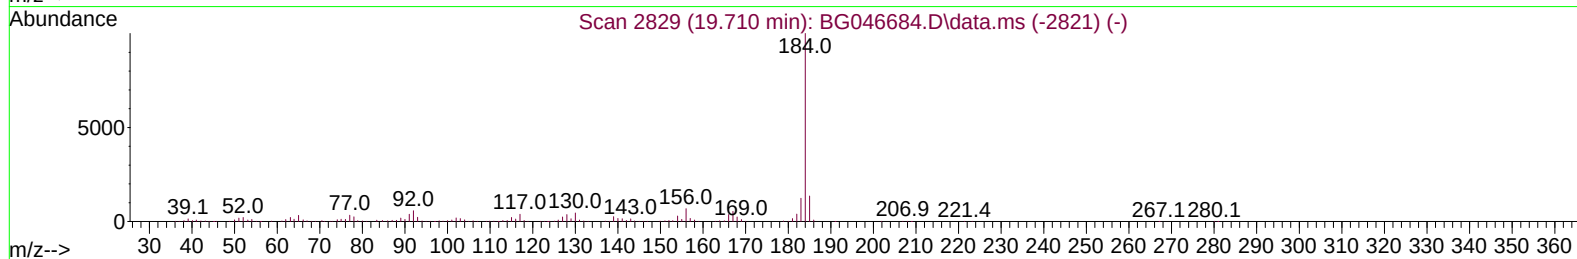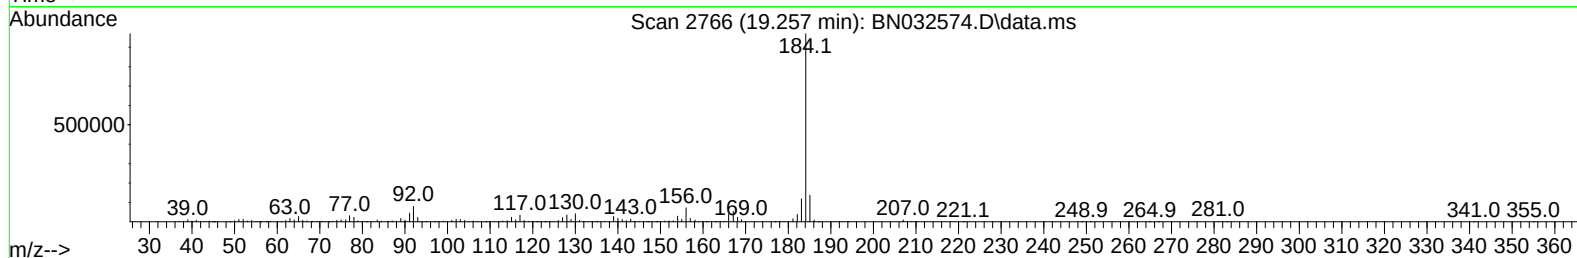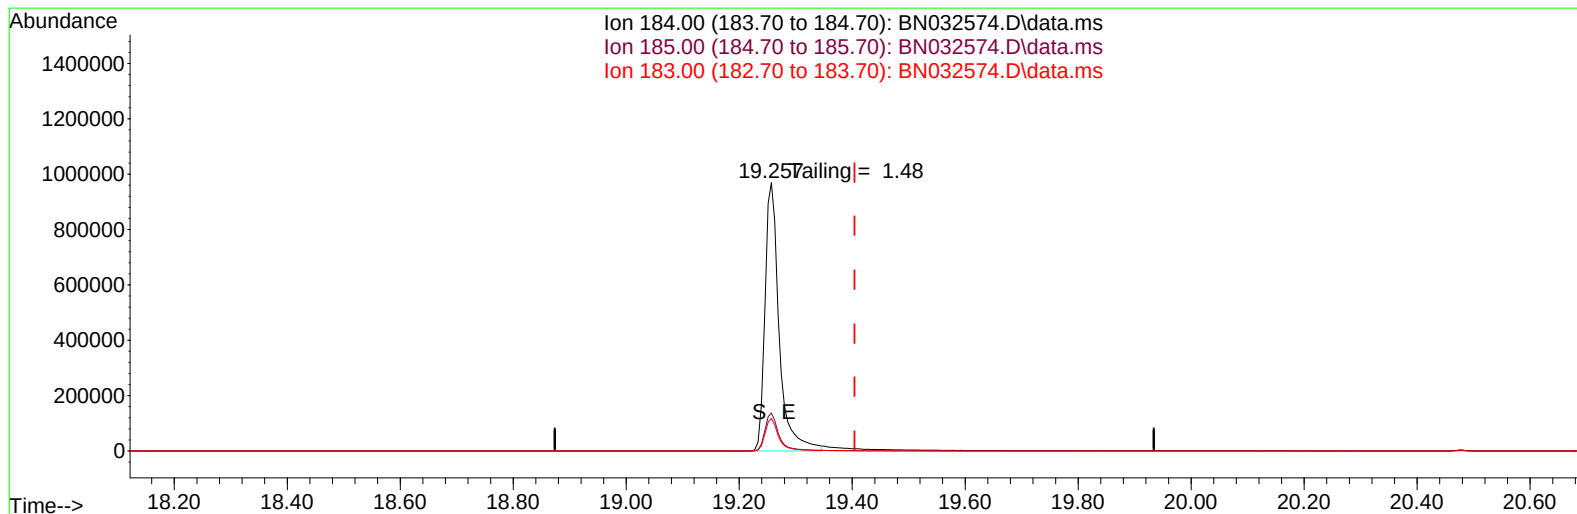

TIC: BN032574.D\data.ms

(77) Benzidine

19.257min (-0.147) 0.00 ng

response 1788829

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.18
183.00	13.20	12.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/9/2024	BNA_N	<u>BN032574.D</u>
Compound Name	Response	Retention Time
DDT	970703	20.48
DDD	10515	20.086
DDE	204	19.527
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10719	981422	1.09

Instrument :
BNA_N
ClientSampleId :
DFTPP