


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032593.D
Acq On : 09 Jul 2024 18:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 02:39:48 2024

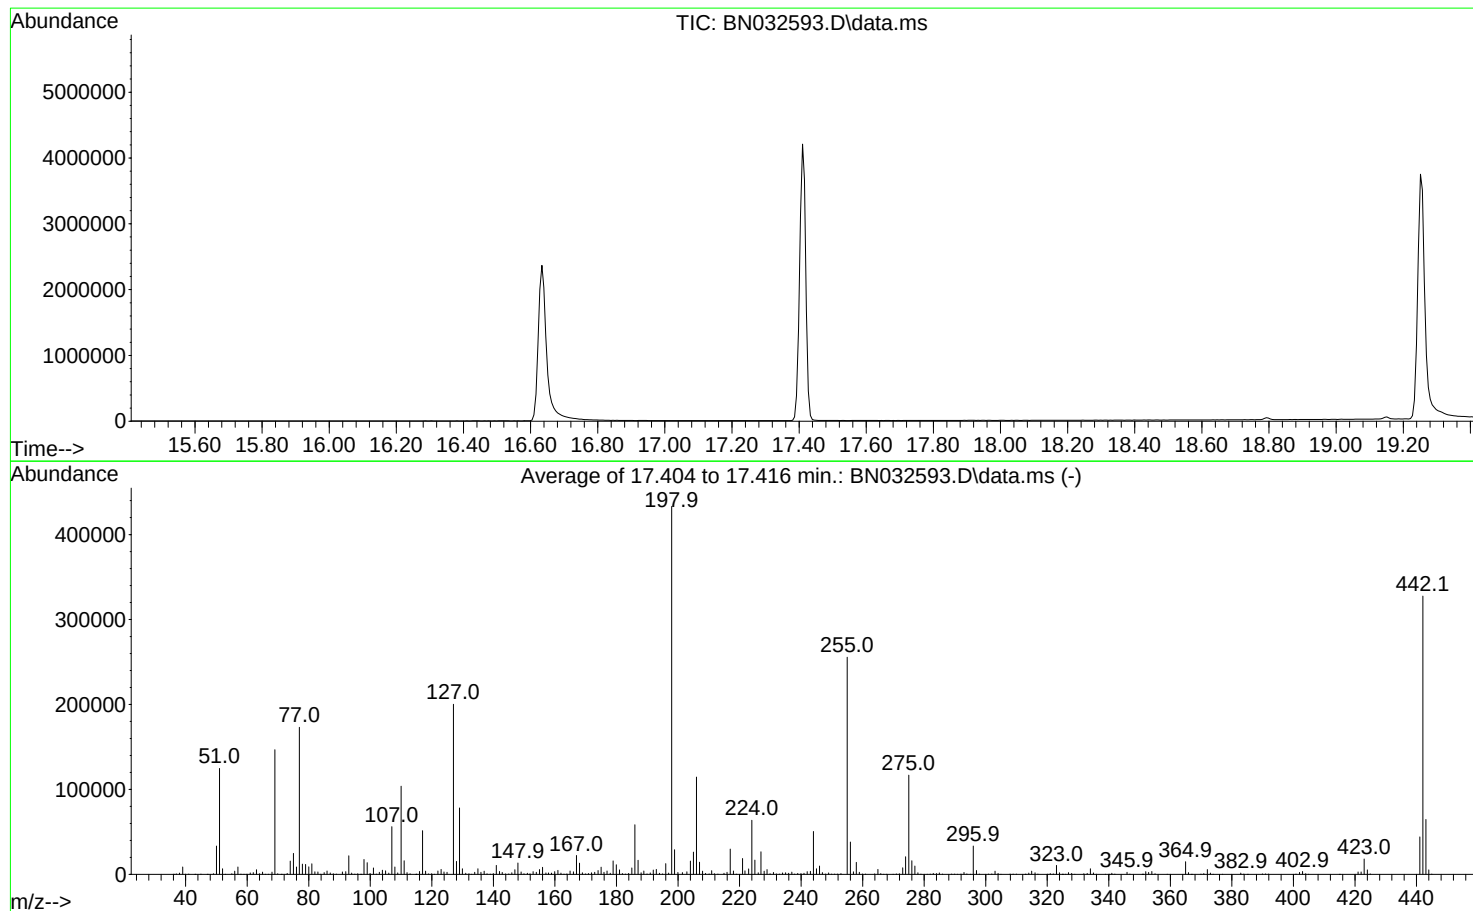




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	124725	PASS
68	69	0.00	2	1.8	2627	PASS
69	198	0.00	100	33.9	146821	PASS
70	69	0.00	2	0.5	680	PASS
127	198	10	80	46.2	200299	PASS
197	198	0.00	2	0.4	1572	PASS
198	198	100	100	100.0	433088	PASS
199	198	5	9	6.7	28987	PASS
275	198	10	60	27.0	116893	PASS
365	198	1	100	3.5	14945	PASS
441	198	0.01	100	10.2	44120	PASS
442	442	50	100	100.0	327680	PASS
443	442	15	24	19.7	64608	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032593.D
Acq On : 09 Jul 2024 18:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 10 01:07:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

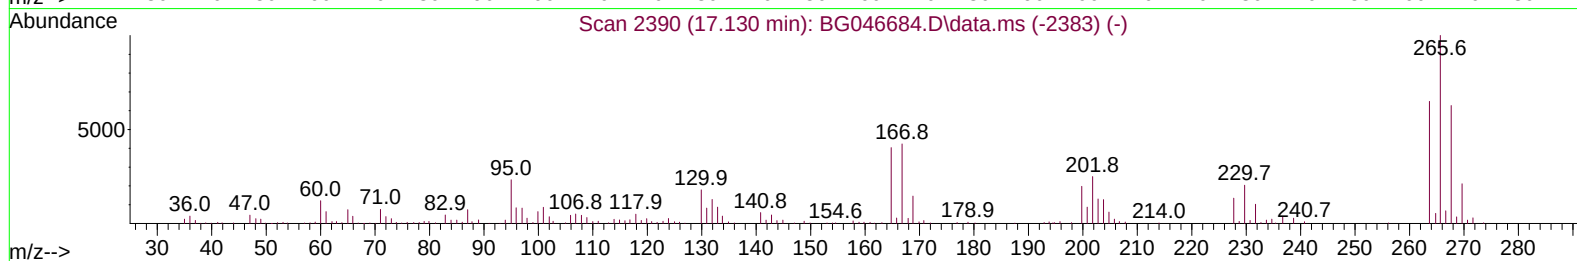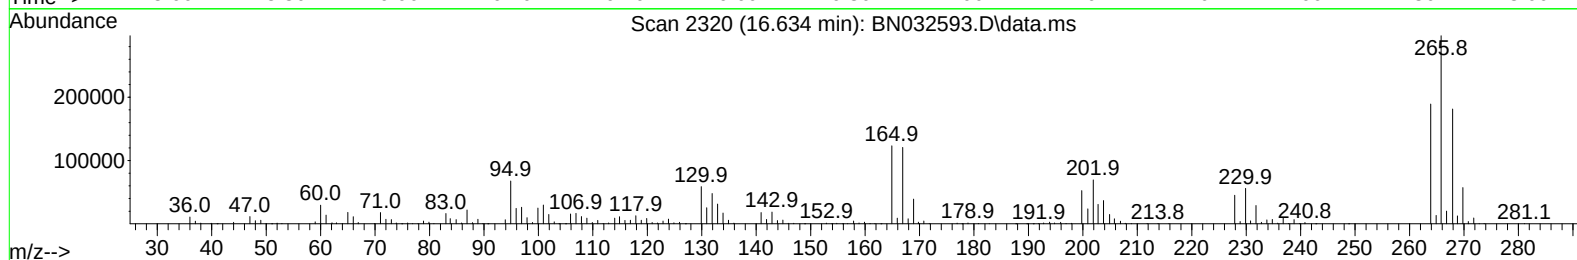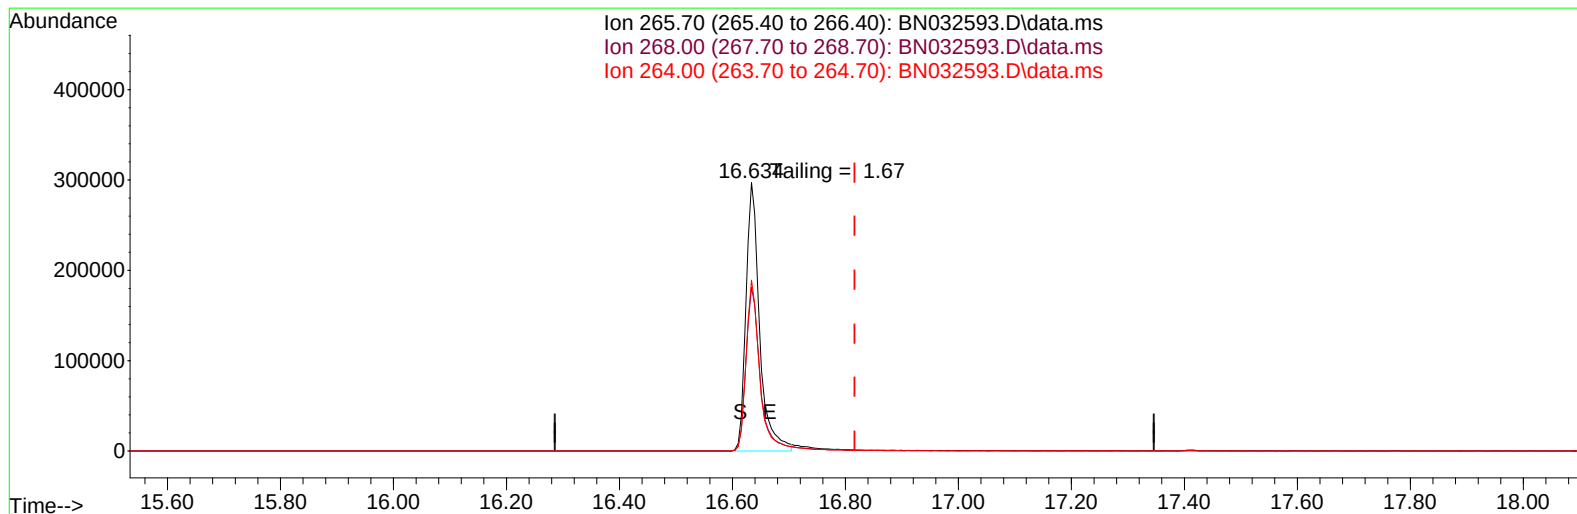

TIC: BN032593.D\data.ms

(70) Pentachlorophenol (C)

16.634min (-0.182) 23870.22 ng




response 521707

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.01
264.00	61.60	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070924\
Data File : BN032593.D
Acq On : 09 Jul 2024 18:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 10 01:07:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

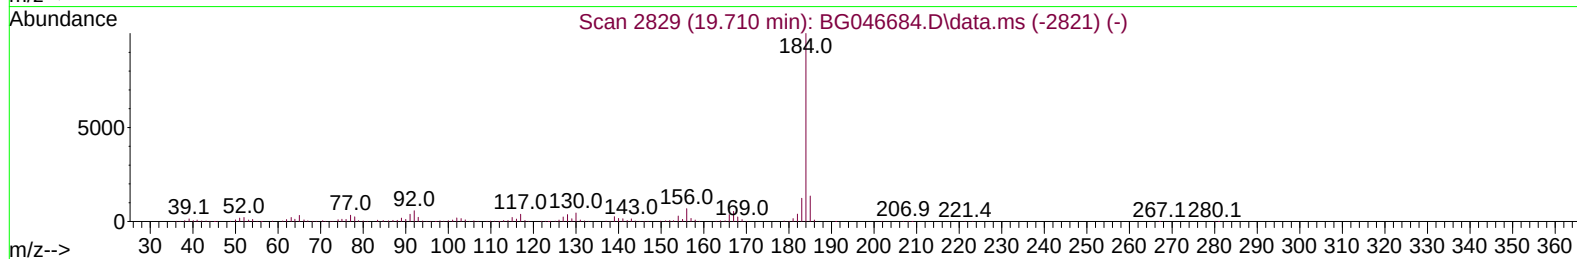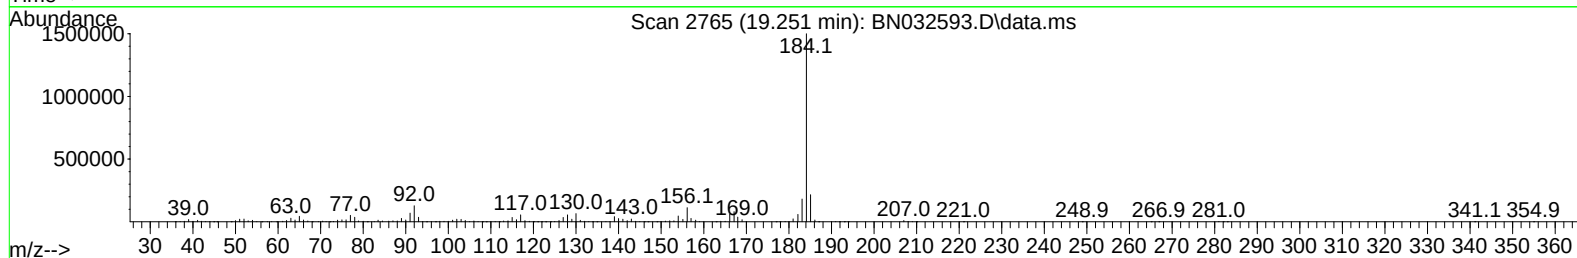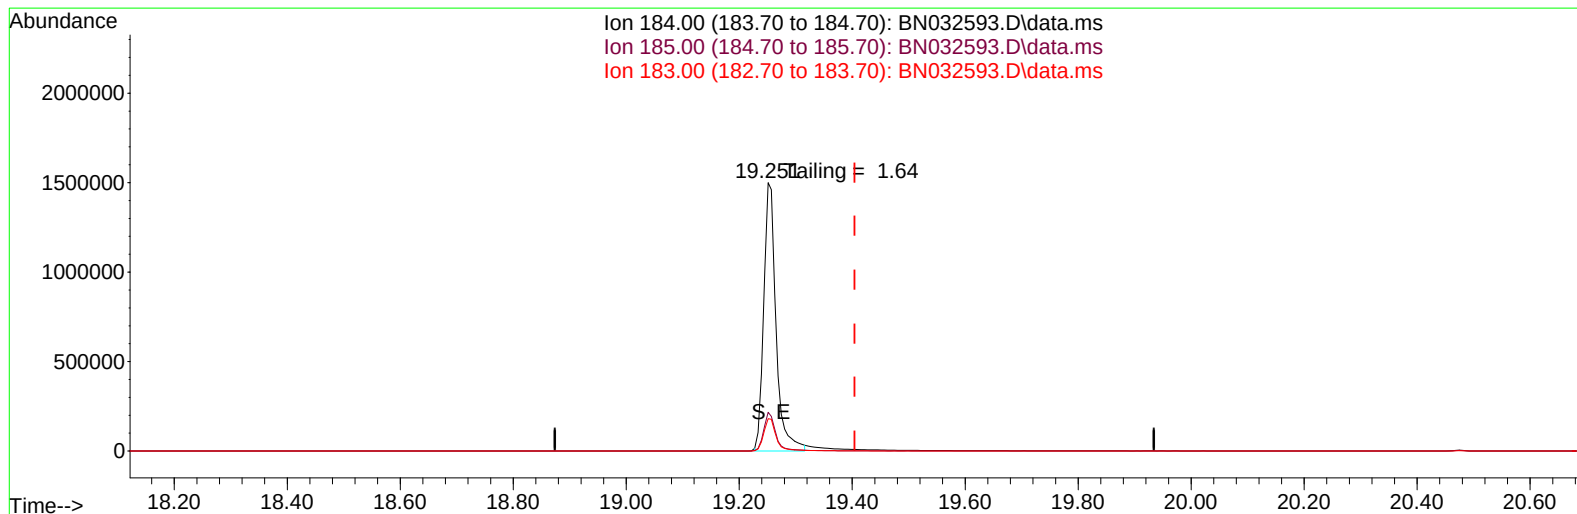

TIC: BN032593.D\data.ms

(77) Benzidine

19.251min (-0.153) 0.00 ng

response 2409899

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/9/2024	BNA_N	<u>BN032593.D</u>
Compound Name	Response	Retention Time
DDT	1351078	20.475
DDD	14836	20.08
DDE	554	19.522
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15390	1366468	1.13

Instrument :
BNA_N
ClientSampleId :
DFTPP