


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071020\
 Data File : BN011131.D
 Acq On : 09 Jul 2020 14:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 09 15:33:27 2020

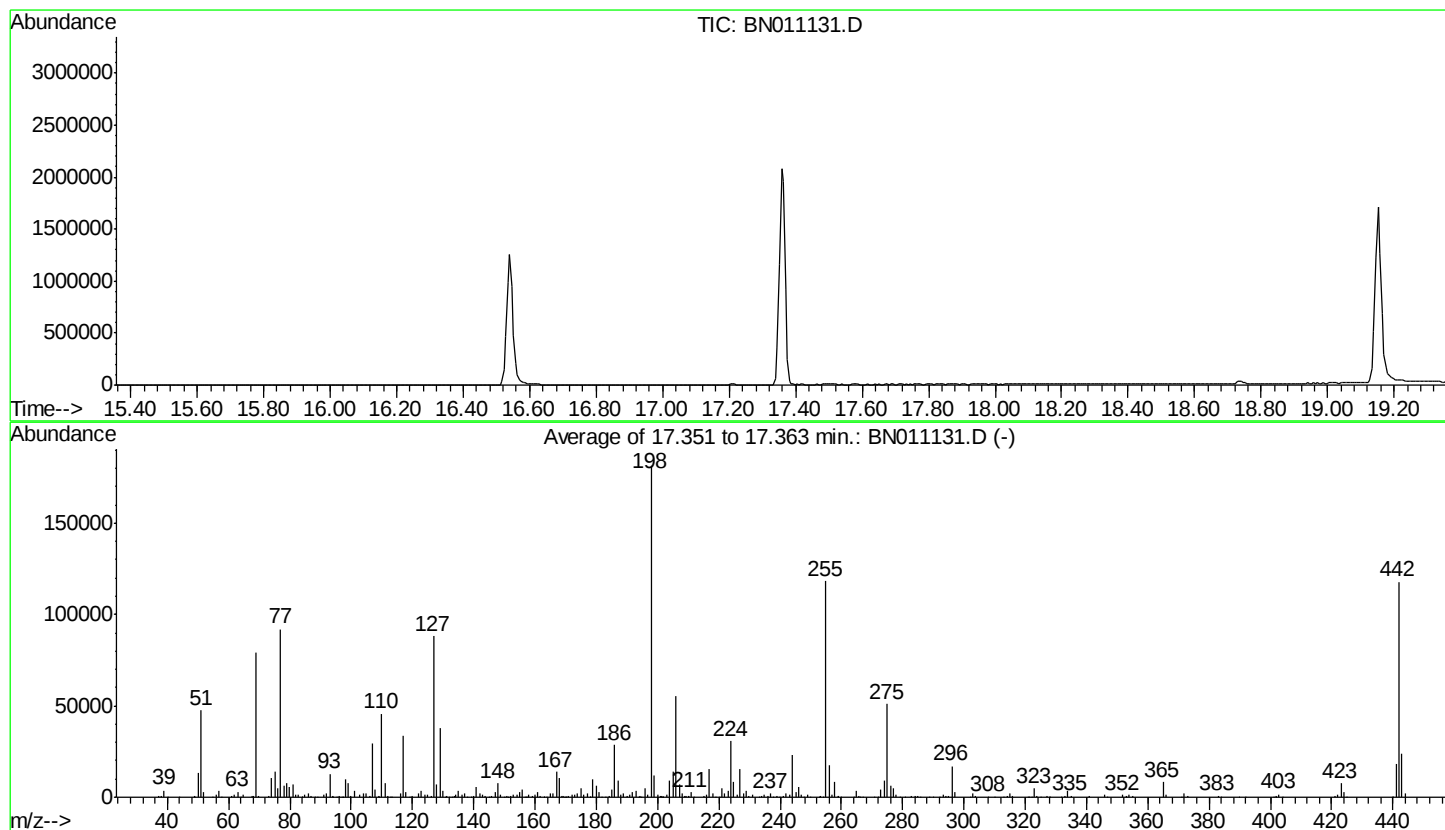

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.1	47338	PASS
68	69	0.00	2	1.2	950	PASS
69	198	0.00	100	43.6	79146	PASS
70	69	0.00	2	0.7	564	PASS
127	198	10	80	48.6	88237	PASS
197	198	0.00	2	0.7	1235	PASS
198	198	100	100	100.0	181405	PASS
199	198	5	9	6.7	12149	PASS
275	198	10	60	28.1	50904	PASS
365	198	1	100	4.5	8093	PASS
441	198	0.01	100	10.1	18333	PASS
442	198	50	100	65.1	118016	PASS
443	442	15	24	20.3	23914	PASS