
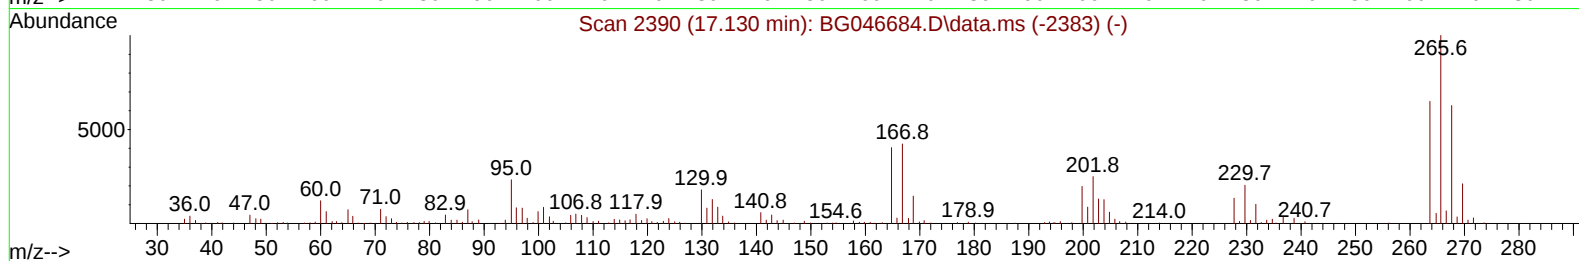
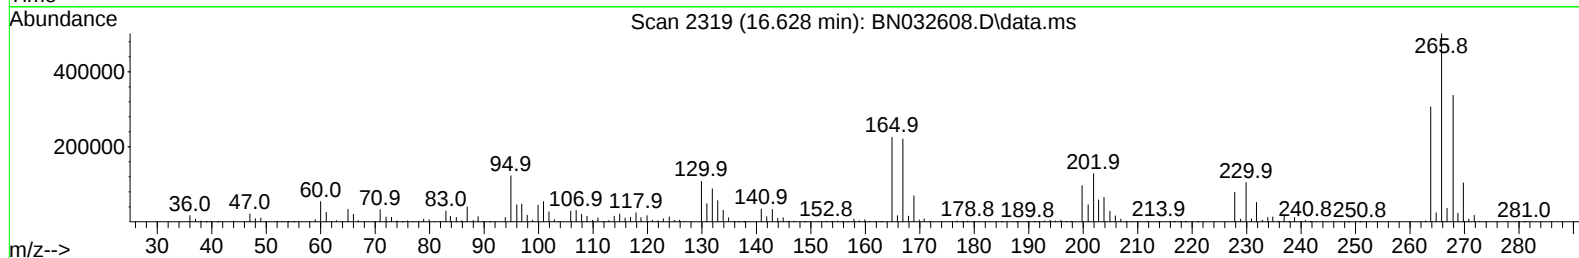


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071024\
Data File : BN032608.D
Acq On : 10 Jul 2024 08:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 20:05:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

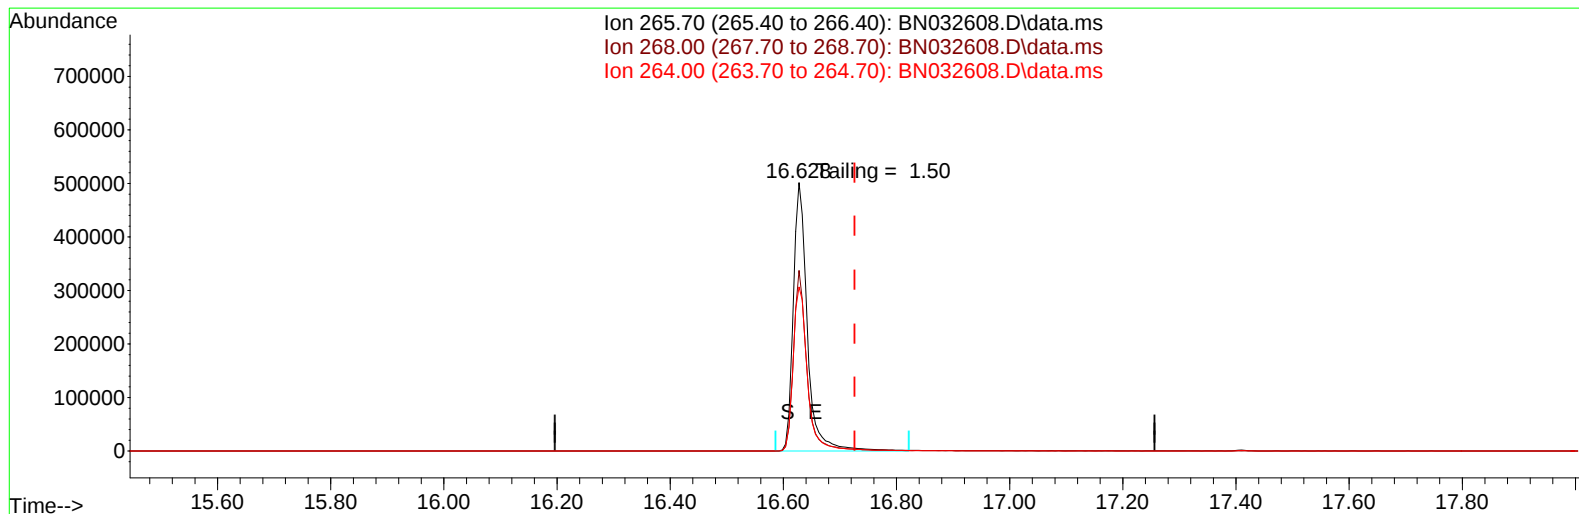

TIC: BN032608.D\data.ms

(70) Pentachlorophenol (C)




16.628min (-0.098) 27615.30 ng

response 869039

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.23
264.00	61.60	61.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071024\
Data File : BN032608.D
Acq On : 10 Jul 2024 08:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 20:05:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

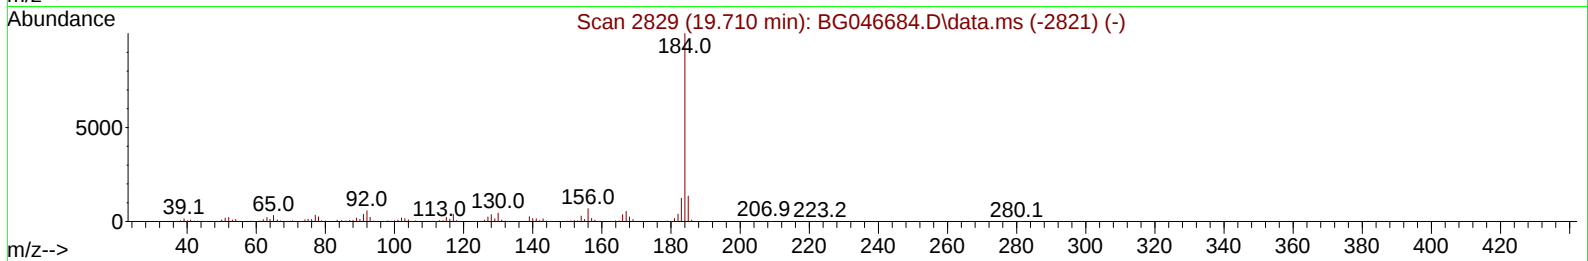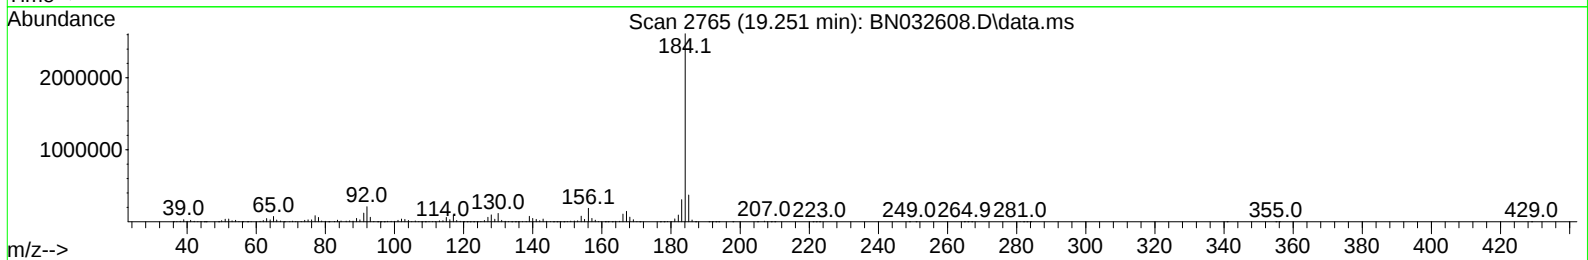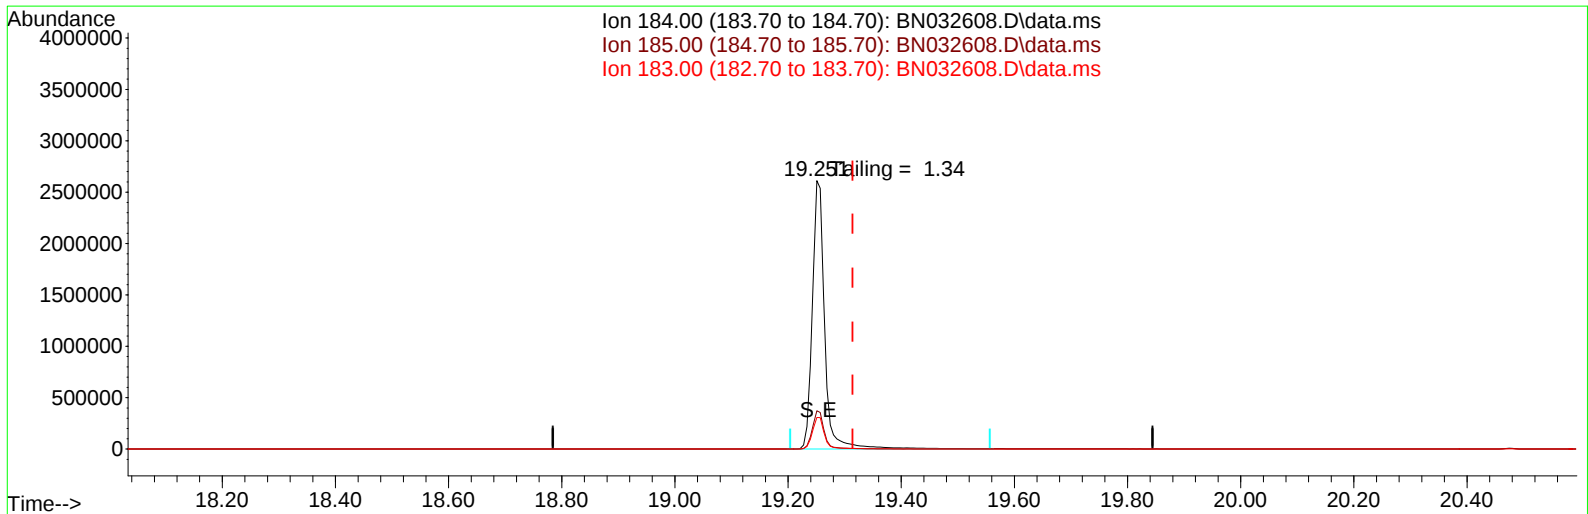

TIC: BN032608.D\data.ms

(77) Benzidine

19.251min (-0.063) 0.00 ng

response 3966449

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.24
183.00	13.20	11.75
0.00	0.00	0.00