


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071024\
Data File : BN032608.D
Acq On : 10 Jul 2024 08:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 02:39:48 2024

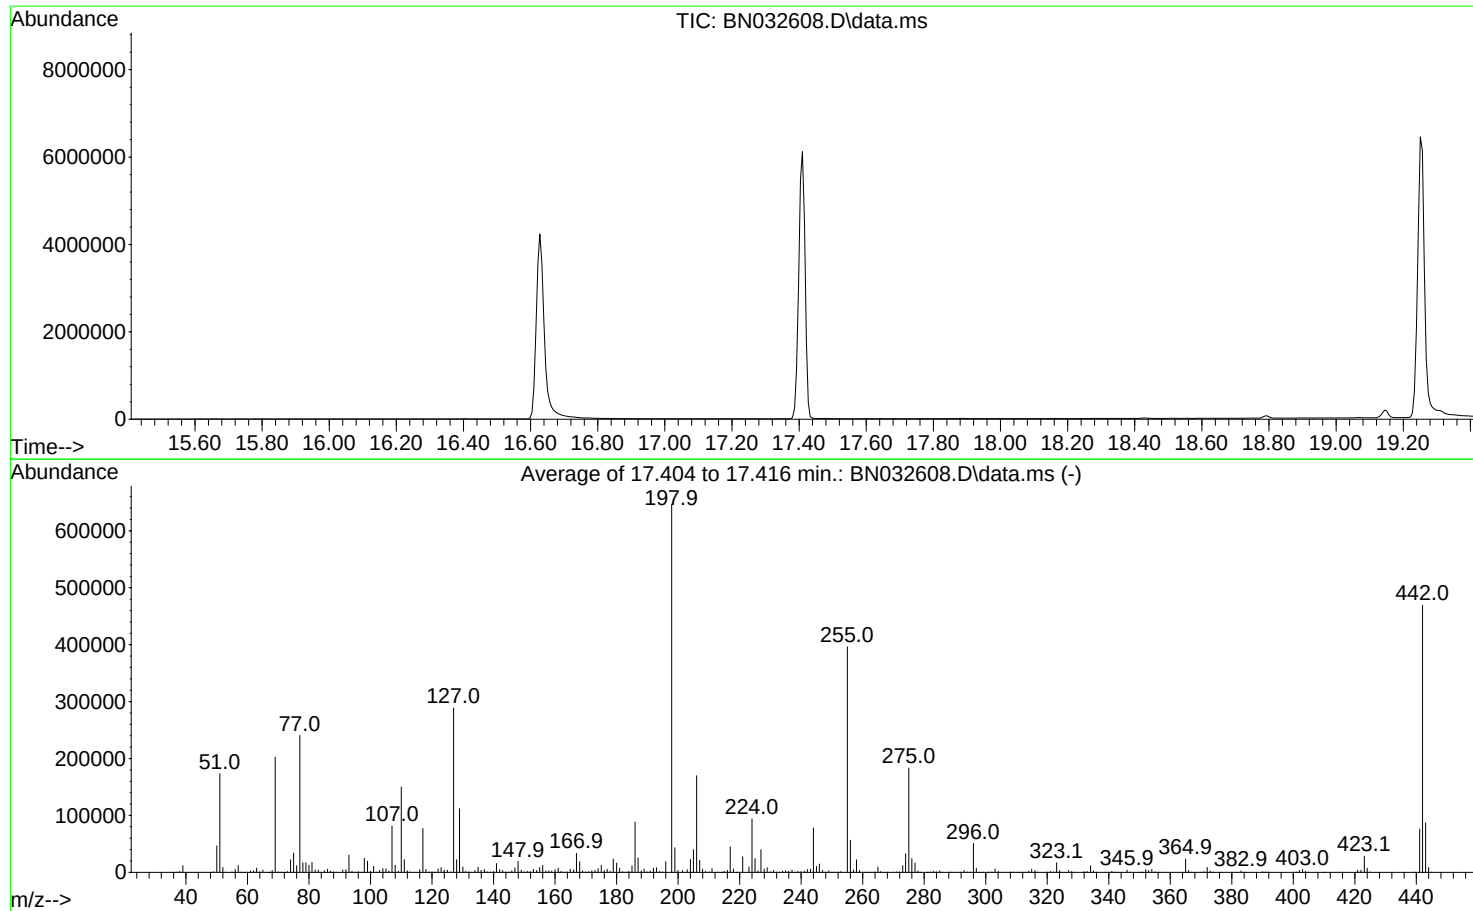

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	173563	PASS
68	69	0.00	2	1.7	3436	PASS
69	198	0.00	100	31.3	202347	PASS
70	69	0.00	2	0.5	1003	PASS
127	198	10	80	44.7	288619	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	646336	PASS
199	198	5	9	6.7	43168	PASS
275	198	10	60	28.4	183381	PASS
365	198	1	100	3.6	23440	PASS
441	198	0.01	100	11.8	76333	PASS
442	442	50	100	100.0	469269	PASS
443	442	15	24	18.5	86960	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/10/2024	BNA_N	<u>BN032608.D</u>
Compound Name	Response	Retention Time
DDT	2163225	20.474
DDD	27039	20.08
DDE	1170	19.522
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28209	2191434	1.29

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071024\
Data File : BN032608.D
Acq On : 10 Jul 2024 08:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 10 20:05:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

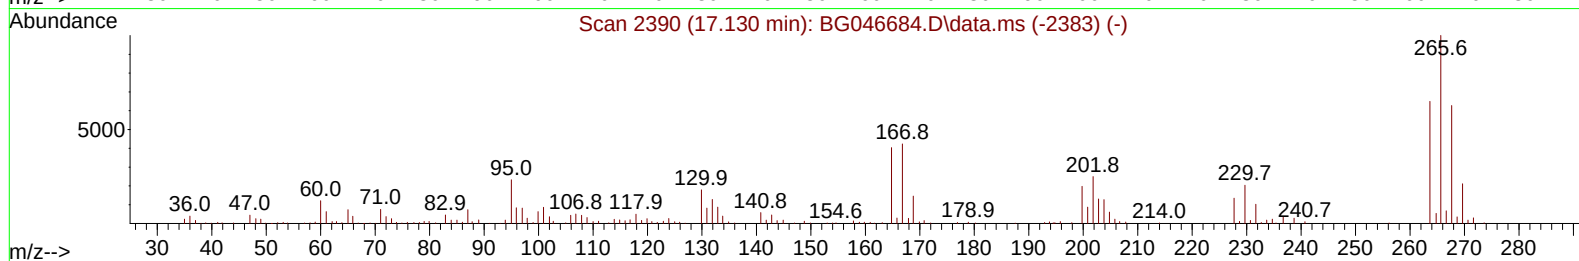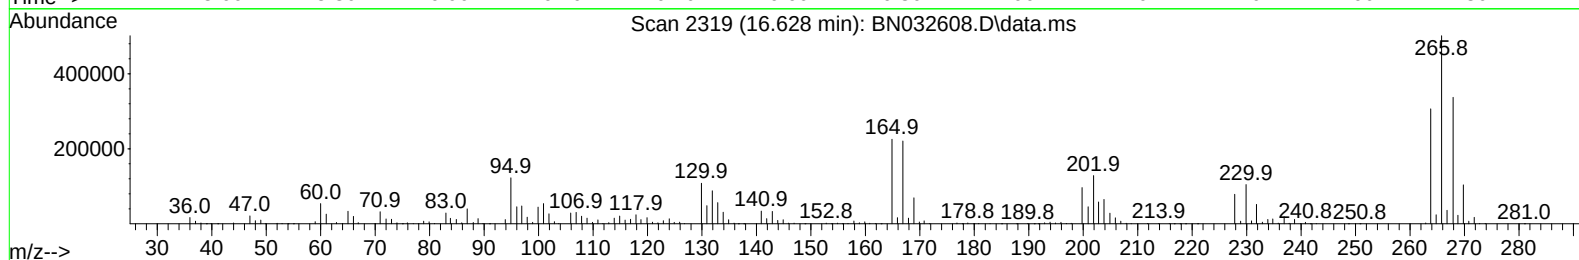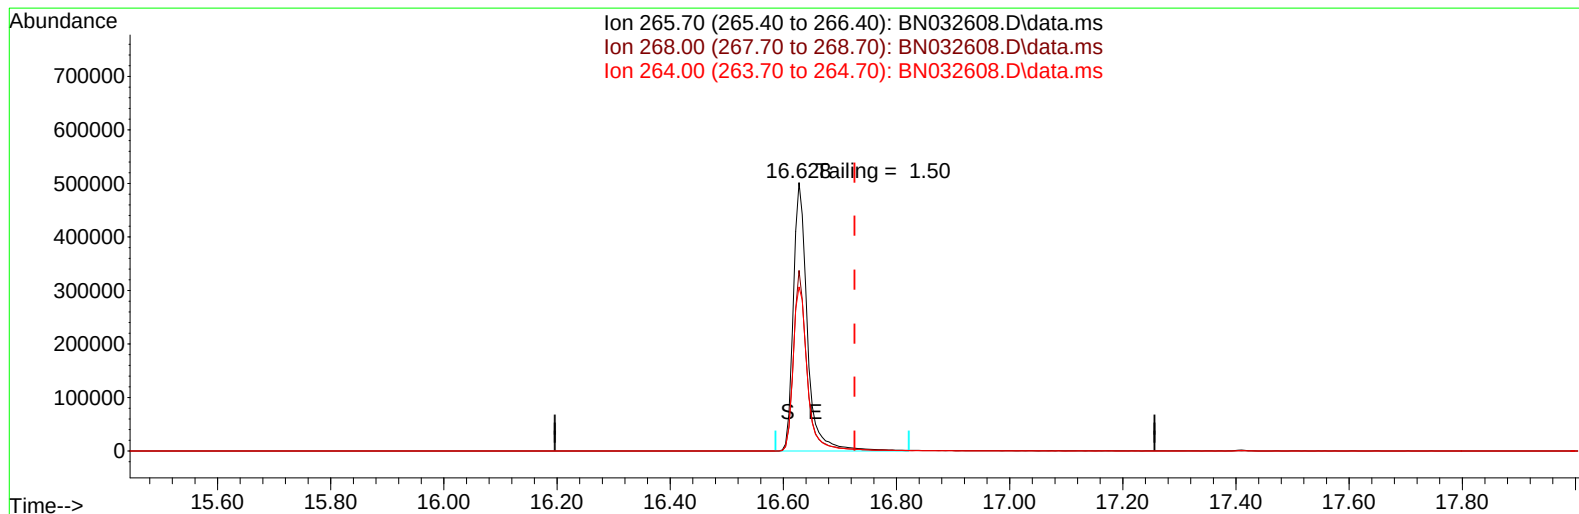

TIC: BN032608.D\data.ms

(70) Pentachlorophenol (C)

16.628min (-0.098) 27615.30 ng




response 869039

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.23
264.00	61.60	61.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071024\
Data File : BN032608.D
Acq On : 10 Jul 2024 08:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 10 20:05:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

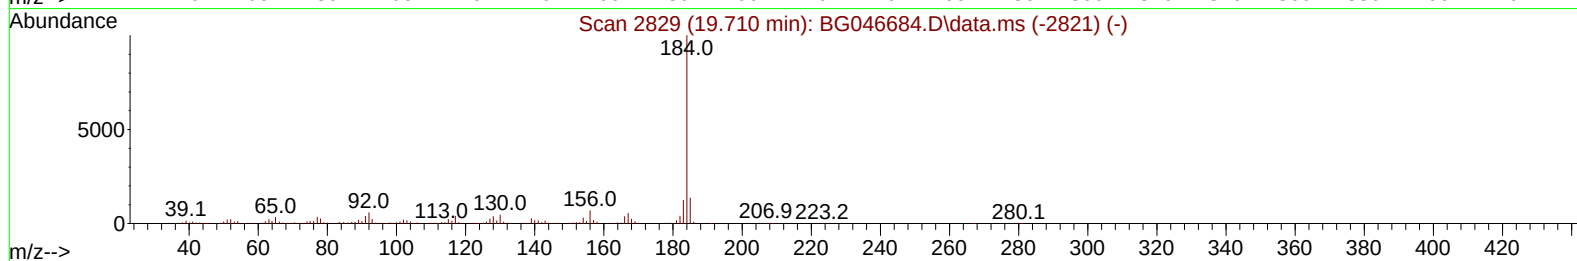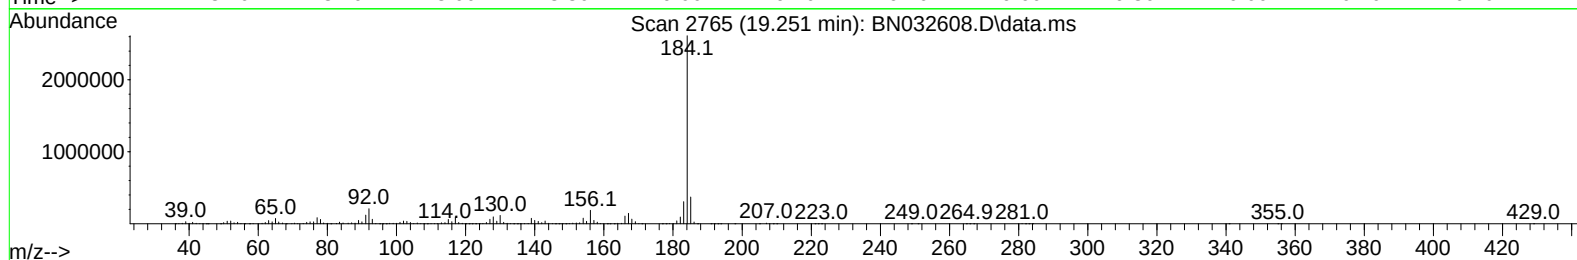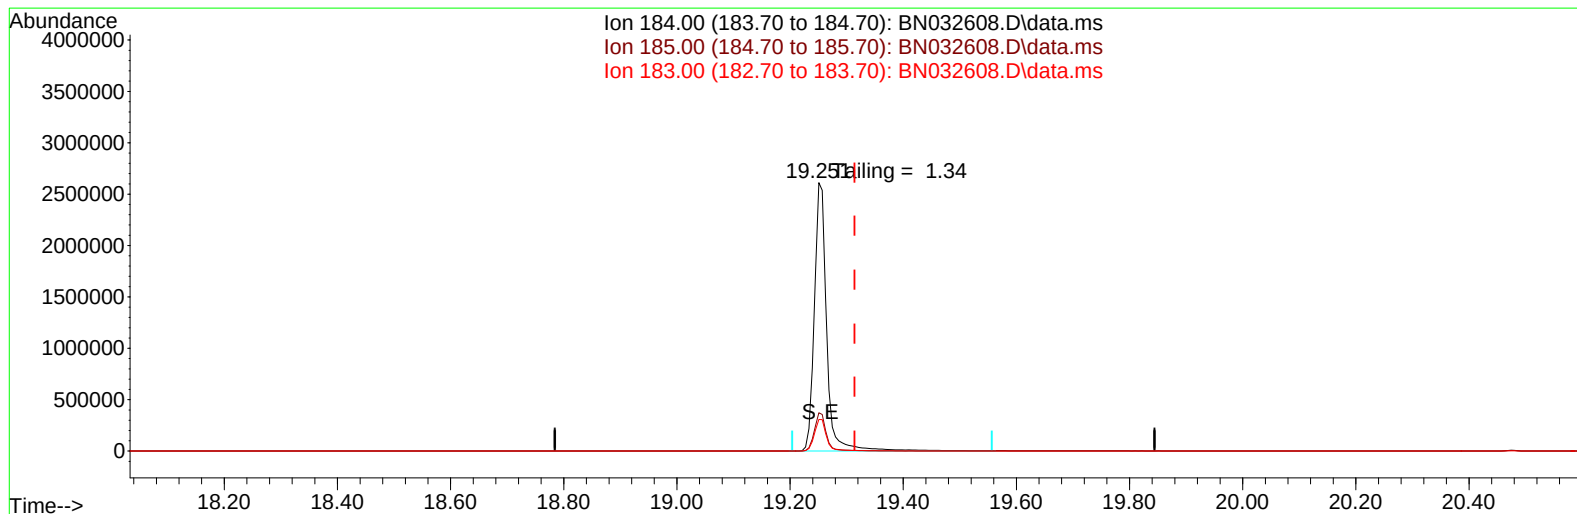

TIC: BN032608.D\data.ms

(77) Benzidine

19.251min (-0.063) 0.00 ng

response 3966449

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.24
183.00	13.20	11.75
0.00	0.00	0.00