


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071025\
Data File : BN037452.D
Acq On : 10 Jul 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN070925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 10 00:48:38 2025

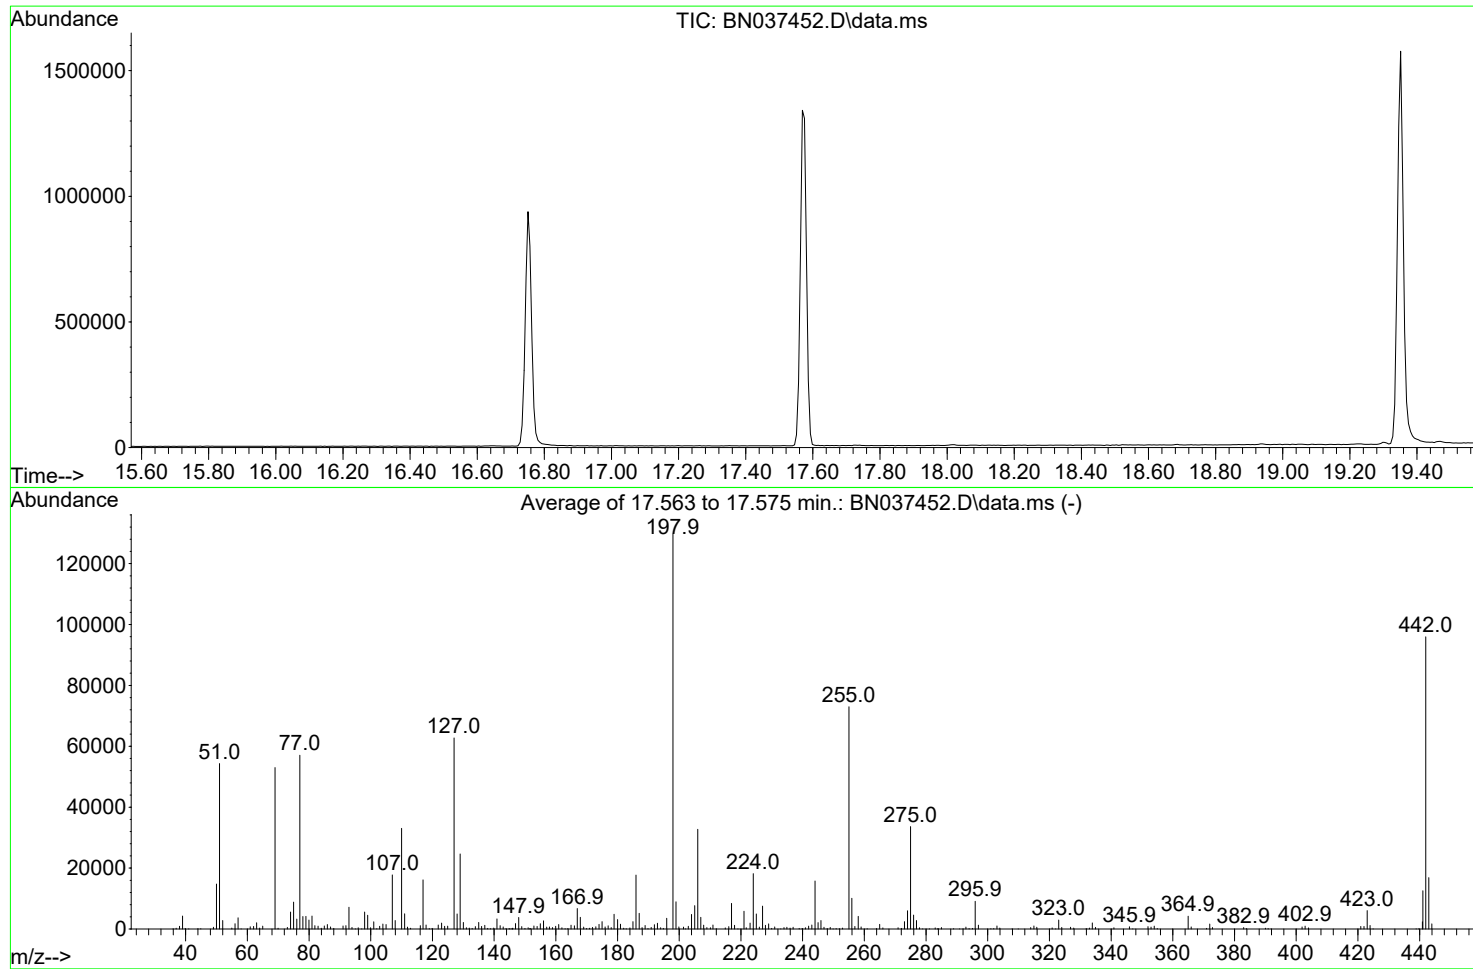

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	53035	PASS
70	69	0.00	2	0.5	282	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	129669	PASS
199	198	5	9	6.9	8956	PASS
365	198	1	100	3.2	4192	PASS
441	443	0.01	150	74.6	12576	PASS
442	442	100	100	100.0	95971	PASS
443	442	15	24	17.6	16859	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/10/2025	BNA_N	<u>BN037452.D</u>
Compound Name	Response	Retention Time
DDT	263840	20.598
DDD	2930	20.157
DDE	271	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3201	267041	1.20

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071025\
Data File : BN037452.D
Acq On : 10 Jul 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 10 17:51:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

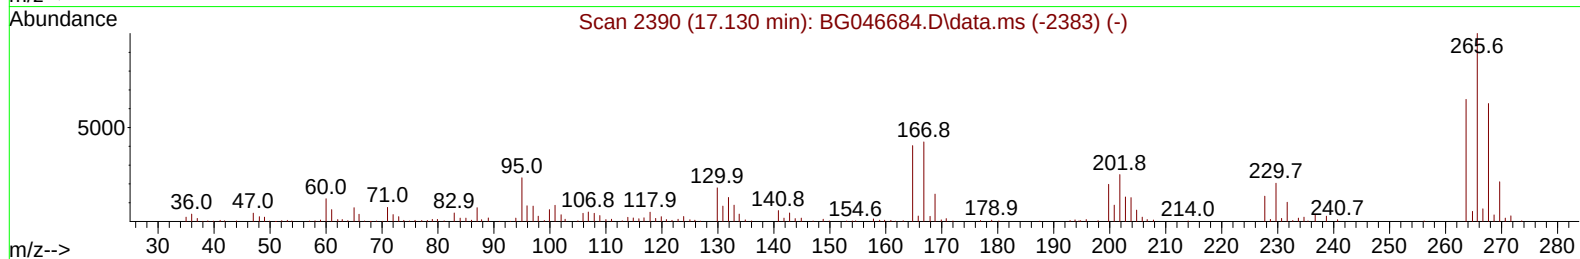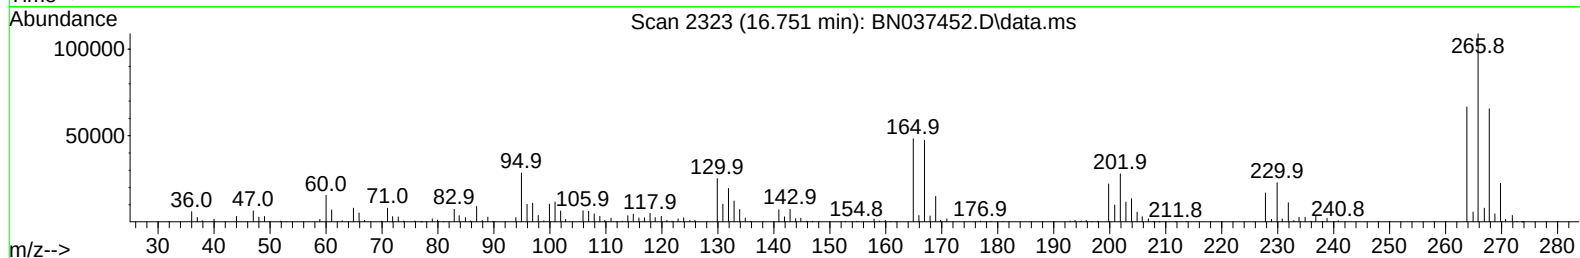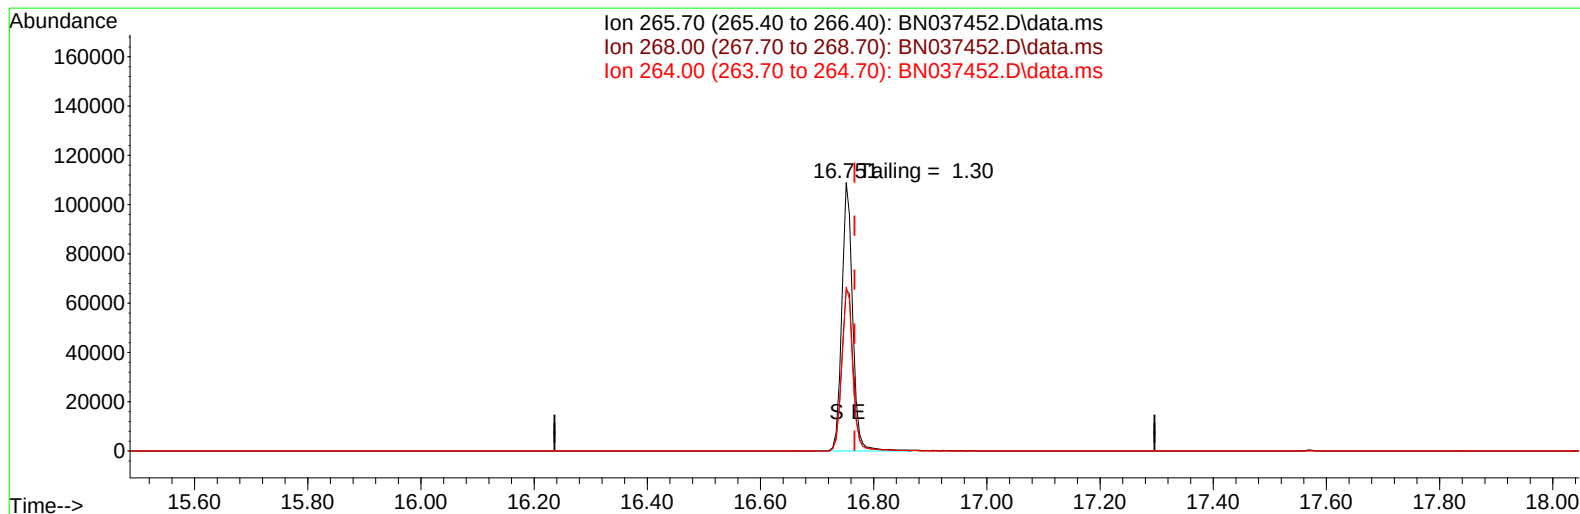

TIC: BN037452.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.015) 24354.64 ng




response 145067

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.16
264.00	61.60	61.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071025\
Data File : BN037452.D
Acq On : 10 Jul 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 10 17:51:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

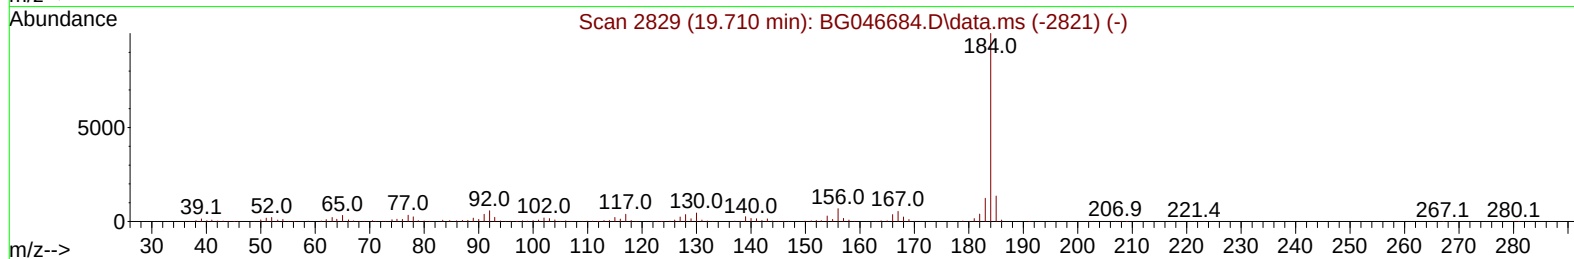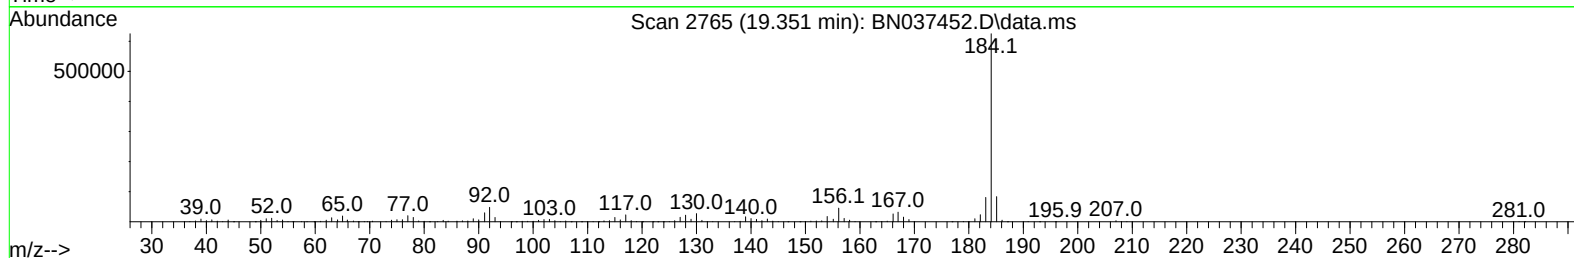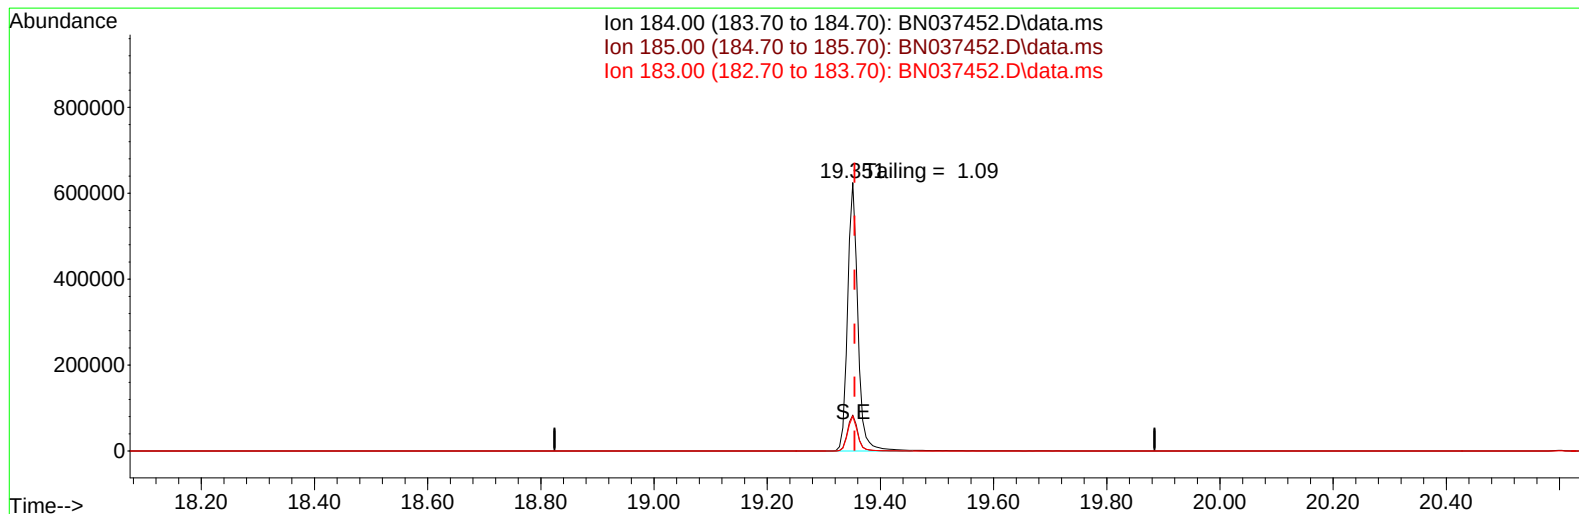

TIC: BN037452.D\data.ms

(77) Benzidine

19.351min (-0.003) 0.00 ng

response 789432

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.42
183.00	13.20	12.94
0.00	0.00	0.00