
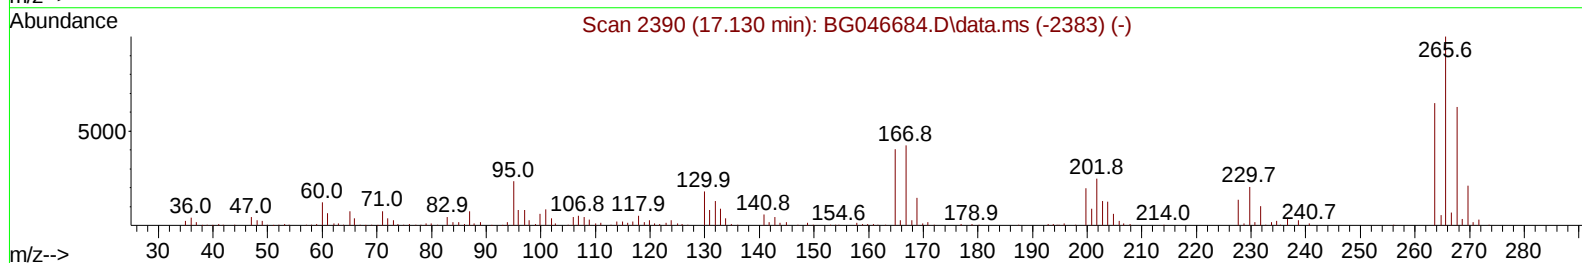
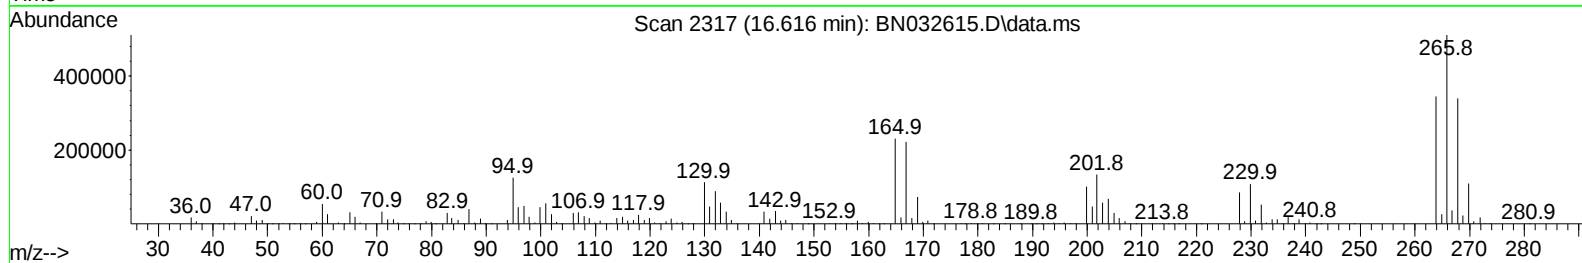


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071124\
Data File : BN032615.D
Acq On : 10 Jul 2024 15:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 03:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration



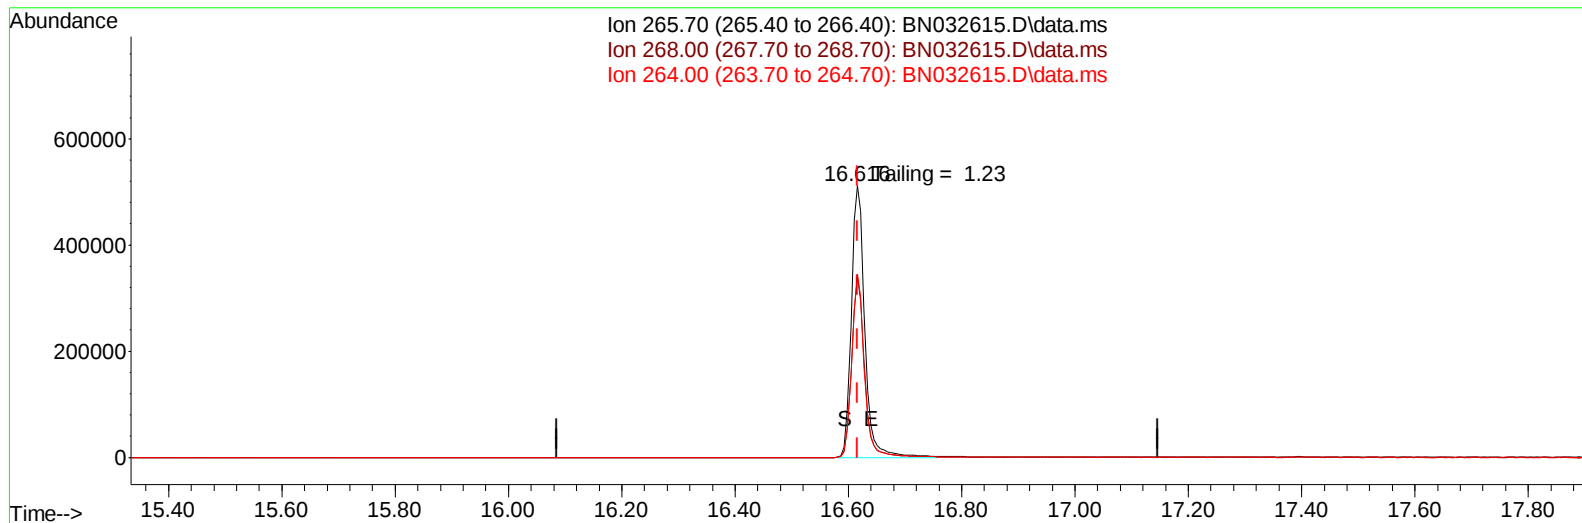


TIC: BN032615.D\data.ms

(70) Pentachlorophenol (C)**16.616min (0.000) 28100.93 ng****response 854109**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.51
264.00	61.60	67.53
0.00	0.00	0.00

Quant Time: Jul 11 03:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

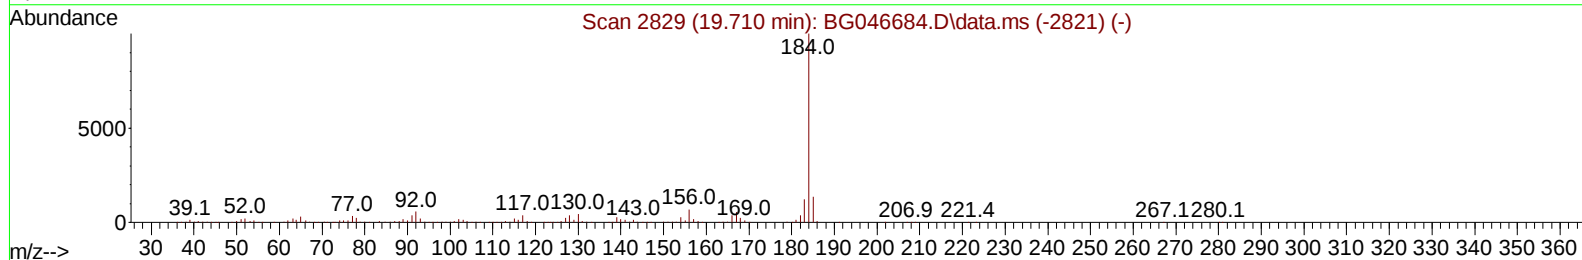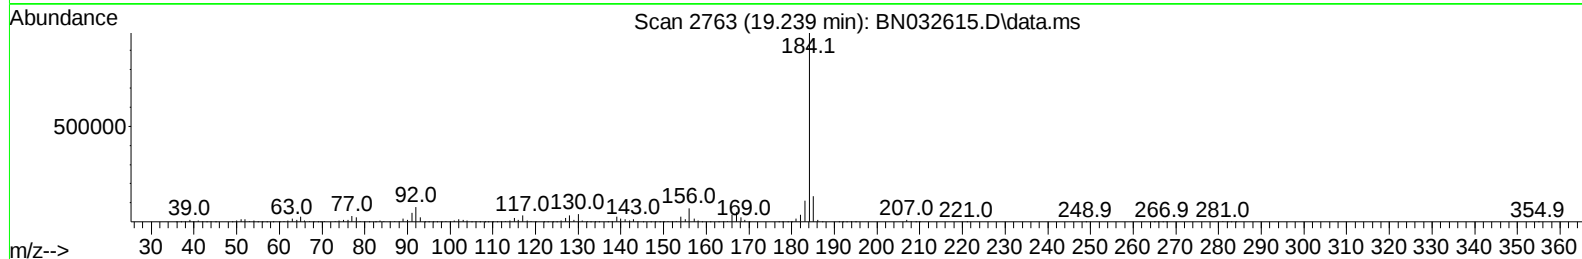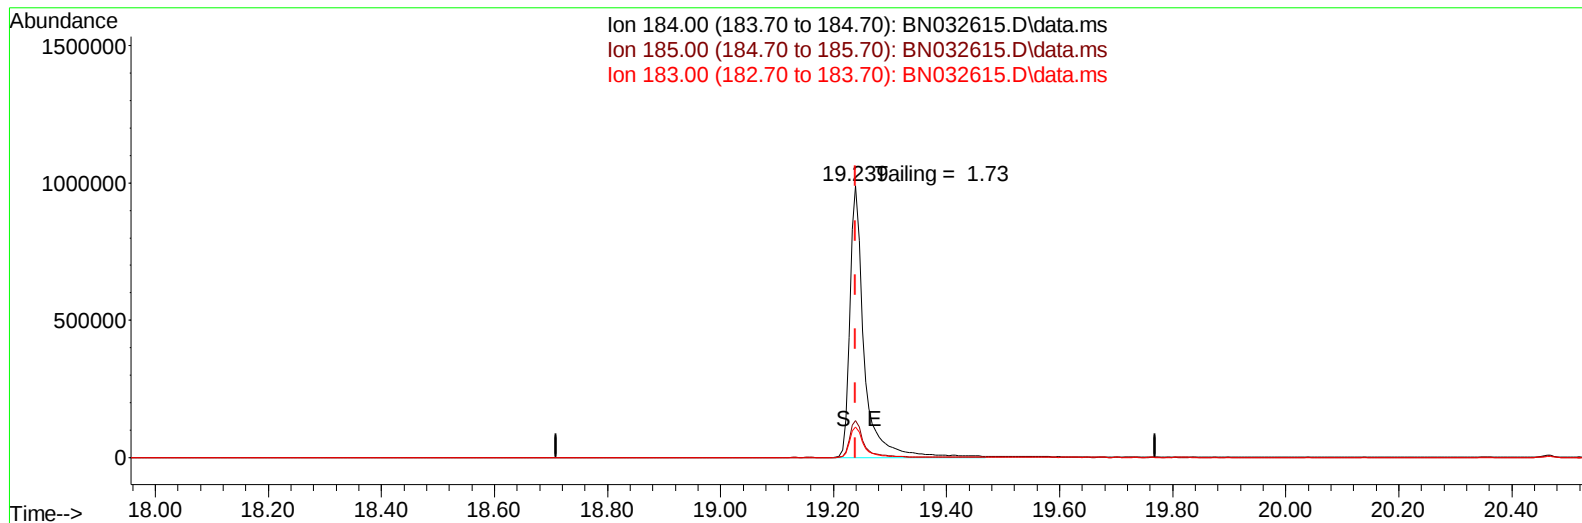

TIC: BN032615.D\data.ms

(77) Benzidine

19.239min (0.000) 190151.31 ng

response **1752584**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.21
0.00	0.00	0.00