
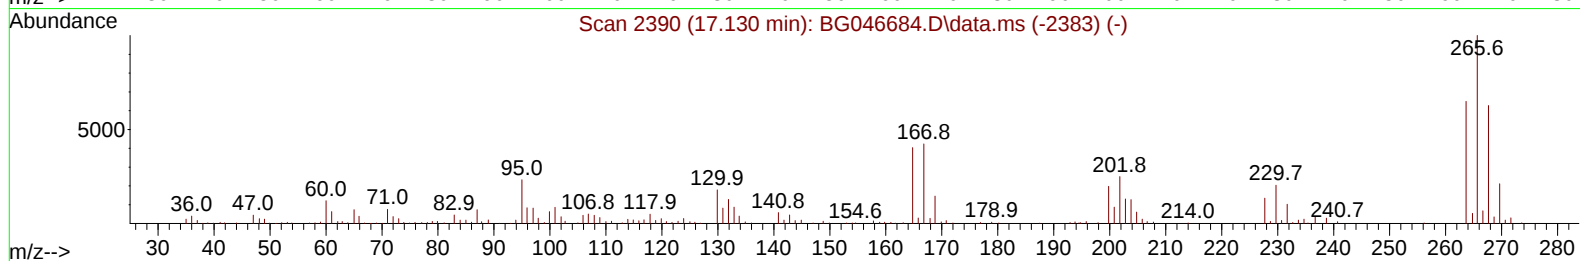
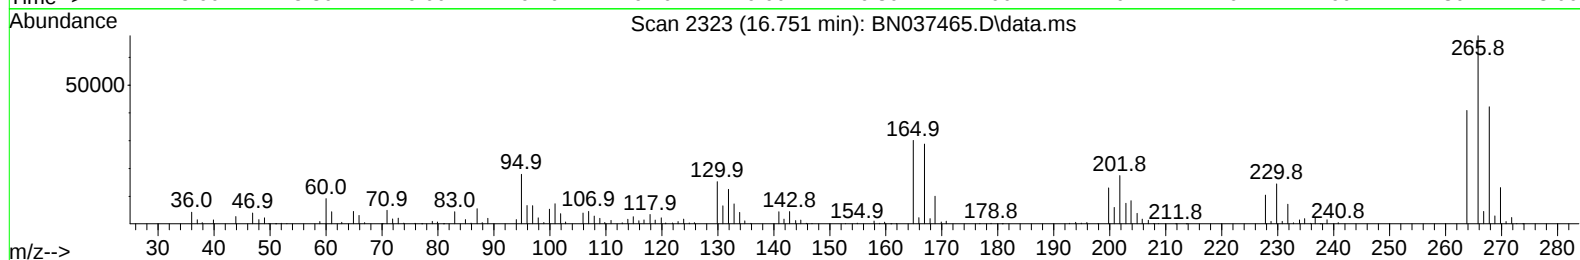


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071125\
Data File : BN037465.D
Acq On : 11 Jul 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 16:46:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

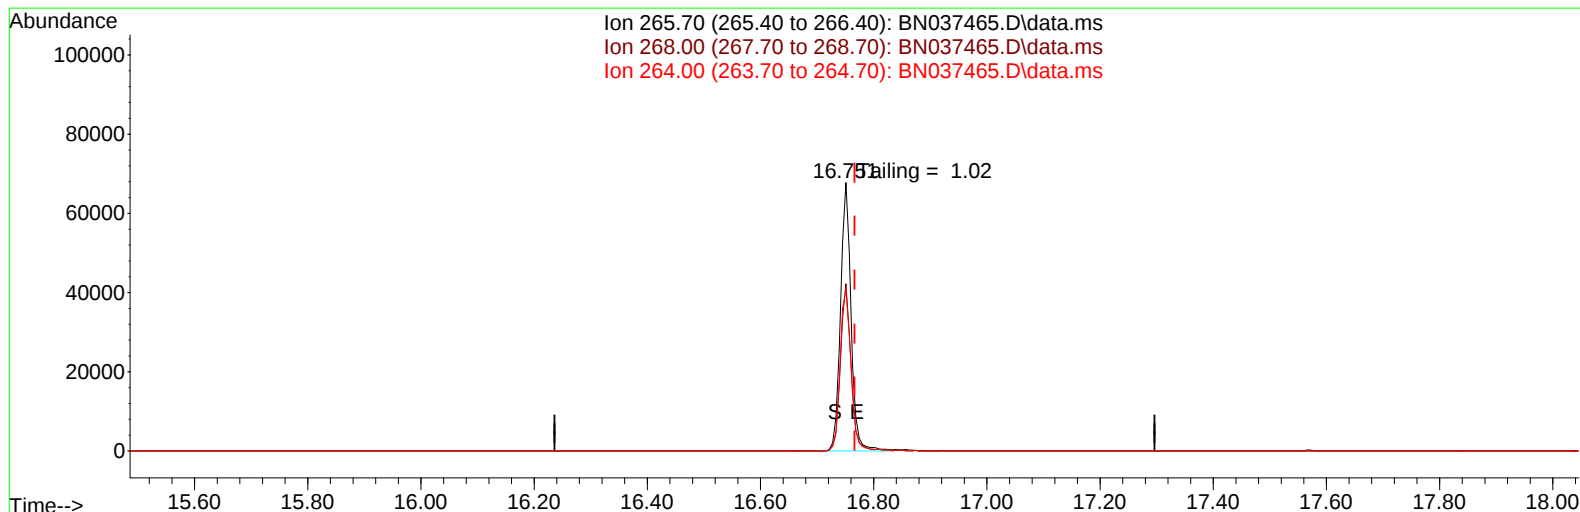

TIC: BN037465.D\data.ms

(70) Pentachlorophenol (C)




16.751min (-0.015) 19733.94 ng

response 87345

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.30
264.00	61.60	60.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071125\
Data File : BN037465.D
Acq On : 11 Jul 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 16:46:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

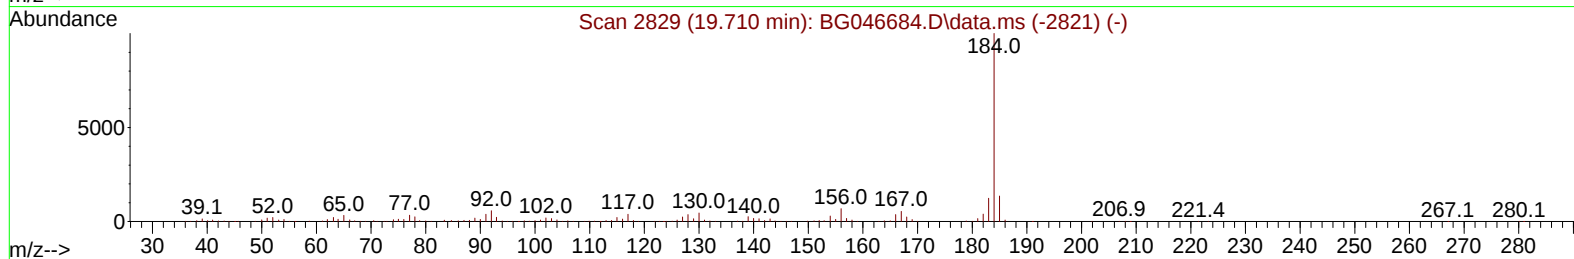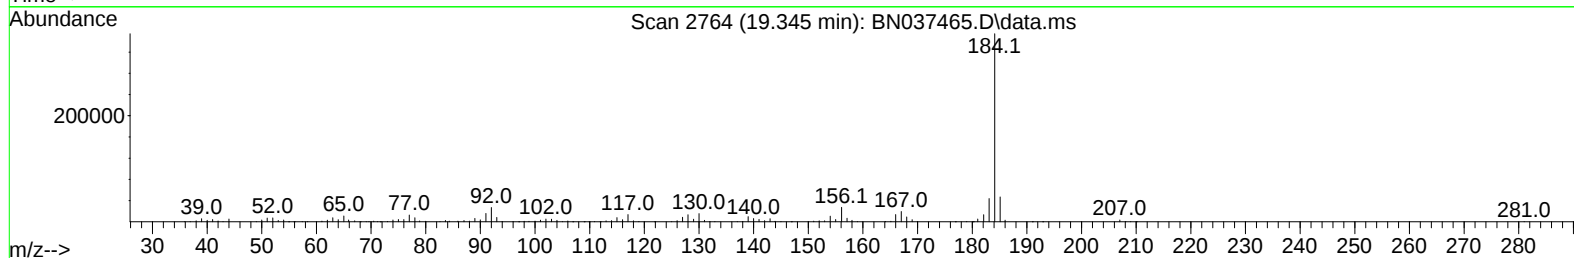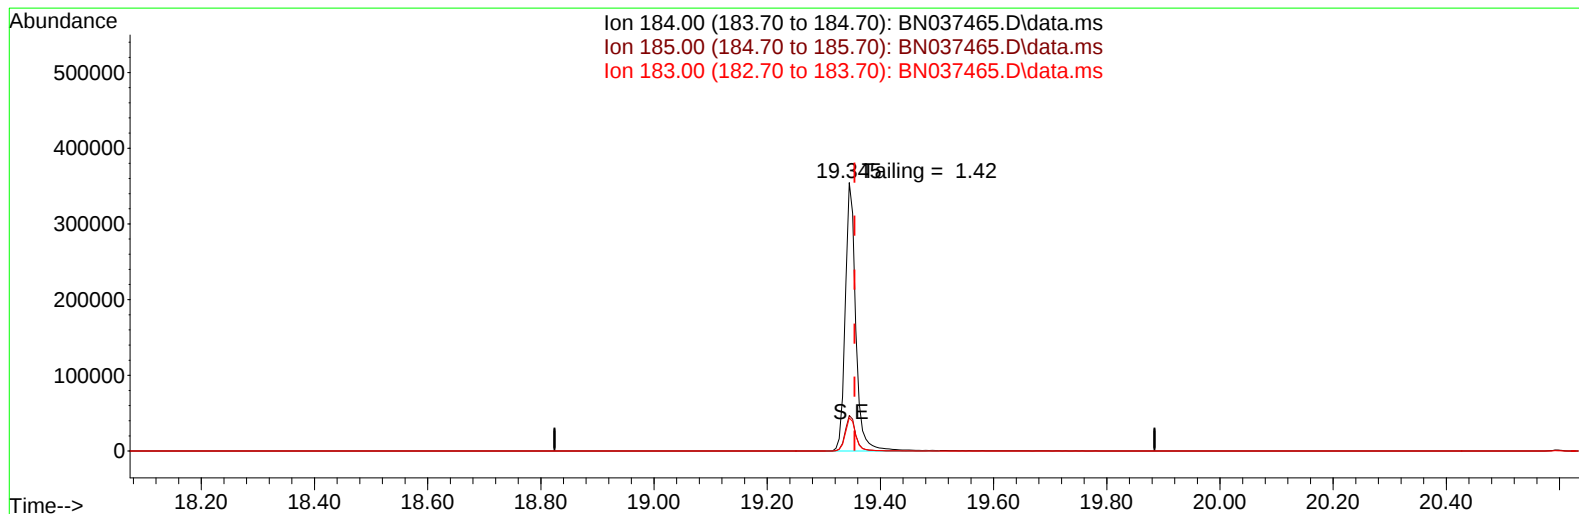

TIC: BN037465.D\data.ms

(77) Benzidine

19.345min (-0.009) 0.00 ng

response 460569

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.26
183.00	13.20	12.35
0.00	0.00	0.00