


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071320\
 Data File : BN011149.D
 Acq On : 13 Jul 2020 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN071120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 11:25:24 2020

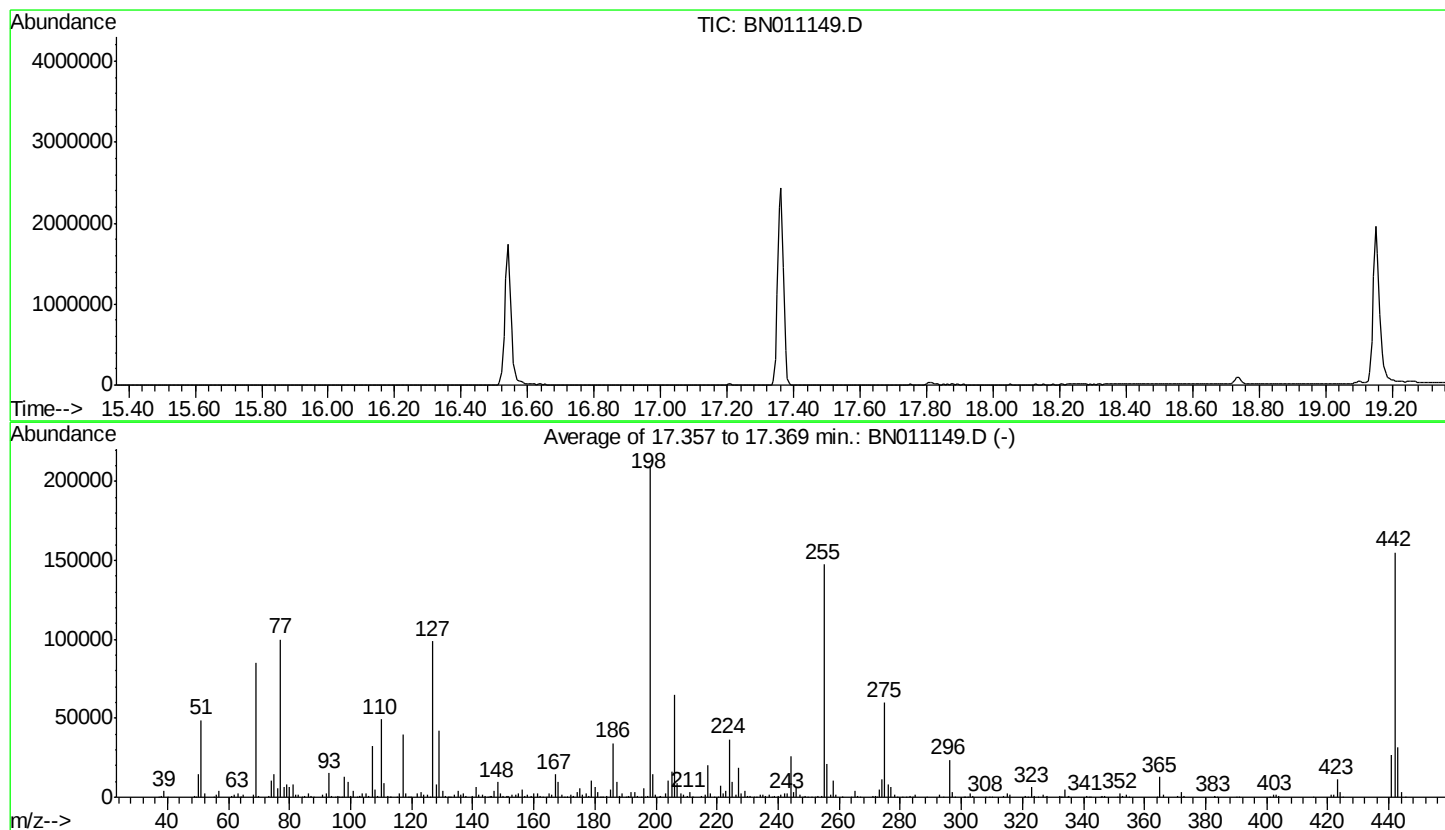

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.3	48978	PASS
68	69	0.00	2	2.0	1676	PASS
69	198	0.00	100	40.5	85085	PASS
70	69	0.00	2	0.6	528	PASS
127	198	10	80	46.9	98658	PASS
197	198	0.00	2	0.3	599	PASS
198	198	100	100	100.0	210154	PASS
199	198	5	9	6.8	14230	PASS
275	198	10	60	28.5	59946	PASS
365	198	1	100	6.0	12663	PASS
441	198	0.01	100	12.9	27130	PASS
442	198	50	100	73.8	155154	PASS
443	442	15	24	20.4	31589	PASS