

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071322\
 Data File : BN020727.D
 Acq On : 13 Jul 2022 13:27
 Operator : CG/JU
 Sample : PB146171BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK171

Quant Time: Jul 14 03:11:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 02 00:47:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	4433	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.612	136	13791	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.470	164	8855	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.222	188	17372	0.400	ng/ul	-0.01
17) Chrysene-d12	21.441	240	10948	0.400	ng/ul	0.00
23) Perylene-d12	23.786	264	10292	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	26878	5.234	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	5089	0.225	ng/ul	0.00
18) Fluoranthene-d10	19.263	212	11779	0.326	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.626	202	1661	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.631	252	2701	0.062	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071322\
Data File : BN020727.D
Acq On : 13 Jul 2022 13:27
Operator : CG/JU
Sample : PB146171BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK171

Quant Time: Jul 14 03:11:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 00:47:40 2022
Response via : Initial Calibration




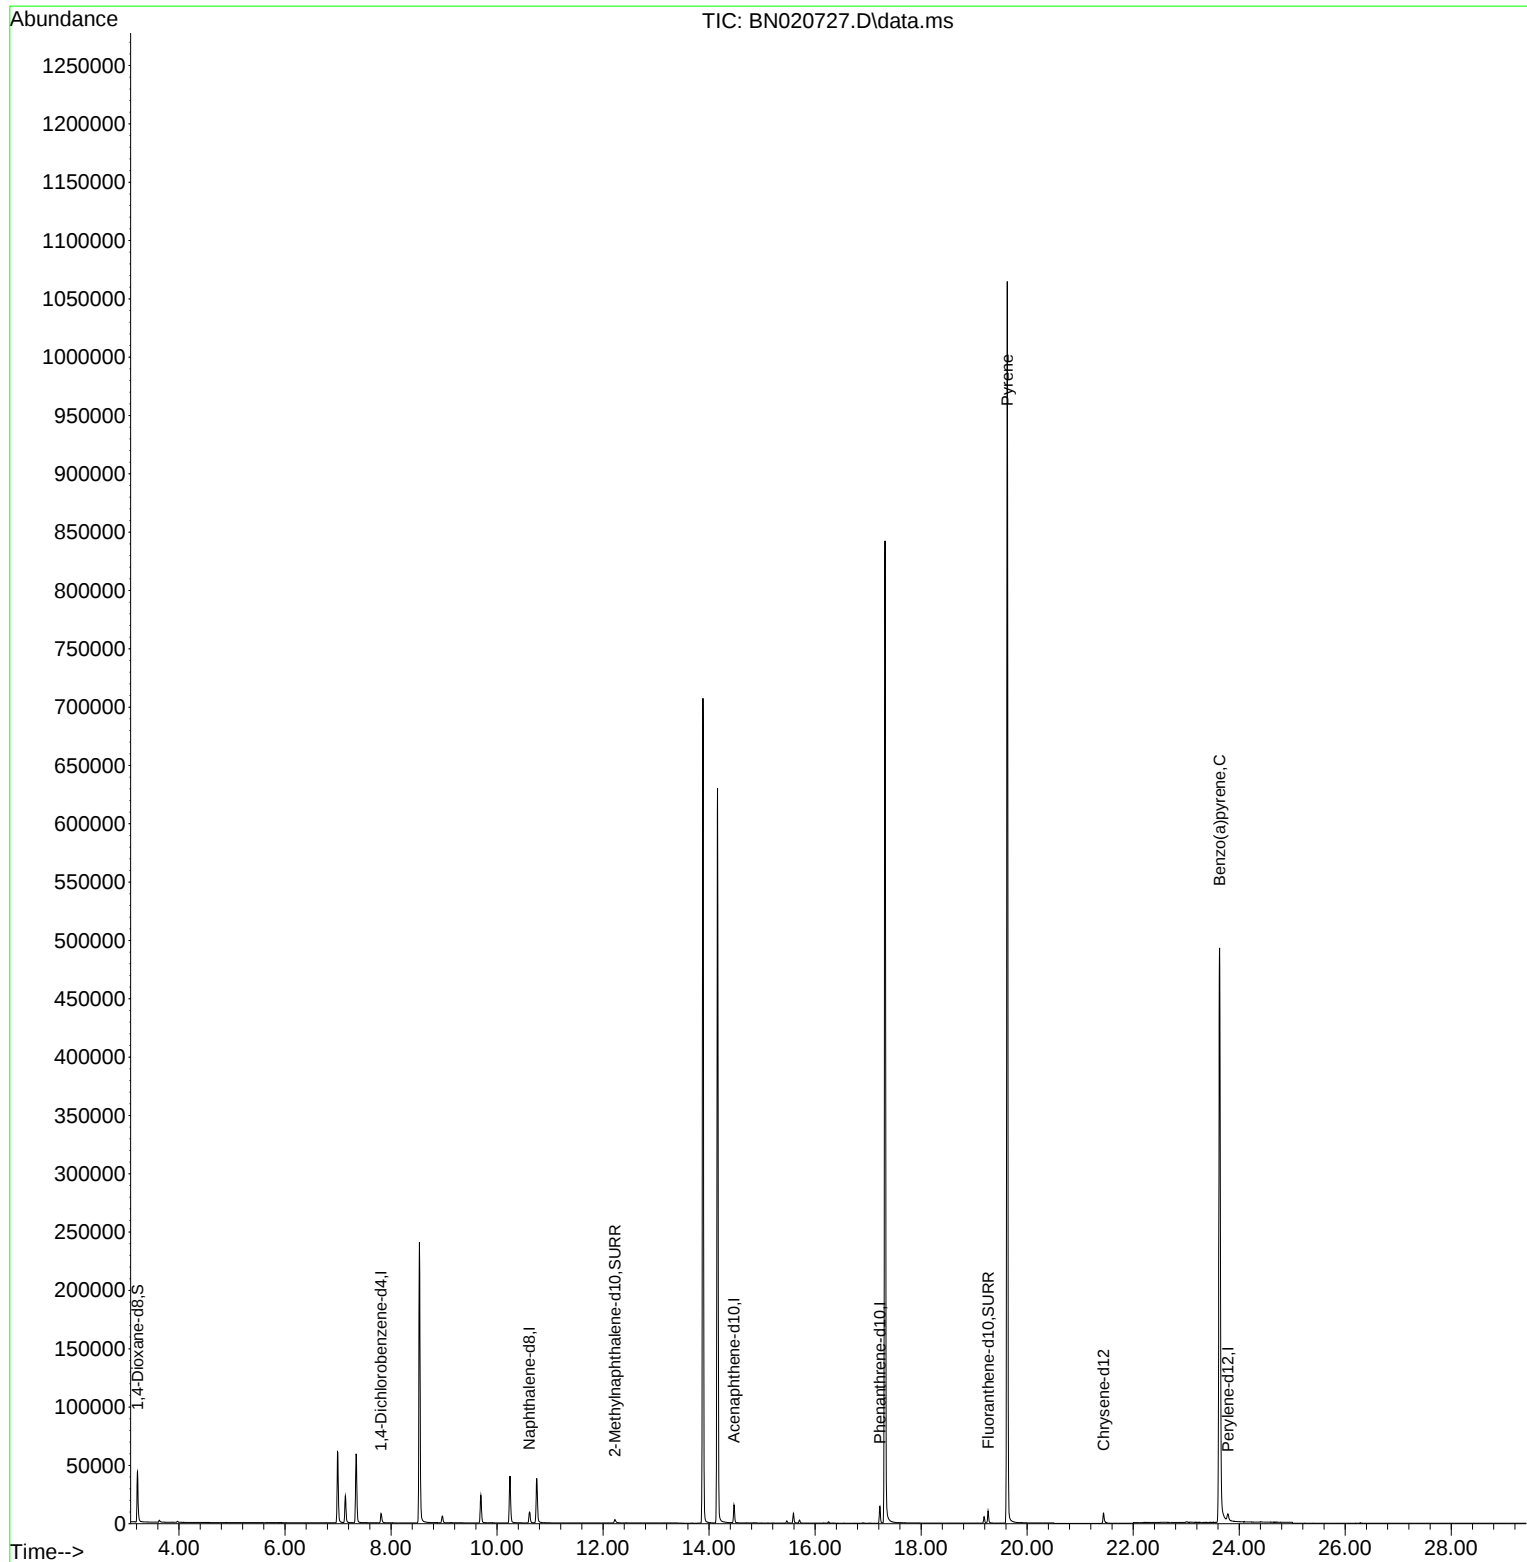


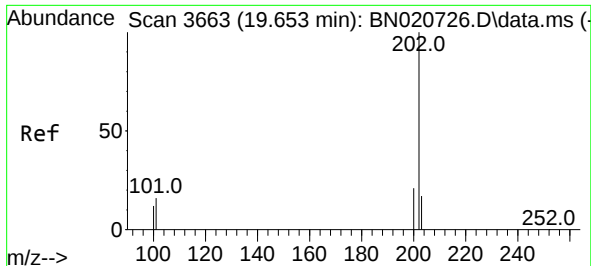

#20
Pyrene
Concen: 0.032 ng/ul
RT: 19.626 min Scan# 3657
Delta R.T. -0.041 min
Lab File: BN020727.D
Acq: 13 Jul 2022 13:27

Instrument :
BNA_N
ClientSampleId :
SBLK171

Tgt Ion:202 Resp: 1661
Ion Ratio Lower Upper
202 100
101 174.1 11.6 17.4#
100 1258.4 9.2 13.8#

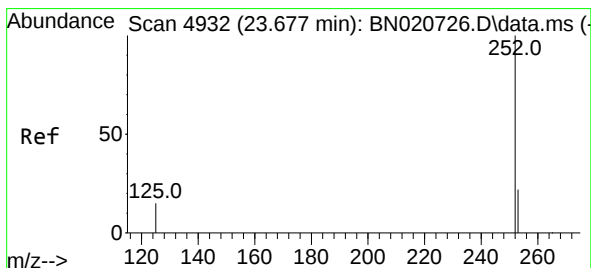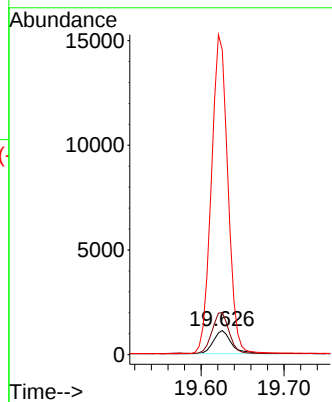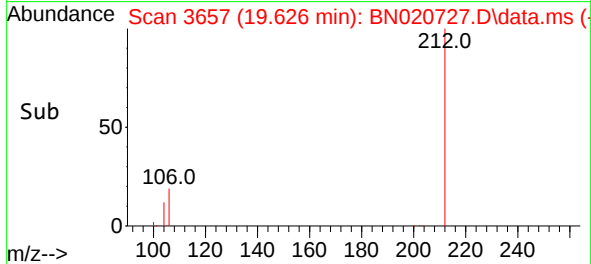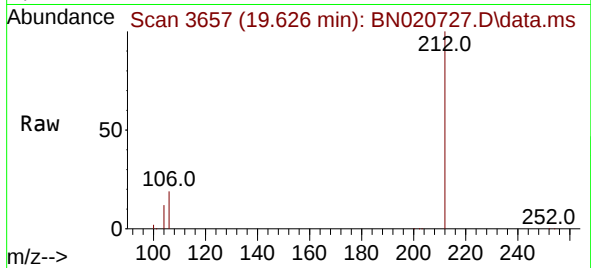

#26
Benzo(a)pyrene
Concen: 0.062 ng/ul
RT: 23.631 min Scan# 4916
Delta R.T. -0.066 min
Lab File: BN020727.D
Acq: 13 Jul 2022 13:27

Tgt Ion:252 Resp: 2701
Ion Ratio Lower Upper
252 100
253 46.0 21.0 31.4#
125 34.8 18.8 28.2#

