

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071322\
 Data File : BN020728.D
 Acq On : 13 Jul 2022 14:22
 Operator : CG/JU
 Sample : N3600-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN4

Quant Time: Jul 14 03:11:21 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 02 00:47:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	4097	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.612	136	14316	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.470	164	8881	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.221	188	17355	0.400	ng/ul	-0.01
17) Chrysene-d12	21.438	240	12168	0.400	ng/ul	0.00
23) Perylene-d12	23.785	264	10125	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	23993	5.055	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.218	152	5826	0.248	ng/ul	-0.01
18) Fluoranthene-d10	19.262	212	11531	0.287	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.464	166	1766	0.044	ng/ul#	14
20) Pyrene	19.625	202	1475	0.026	ng/ul#	1
26) Benzo(a)pyrene	23.630	252	2350	0.055	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071322\
Data File : BN020728.D
Acq On : 13 Jul 2022 14:22
Operator : CG/JU
Sample : N3600-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN4

Quant Time: Jul 14 03:11:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 00:47:40 2022
Response via : Initial Calibration




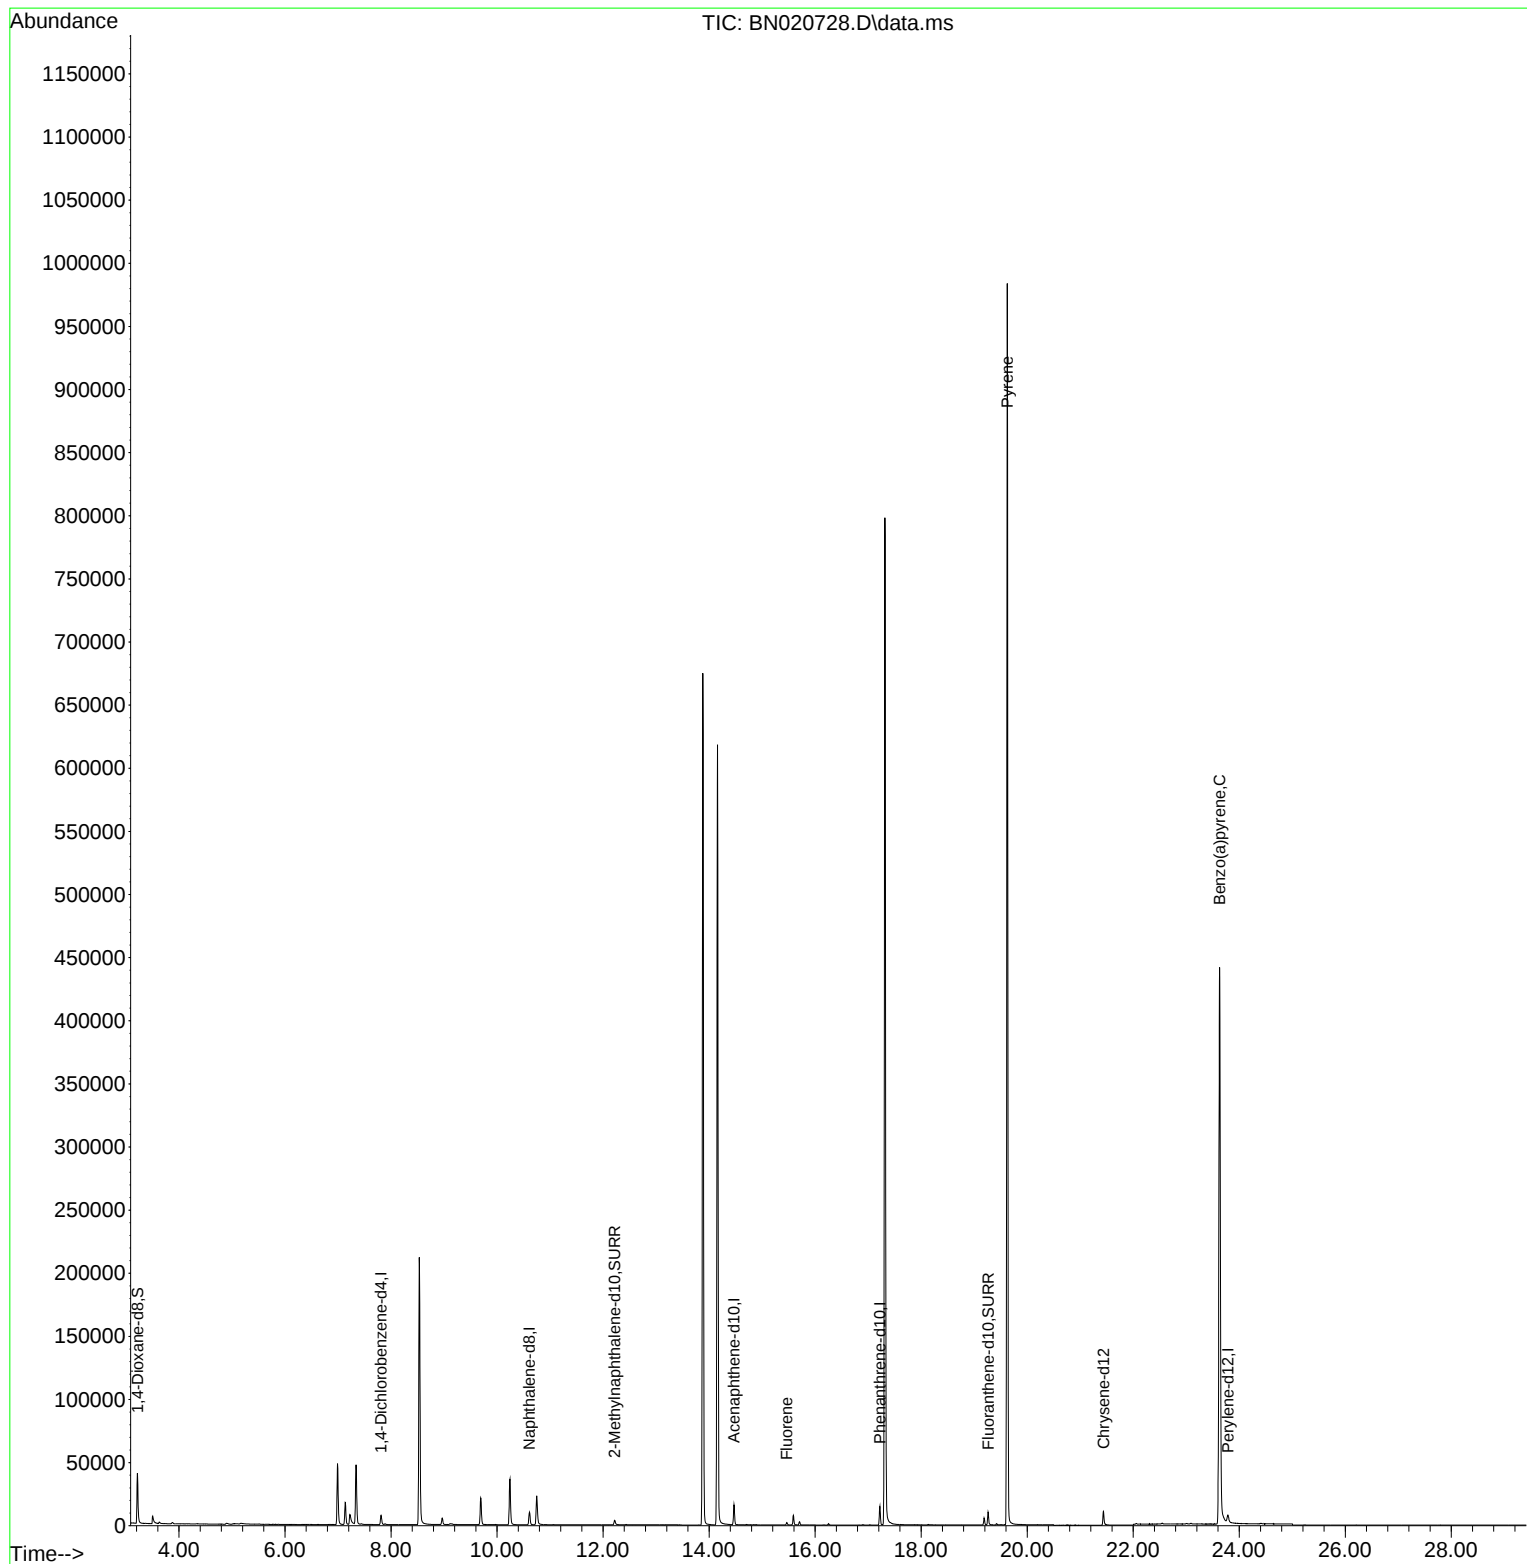


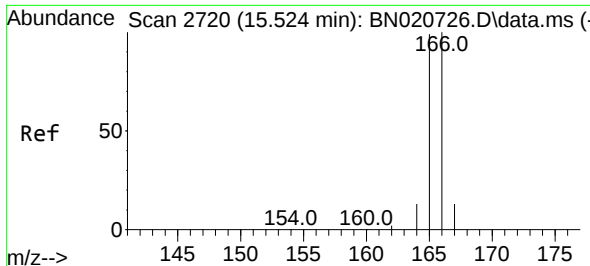

#12
Fluorene
Concen: 0.044 ng/ul
RT: 15.464 min Scan# 21
Delta R.T. -0.069 min
Lab File: BN020728.D
Acq: 13 Jul 2022 14:22




Instrument :
BNA_N
ClientSampleId :
C0AN4


Tgt Ion:166 Resp: 1766
Ion Ratio Lower Upper
166 100
165 8.0 78.2 117.2#
167 33.8 11.3 16.9#

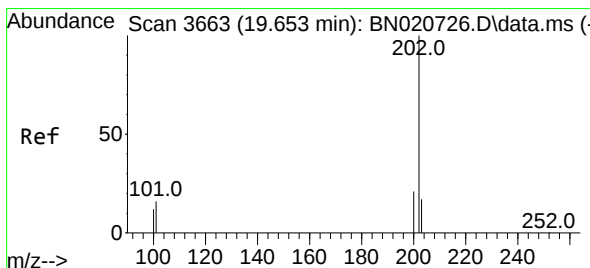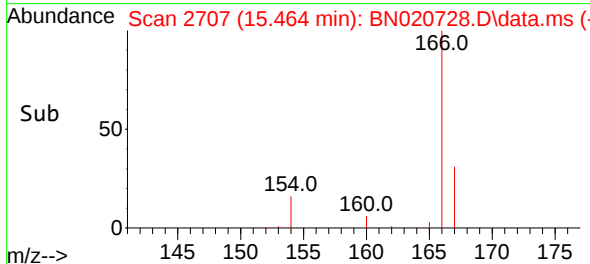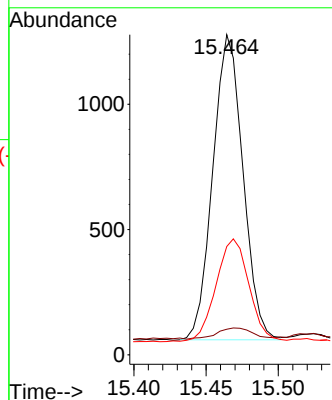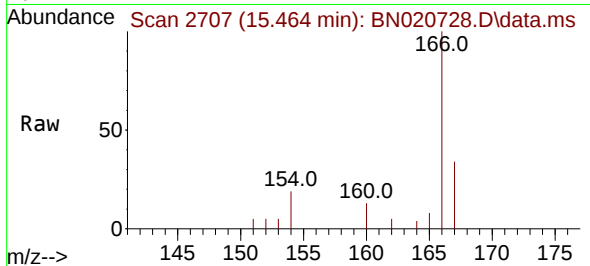

#20
Pyrene
Concen: 0.026 ng/ul
RT: 19.625 min Scan# 3657
Delta R.T. -0.042 min
Lab File: BN020728.D
Acq: 13 Jul 2022 14:22

Tgt Ion:202 Resp: 1475
Ion Ratio Lower Upper
202 100
101 174.0 11.6 17.4#
100 1279.9 9.2 13.8#

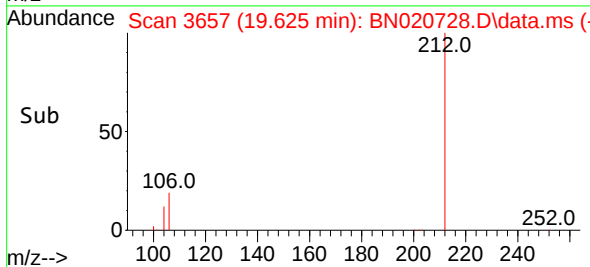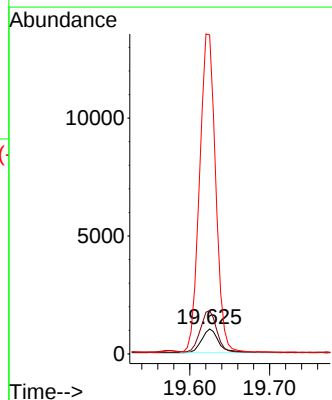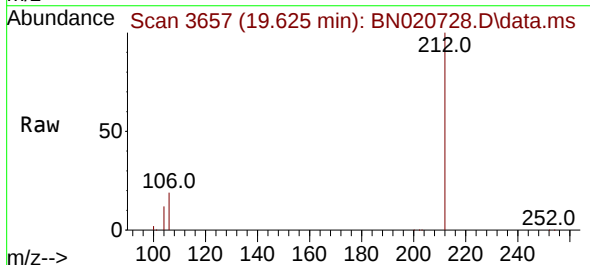

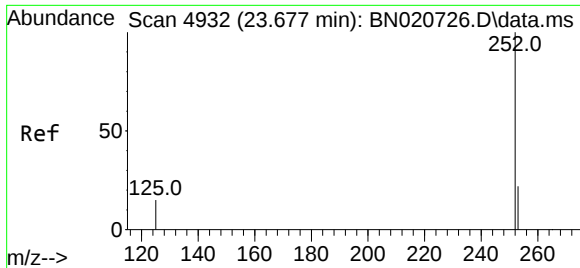

#26

Benzo(a)pyrene

Concen: 0.055 ng/ul

RT: 23.630 min Scan# 4916

Delta R.T. -0.067 min

Lab File: BN020728.D


Acq: 13 Jul 2022 14:22

Instrument :

BNA_N

ClientSampleId :

C0AN4

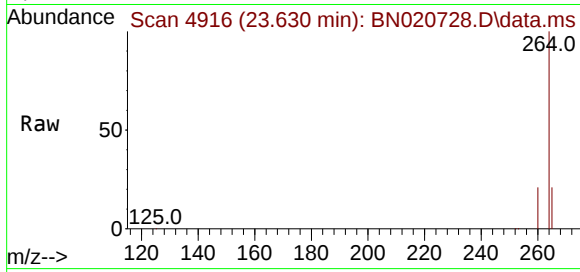

Tgt Ion:252 Resp: 2350

Ion Ratio Lower Upper

252 100

253 49.3 21.0 31.4#

125 40.9 18.8 28.2#

