
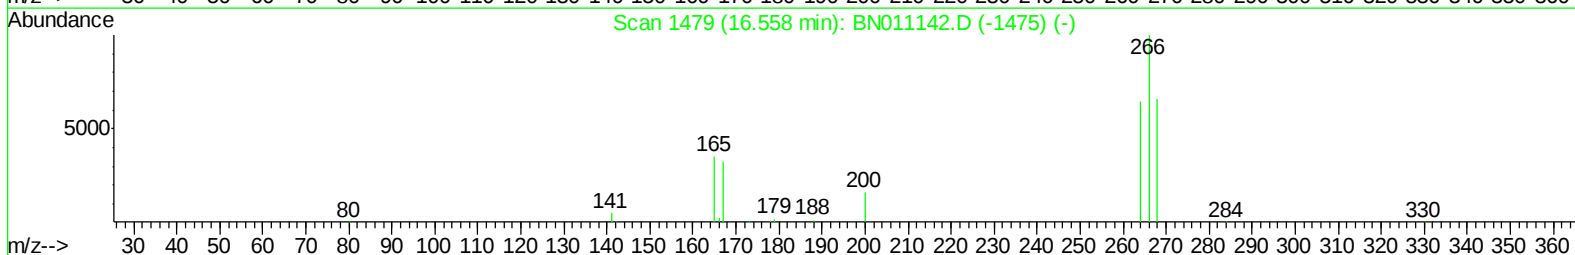
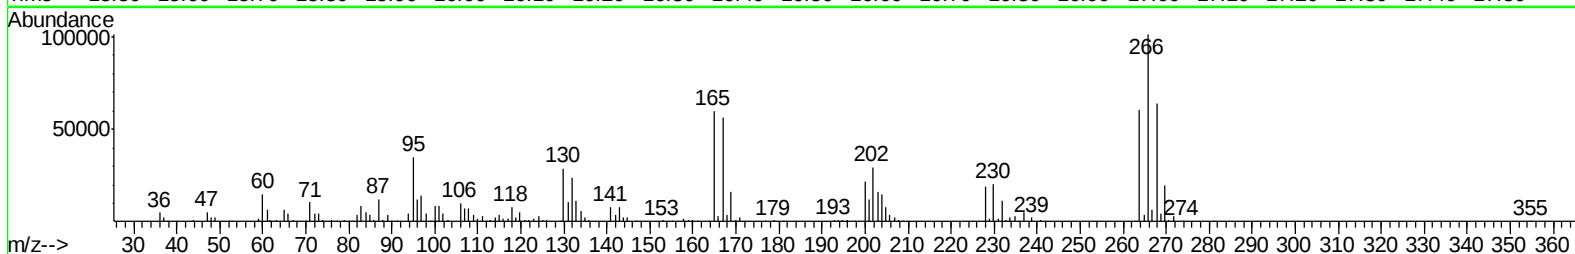


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071420\
 Data File : BN011159.D
 Acq On : 14 Jul 2020 13:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 02:34:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN071120.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 14 15:08:13 2020
 Response via : Initial Calibration

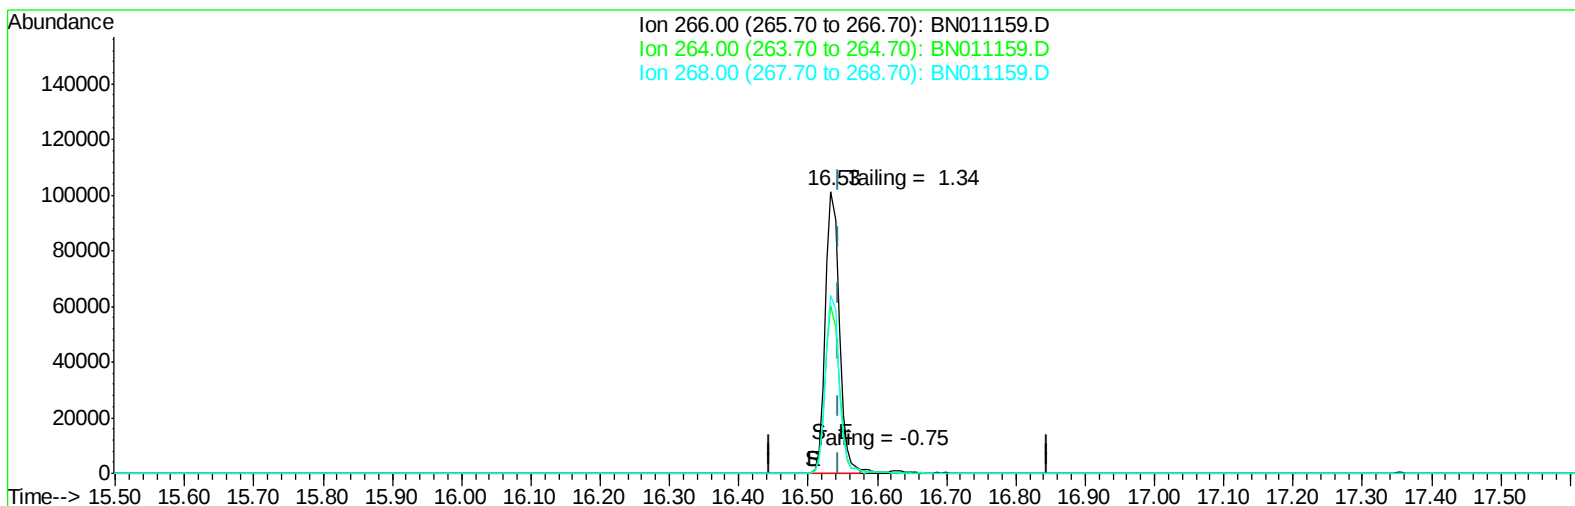

TIC: BN011159.D

(24) Pentachlorophenol

16.533min (-0.012) 0.00ng

response 142013

Ion	Exp%	Act%
266.00	100	100
264.00	65.60	60.65
268.00	61.10	61.21
0.00	0.00	0.00