


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071420\
 Data File : BN011159.D
 Acq On : 14 Jul 2020 13:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN071120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 14 15:08:13 2020

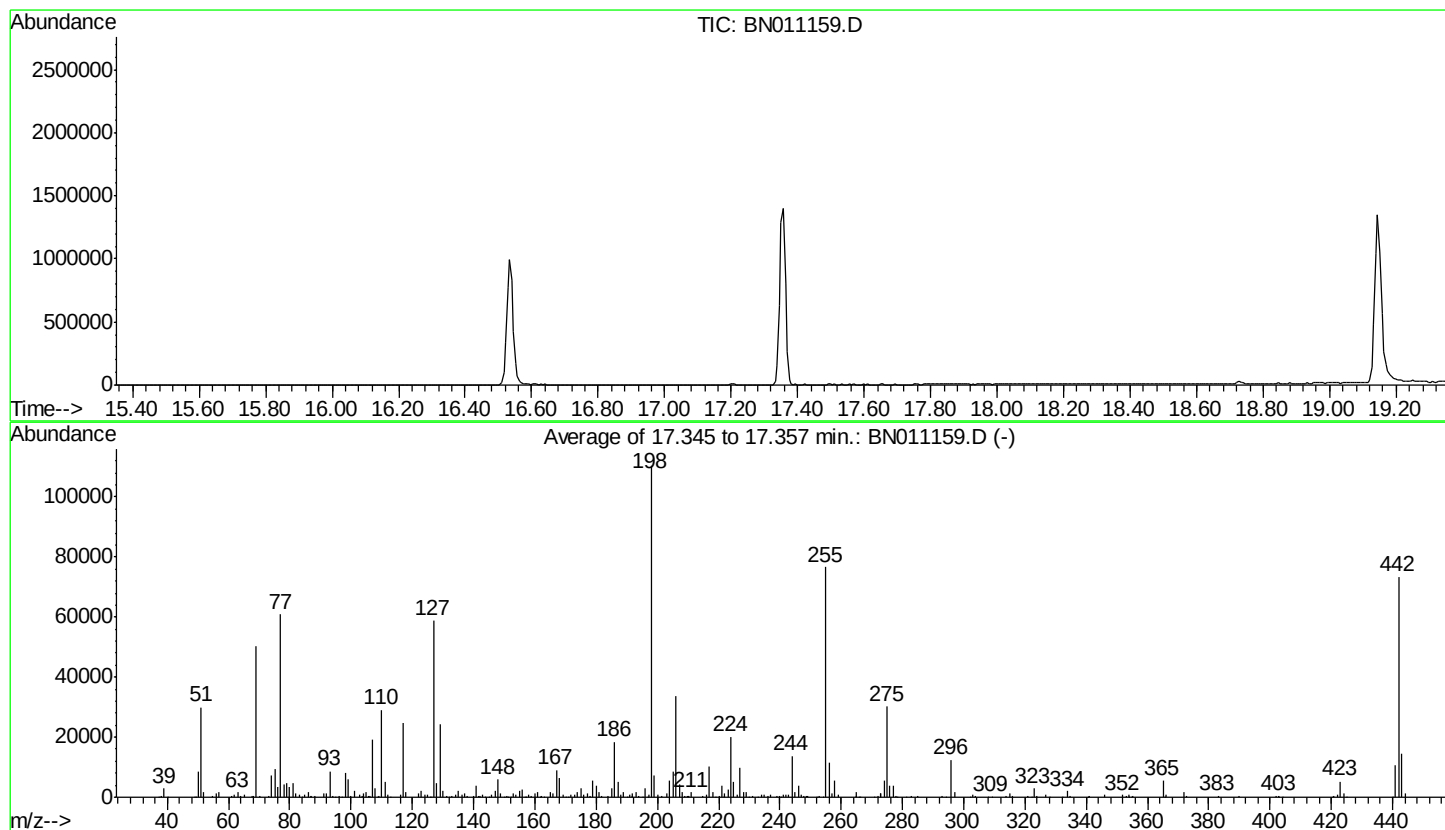

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.2	29994	PASS
68	69	0.00	2	0.9	429	PASS
69	198	0.00	100	45.5	50194	PASS
70	69	0.00	2	0.5	235	PASS
127	198	10	80	53.2	58698	PASS
197	198	0.00	2	0.7	743	PASS
198	198	100	100	100.0	110437	PASS
199	198	5	9	6.5	7125	PASS
275	198	10	60	27.3	30118	PASS
365	198	1	100	5.0	5524	PASS
441	198	0.01	100	9.8	10780	PASS
442	198	50	100	66.6	73544	PASS
443	442	15	24	19.6	14392	PASS