

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071522\
 Data File : BN020750.D
 Acq On : 15 Jul 2022 17:10
 Operator : CG/JU
 Sample : N3735-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GWOW-BR-01-79-91-071322

Quant Time: Jul 16 03:23:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 16 03:21:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.818	152	2577	0.400	ng	0.00
7) Naphthalene-d8	10.615	136	9031	0.400	ng	# 0.00
13) Acenaphthene-d10	14.463	164	5139	0.400	ng	0.00
19) Phenanthrene-d10	17.215	188	12778	0.400	ng	# 0.00
29) Chrysene-d12	21.431	240	11771	0.400	ng	# 0.00
35) Perylene-d12	23.779	264	9972	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.413	112	663	0.093	ng	0.01
5) Phenol-d6	7.024	99	439	0.051	ng	0.01
8) Nitrobenzene-d5	8.982	82	1648	0.225	ng	0.01
11) 2-Methylnaphthalene-d10	12.215	152	4833	0.312	ng	0.00
14) 2,4,6-Tribromophenol	15.964	330	639	0.330	ng	-0.01
15) 2-Fluorobiphenyl	13.095	172	5973	0.282	ng	0.00
27) Fluoranthene-d10	19.261	212	14859	0.391	ng	0.00
31) Terphenyl-d14	19.864	244	12440	0.442	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.254	88	303	0.090	ng	# 78
9) Naphthalene	10.669	128	13038	0.483	ng	99
12) 2-Methylnaphthalene	12.291	142	2151	0.120	ng	98
25) Phenanthrene	17.266	178	2018	0.047	ng	100
28) Fluoranthene	19.291	202	1204	0.026	ng	# 64
30) Pyrene	19.653	202	1158	0.023	ng	97
34) Bis(2-ethylhexyl)phtha...	21.351	149	2208	0.093	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071522\
Data File : BN020750.D
Acq On : 15 Jul 2022 17:10
Operator : CG/JU
Sample : N3735-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GWOW-BR-01-79-91-071322


Quant Time: Jul 16 03:23:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 16 03:21:59 2022
Response via : Initial Calibration

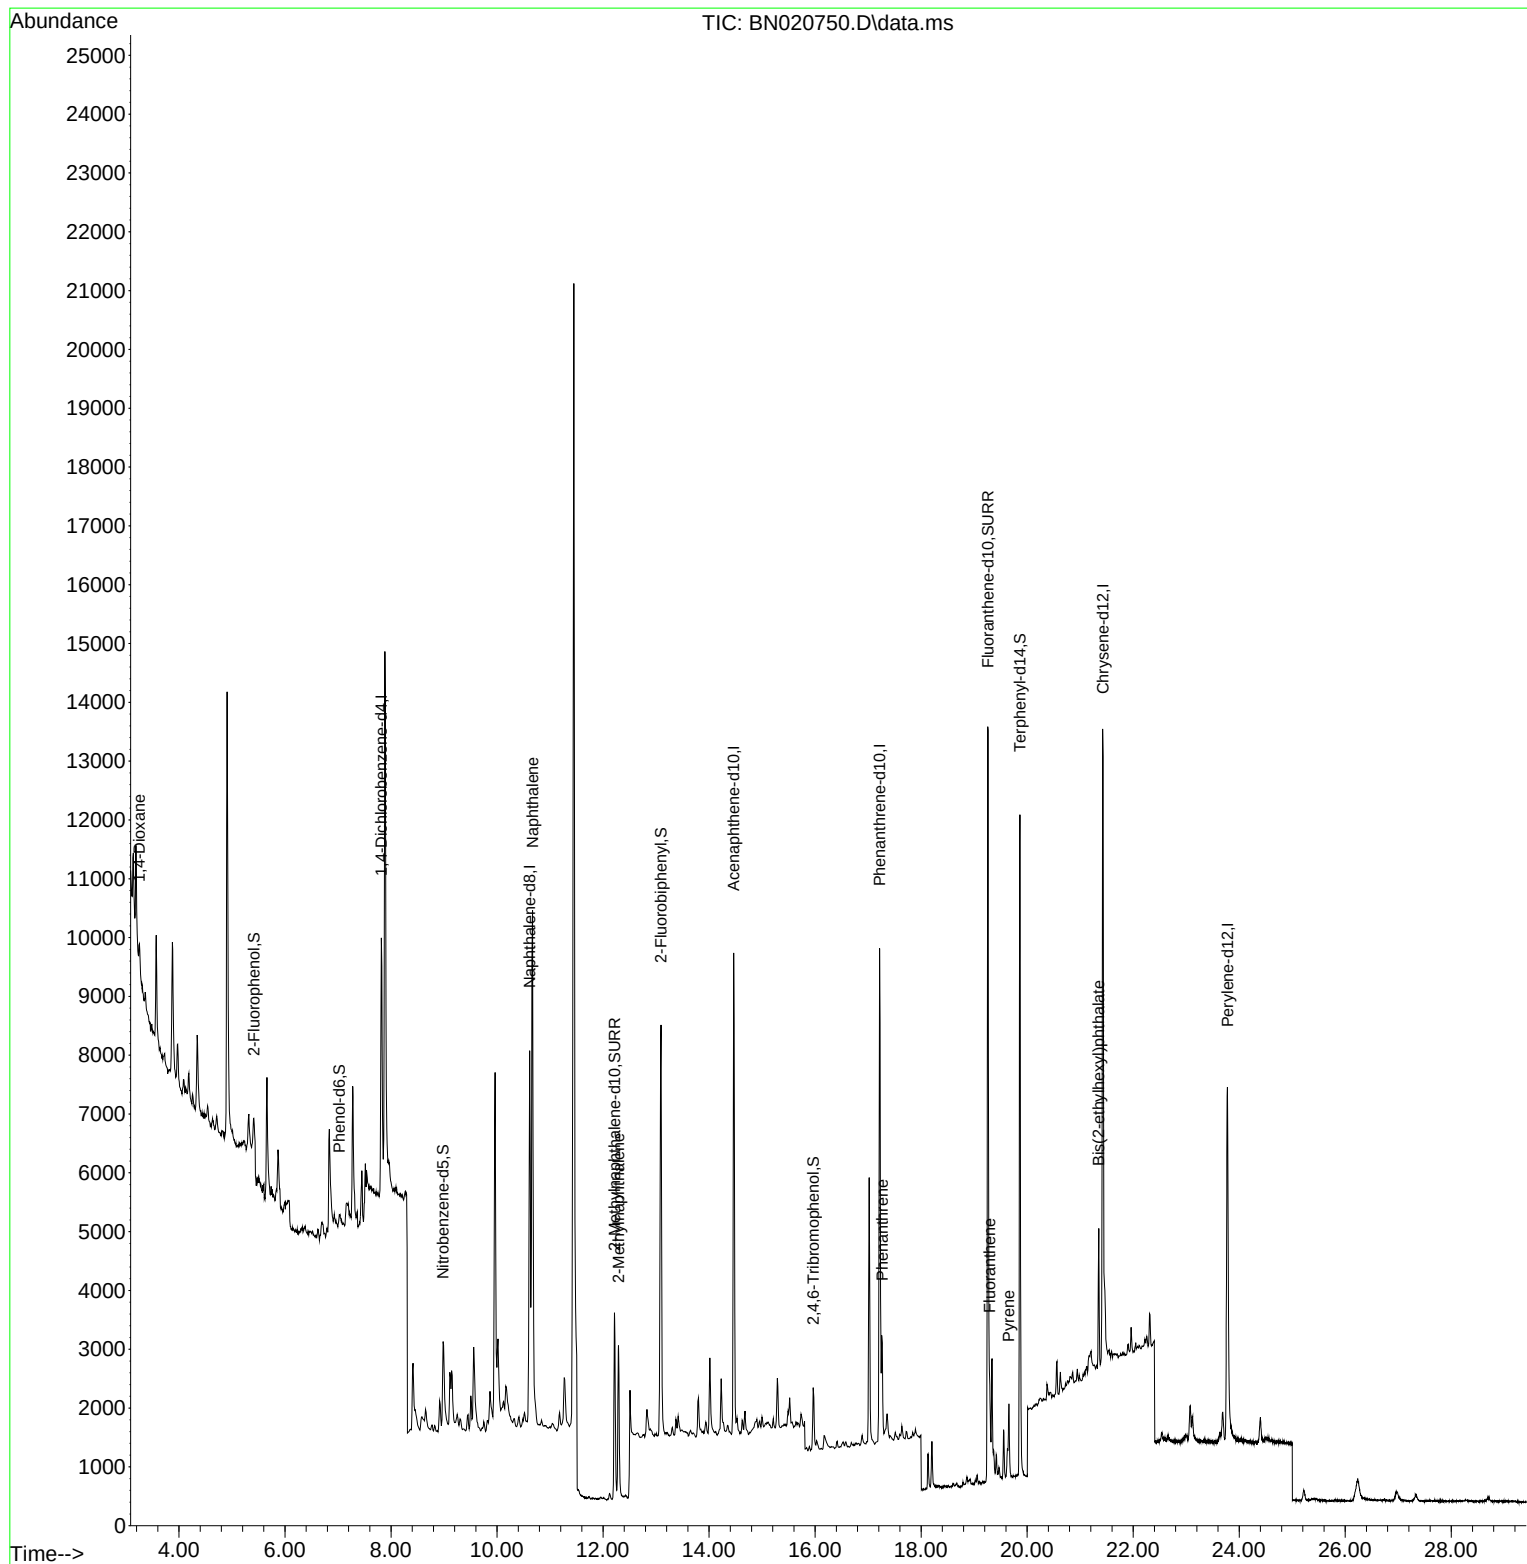






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.818 min Scan# 61
 Delta R.T. 0.007 min
 Lab File: BN020750.D
 Acq: 15 Jul 2022 17:10

Instrument :
 BNA_N
 ClientSampleId :
 GWOW-BR-01-79-91-071322



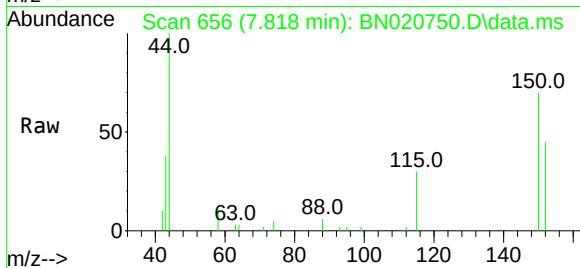



Tgt Ion:152 Resp: 2577
 Ion Ratio Lower Upper
 152 100
 150 155.4 127.9 191.9
 115 66.7 51.4 77.2

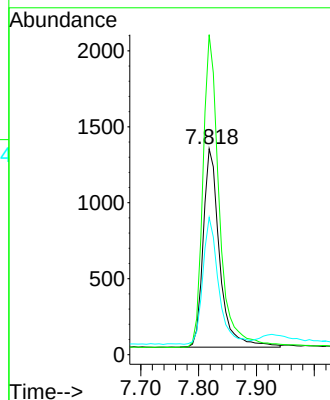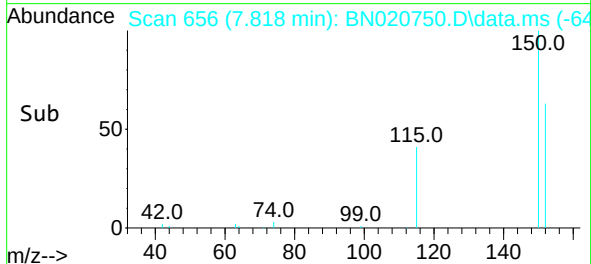

#2
 1,4-Dioxane
 Concen: 0.090 ng
 RT: 3.254 min Scan# 24
 Delta R.T. -0.000 min
 Lab File: BN020750.D
 Acq: 15 Jul 2022 17:10

Tgt Ion: 88 Resp: 303
 Ion Ratio Lower Upper
 88 100
 43 0.0 30.2 45.2#
 58 86.8 73.0 109.6


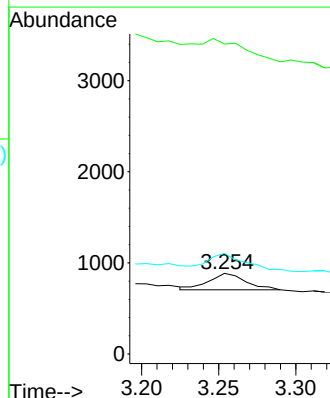
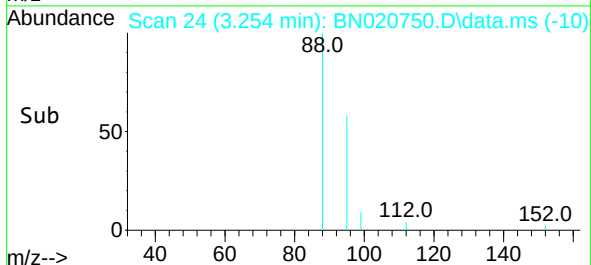
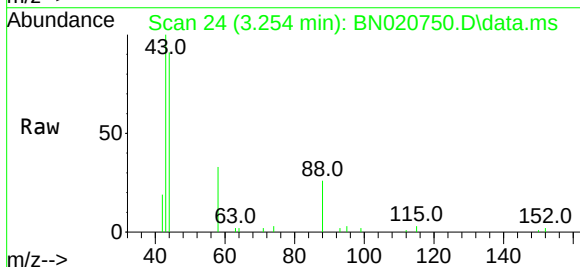




#4
2-Fluorophenol
Concen: 0.093 ng
RT: 5.413 min Scan# 314
Delta R.T. 0.014 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10




Instrument :
BNA_N
ClientSampleId :
GWOW-BR-01-79-91-071322


Tgt Ion:112 Resp: 663
Ion Ratio Lower Upper
112 100
64 62.4 49.1 73.7
63 36.3 26.3 39.5

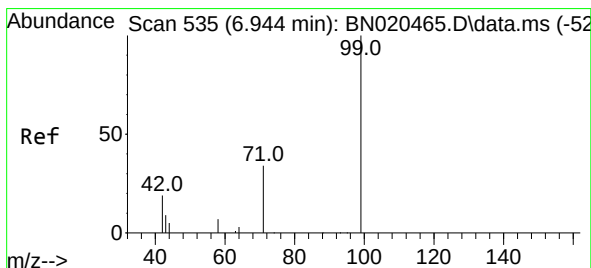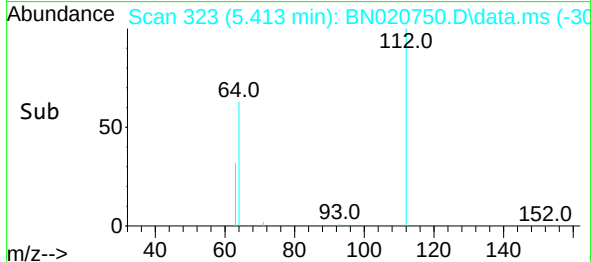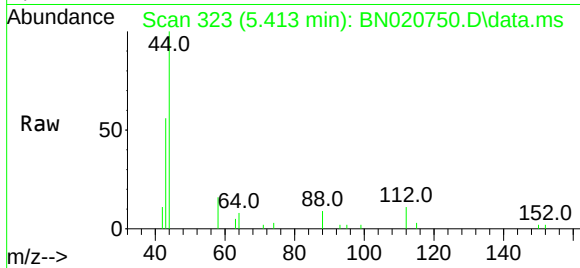

#5
Phenol-d6
Concen: 0.051 ng
RT: 7.024 min Scan# 546
Delta R.T. 0.014 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10

Tgt Ion: 99 Resp: 439
Ion Ratio Lower Upper
99 100
42 0.0 19.3 28.9#
71 33.5 27.5 41.3


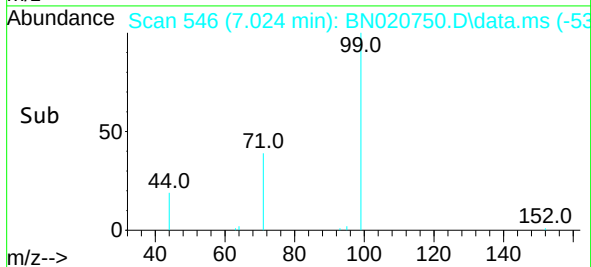

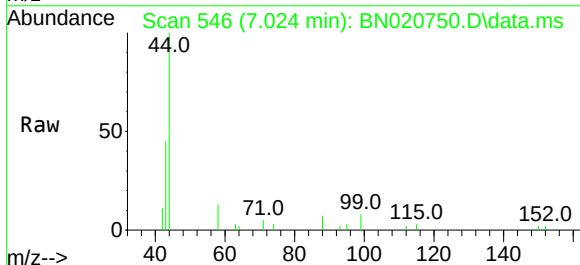




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.615 min Scan# 94
Delta R.T. -0.000 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10




Instrument :
BNA_N
ClientSampleId :
GWOW-BR-01-79-91-071322


Tgt Ion:136	Resp:	9031
Ion Ratio	Lower	Upper
136	100	
137	11.6	9.0 13.6
54	11.3	6.2 9.2#
68	7.7	4.4 6.6#

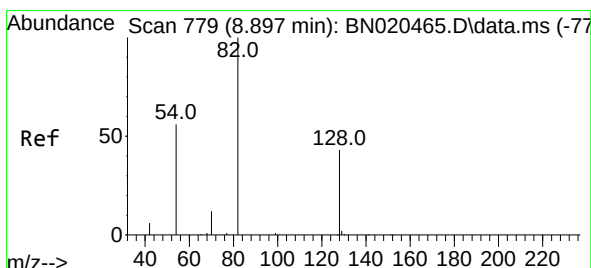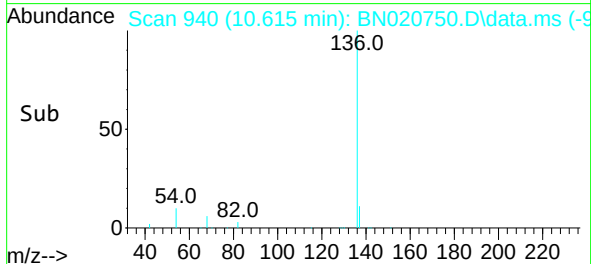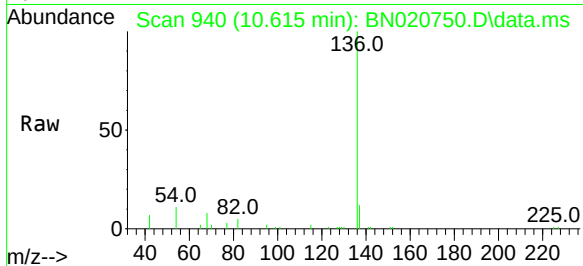

#8
Nitrobenzene-d5
Concen: 0.225 ng
RT: 8.982 min Scan# 787
Delta R.T. 0.011 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10

Tgt Ion: 82	Resp:	1648
Ion Ratio	Lower	Upper
82	100	
128	39.5	35.0 52.6
54	70.1	46.2 69.4#


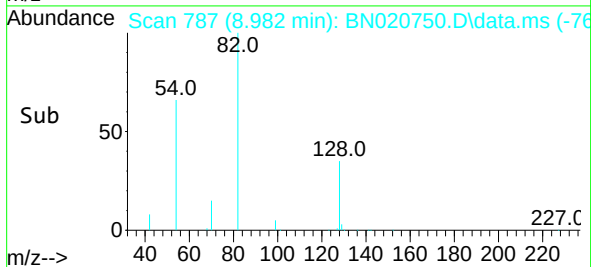

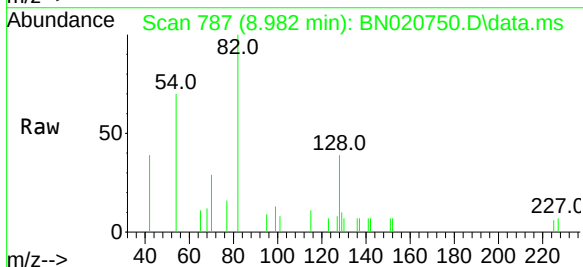




#9
Naphthalene
Concen: 0.483 ng
RT: 10.669 min Scan# 94
Delta R.T. 0.011 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10




Instrument :
BNA_N
ClientSampleId :
GWOW-BR-01-79-91-071322


Tgt Ion:128 Resp: 13038
Ion Ratio Lower Upper
128 100
129 12.1 8.9 13.3
127 13.4 10.8 16.2

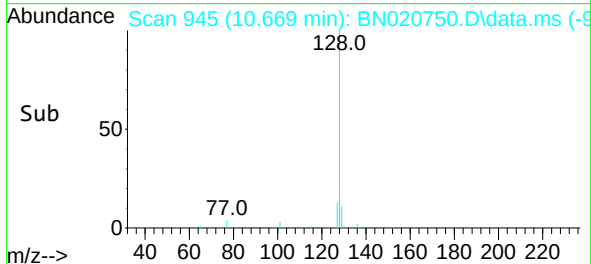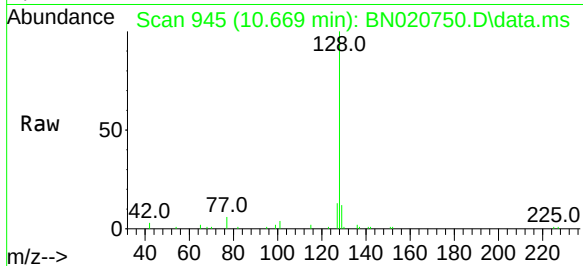

#11
2-Methylnaphthalene-d10
Concen: 0.312 ng
RT: 12.215 min Scan# 1210
Delta R.T. 0.004 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10


Tgt Ion:152 Resp: 4833
Ion Ratio Lower Upper
152 100
151 20.4 16.2 24.4

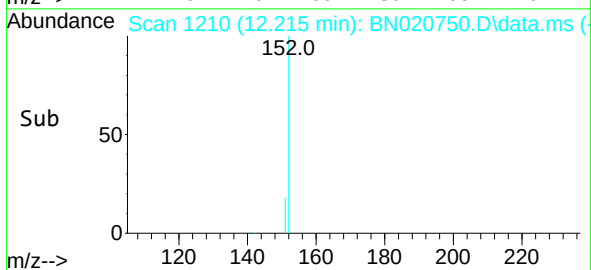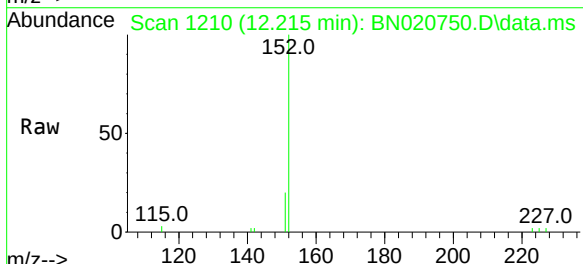






#12
2-Methylnaphthalene
Concen: 0.120 ng
RT: 12.291 min Scan# 11
Delta R.T. 0.004 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10


Instrument :
BNA_N
ClientSampleId :
GWOW-BR-01-79-91-071322

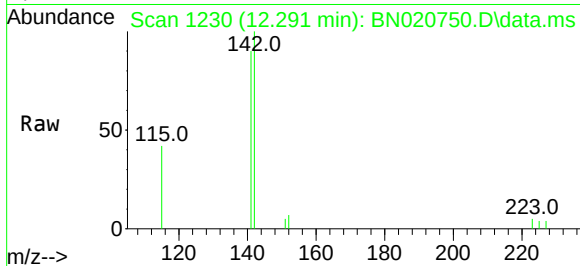



Tgt Ion	Ratio	Lower	Upper
142	100		
141	89.5	71.6	107.4
115	41.8	29.8	44.8

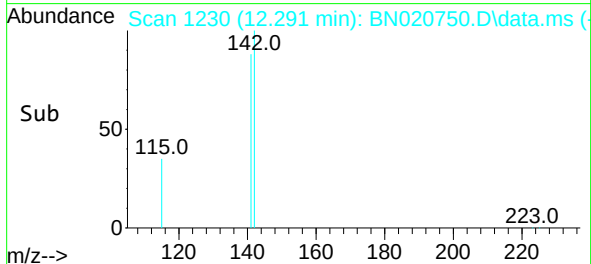


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.463 min Scan# 1470
Delta R.T. -0.000 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10

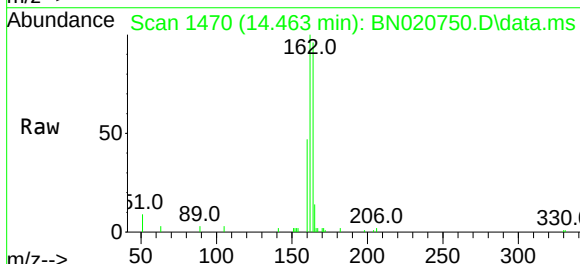


Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.1	82.1	123.1
160	49.4	38.6	58.0

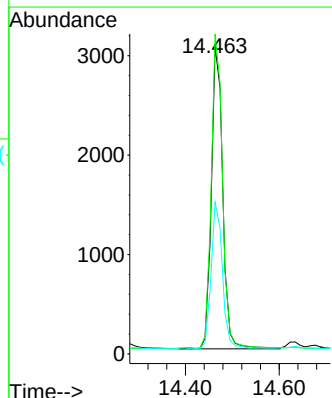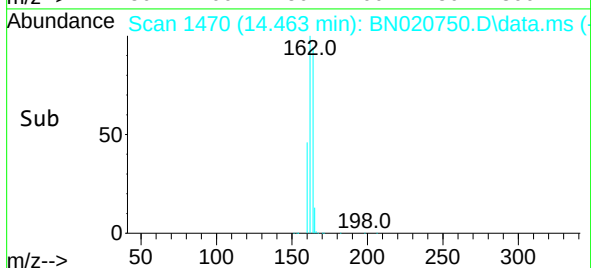



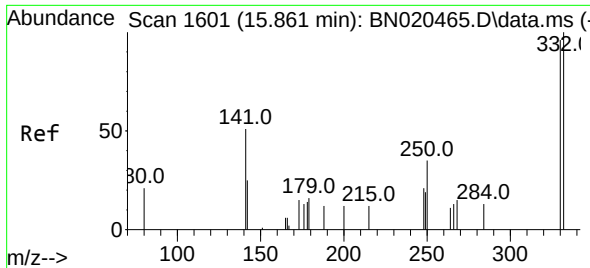


#14
2,4,6-Tribromophenol
Concen: 0.330 ng
RT: 15.964 min Scan# 1
Delta R.T. -0.010 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10

Instrument :
BNA_N
ClientSampleId :
GWOW-BR-01-79-91-071322



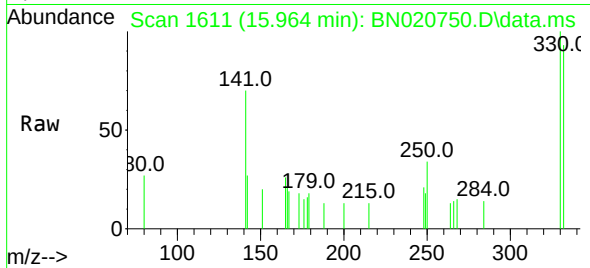



Tgt Ion:330 Resp: 639
Ion Ratio Lower Upper
330 100
332 95.8 77.6 116.4
141 56.0 41.0 61.4

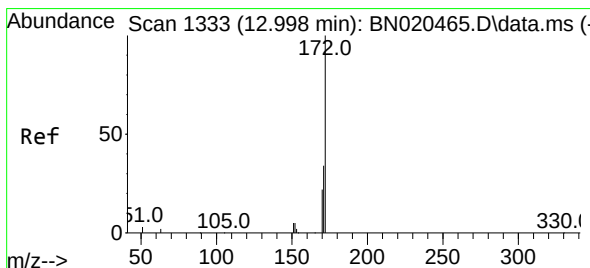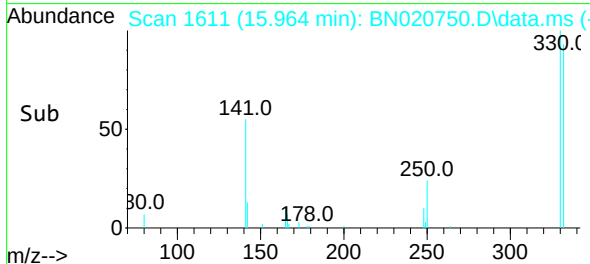

#15
2-Fluorobiphenyl
Concen: 0.282 ng
RT: 13.095 min Scan# 1342
Delta R.T. -0.000 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10

Tgt Ion:172 Resp: 5973
Ion Ratio Lower Upper
172 100
171 35.4 27.2 40.8
170 24.2 18.2 27.4


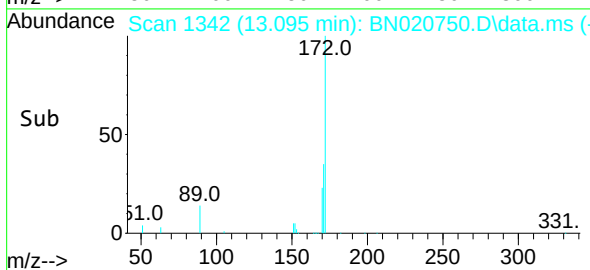

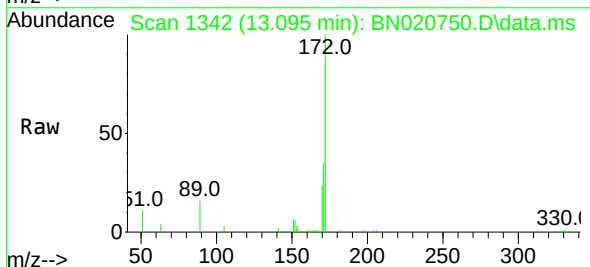


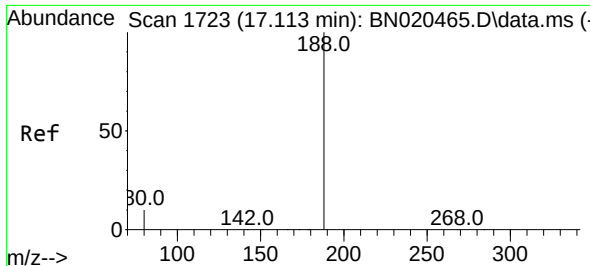

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.215 min Scan# 1733
Delta R.T. -0.000 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10




Instrument :
BNA_N
ClientSampleId :
GWOW-BR-01-79-91-071322


Tgt Ion:188 Resp: 12778
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.8 7.4 11.2#

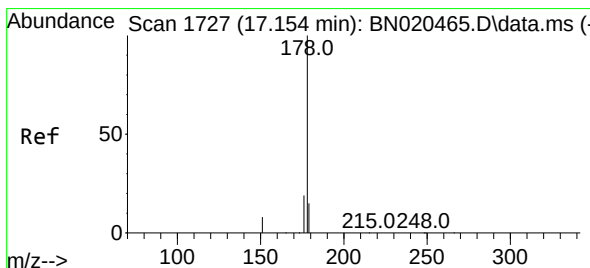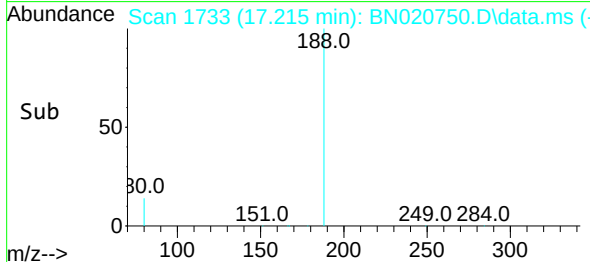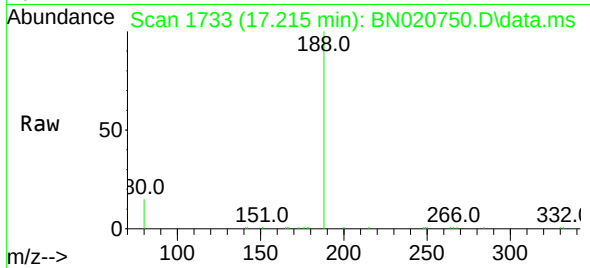

#25
Phenanthrene
Concen: 0.047 ng
RT: 17.266 min Scan# 1738
Delta R.T. 0.010 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10

Tgt Ion:178 Resp: 2018
Ion Ratio Lower Upper
178 100
176 18.9 15.3 22.9
179 15.4 12.2 18.4


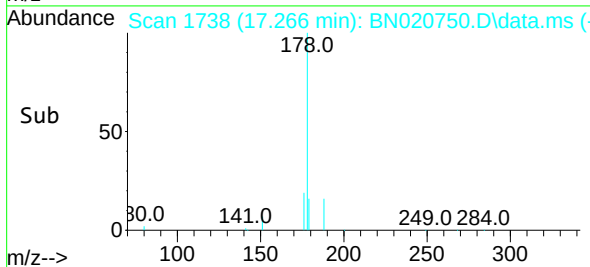

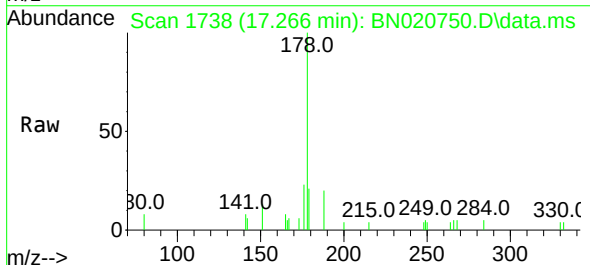


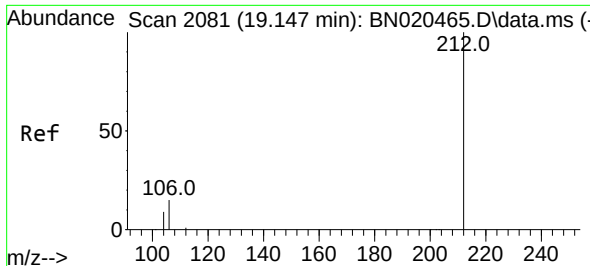

#27
Fluoranthene-d10
Concen: 0.391 ng
RT: 19.261 min Scan# 2115
Delta R.T. -0.000 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10




Instrument :
BNA_N
ClientSampleId :
GWOW-BR-01-79-91-071322


Tgt Ion:212 Resp: 14859
Ion Ratio Lower Upper
212 100
106 16.6 12.6 19.0
104 9.6 7.2 10.8

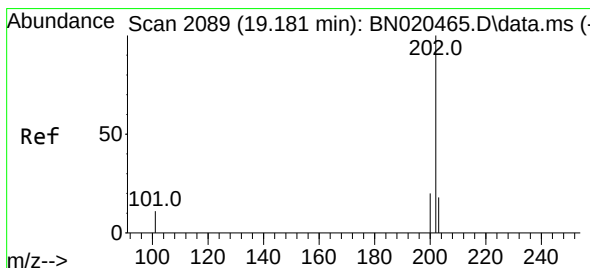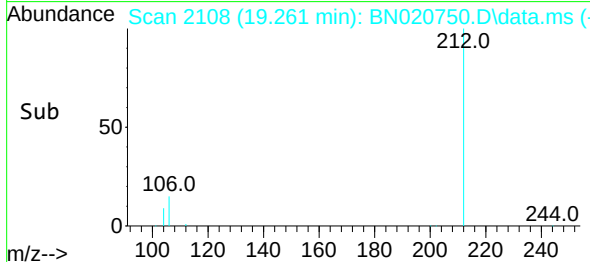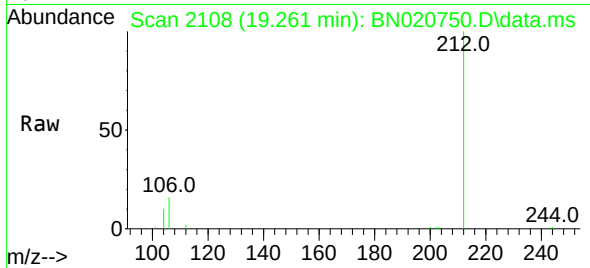

#28
Fluoranthene
Concen: 0.026 ng
RT: 19.291 min Scan# 2115
Delta R.T. -0.000 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10

Tgt Ion:202 Resp: 1204
Ion Ratio Lower Upper
202 100
101 24.3 9.6 14.4#
203 33.6 13.5 20.3#


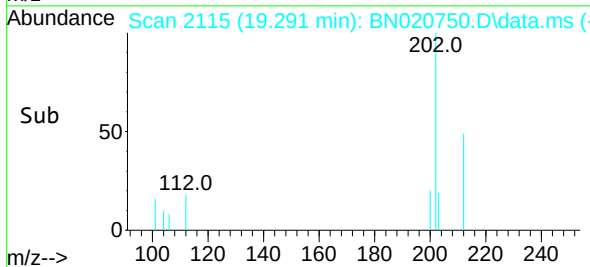

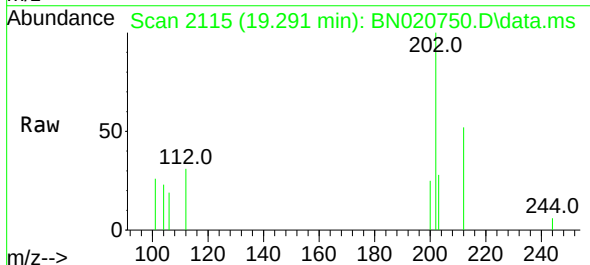


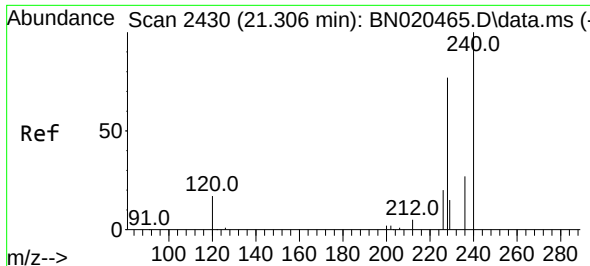

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.431 min Scan# 2444
Delta R.T. -0.000 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10




Instrument :
BNA_N
ClientSampleId :
GWOW-BR-01-79-91-071322


Tgt Ion:240 Resp: 11771
Ion Ratio Lower Upper
240 100
120 11.4 14.6 21.8#
236 27.4 22.6 33.8

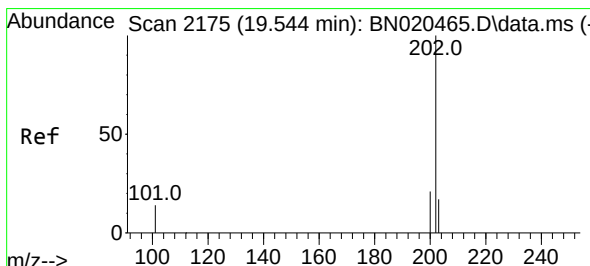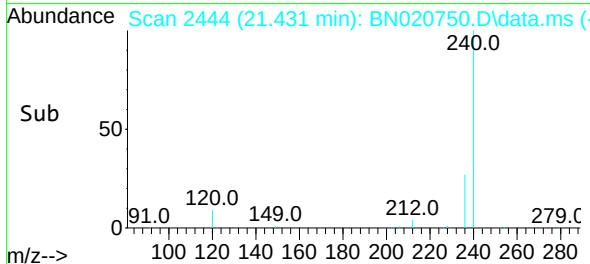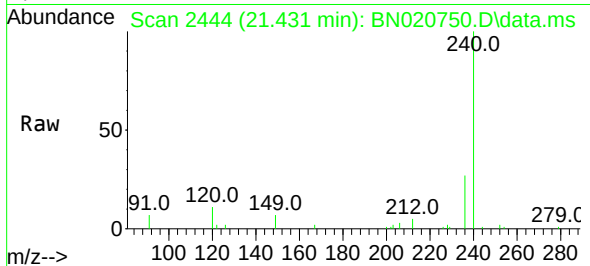

#30
Pyrene
Concen: 0.023 ng
RT: 19.653 min Scan# 2201
Delta R.T. -0.000 min
Lab File: BN020750.D
Acq: 15 Jul 2022 17:10

Tgt Ion:202 Resp: 1158
Ion Ratio Lower Upper
202 100
200 20.4 16.6 25.0
203 20.1 14.2 21.2


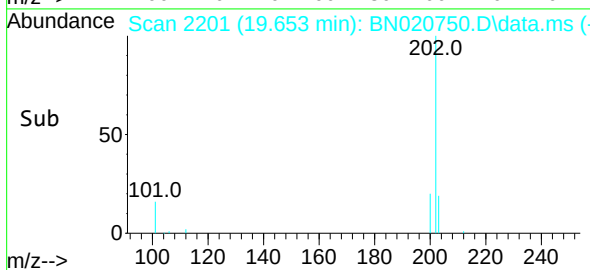

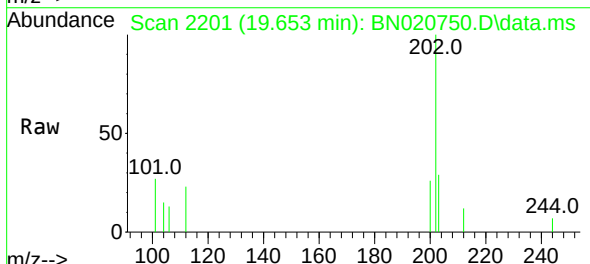




#31
 Terphenyl-d14
 Concen: 0.442 ng
 RT: 19.864 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN020750.D
 Acq: 15 Jul 2022 17:10




Instrument :
 BNA_N
 ClientSampleId :
 GWOW-BR-01-79-91-071322


Tgt Ion:244 Resp: 12440
 Ion Ratio Lower Upper
 244 100
 212 9.0 7.1 10.7
 122 0.0 0.0 0.0

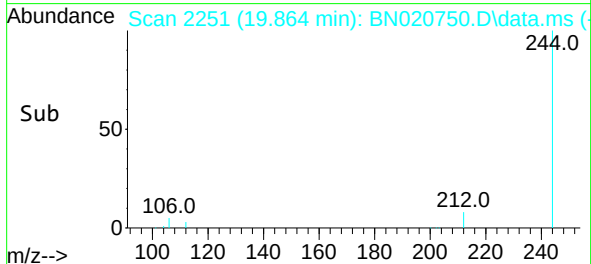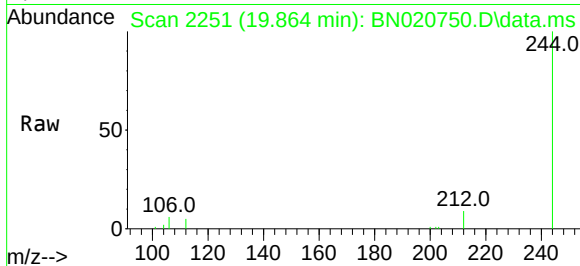

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.093 ng
 RT: 21.351 min Scan# 2435
 Delta R.T. -0.000 min
 Lab File: BN020750.D
 Acq: 15 Jul 2022 17:10


Tgt Ion:149 Resp: 2208
 Ion Ratio Lower Upper
 149 100
 167 26.3 21.7 32.5
 279 3.3 2.2 3.2#

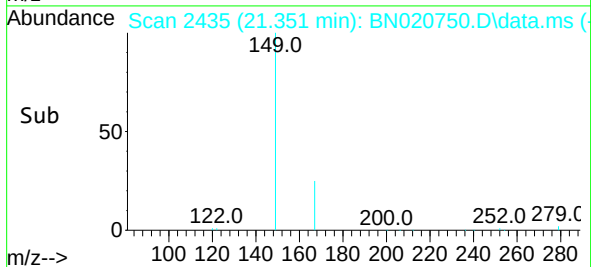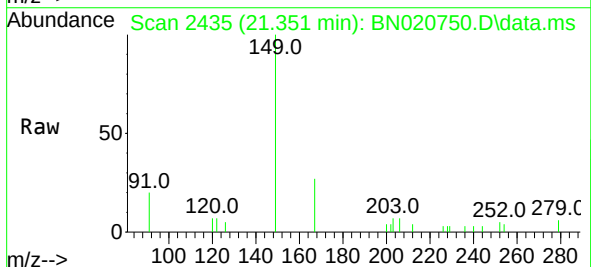

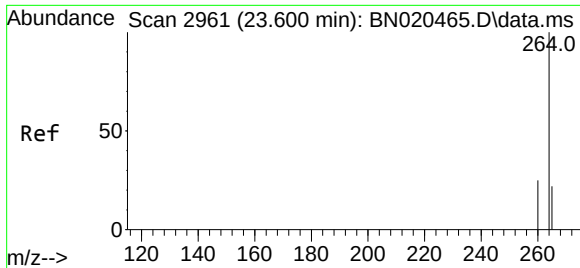

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.779 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN020750.D
 Acq: 15 Jul 2022 17:10

Instrument :
 BNA_N
 ClientSampleId :
 GWOW-BR-01-79-91-071322

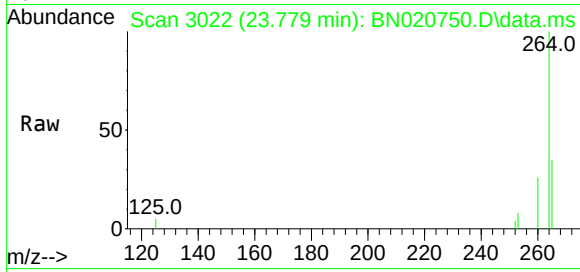

Tgt Ion:264 Resp: 9972

Ion	Ratio	Lower	Upper
264	100		
260	25.6	20.9	31.3
265	34.5	28.0	42.0

