

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071620\
 Data File : BN011193.D
 Acq On : 16 Jul 2020 17:10
 Operator : CG/JU
 Sample : L3295-01RX
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG098RX

Quant Time: Jul 16 17:41:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 16 09:28:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	157429	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	652651	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.12	164	445485	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	933746	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1077600	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	1058754	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	18655	4.53	ng/uL	0.00
5) Phenol-d5	6.69	99	5205	0.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	210295	31.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	220683	20.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	46223	4.48	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	193562	36.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.34	143	179112	31.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.87	165	306079	28.03	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.54	166	1315604	36.42	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	42097	0.98	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	31999	4.96	ng/ul	0.01
58) Fluorene-d10	15.12	176	1016402	31.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	181475	31.85	ng/ul	0.00
71) Anthracene-d10	16.97	188	277564	6.11	ng/ul	0.00
79) Pyrene-d10	19.28	212	504304	9.39	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	602014	10.49	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.59	163	64503	1.690 ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071620\
Data File : BN011193.D
Acq On : 16 Jul 2020 17:10
Operator : CG/JU
Sample : L3295-01RX
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG098RX

Quant Time: Jul 16 17:41:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 16 09:28:14 2020
Response via : Initial Calibration

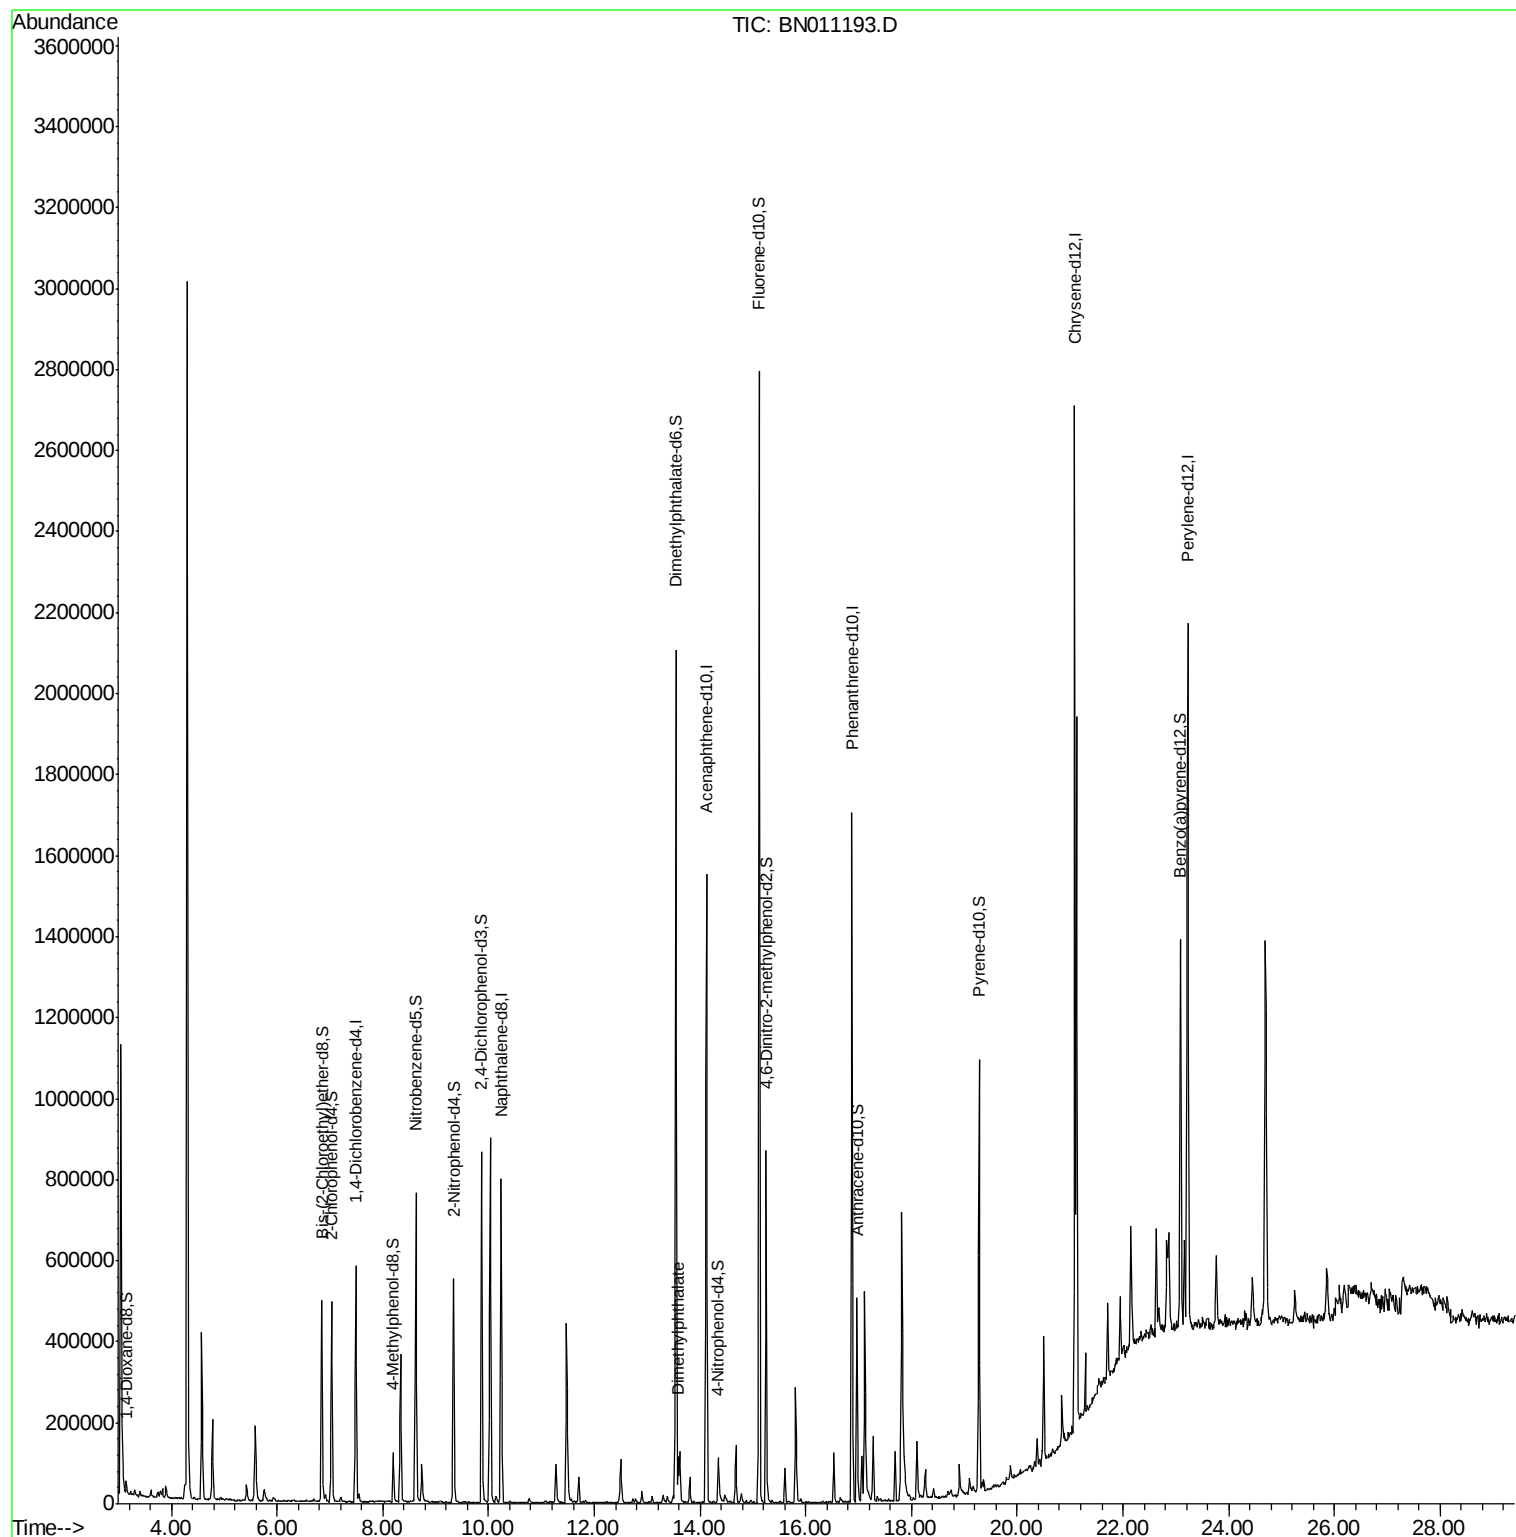

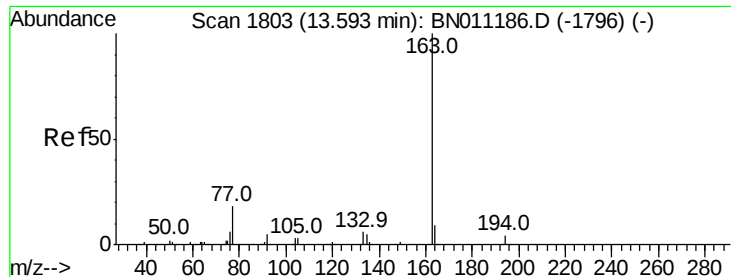

#45

Dimethylphthalate

Concen: 1.690 ng/ul

RT: 13.59 min Scan# 1802

Delta R.T. -0.01 min

Lab File: BN011193.D

Acq: 16 Jul 2020 17:10

Instrument :

BNA_N

ClientSampleId :

BG098RX


Tot Ion:163 Resp: 64503

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 9.9 7.8 11.8

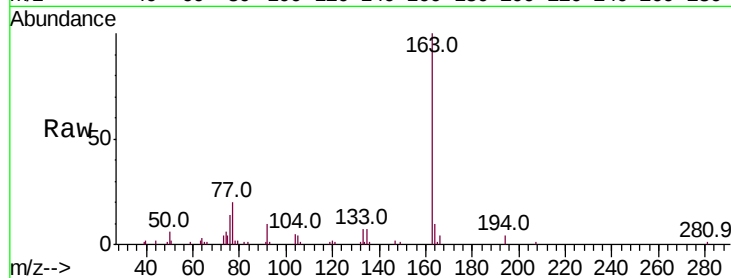

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

