




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032758.D
Acq On : 17 Jul 2024 02:08
Operator : MA/JU
Sample : PB161887BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK887

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 17 02:35:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

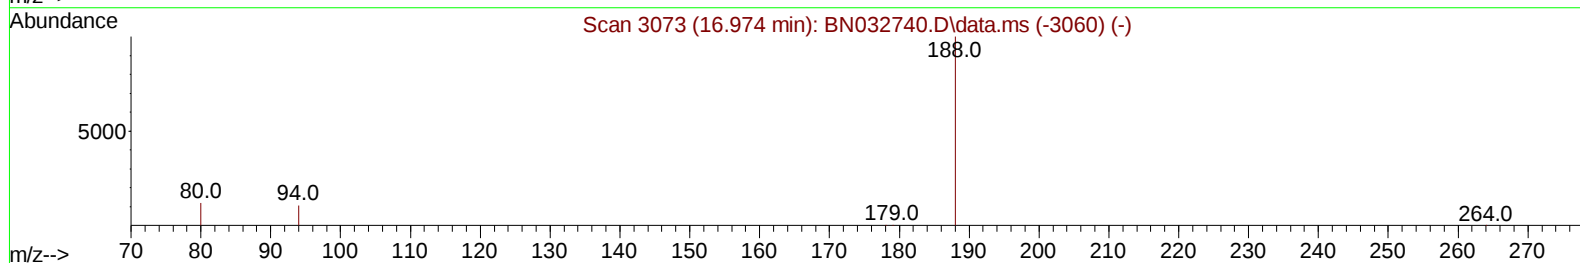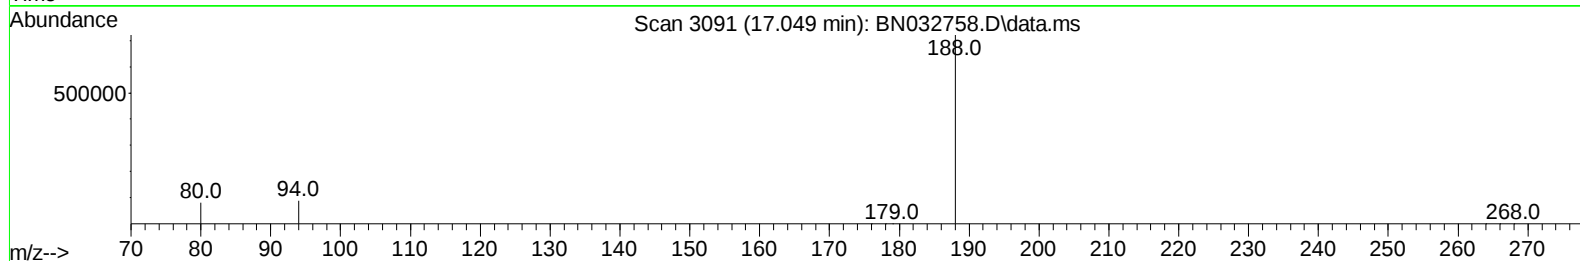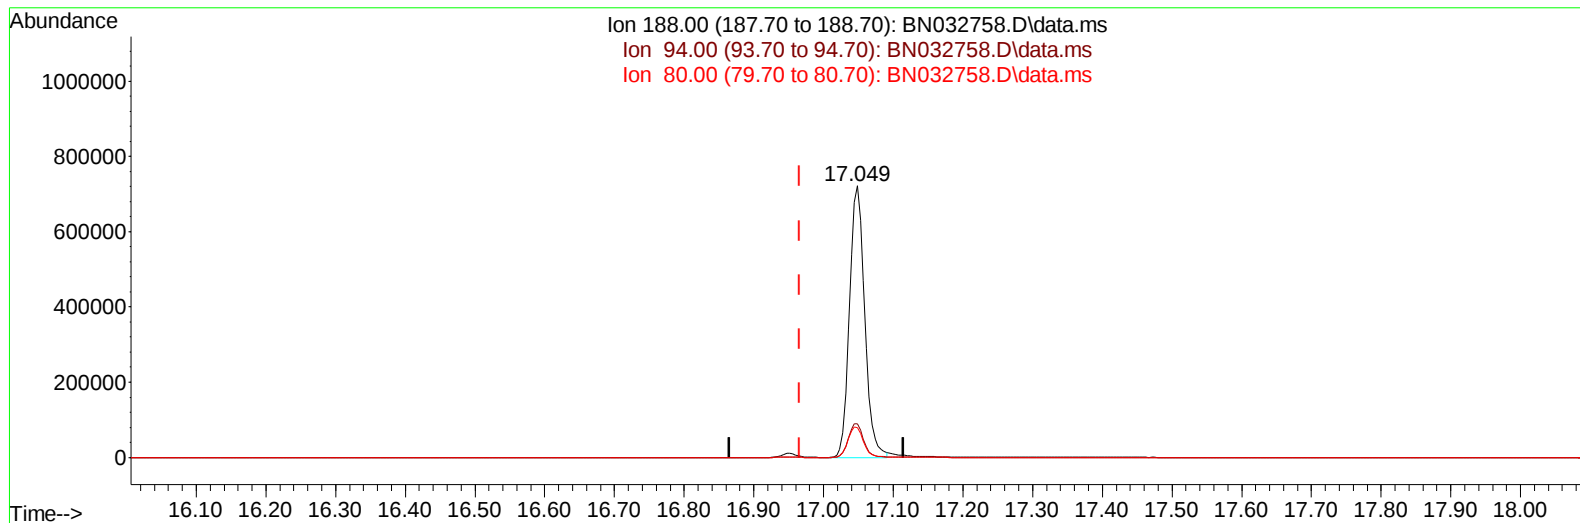

TIC: BN032758.D\data.ms

(13) Phenanthrene-d10 (I)

17.049min (+ 0.083) 0.40 ng/u1

response 1091937

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	12.30
80.00	12.00	11.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032758.D
Acq On : 17 Jul 2024 02:08
Operator : MA/JU
Sample : PB161887BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK887

Manual IntegrationsAPPROVED

Quant Time: Jul 17 02:35:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

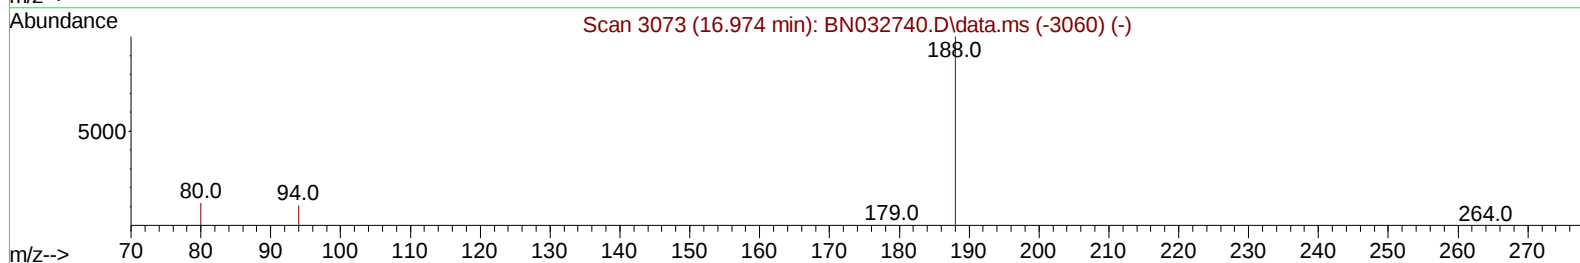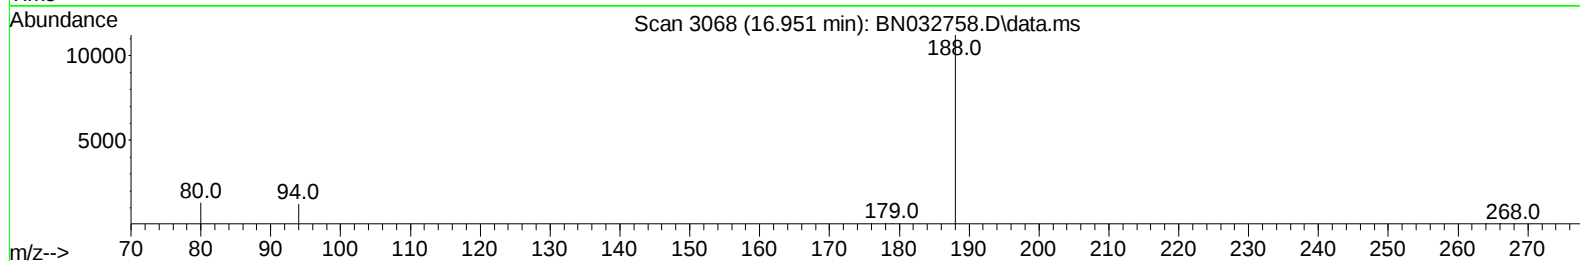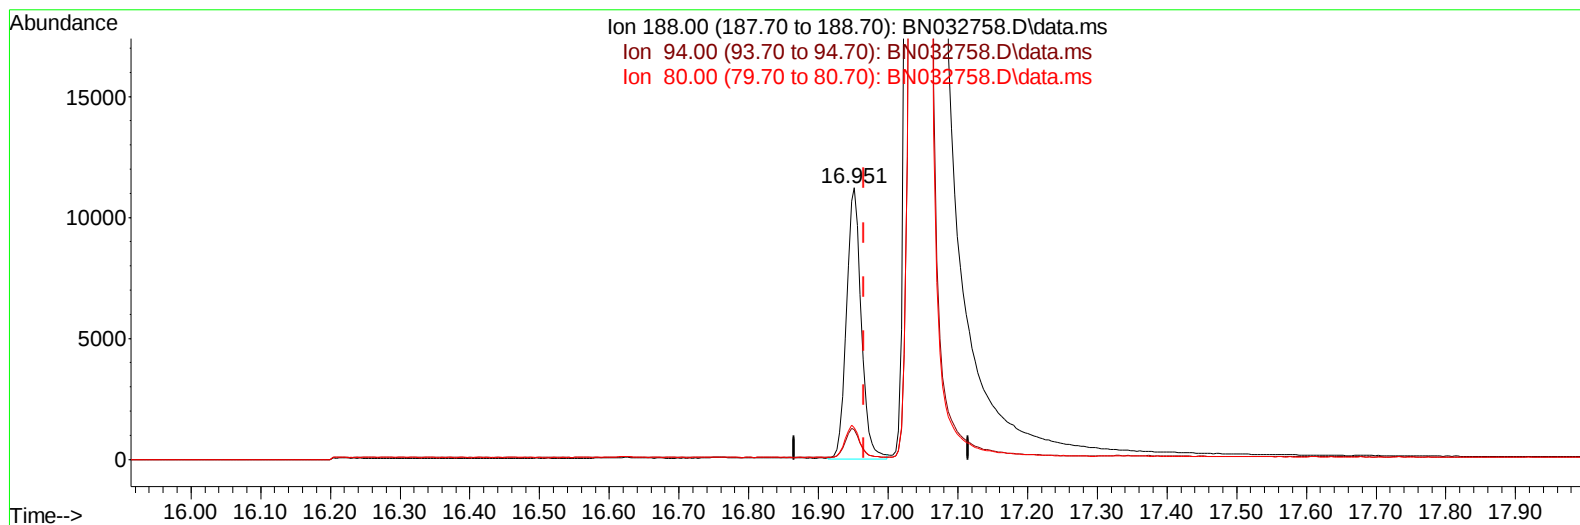

TIC: BN032758.D\data.ms

(13) Phenanthrene-d10 (I)

16.951min (-0.014) 0.40 ng/ul m

response 16398

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	10.92
80.00	12.00	11.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032758.D
Acq On : 17 Jul 2024 02:08
Operator : MA/JU
Sample : PB161887BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK887

Manual IntegrationsAPPROVED

Quant Time: Jul 17 02:35:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

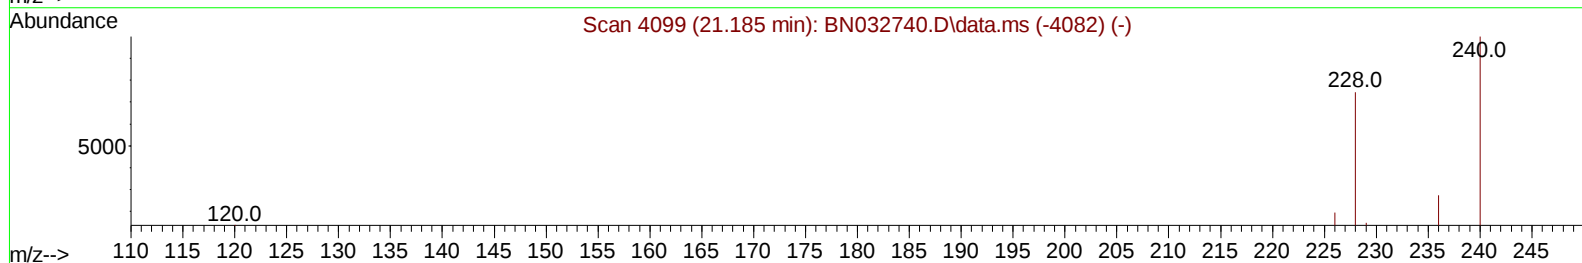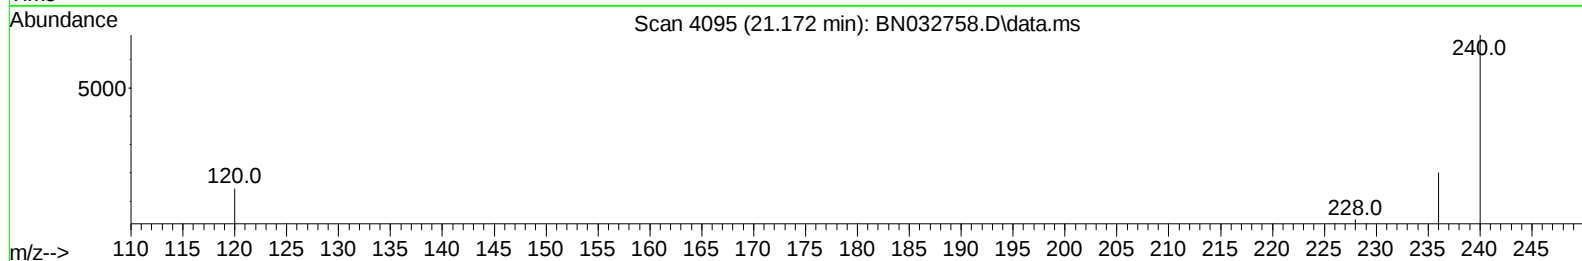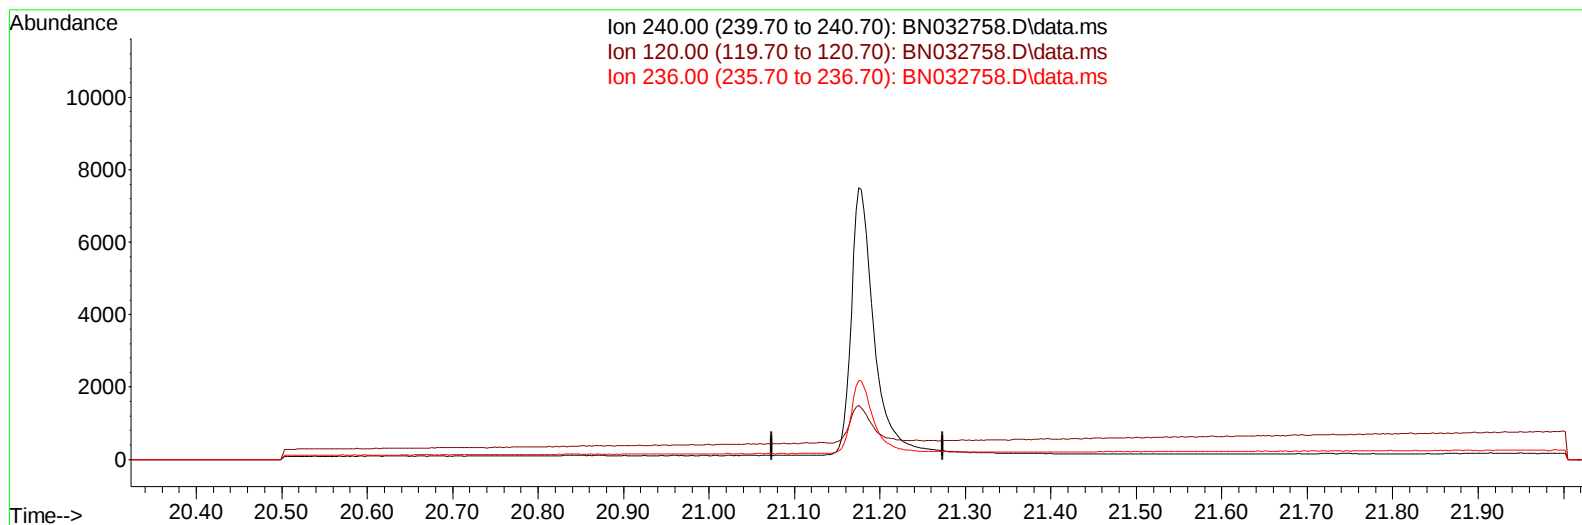

TIC: BN032758.D\data.ms

(17) Chrysene-d12

21.174min (-21.174) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	18.00	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032758.D
Acq On : 17 Jul 2024 02:08
Operator : MA/JU
Sample : PB161887BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK887

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 17 02:35:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

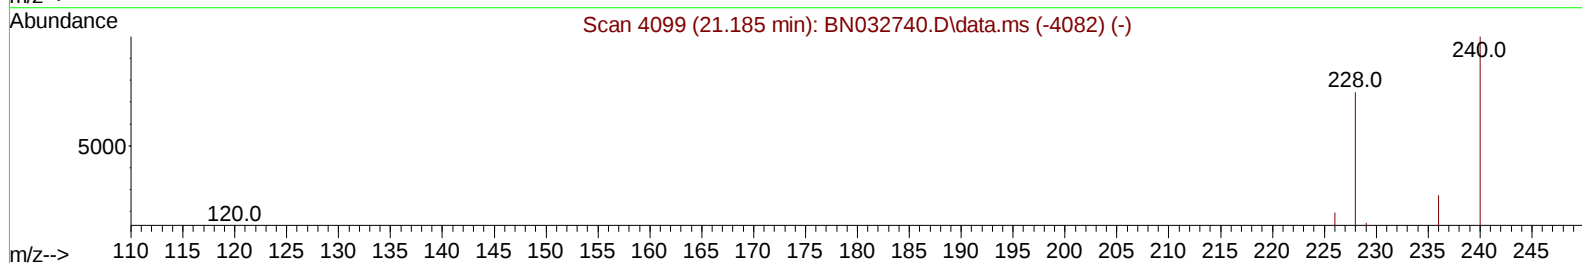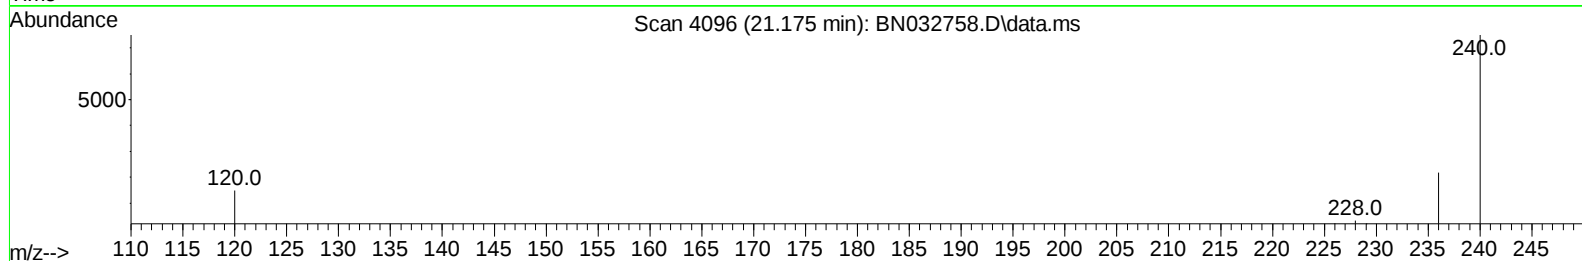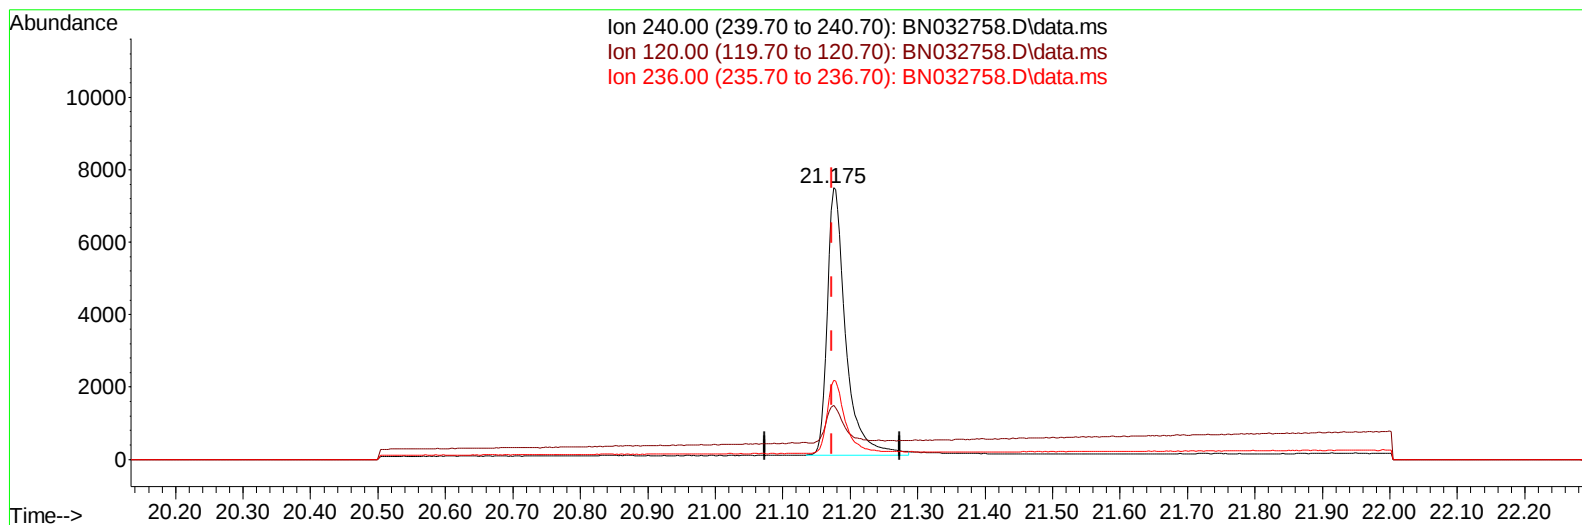

TIC: BN032758.D\data.ms

(17) Chrysene-d12

21.175min (+ 0.002) 0.40 ng/ul m

response 13962

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.00	20.02
236.00	28.40	29.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032758.D
Acq On : 17 Jul 2024 02:08
Operator : MA/JU
Sample : PB161887BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK887

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 17 02:35:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

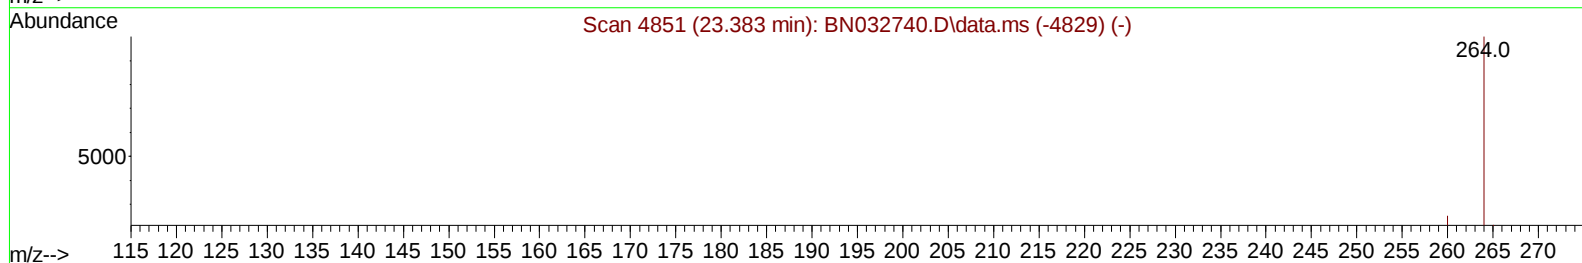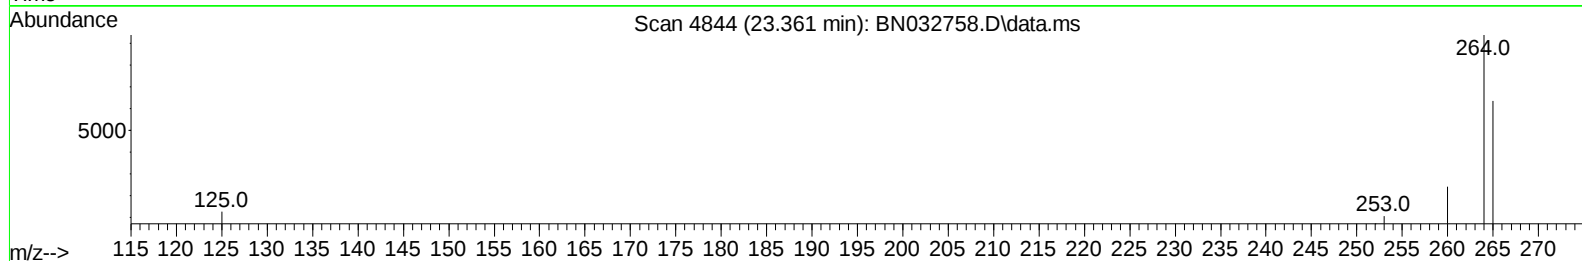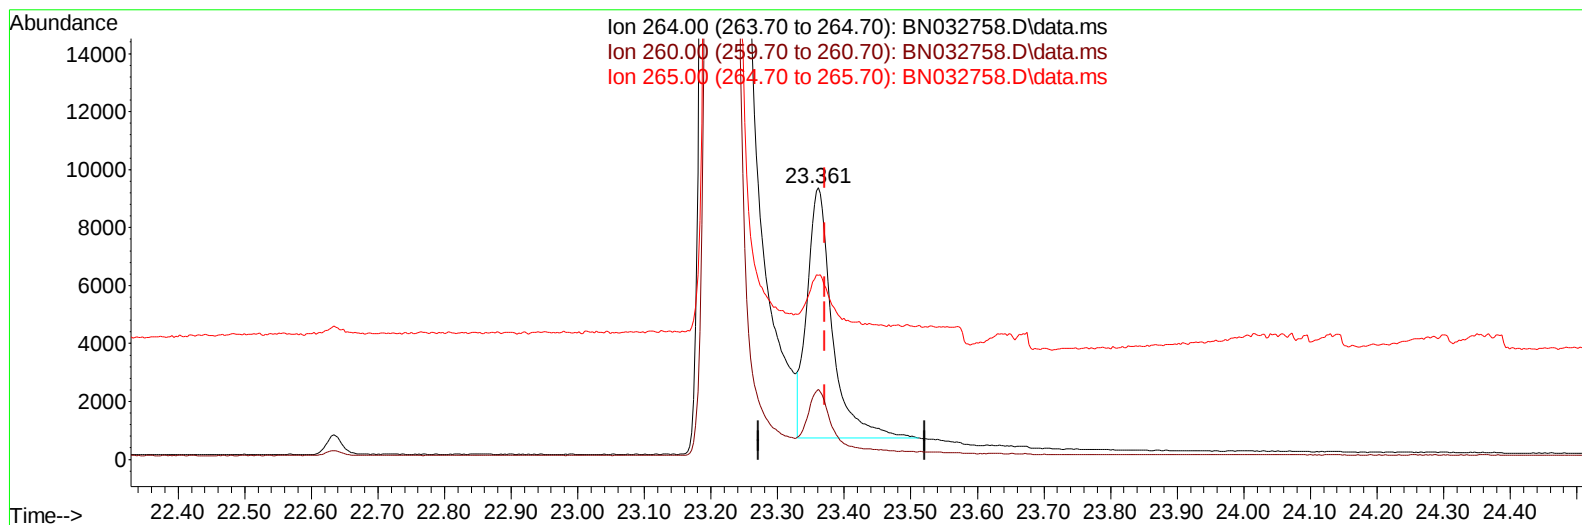

TIC: BN032758.D\data.ms

(23) Perylene-d12 (I)

23.361min (-0.010) 0.40 ng/u1

response 22715

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	25.85
265.00	95.50	67.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032758.D
Acq On : 17 Jul 2024 02:08
Operator : MA/JU
Sample : PB161887BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK887

Manual IntegrationsAPPROVED

Quant Time: Jul 17 02:35:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

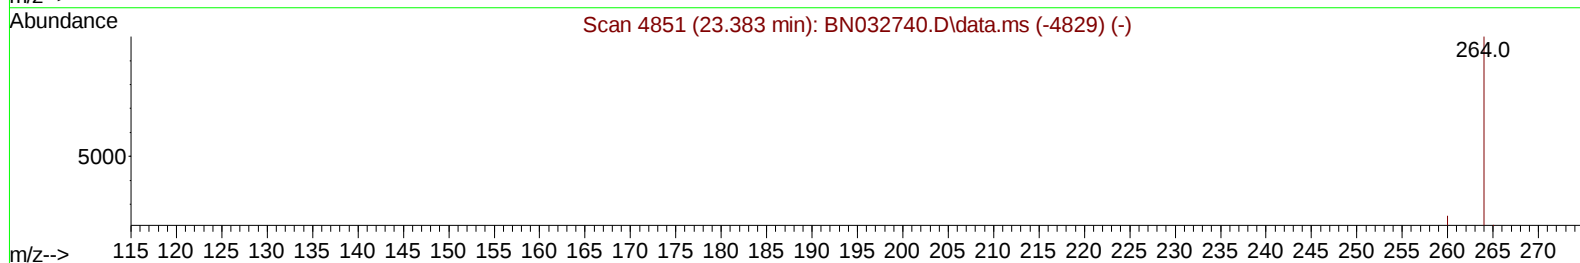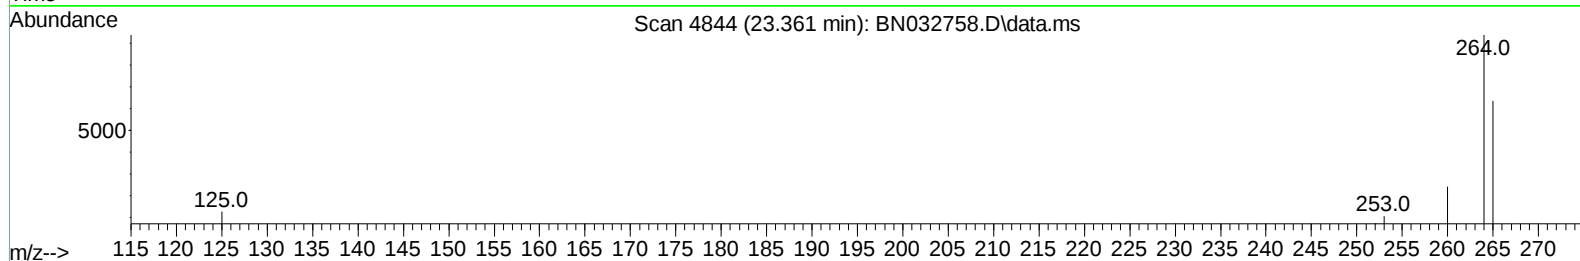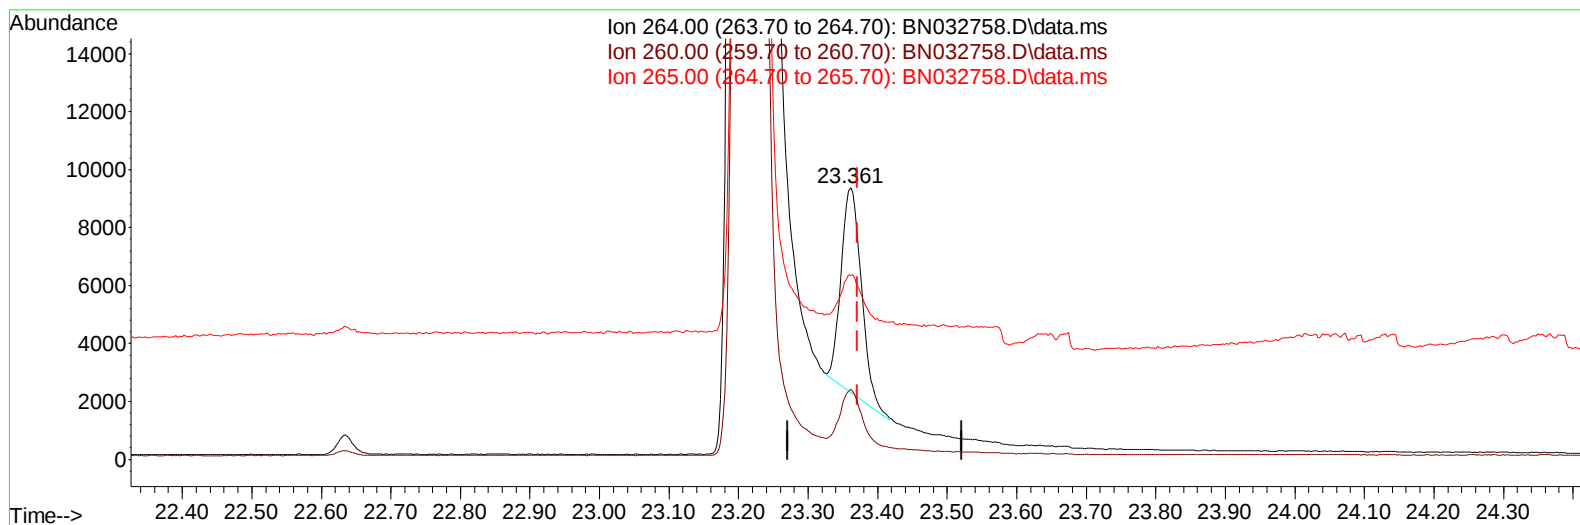

TIC: BN032758.D\data.ms

(23) Perylene-d12 (I)

23.361min (-0.010) 0.40 ng/ul m

response 14286

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	25.85
265.00	95.50	67.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
 Data File : BN032758.D
 Acq On : 17 Jul 2024 02:08
 Operator : MA/JU
 Sample : PB161887BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK887

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 17 02:35:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 17 02:35:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.544	152	5664	0.400	ng/ul	0.00
4) Naphthalene-d8	10.309	136	16990	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.192	164	9143	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.951	188	16398m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.175	240	13962m	0.400	ng/ul	0.00
23) Perylene-d12	23.361	264	14286m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	39445	5.800	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.931	152	6260	0.244	ng/ul	0.00
18) Fluoranthene-d10	18.993	212	13263	0.291	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032758.D
Acq On : 17 Jul 2024 02:08
Operator : MA/JU
Sample : PB161887BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK887

Manual IntegrationsAPPROVED

Quant Time: Jul 17 02:35:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

