




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

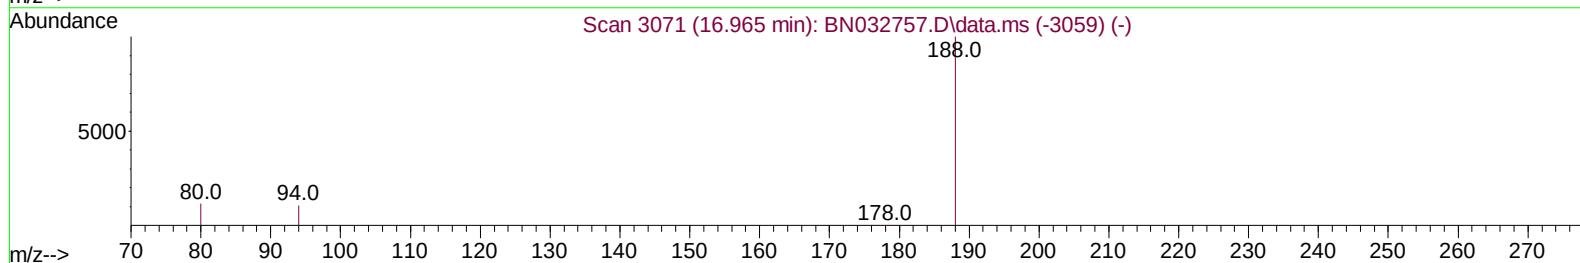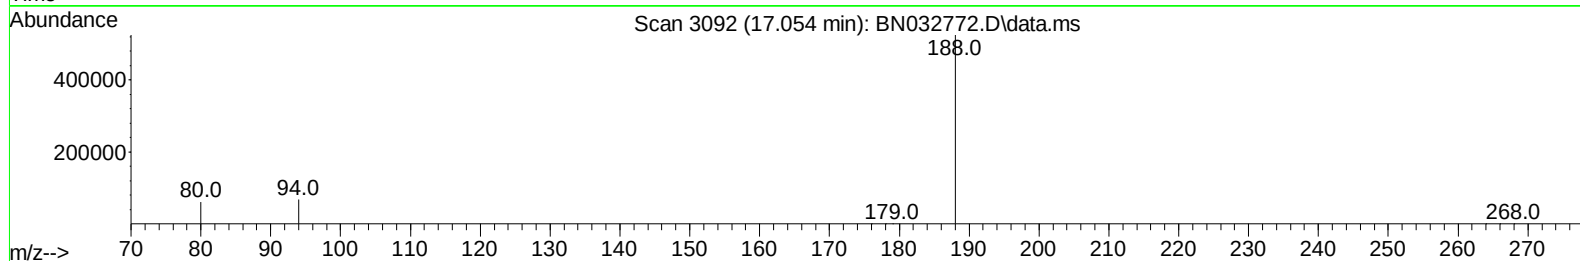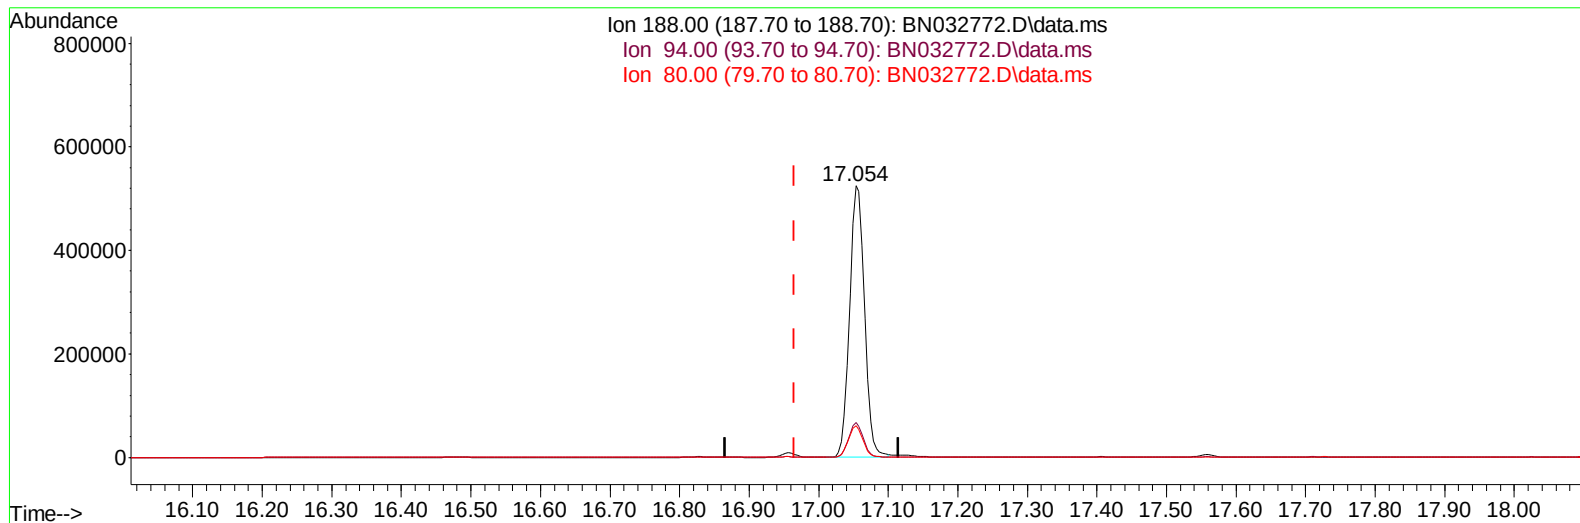

TIC: BN032772.D\data.ms

(13) Phenanthrene-d10 (I)

17.054min (+ 0.088) 0.40 ng/u1

response 780128

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	12.86
80.00	12.00	11.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

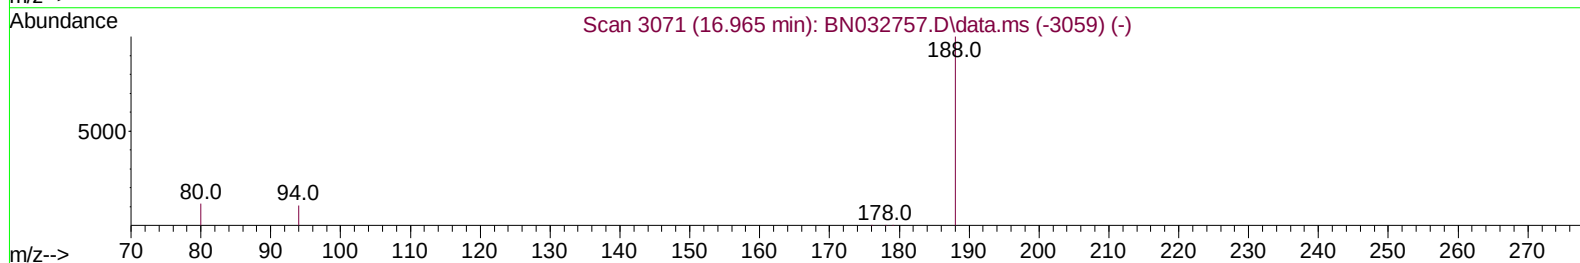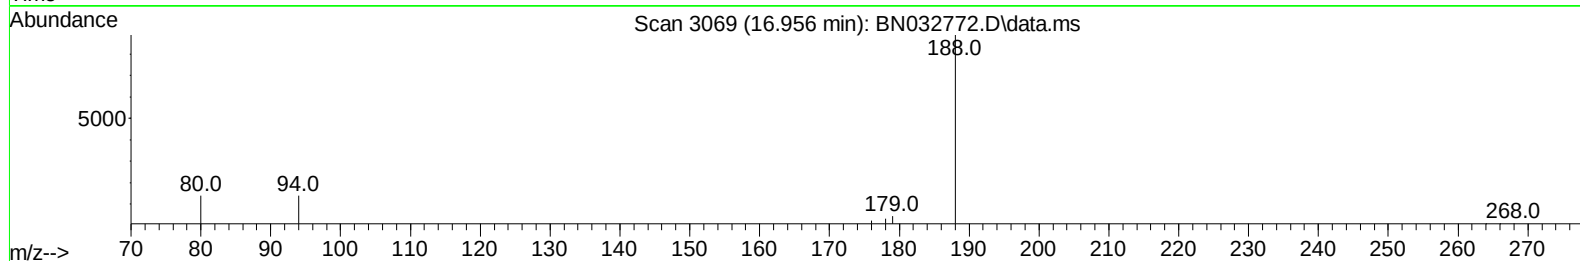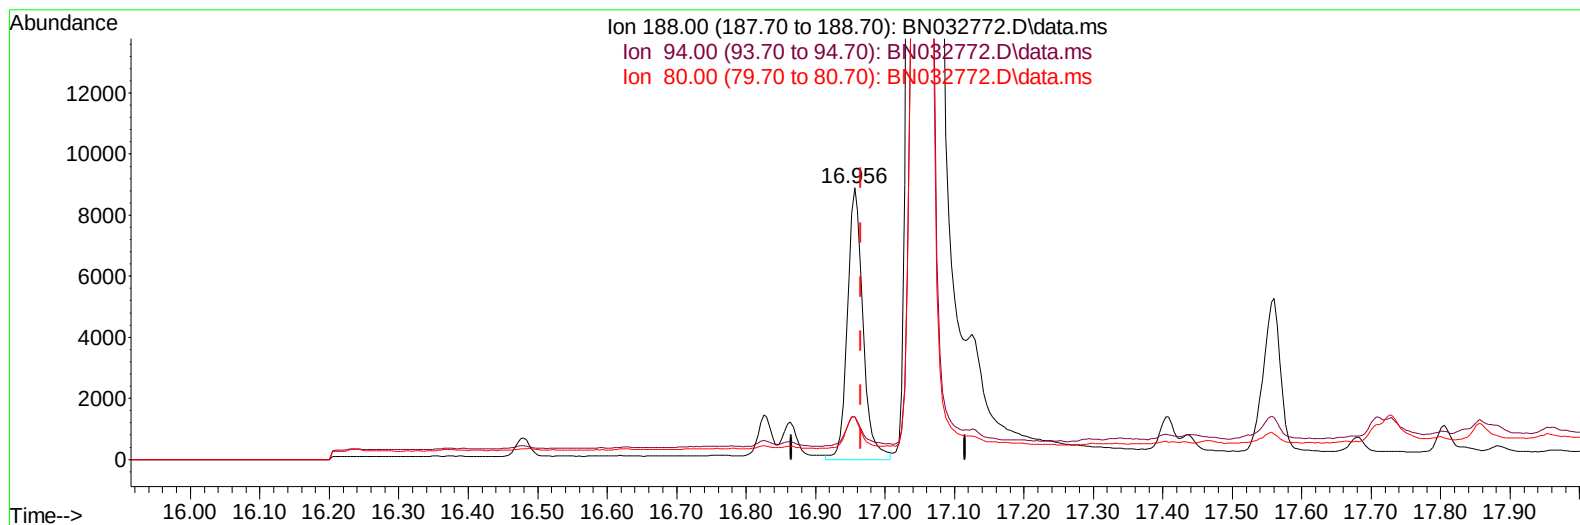

TIC: BN032772.D\data.ms

(13) Phenanthrene-d10 (I)

16.956min (-0.009) 0.40 ng/ul m

response 13876

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	15.70#
80.00	12.00	15.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

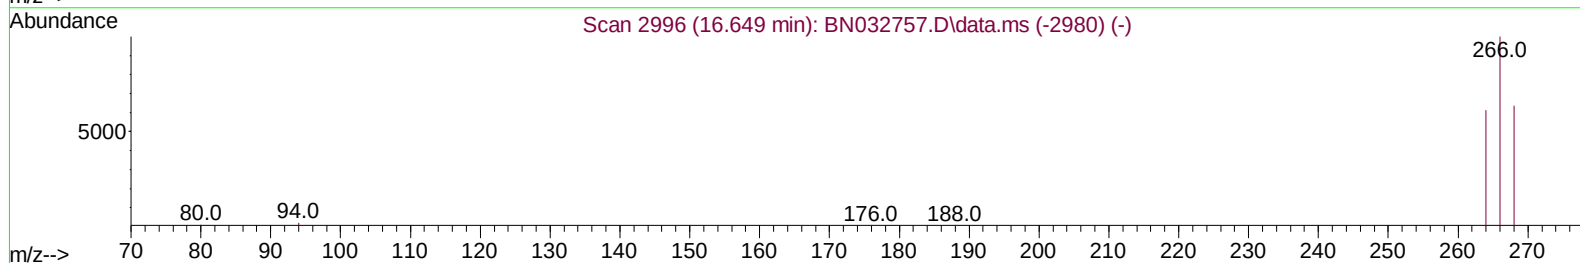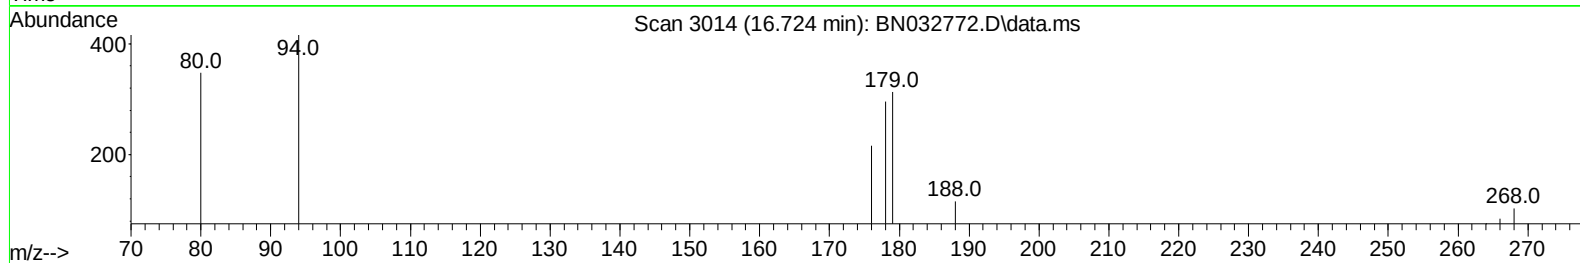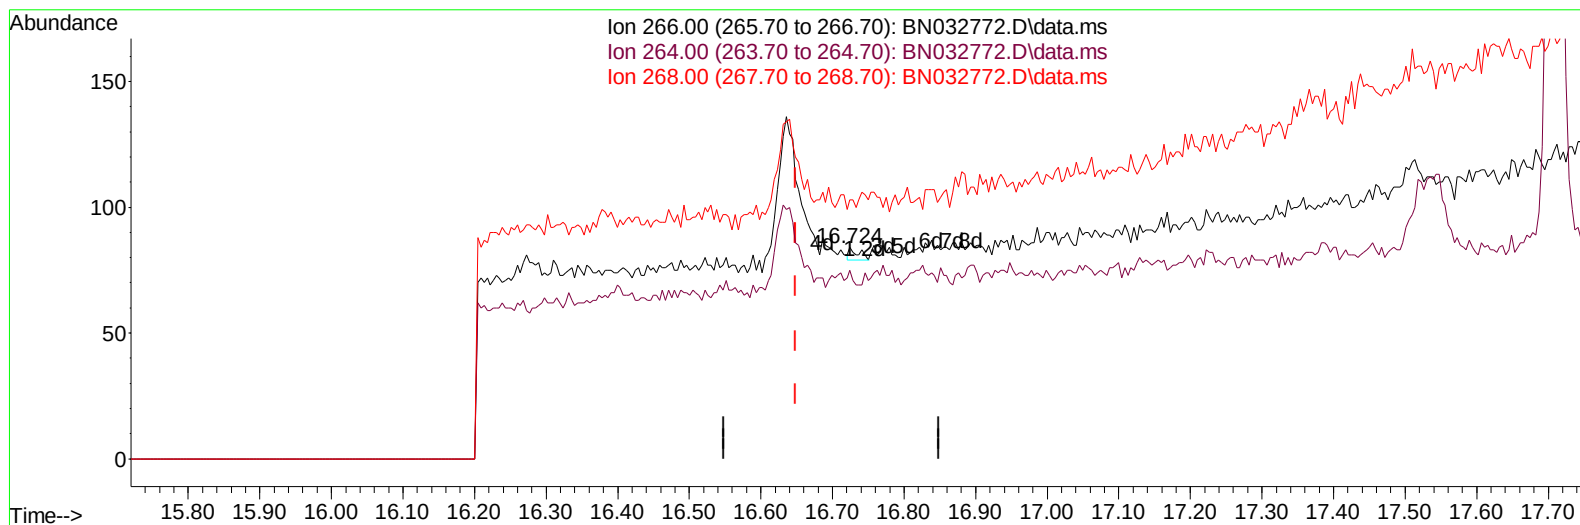

TIC: BN032772.D\data.ms

(14) Pentachlorophenol

16.724min (+ 0.075) 0.00 ng/u1

response	5	
Ion	Exp%	Act%
266.00	100.00	100.00
264.00	61.80	140.00#
268.00	64.50	80.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

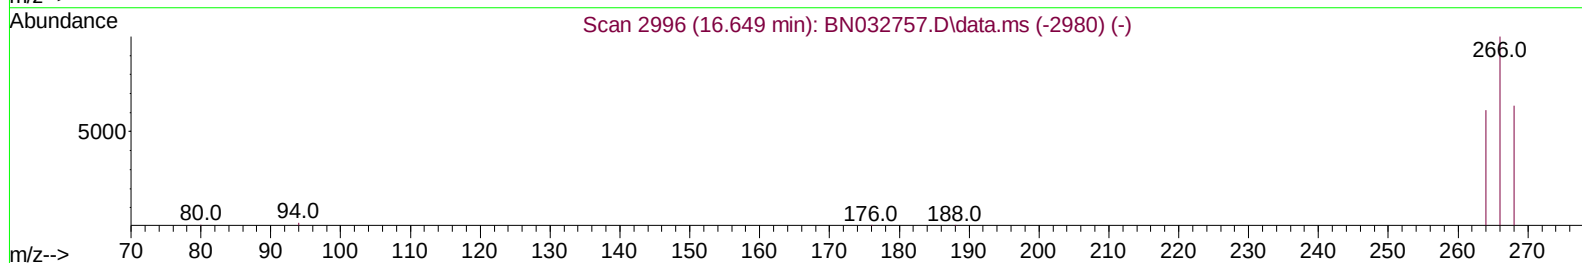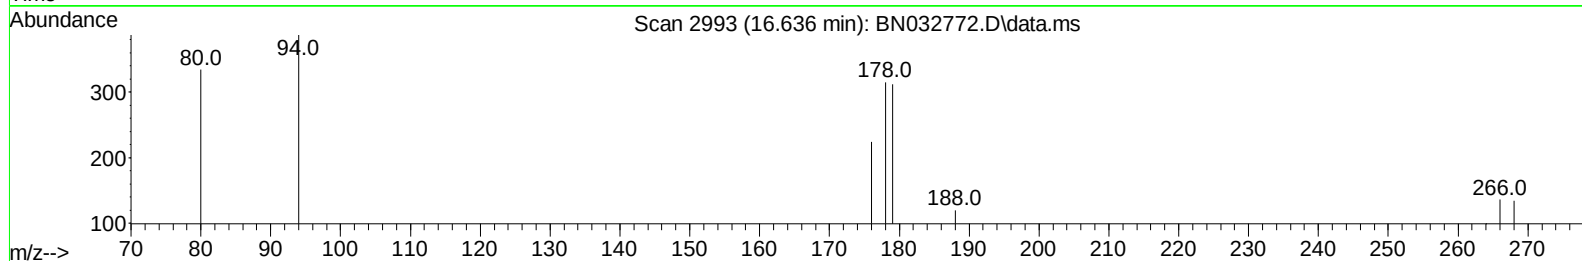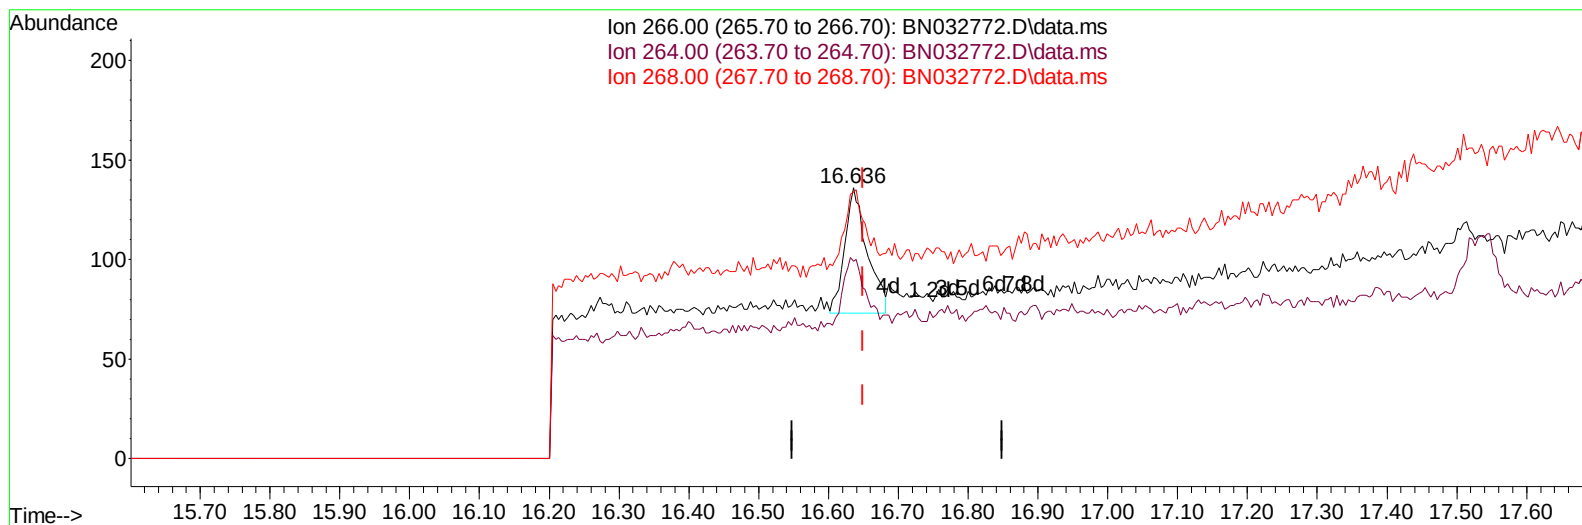

TIC: BN032772.D\data.ms

(14) Pentachlorophenol

16.636min (-0.013) 0.06 ng/ul m

response 141

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	61.80	4.96#
268.00	64.50	2.84#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

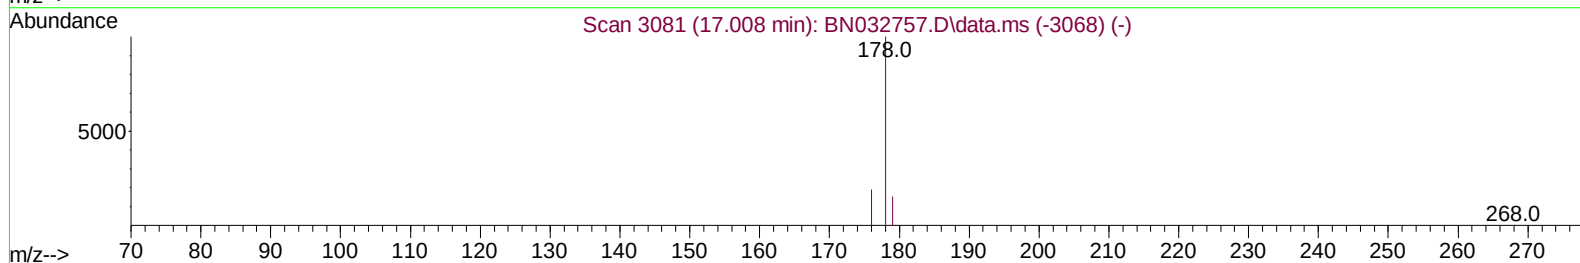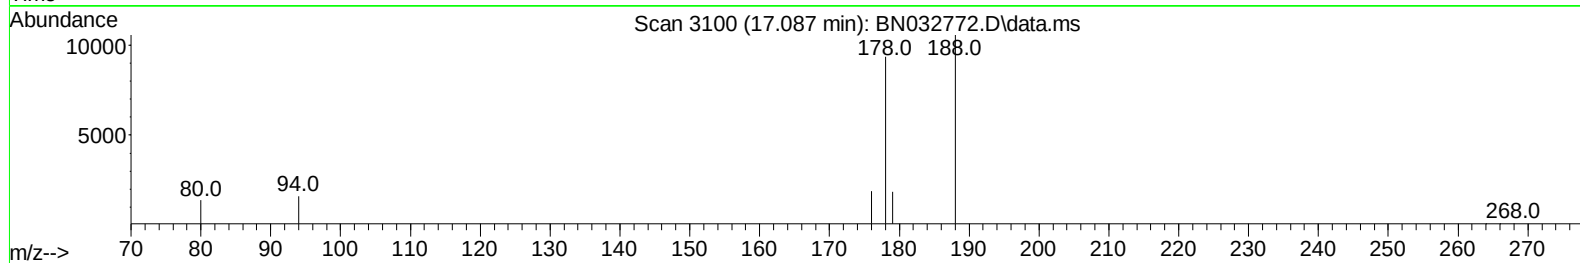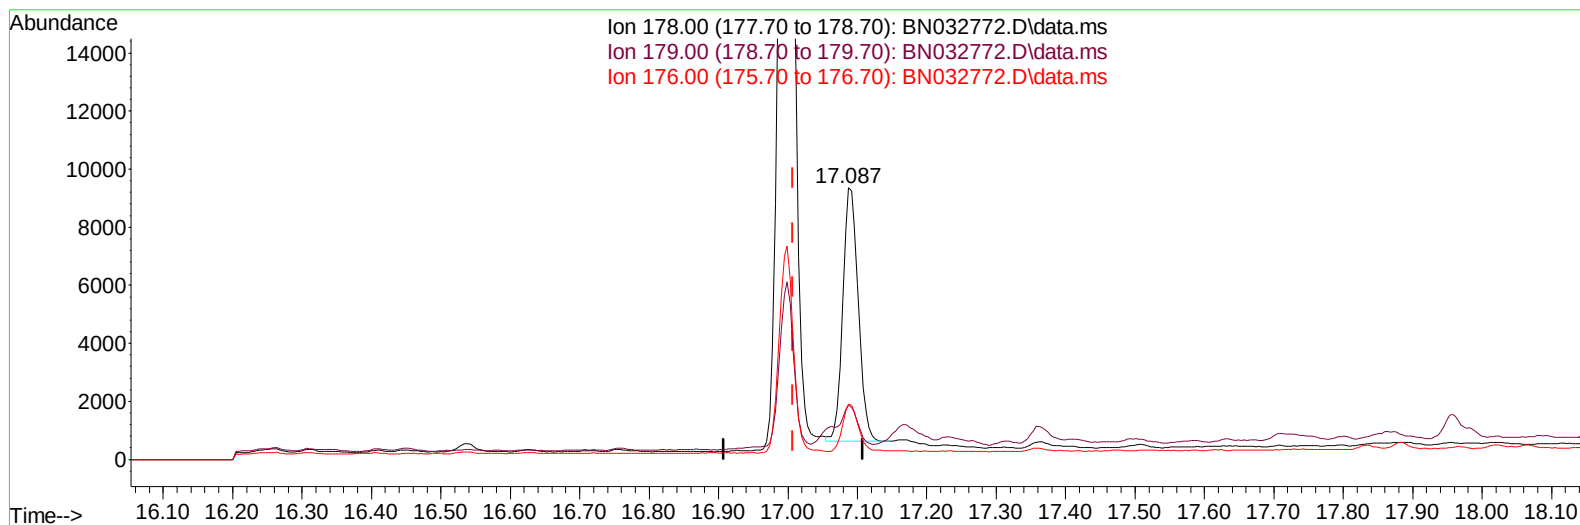

TIC: BN032772.D\data.ms

(15) Phenanthrene

17.087min (+ 0.080) 0.36 ng/ul

response 13534

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.20	19.85#
176.00	19.50	20.36
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
 Data File : BN032772.D
 Acq On : 17 Jul 2024 10:35
 Operator : MA/JU
 Sample : P3177-03
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 17 02:35:25 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :mohammad ahmed 07/19/2024

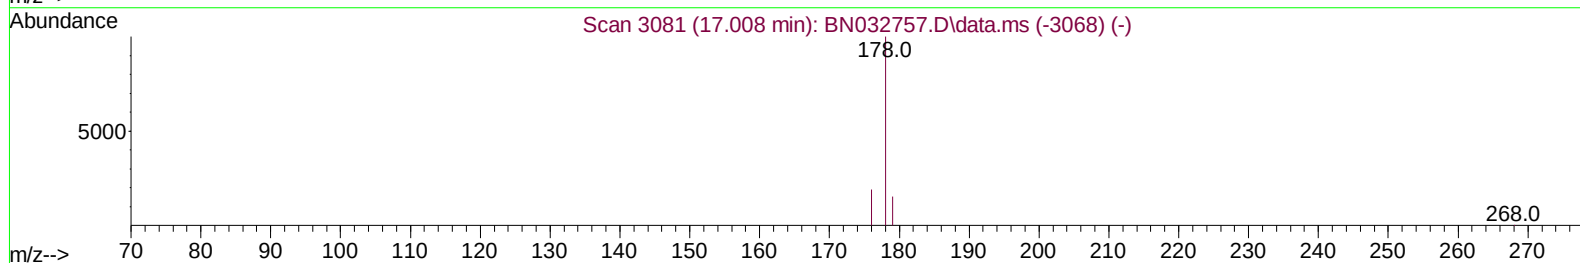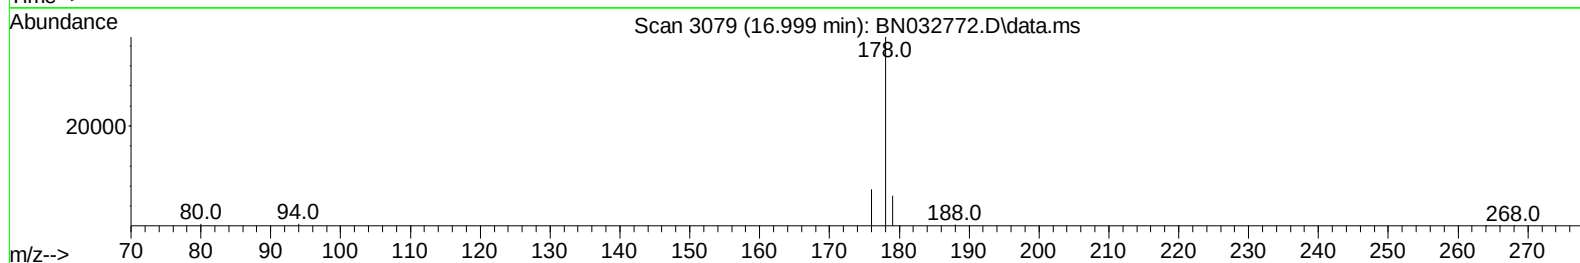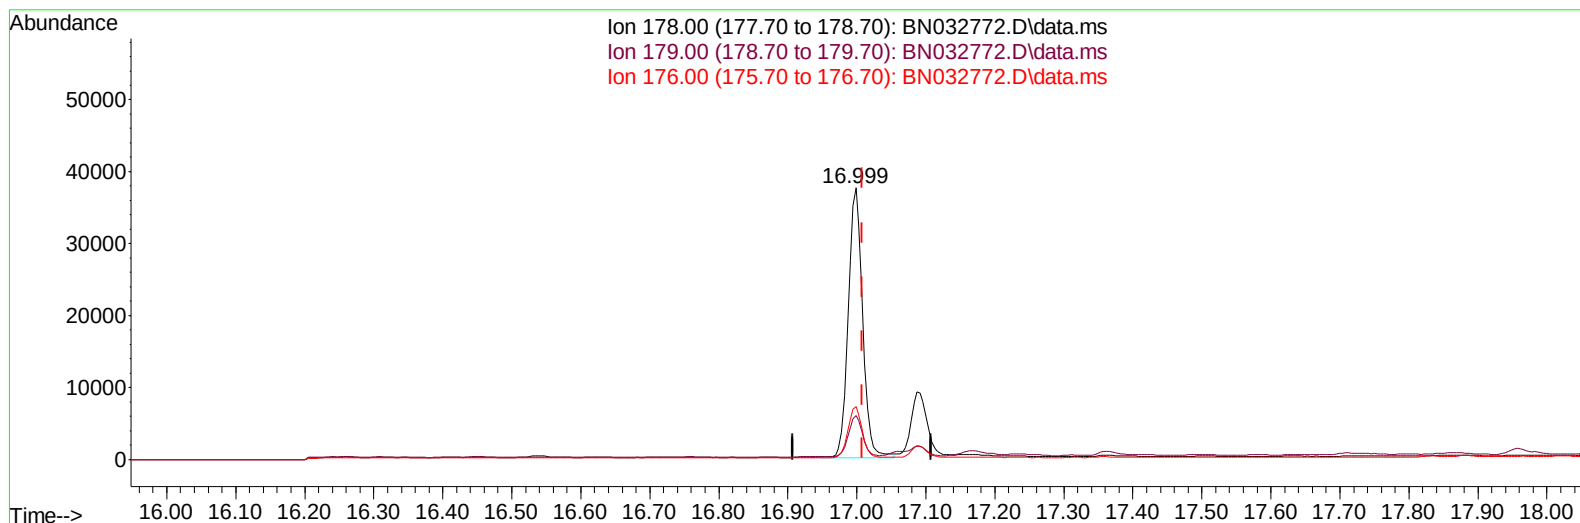

TIC: BN032772.D\data.ms

(15) Phenanthrene

16.999min (-0.009) 1.44 ng/ul m

response 54521

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.20	16.20
176.00	19.50	19.49
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

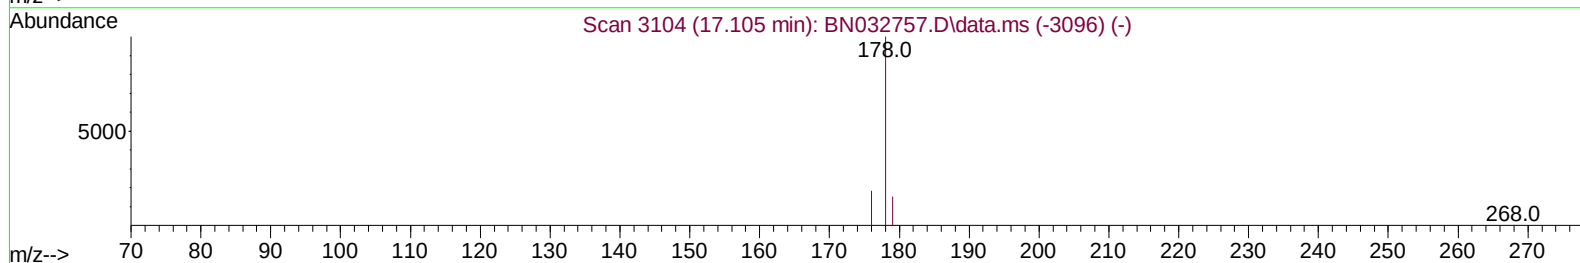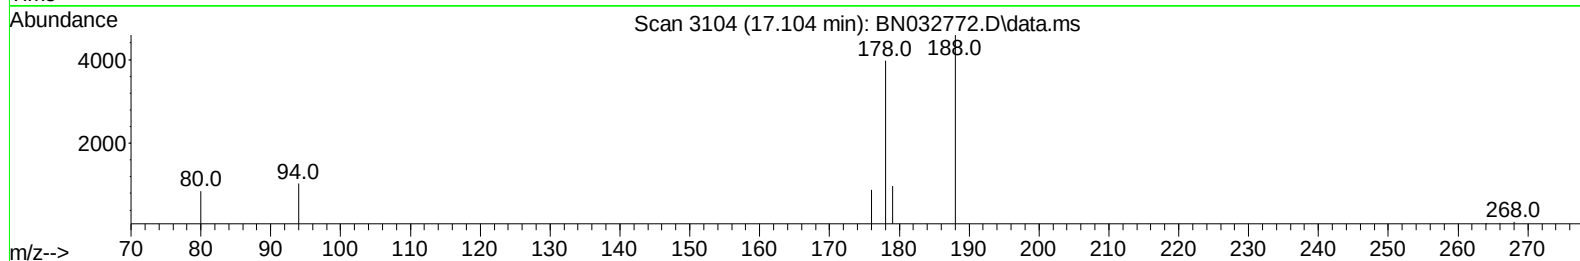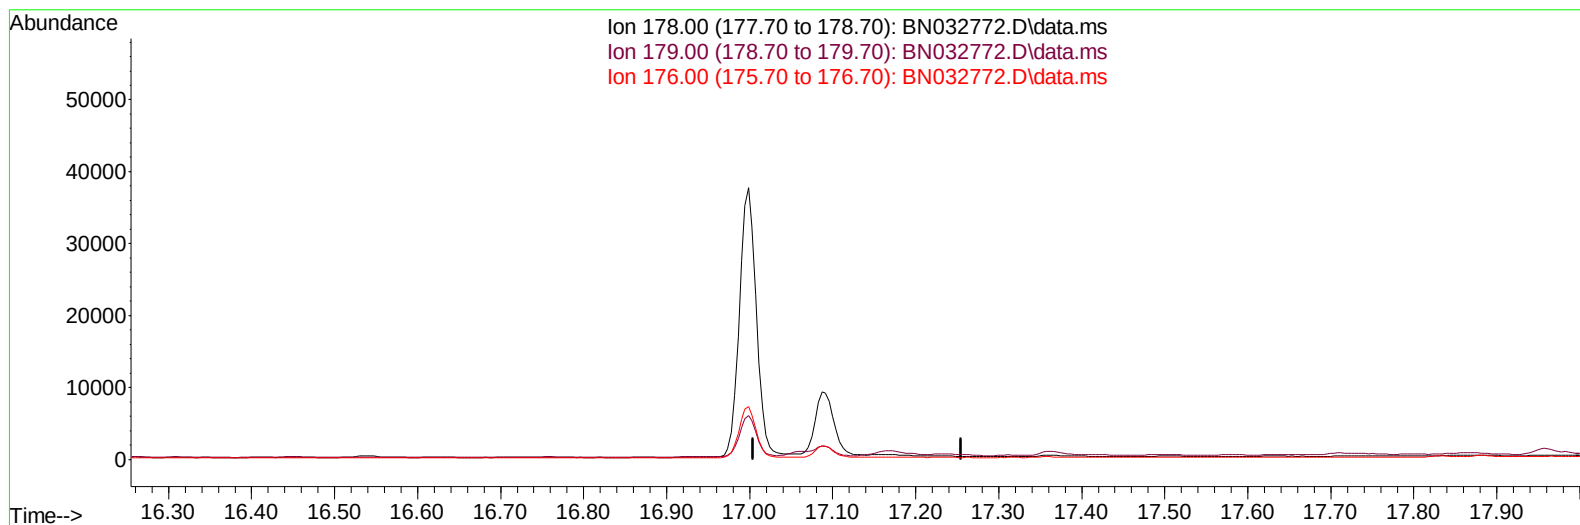

TIC: BN032772.D\data.ms

(16) Anthracene

17.105min (-17.105) 0.00 ng/u1

response 0

Ion	Exp%	Act%
178.00	100.00	0.00
179.00	16.80	0.00#
176.00	19.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

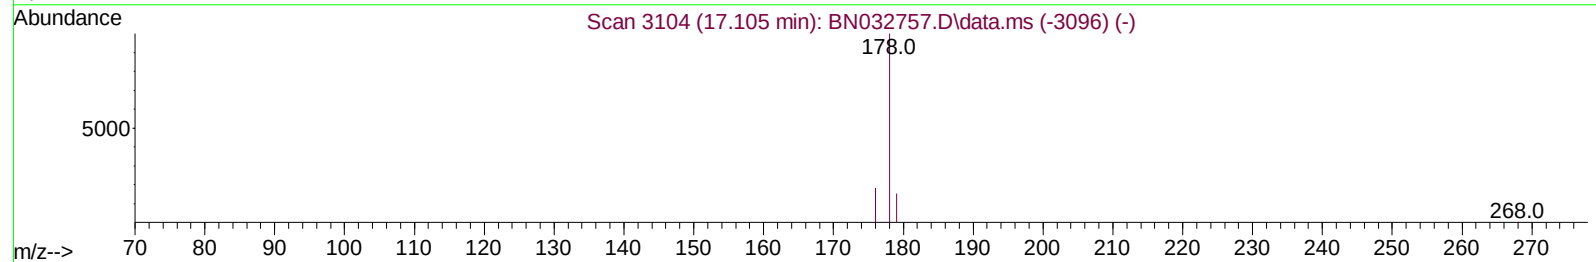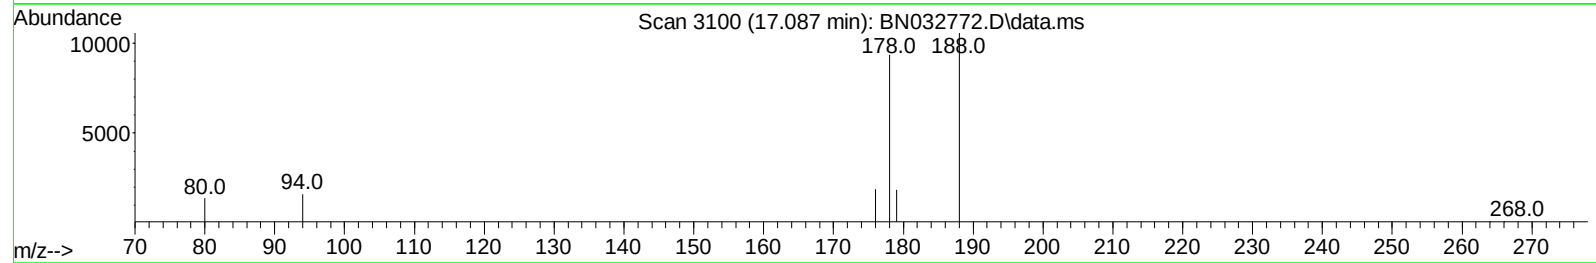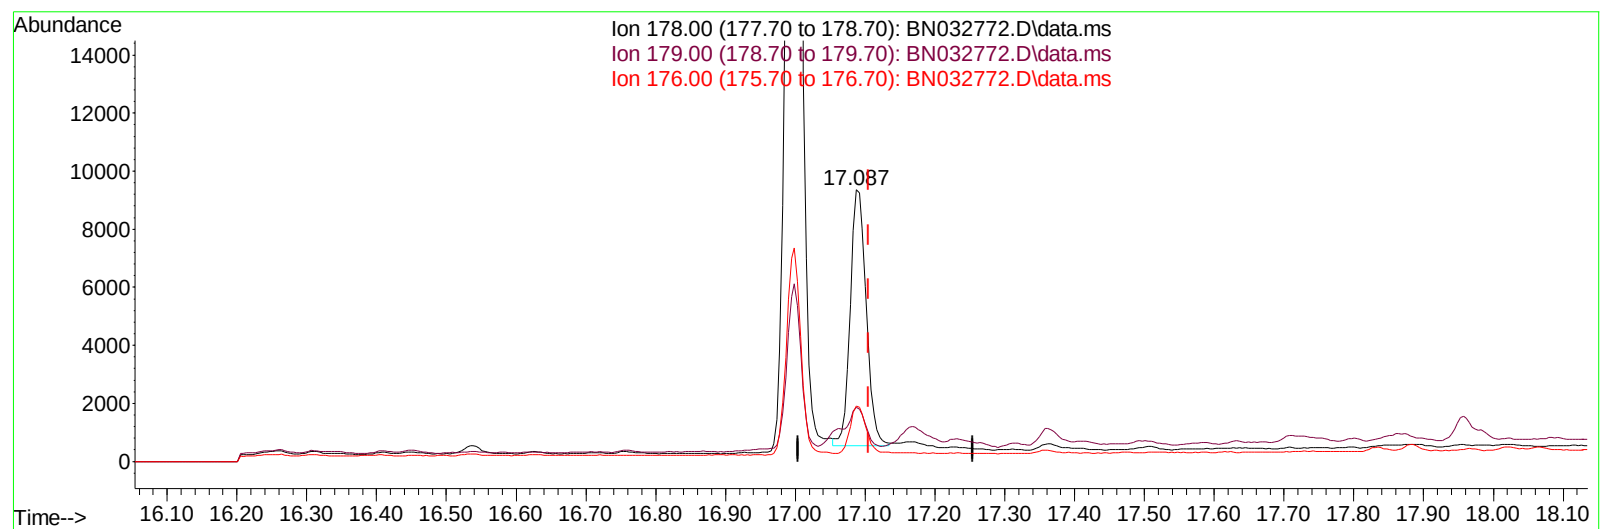

TIC: BN032772.D\data.ms

(16) Anthracene

17.087min (-0.017) 0.45 ng/ul m

response 13952

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.80	19.85
176.00	19.20	20.36
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

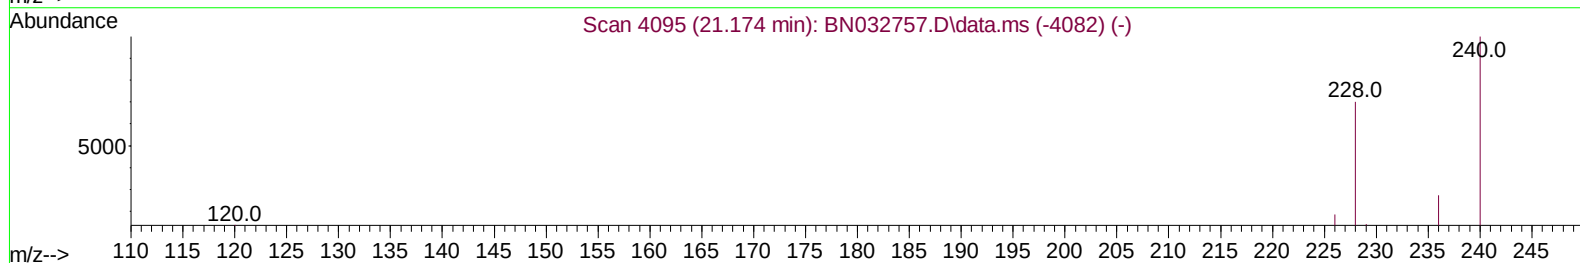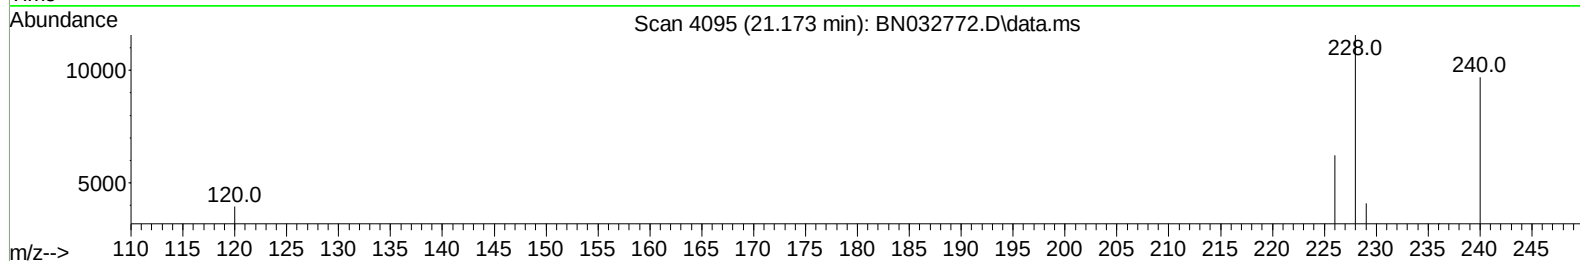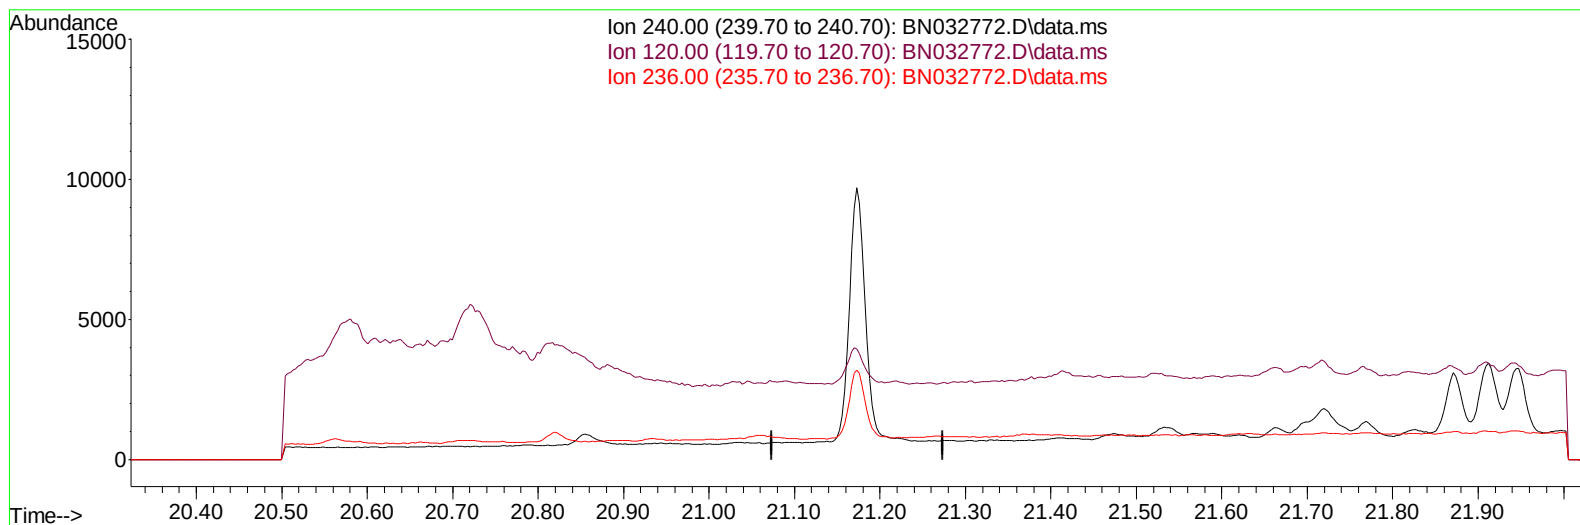

TIC: BN032772.D\data.ms

(17) Chrysene-d12

21.174min (-21.174) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	18.00	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

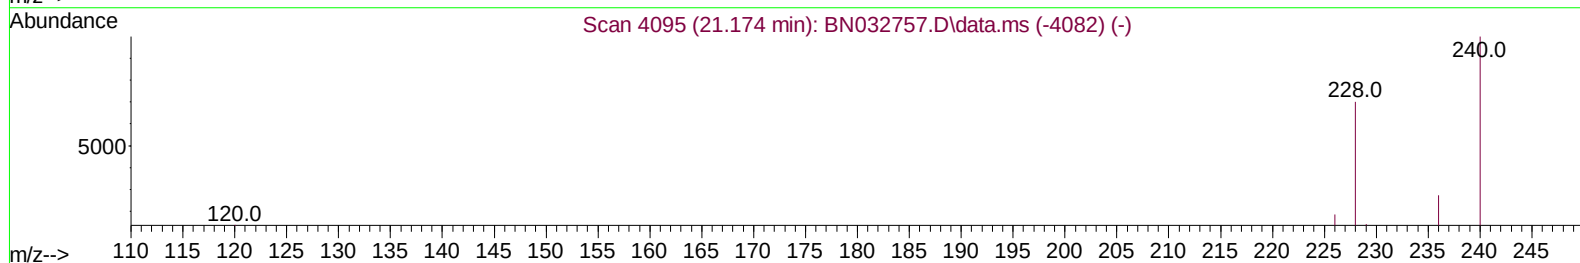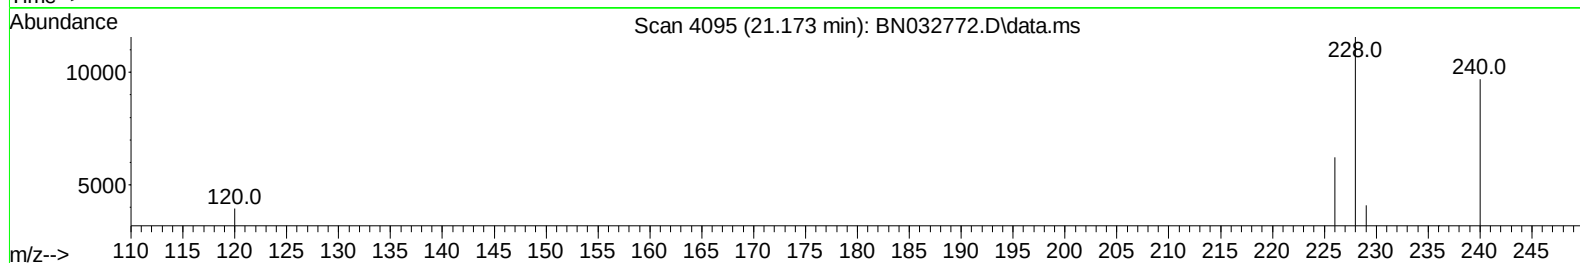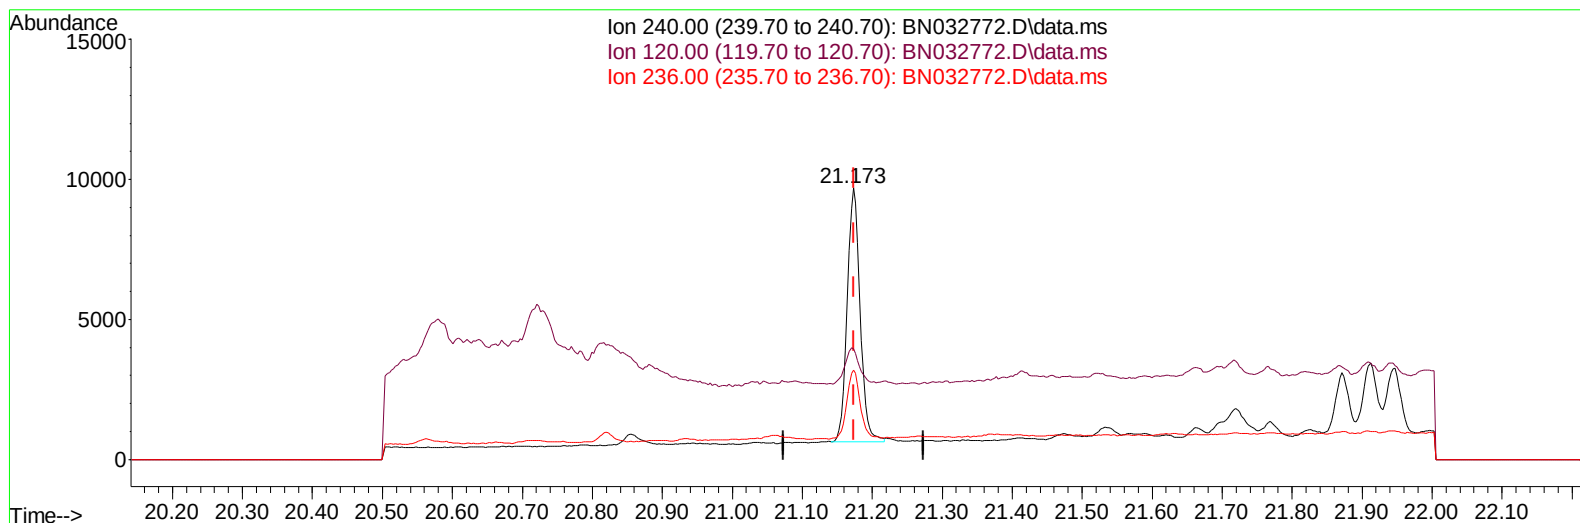

TIC: BN032772.D\data.ms

(17) Chrysene-d12

21.173min (-0.001) 0.40 ng/ul m

response 11700

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.00	40.79#
236.00	28.40	32.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

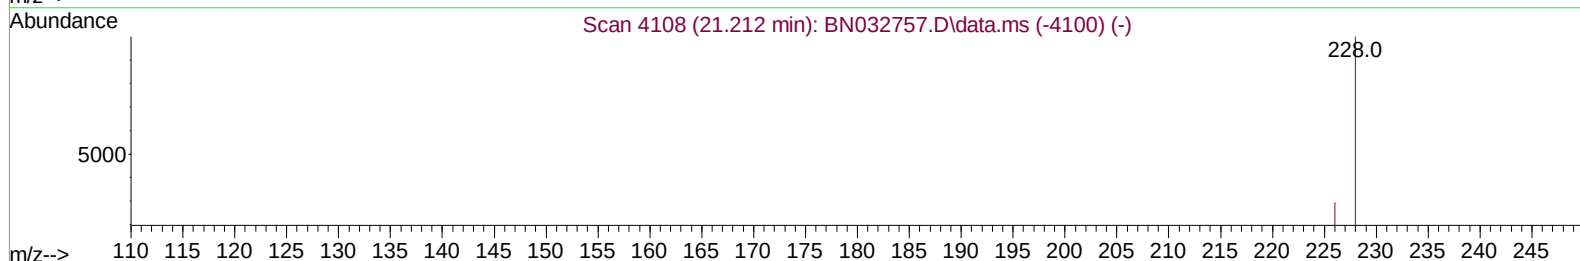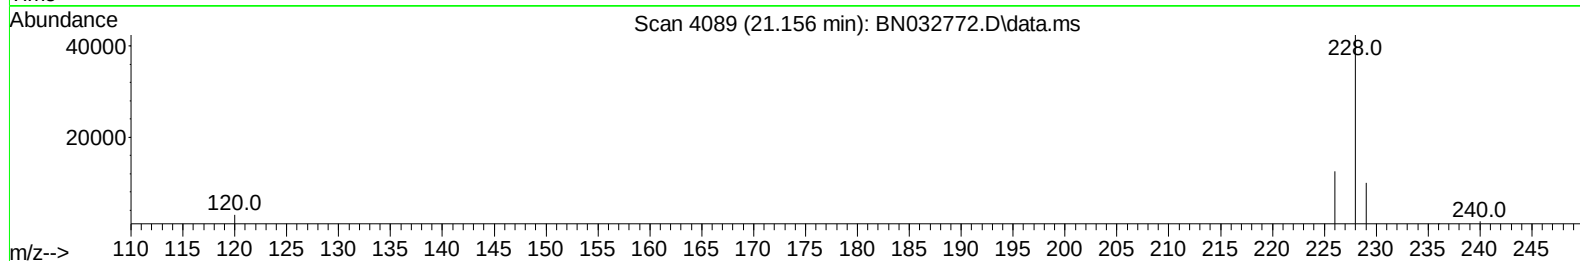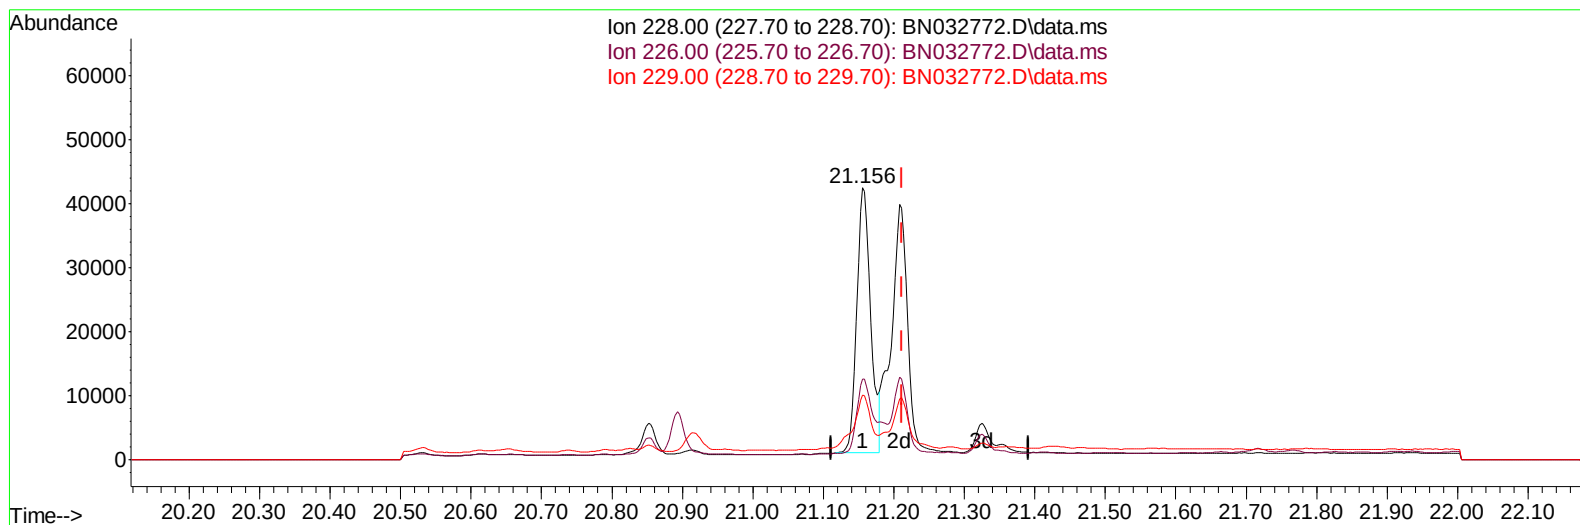

TIC: BN032772.D\data.ms

(22) Chrysene

21.156min (-0.056) 1.06 ng/u1

response 56872

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.00	29.58
229.00	19.70	23.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

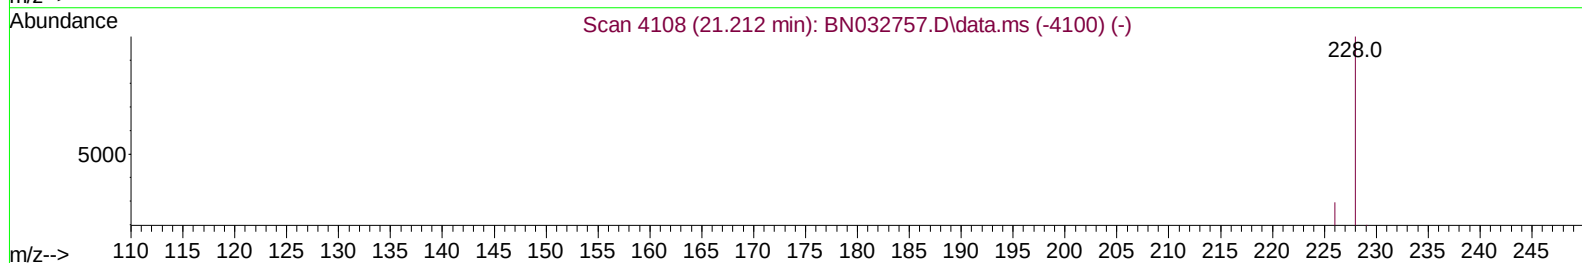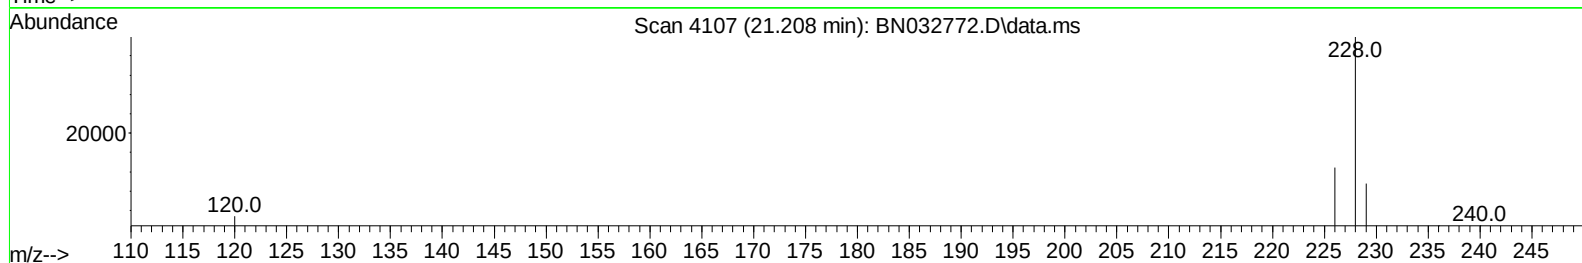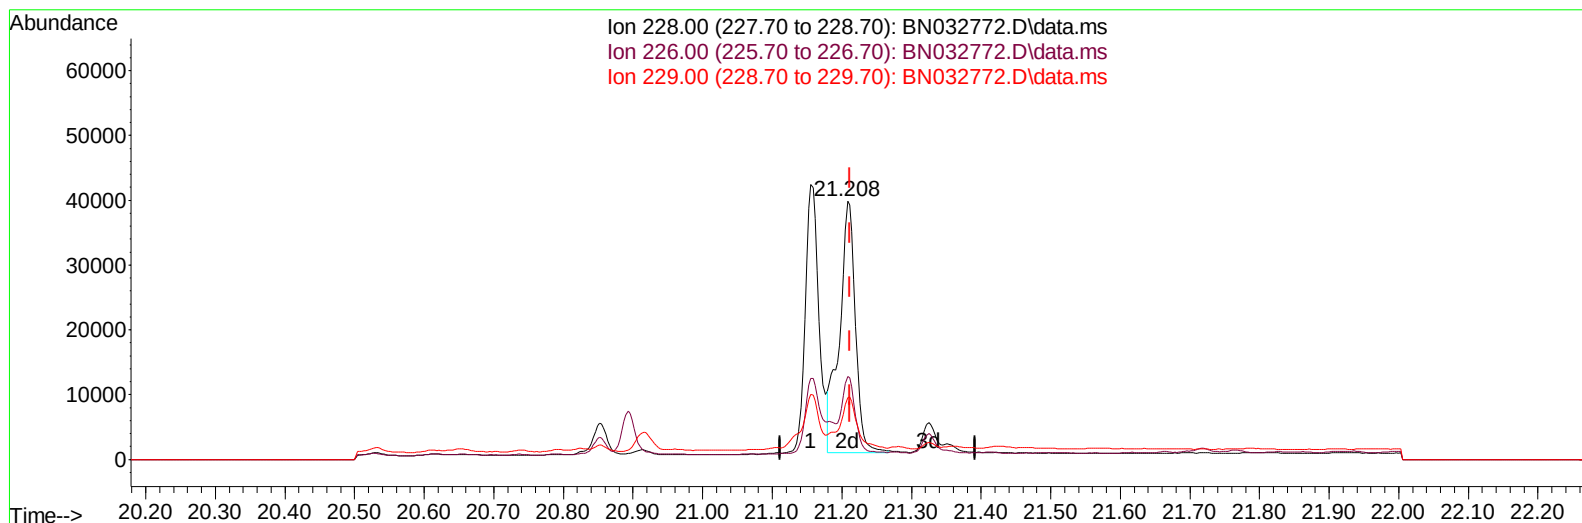

TIC: BN032772.D\data.ms

(22) Chrysene

21.208min (-0.003) 1.15 ng/ul m

response 62185

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.00	32.14
229.00	19.70	23.84#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

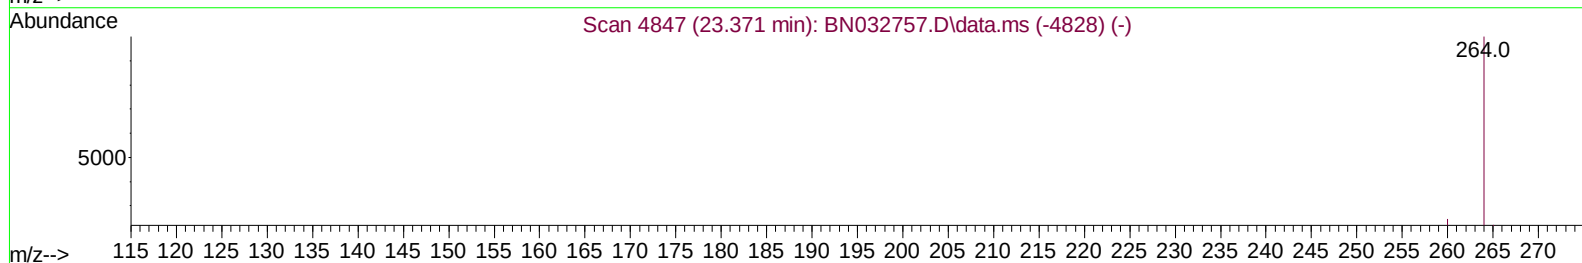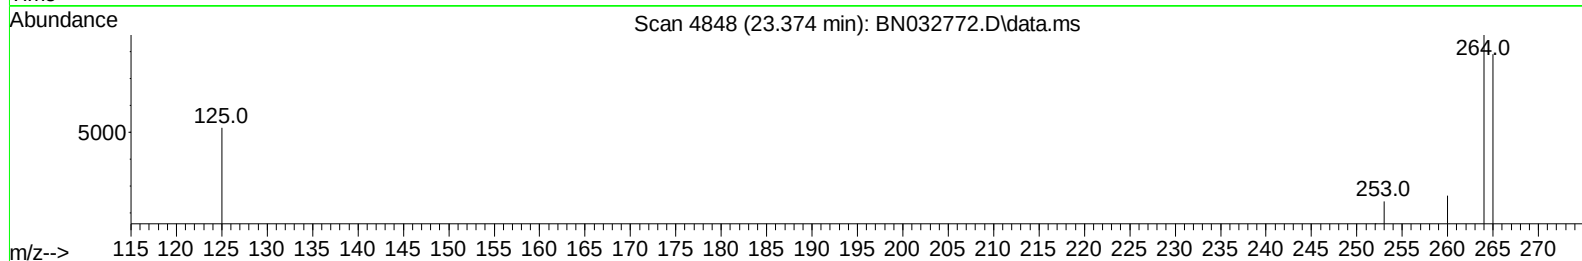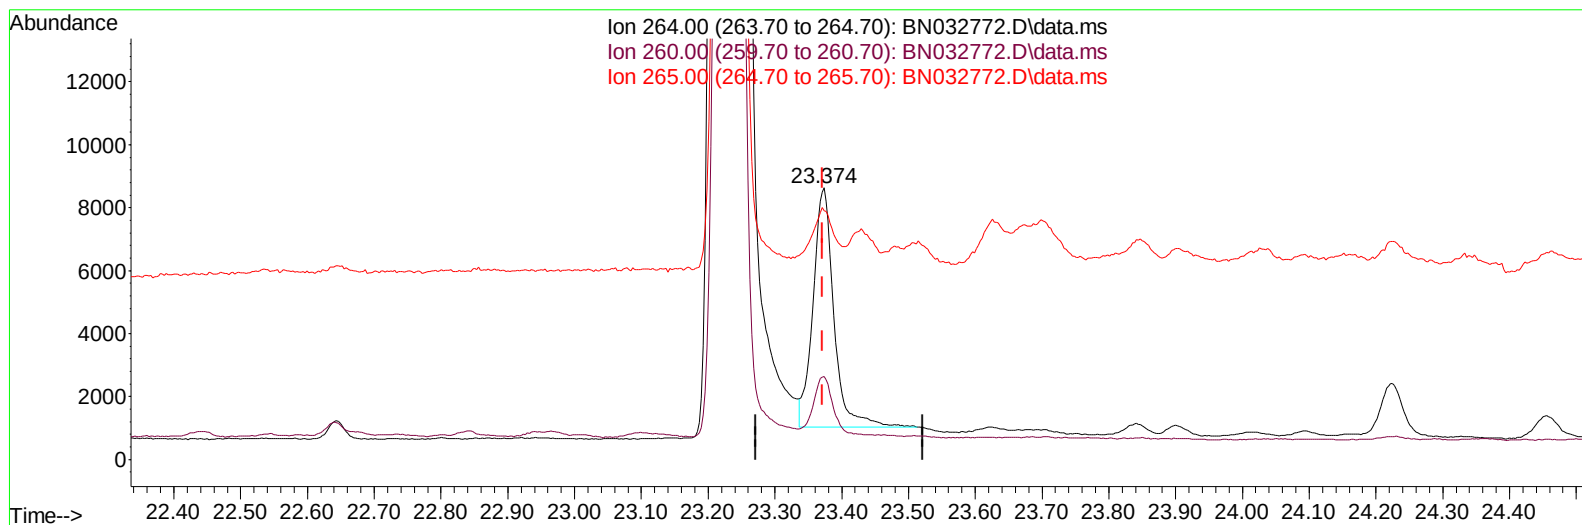

TIC: BN032772.D\data.ms

(23) Perylene-d12 (I)

23.374min (+ 0.002) 0.40 ng/ul

response 16543

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	30.61
265.00	95.50	91.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

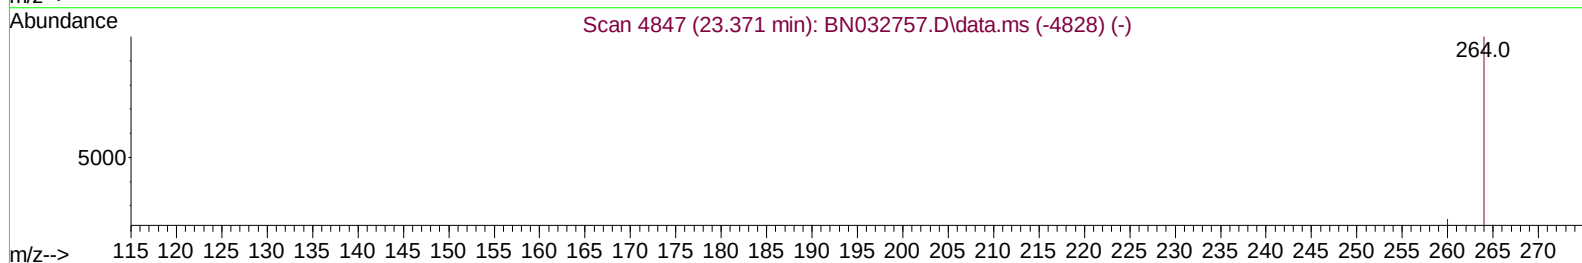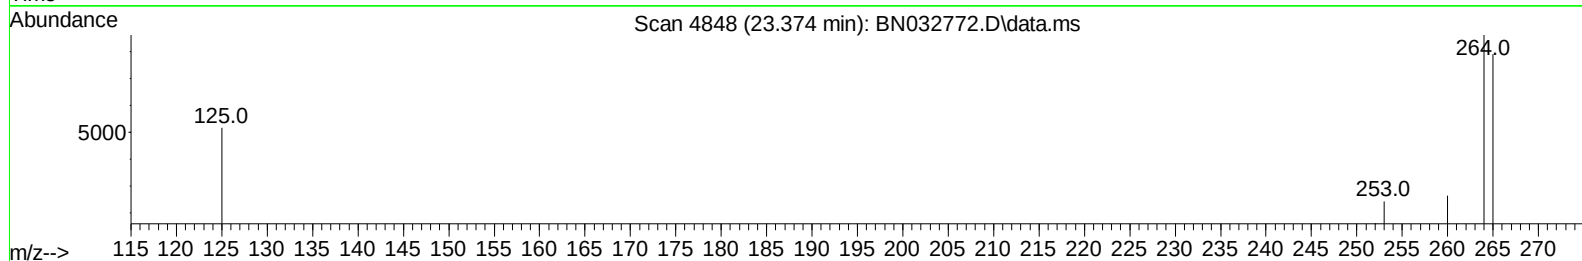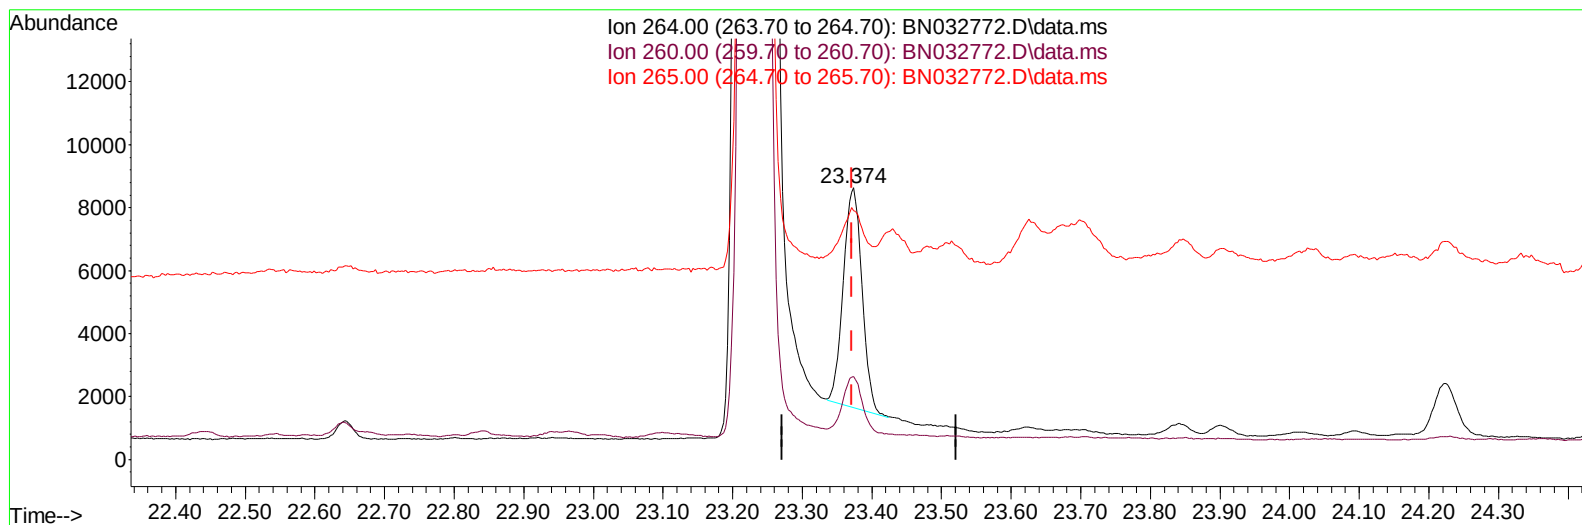

TIC: BN032772.D\data.ms

(23) Perylene-d12 (I)

23.374min (+ 0.002) 0.40 ng/ul m

response 12886

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	30.61
265.00	95.50	91.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

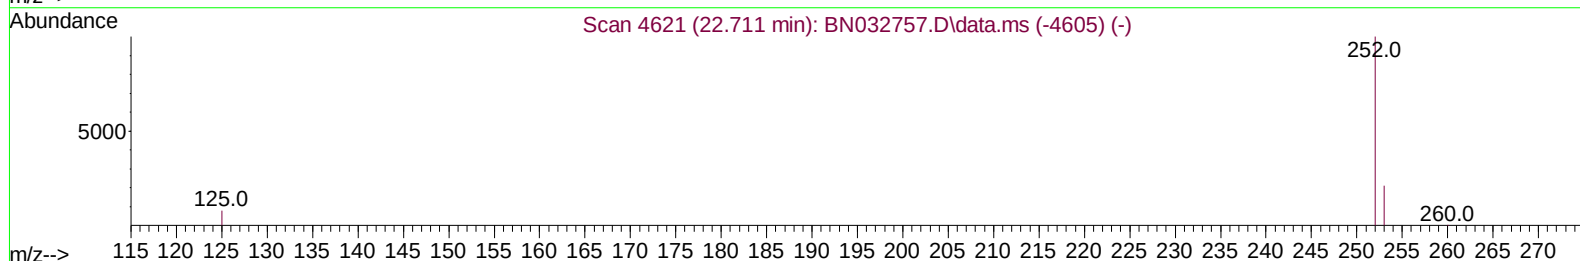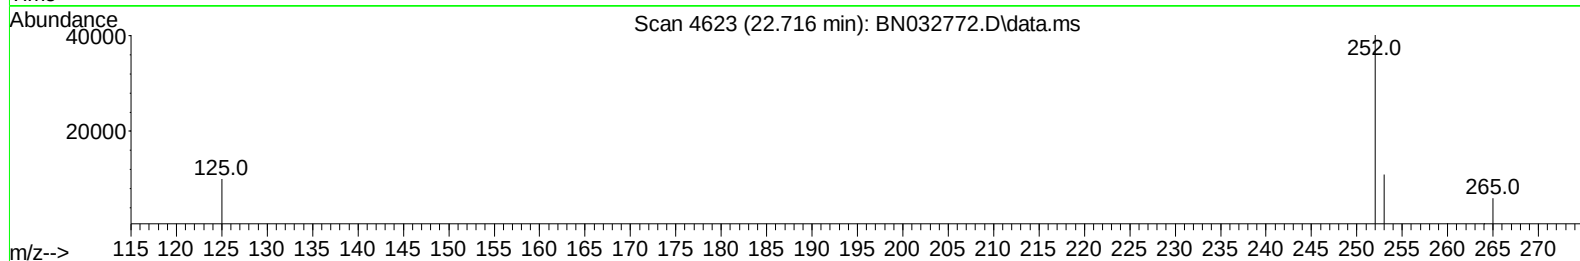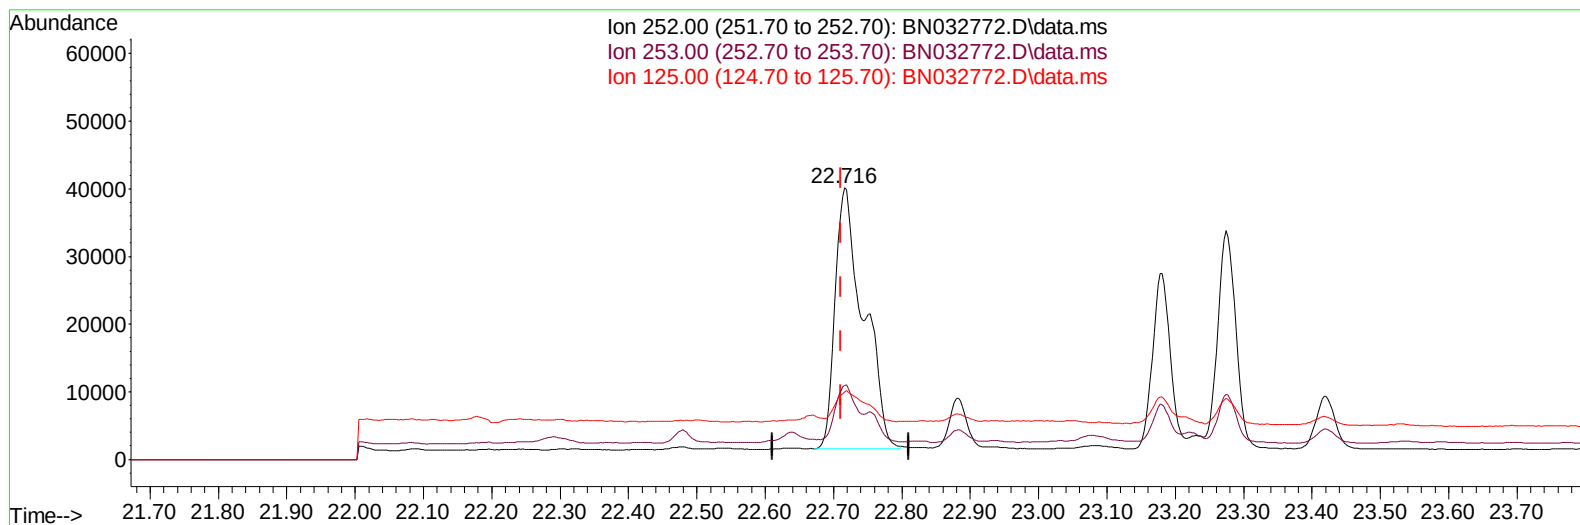

TIC: BN032772.D\data.ms

(24) Benzo(b)fluoranthene

22.716min (+ 0.005) 2.44 ng/u1

response 111091

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	27.23
125.00	18.00	24.93
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

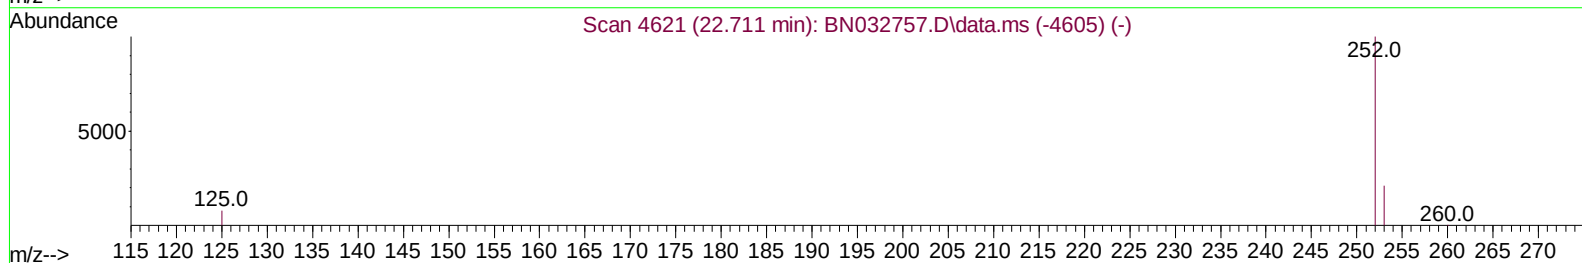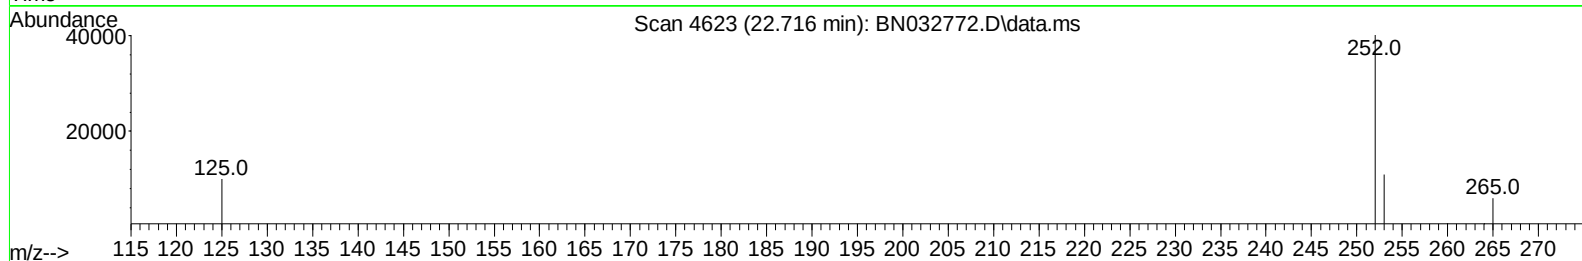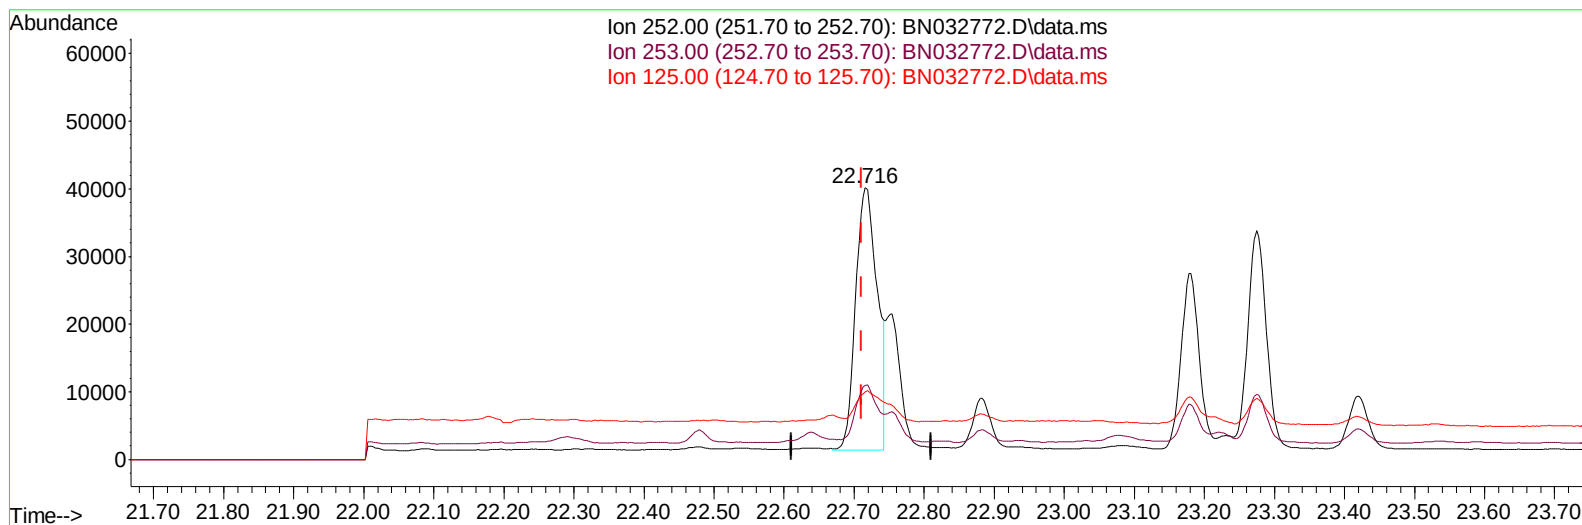

TIC: BN032772.D\data.ms

(24) Benzo(b)fluoranthene

22.716min (+ 0.005) 1.82 ng/ul m

response 82974

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	27.23
125.00	18.00	24.93
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

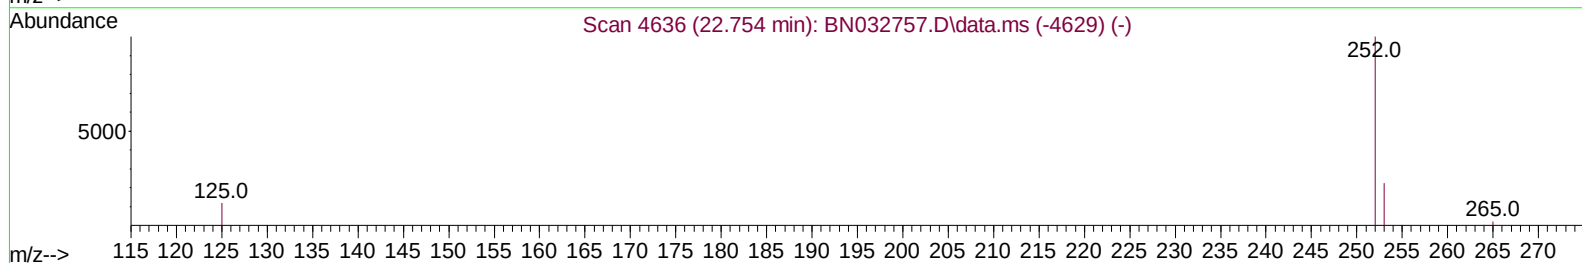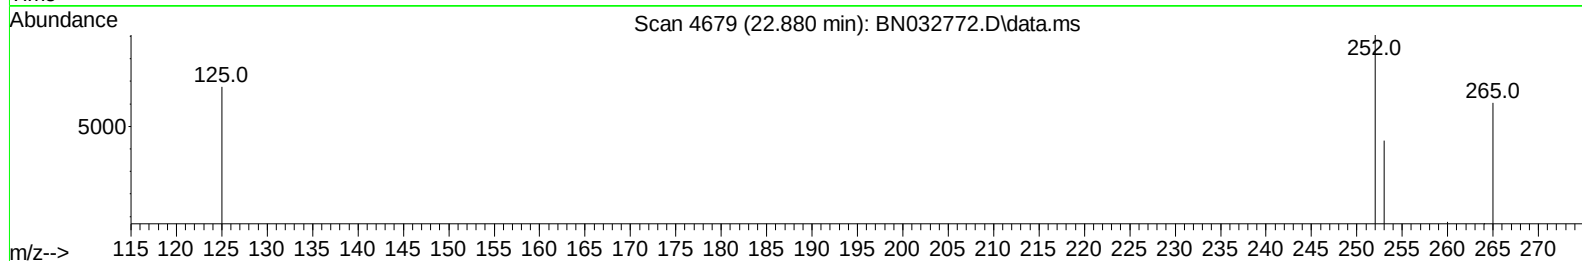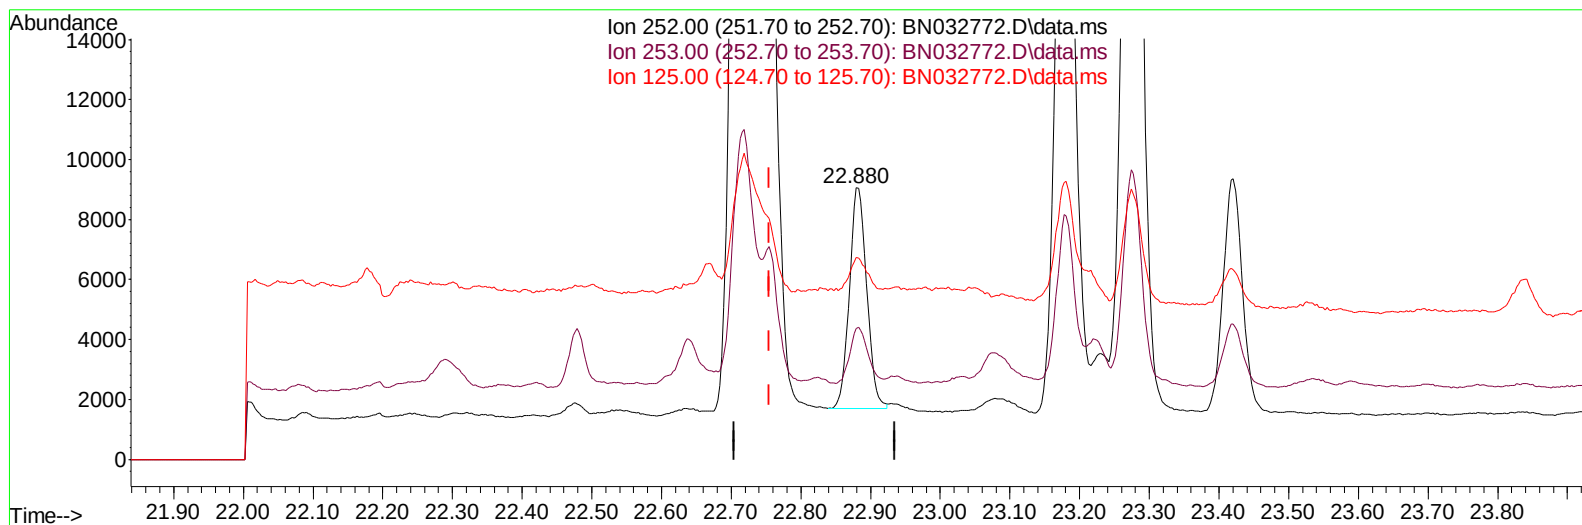

TIC: BN032772.D\data.ms

(25) Benzo(k)fluoranthene

22.880min (+ 0.125) 0.23 ng/u1

response 12706

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	48.13#
125.00	18.50	74.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

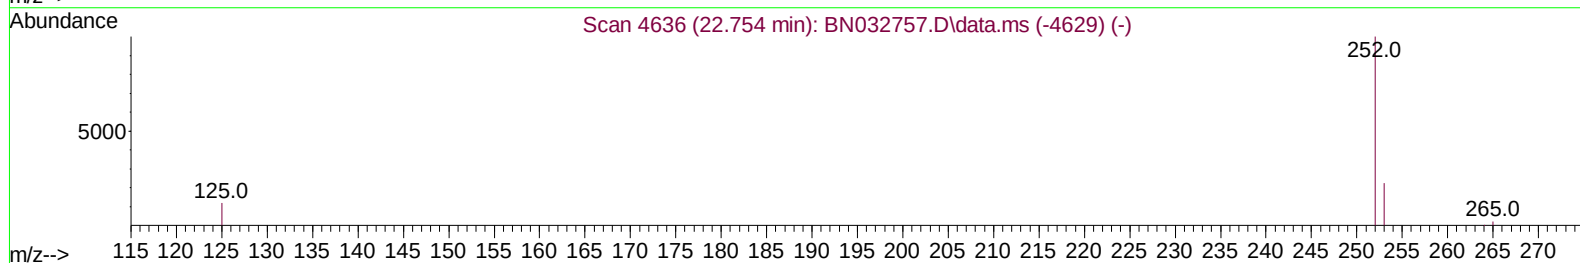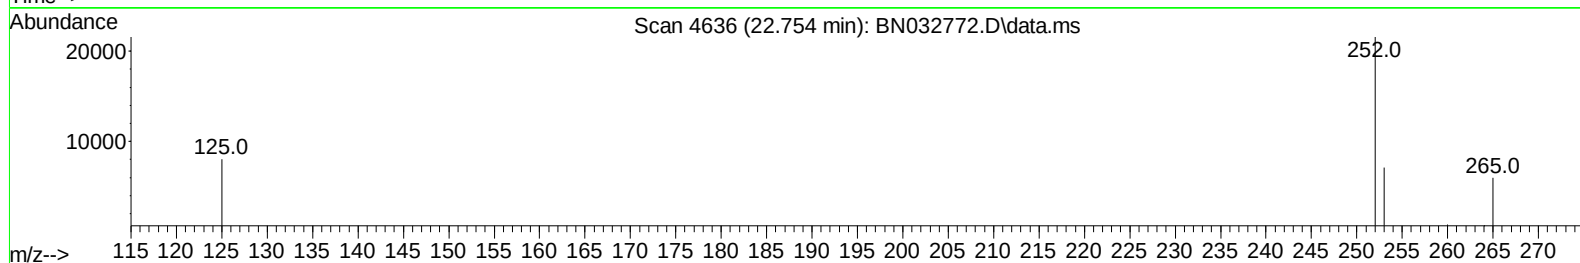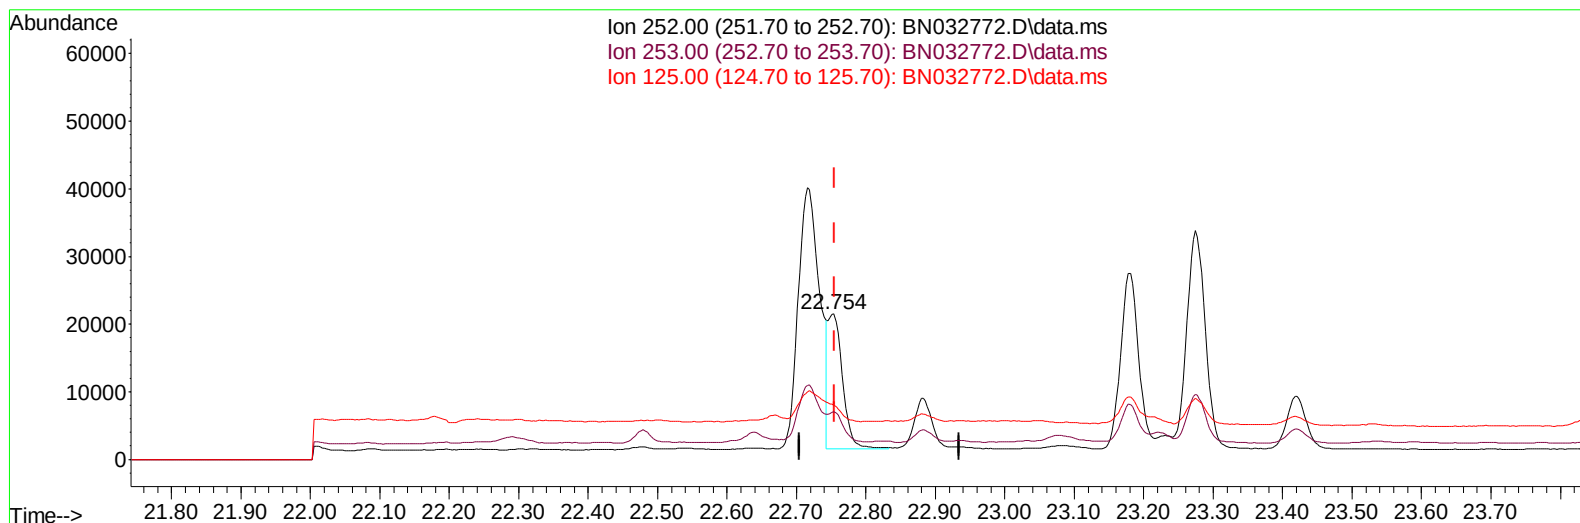

TIC: BN032772.D\data.ms

(25) Benzo(k)fluoranthene

22.754min (-0.001) 0.53 ng/ul m

response 29342

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	32.91#
125.00	18.50	37.23#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
 Data File : BN032772.D
 Acq On : 17 Jul 2024 10:35
 Operator : MA/JU
 Sample : P3177-03
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BS1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 17 11:30:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 17 02:35:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.544	152	3417	0.400	ng/ul	0.00
4) Naphthalene-d8	10.315	136	11866	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.197	164	6547	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.956	188	13876m	0.400	ng/ul	0.00
17) Chrysene-d12	21.173	240	11700m	0.400	ng/ul	0.00
23) Perylene-d12	23.374	264	12886m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	21052	5.131	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.916	152	4736	0.264	ng/ul	-0.02
18) Fluoranthene-d10	18.998	212	9890	0.259	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.365	128	3605	0.113	ng/ul#	93
7) 2-Methylnaphthalene	11.993	142	1510	0.076	ng/ul	95
8) 1-Methylnaphthalene	12.218	142	943	0.046	ng/ul	99
10) Acenaphthylene	13.915	152	7695	0.291	ng/ul	96
11) Acenaphthene	14.257	153	2549	0.117	ng/ul	98
12) Fluorene	15.257	166	3254	0.130	ng/ul#	96
14) Pentachlorophenol	16.636	266	141m	0.058	ng/ul	
15) Phenanthrene	16.999	178	54521m	1.443	ng/ul	
16) Anthracene	17.087	178	13952m	0.452	ng/ul	
19) Fluoranthene	19.031	202	109042	2.292	ng/ul	99
20) Pyrene	19.393	202	107164	2.176	ng/ul	100
21) Benzo(a)anthracene	21.156	228	58022	1.558	ng/ul	94
22) Chrysene	21.208	228	62185m	1.154	ng/ul	
24) Benzo(b)fluoranthene	22.716	252	82974m	1.825	ng/ul	
25) Benzo(k)fluoranthene	22.754	252	29342m	0.530	ng/ul	
26) Benzo(a)pyrene	23.274	252	59642	1.516	ng/ul	96
27) Indeno(1,2,3-cd)pyrene	25.585	276	42605	0.800	ng/ul#	91
28) Dibenzo(a,h)anthracene	25.585	278	10867	0.263	ng/ul#	33
29) Benzo(g,h,i)perylene	26.270	276	44452	0.998	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032772.D
Acq On : 17 Jul 2024 10:35
Operator : MA/JU
Sample : P3177-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BS1

Manual IntegrationsAPPROVED

Quant Time: Jul 17 11:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

